

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD102821\  
 Data File : PD066592.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 28 Oct 2021 00:12  
 Operator : AJ\MA  
 Sample : PCHLORICV500  
 Misc :  
 ALS Vial : 43 Sample Multiplier: 1

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Oct 28 02:01:25 2021  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD102821.M  
 Quant Title : GC Extractables  
 QLast Update : Thu Oct 28 02:00:45 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm



|                             | Compound        | RT#1  | RT#2  | Resp#1   | Resp#2  | ng/ml   | ng/ml   |
|-----------------------------|-----------------|-------|-------|----------|---------|---------|---------|
| -----                       |                 |       |       |          |         |         |         |
| System Monitoring Compounds |                 |       |       |          |         |         |         |
| 1)                          | SA Tetrachlo... | 3.439 | 3.970 | 117.3E6  | 415.4E6 | 52.710  | 51.333  |
| 28)                         | SA Decachlor... | 8.167 | 9.023 | 60177021 | 275.7E6 | 50.793  | 50.707  |
| Target Compounds            |                 |       |       |          |         |         |         |
| 23)                         | Chlordane-1     | 4.302 | 4.959 | 38491100 | 148.1E6 | 520.171 | 533.507 |
| 24)                         | Chlordane-2     | 4.799 | 5.427 | 44812907 | 152.3E6 | 528.241 | 513.294 |
| 25)                         | Chlordane-3     | 5.363 | 6.073 | 129.8E6  | 548.6E6 | 530.121 | 508.782 |
| 26)                         | Chlordane-4     | 5.420 | 6.145 | 107.6E6  | 642.1E6 | 528.091 | 509.510 |
| 27)                         | Chlordane-5     | 6.254 | 6.955 | 43592674 | 141.6E6 | 515.456 | 519.578 |
| -----                       |                 |       |       |          |         |         |         |


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD102821\  
Data File : PD066592.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 28 Oct 2021 00:12  
Operator : AJ\MA  
Sample : PCHLORICV500  
Misc :  
ALS Vial : 43 Sample Multiplier: 1

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Oct 28 02:01:25 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD102821.M  
Quant Title : GC Extractables  
QLast Update : Thu Oct 28 02:00:45 2021  
Response via : Initial Calibration  
Integrator: ChemStation


Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

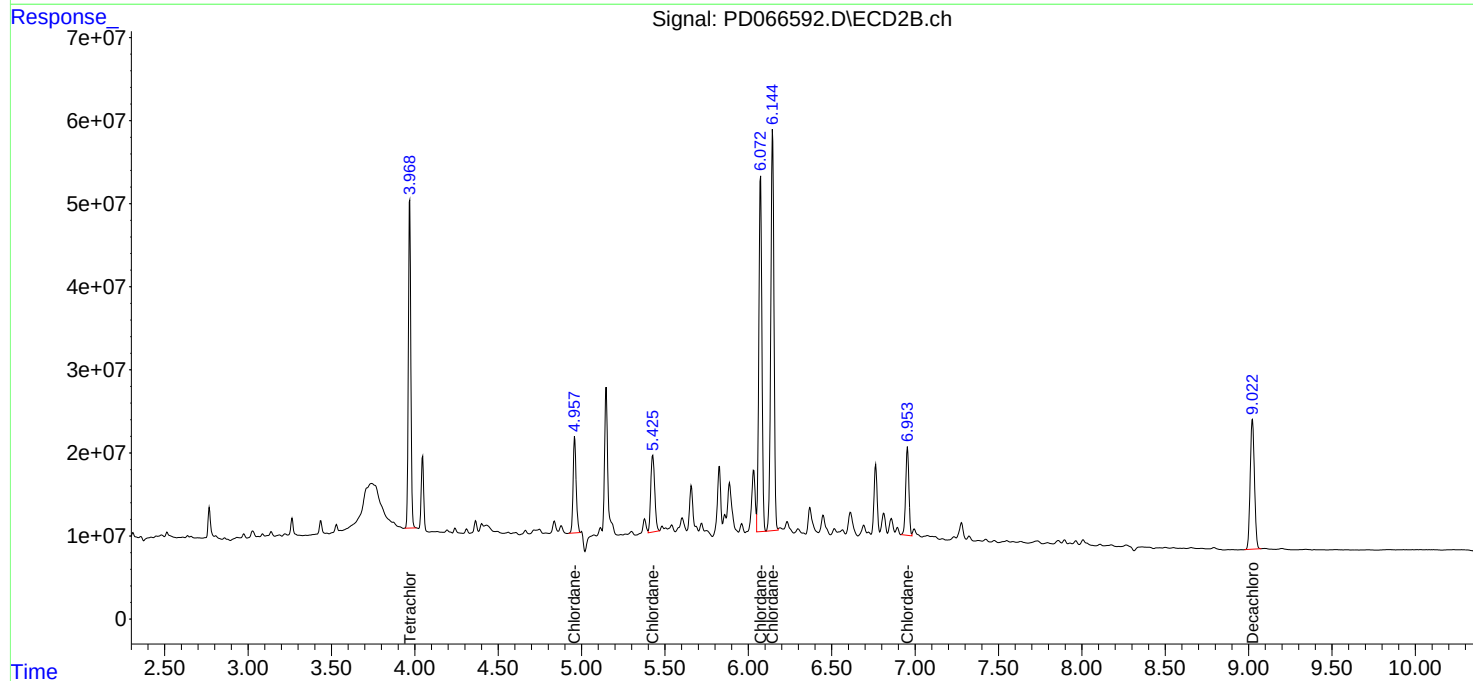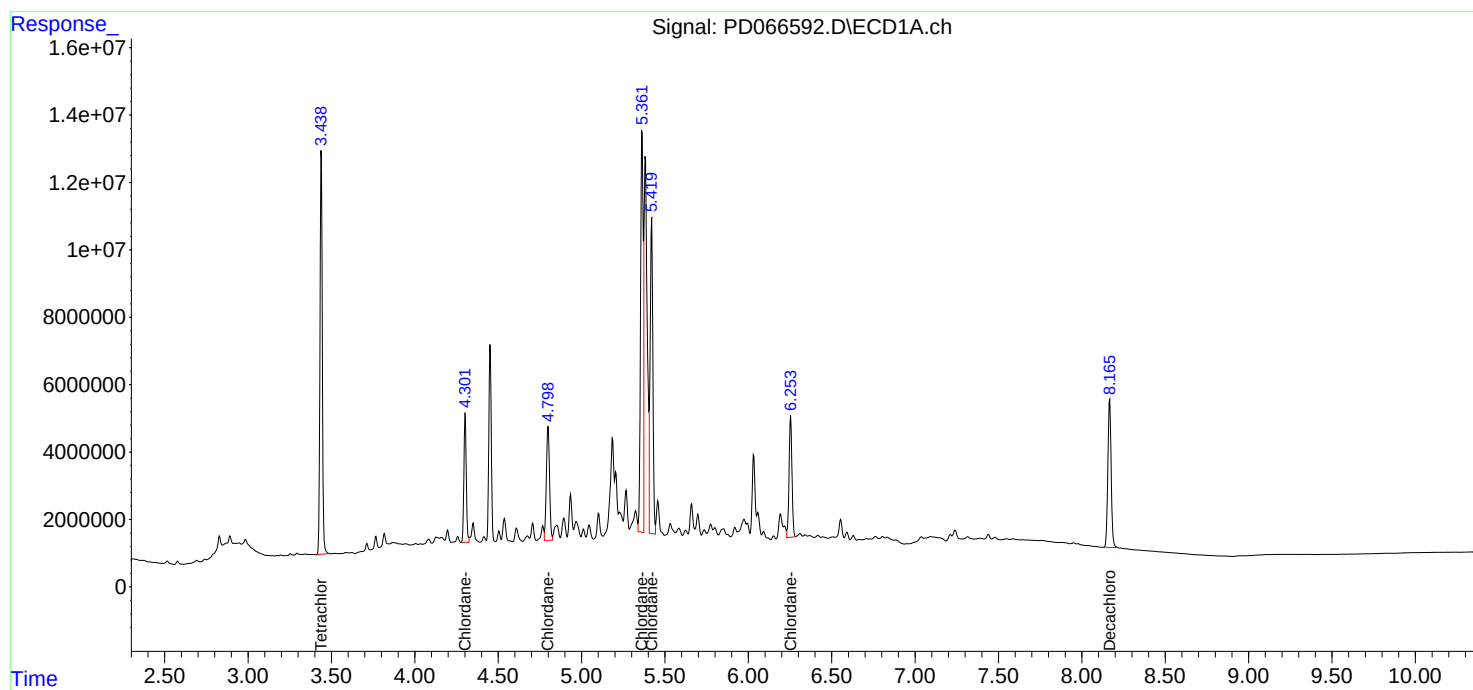

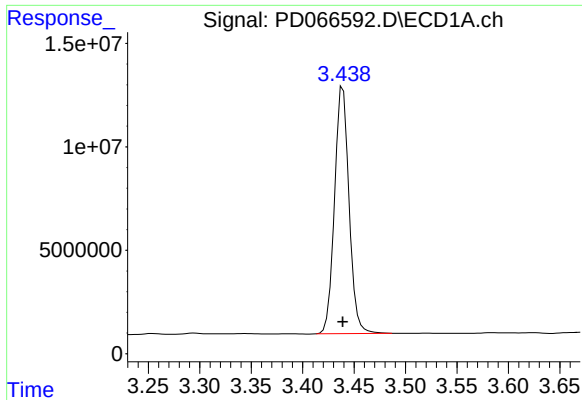


#1 Tetrachloro-m-xylene

R.T.: 3.439 min  
Delta R.T.: 0.000 min  
Response: 117320760  
Conc: 52.71 ng/ml

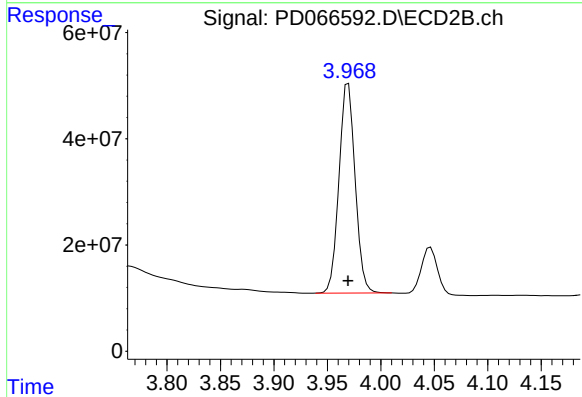


#1 Tetrachloro-m-xylene

R.T.: 3.970 min  
Delta R.T.: 0.000 min  
Response: 415376870  
Conc: 51.33 ng/ml

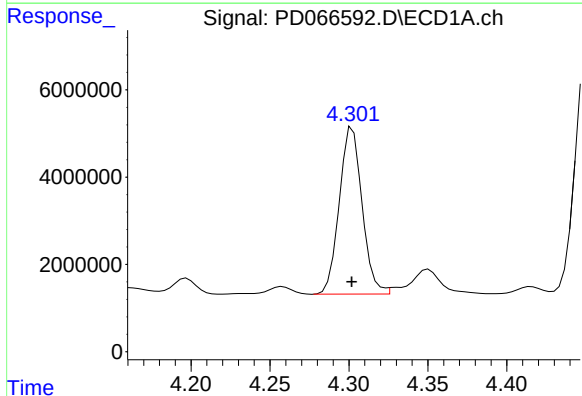


#23 Chlordane-1

R.T.: 4.302 min  
Delta R.T.: 0.000 min  
Response: 38491100  
Conc: 520.17 ng/ml

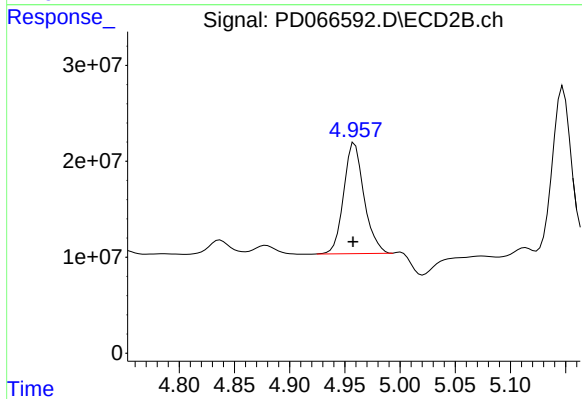


#23 Chlordane-1

R.T.: 4.959 min  
Delta R.T.: 0.001 min  
Response: 148119825  
Conc: 533.51 ng/ml

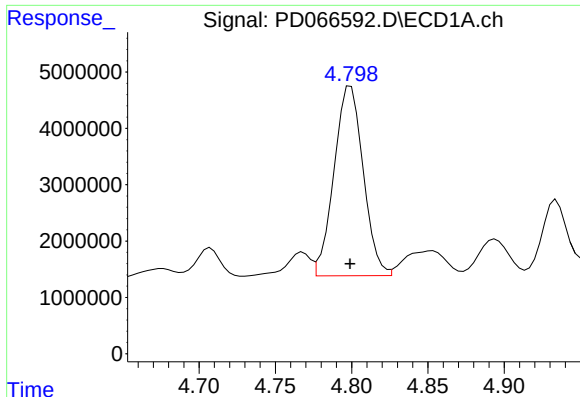


#24 Chlordane-2

R.T.: 4.799 min  
Delta R.T.: 0.000 min  
Response: 44812907  
Conc: 528.24 ng/ml

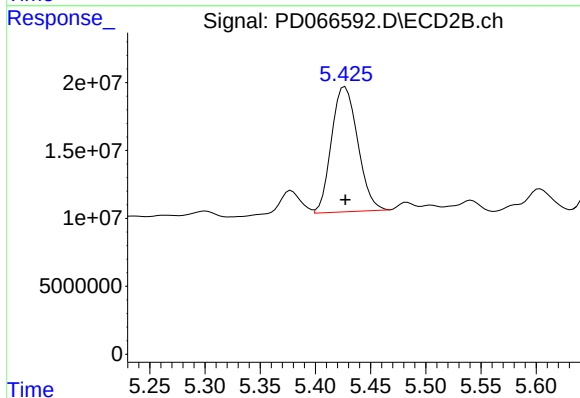


#24 Chlordane-2

R.T.: 5.427 min  
Delta R.T.: 0.000 min  
Response: 152252767  
Conc: 513.29 ng/ml

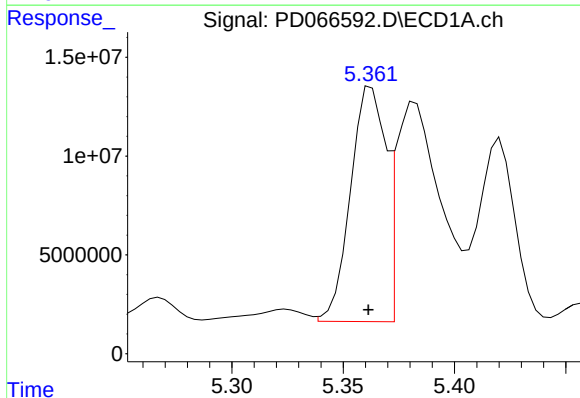


#25 Chlordane-3

R.T.: 5.363 min  
Delta R.T.: 0.001 min  
Response: 129797718  
Conc: 530.12 ng/ml

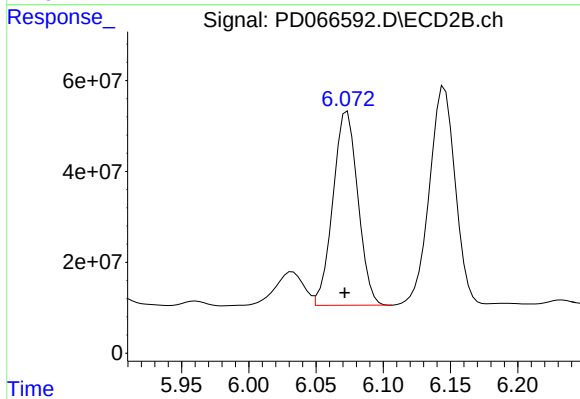


#25 Chlordane-3

R.T.: 6.073 min  
Delta R.T.: 0.002 min  
Response: 548554946  
Conc: 508.78 ng/ml

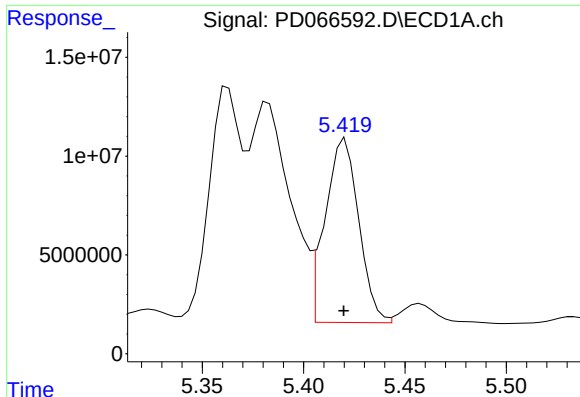


#26 Chlordane-4

R.T.: 5.420 min  
Delta R.T.: 0.000 min  
Response: 107572116  
Conc: 528.09 ng/ml

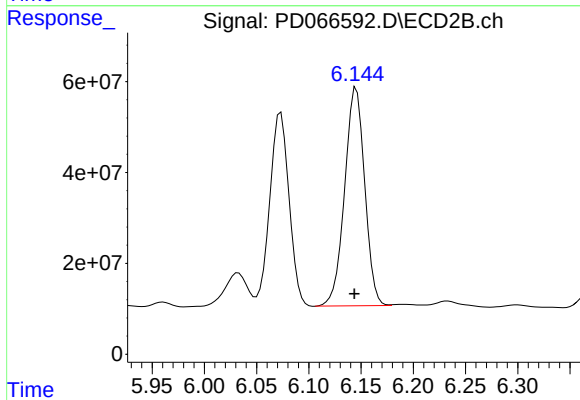


#26 Chlordane-4

R.T.: 6.145 min  
Delta R.T.: 0.002 min  
Response: 642097249  
Conc: 509.51 ng/ml

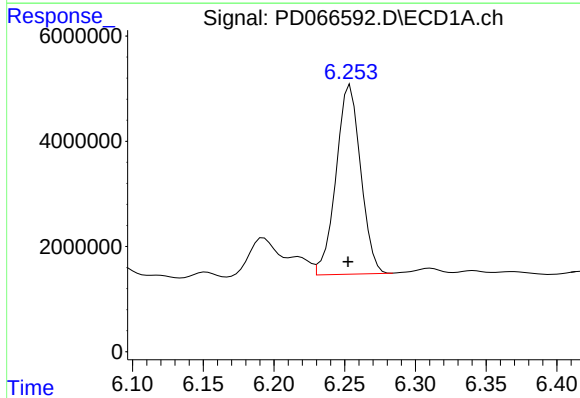


#27 Chlordane-5

R.T.: 6.254 min  
Delta R.T.: 0.002 min  
Response: 43592674  
Conc: 515.46 ng/ml

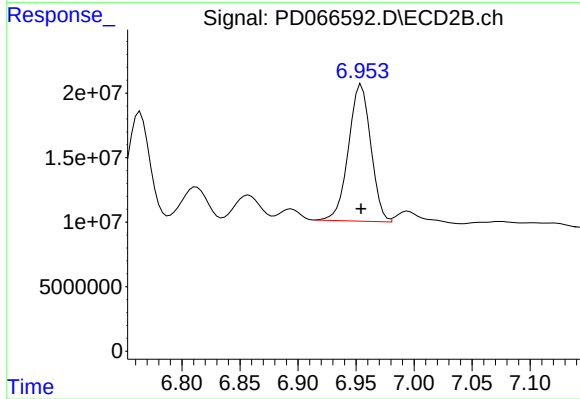


#27 Chlordane-5

R.T.: 6.955 min  
Delta R.T.: 0.000 min  
Response: 141602004  
Conc: 519.58 ng/ml

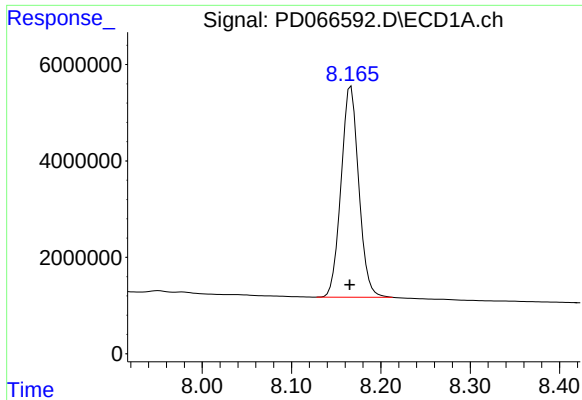

#28 Decachlorobiphenyl

R.T.: 8.167 min  
Delta R.T.: 0.001 min  
Response: 60177021  
Conc: 50.79 ng/ml

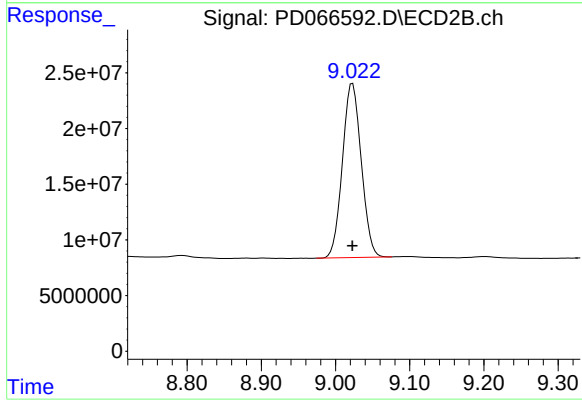

#28 Decachlorobiphenyl

R.T.: 9.023 min  
Delta R.T.: 0.000 min  
Response: 275718308  
Conc: 50.71 ng/ml