

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102821\
 Data File : PD066581.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Oct 2021 21:40
 Operator : AJ\MA
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 01:41:12 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102821.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 28 01:40:01 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.439	3.970	223.0E6	726.9E6	97.884	91.173
28)	SA Decachlor...	8.167	9.023	106.6E6	487.4E6	90.487	90.319
Target Compounds							
23)	Chlordane-1	4.302	4.959	73442826	271.3E6	996.928	962.775
24)	Chlordane-2	4.799	5.427	81018884	265.4E6	1002.044	900.439
25)	Chlordane-3	5.362	6.073	250.0E6	997.6E6	1001.166	942.674
26)	Chlordane-4	5.420	6.145	204.1E6	1160.5E6	974.812	953.671
27)	Chlordane-5	6.254	6.954	79955586	254.7E6	902.533	895.647



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102821\
Data File : PD066581.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Oct 2021 21:40
Operator : AJ\MA
Sample : PCHLORICC1000
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 01:41:12 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102821.M
Quant Title : GC Extractables
QLast Update : Thu Oct 28 01:40:01 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

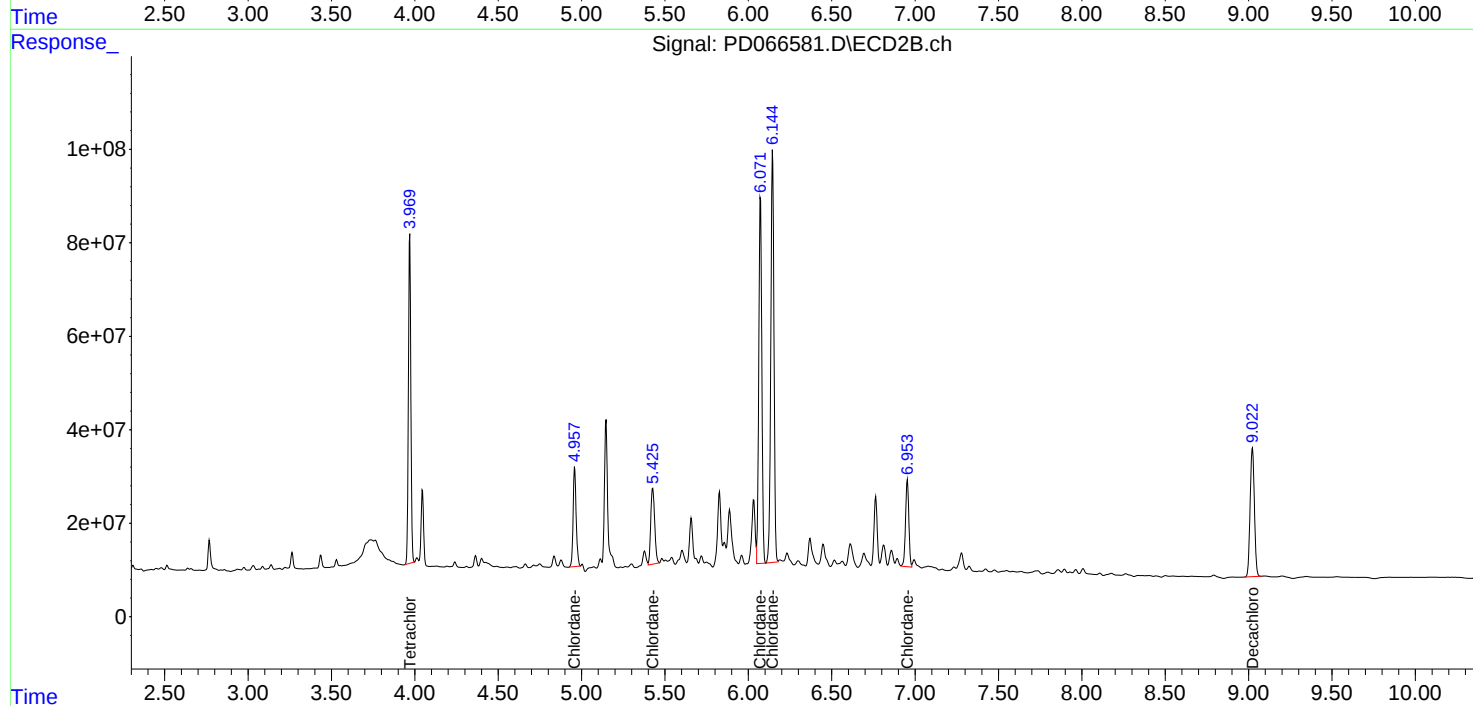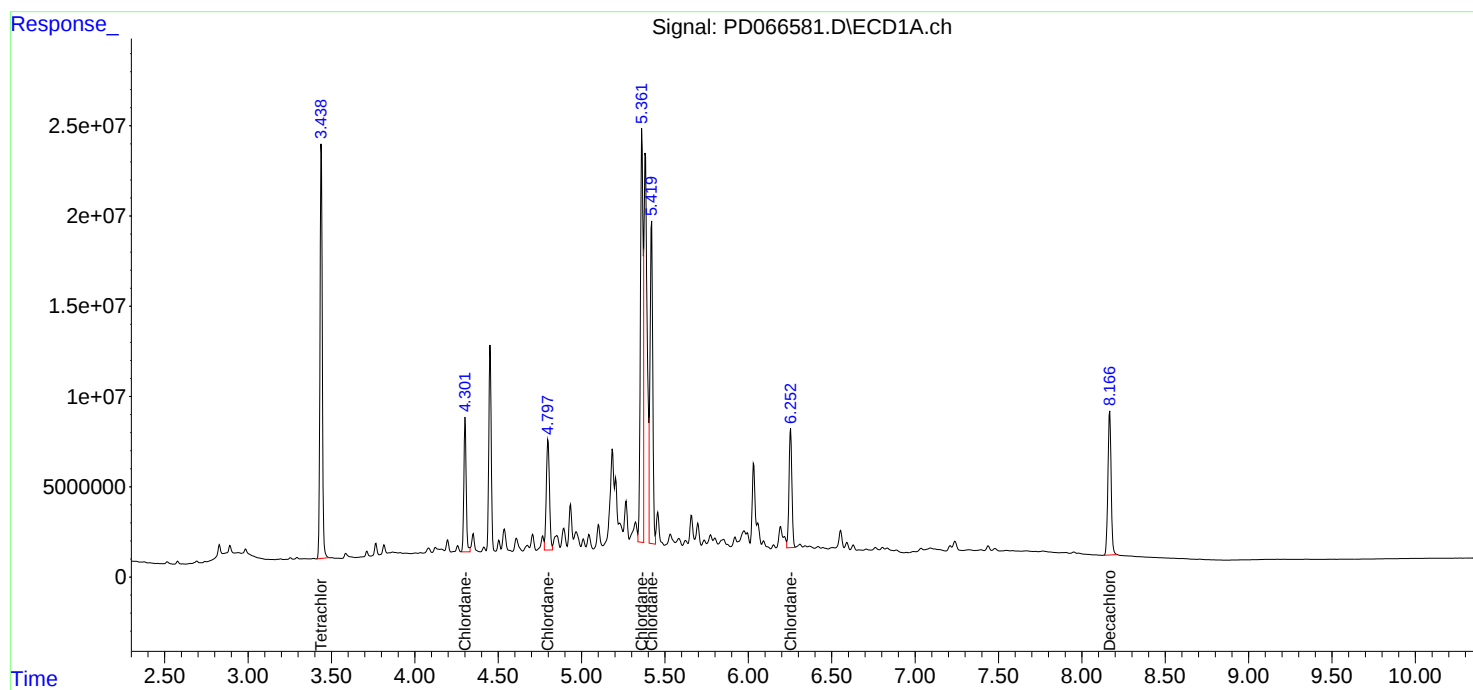


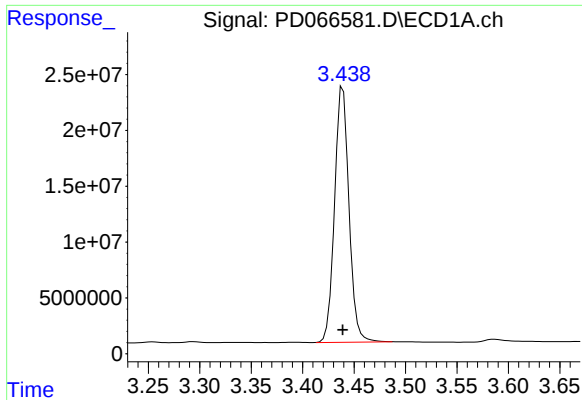

#1 Tetrachloro-m-xylene


R.T.: 3.439 min
Delta R.T.: 0.000 min
Response: 222975162
Conc: 97.88 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

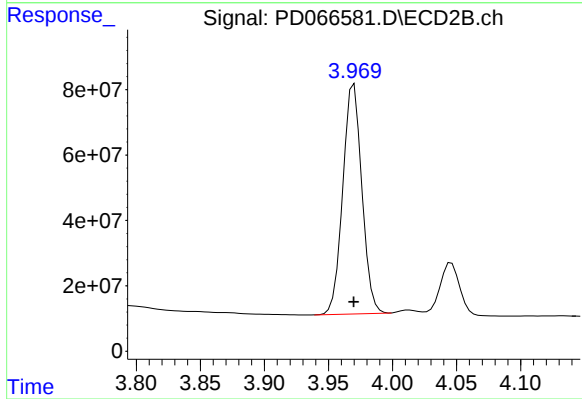


#1 Tetrachloro-m-xylene

R.T.: 3.970 min
Delta R.T.: 0.000 min
Response: 726868536
Conc: 91.17 ng/ml

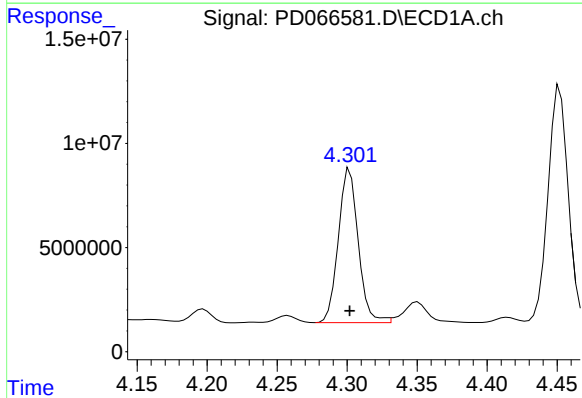


#23 Chlordane-1

R.T.: 4.302 min
Delta R.T.: 0.000 min
Response: 73442826
Conc: 996.93 ng/ml

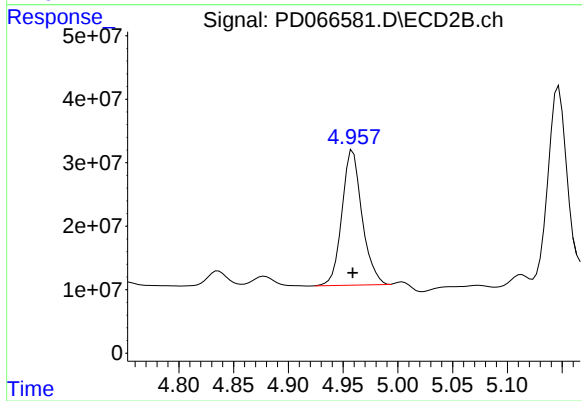

#23 Chlordane-1


R.T.: 4.959 min
Delta R.T.: 0.000 min
Response: 271274625
Conc: 962.77 ng/ml

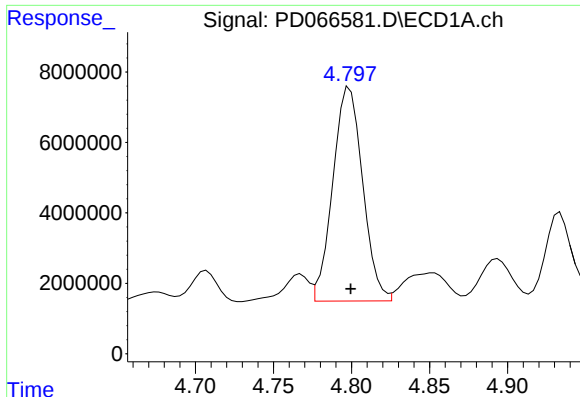

#24 Chlordane-2


R.T.: 4.799 min
Delta R.T.: 0.000 min
Response: 81018884
Conc: 1002.04 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

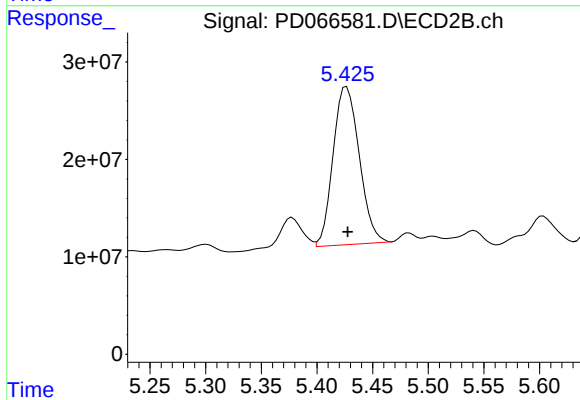


#24 Chlordane-2

R.T.: 5.427 min
Delta R.T.: 0.000 min
Response: 265427070
Conc: 900.44 ng/ml

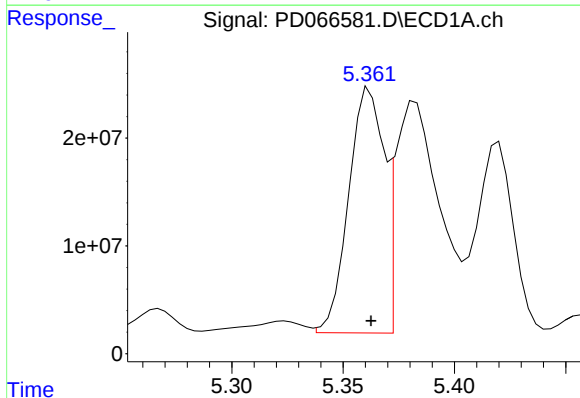


#25 Chlordane-3

R.T.: 5.362 min
Delta R.T.: 0.000 min
Response: 249989669
Conc: 1001.17 ng/ml

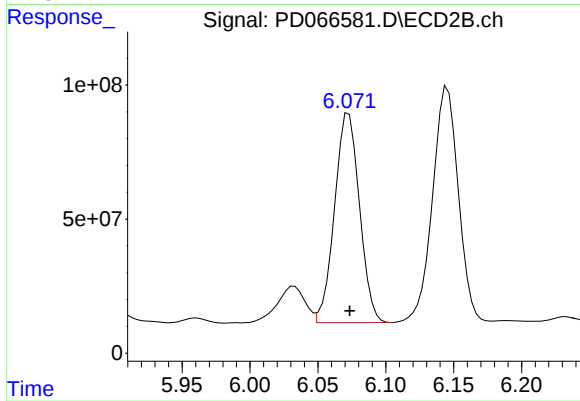

#25 Chlordane-3


R.T.: 6.073 min
Delta R.T.: 0.000 min
Response: 997583874
Conc: 942.67 ng/ml

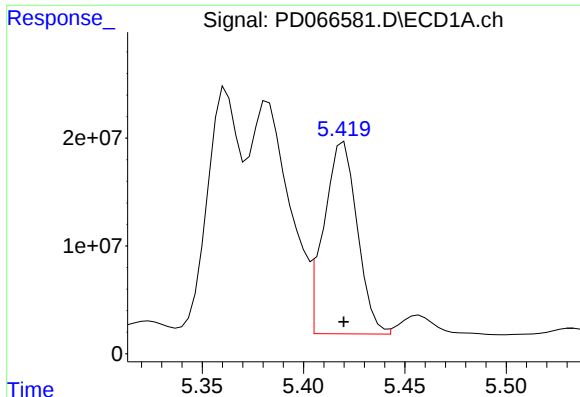

#26 Chlordane-4


R.T.: 5.420 min
Delta R.T.: 0.000 min
Response: 204090108
Conc: 974.81 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

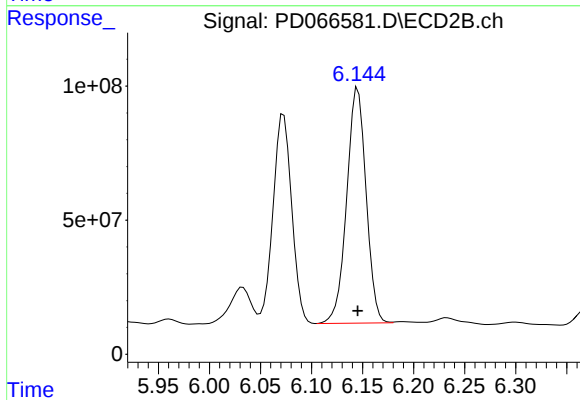


#26 Chlordane-4

R.T.: 6.145 min
Delta R.T.: 0.000 min
Response: 1160451318
Conc: 953.67 ng/ml

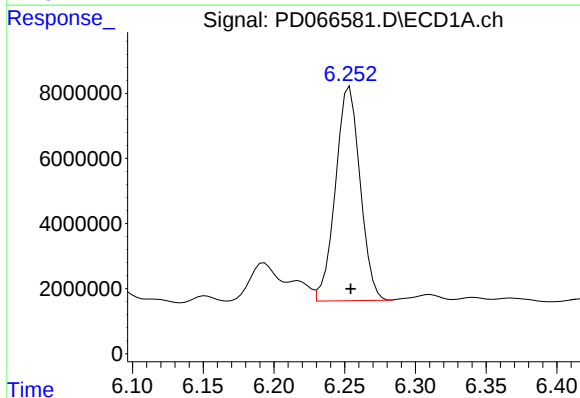


#27 Chlordane-5

R.T.: 6.254 min
Delta R.T.: 0.000 min
Response: 79955586
Conc: 902.53 ng/ml

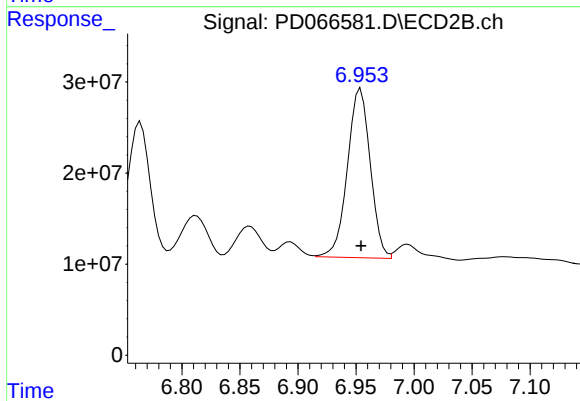

#27 Chlordane-5


R.T.: 6.954 min
Delta R.T.: 0.000 min
Response: 254704851
Conc: 895.65 ng/ml

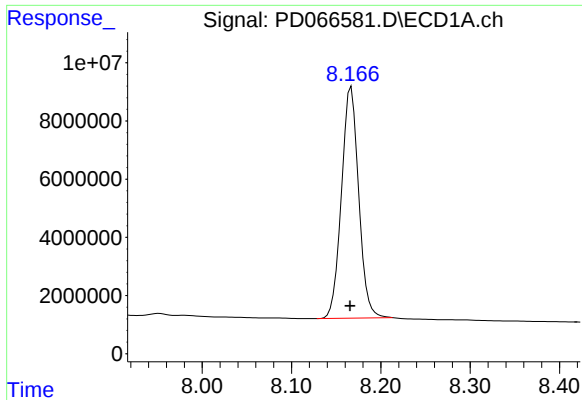

#28 Decachlorobiphenyl

R.T.: 8.167 min
Delta R.T.: 0.001 min
Response: 106615642
Conc: 90.49 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

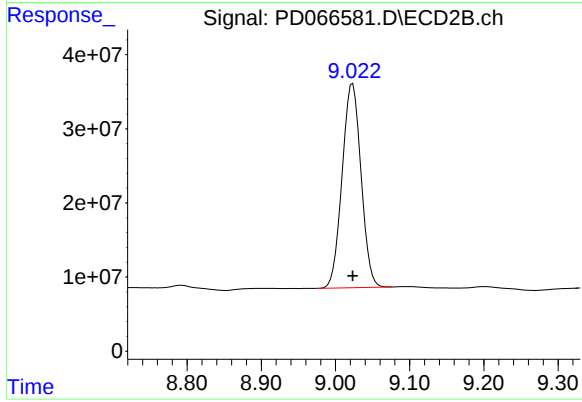

#28 Decachlorobiphenyl

R.T.: 9.023 min
Delta R.T.: 0.000 min
Response: 487416062
Conc: 90.32 ng/ml