

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102821\
 Data File : PD066582.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Oct 2021 21:54
 Operator : AJ\MA
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 01:41:19 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102821.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 28 01:40:01 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.439	3.969	160.7E6	545.7E6	70.554	68.452
28)	SA Decachlor...	8.166	9.023	79864578	367.1E6	67.783	68.022
Target Compounds							
23)	Chlordane-1	4.302	4.959	53338946	200.4E6	724.034	711.192
24)	Chlordane-2	4.800	5.427	59949381	200.9E6	741.456	681.589
25)	Chlordane-3	5.362	6.073	180.2E6	737.3E6	721.700	696.737
26)	Chlordane-4	5.421	6.145	147.2E6	858.7E6	703.102	705.717
27)	Chlordane-5	6.254	6.955	58826891	189.5E6	664.034	666.506



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102821\
Data File : PD066582.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Oct 2021 21:54
Operator : AJ\MA
Sample : PCHLORICC750
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 01:41:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102821.M
Quant Title : GC Extractables
QLast Update : Thu Oct 28 01:40:01 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

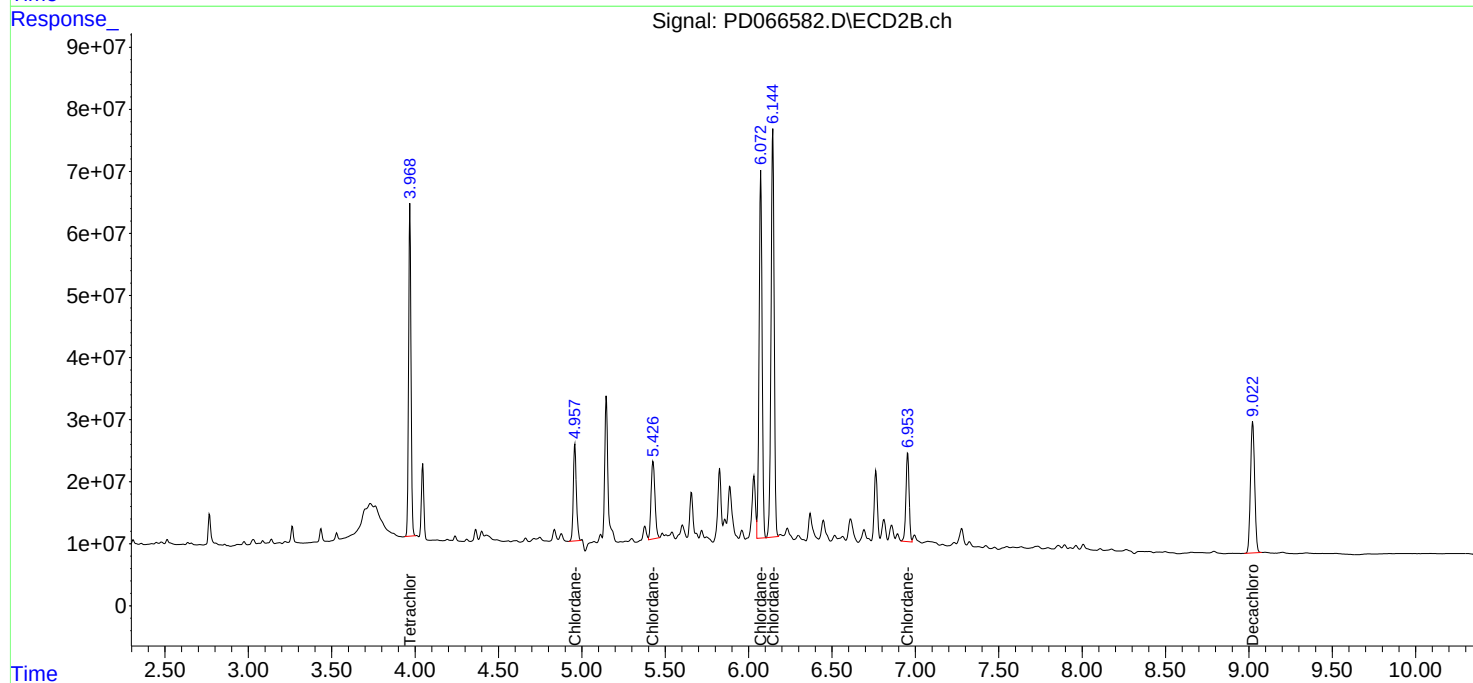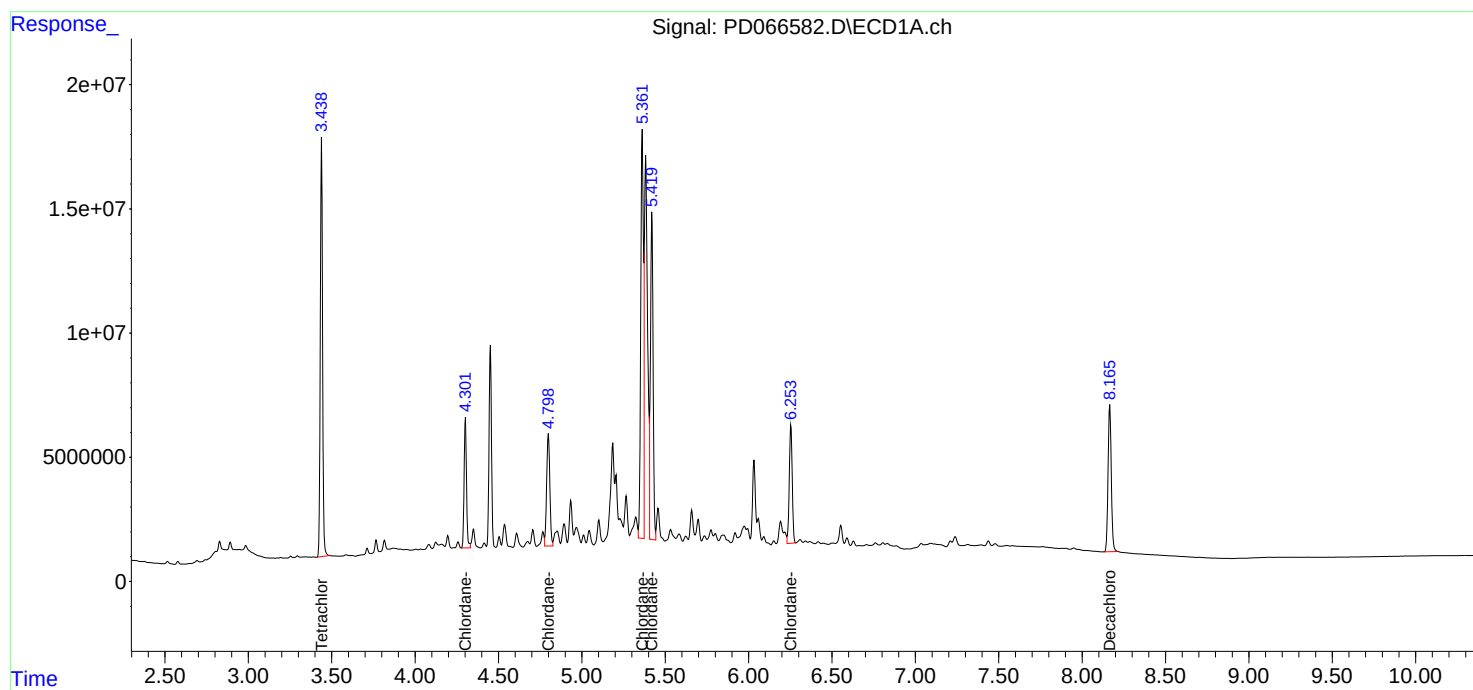


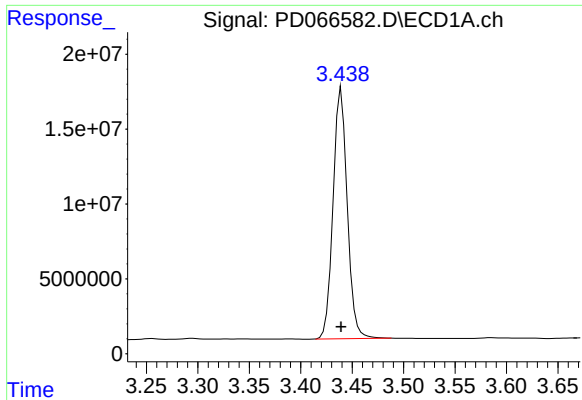

#1 Tetrachloro-m-xylene


R.T.: 3.439 min
Delta R.T.: 0.000 min
Response: 160717789
Conc: 70.55 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

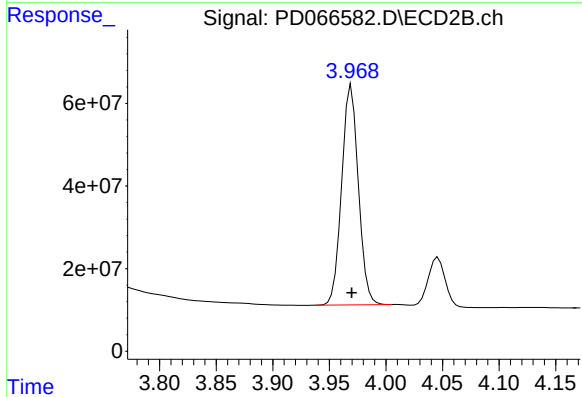


#1 Tetrachloro-m-xylene

R.T.: 3.969 min
Delta R.T.: 0.000 min
Response: 545728586
Conc: 68.45 ng/ml

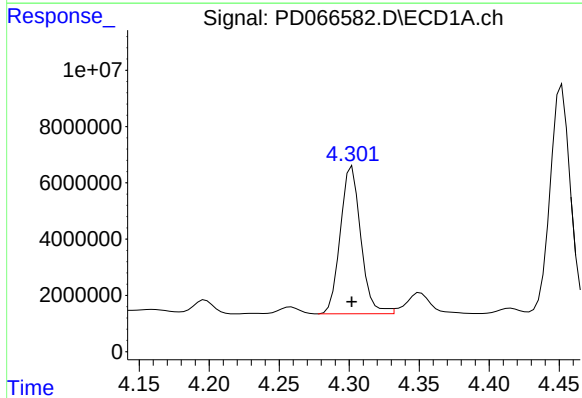


#23 Chlordane-1

R.T.: 4.302 min
Delta R.T.: 0.000 min
Response: 53338946
Conc: 724.03 ng/ml

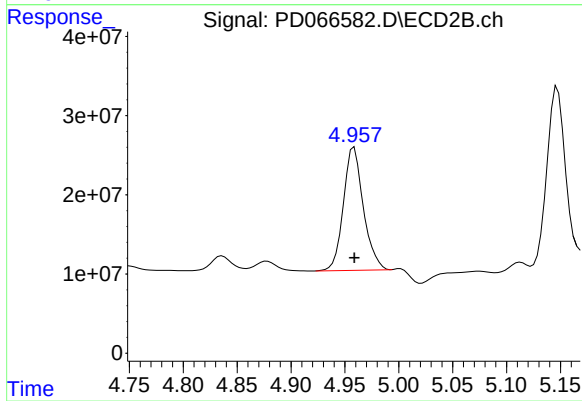

#23 Chlordane-1


R.T.: 4.959 min
Delta R.T.: 0.000 min
Response: 200387865
Conc: 711.19 ng/ml

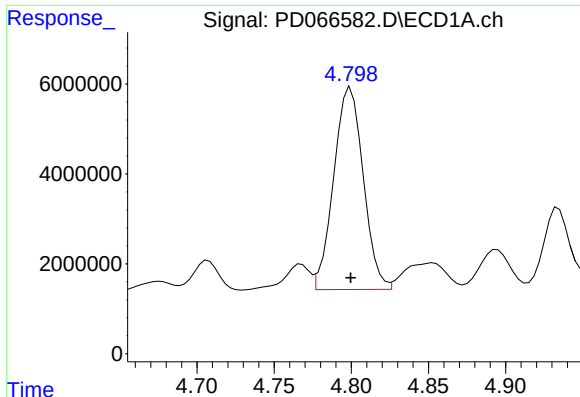

#24 Chlordane-2


R.T.: 4.800 min
Delta R.T.: 0.000 min
Response: 59949381
Conc: 741.46 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

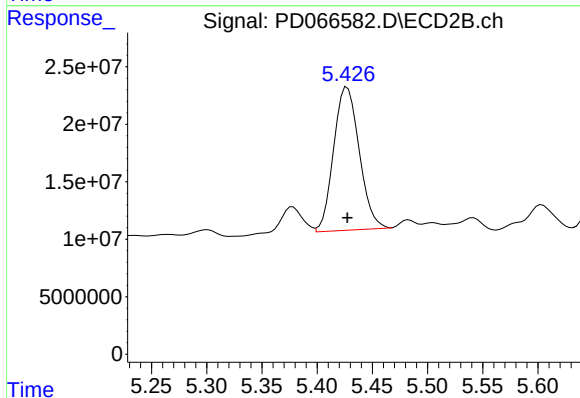


#24 Chlordane-2

R.T.: 5.427 min
Delta R.T.: 0.000 min
Response: 200915501
Conc: 681.59 ng/ml

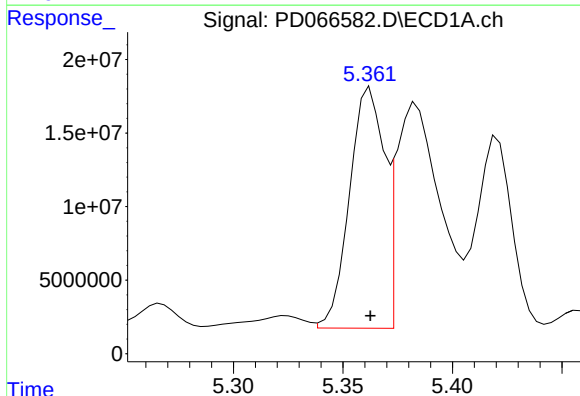


#25 Chlordane-3

R.T.: 5.362 min
Delta R.T.: 0.000 min
Response: 180207396
Conc: 721.70 ng/ml

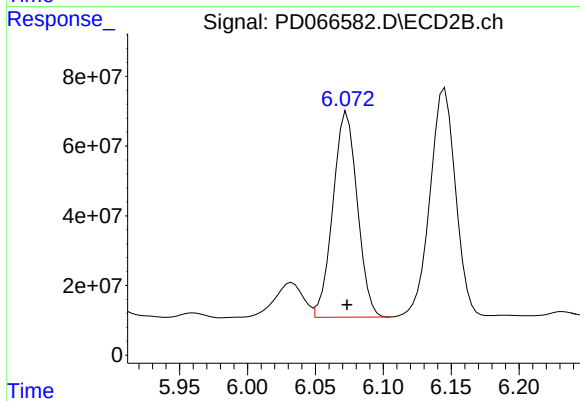

#25 Chlordane-3


R.T.: 6.073 min
Delta R.T.: 0.000 min
Response: 737321663
Conc: 696.74 ng/ml

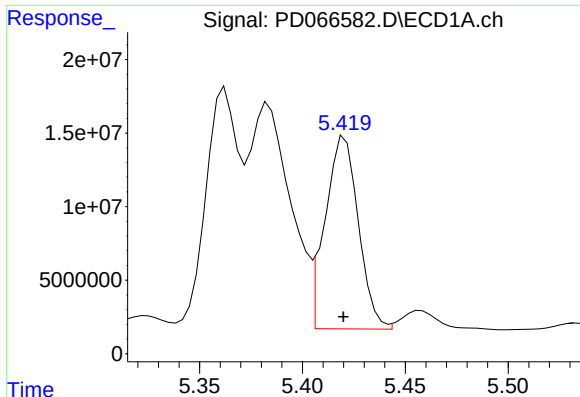

#26 Chlordane-4


R.T.: 5.421 min
Delta R.T.: 0.000 min
Response: 147203837
Conc: 703.10 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

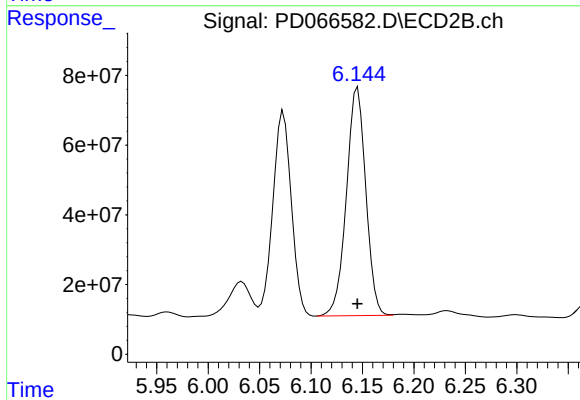


#26 Chlordane-4

R.T.: 6.145 min
Delta R.T.: 0.000 min
Response: 858733587
Conc: 705.72 ng/ml

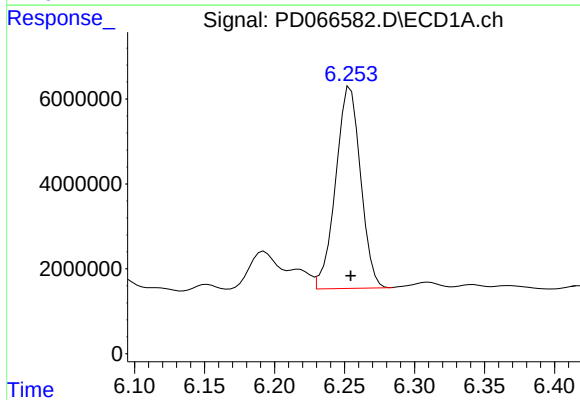


#27 Chlordane-5

R.T.: 6.254 min
Delta R.T.: 0.000 min
Response: 58826891
Conc: 664.03 ng/ml

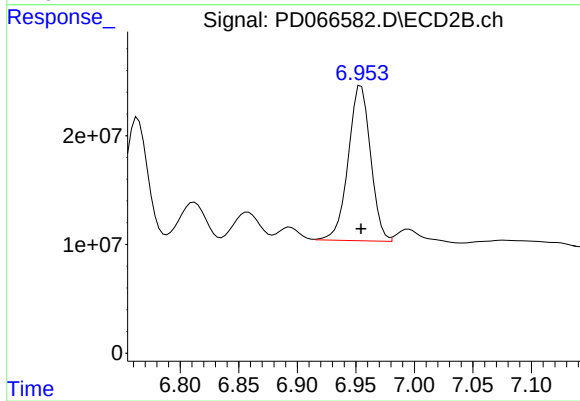

#27 Chlordane-5


R.T.: 6.955 min
Delta R.T.: 0.000 min
Response: 189541343
Conc: 666.51 ng/ml

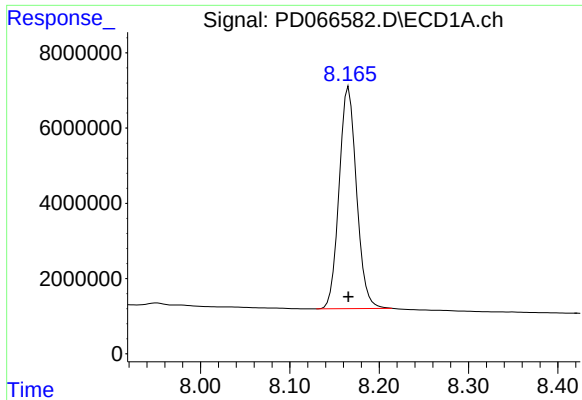

#28 Decachlorobiphenyl

R.T.: 8.166 min
Delta R.T.: 0.000 min
Response: 79864578
Conc: 67.78 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

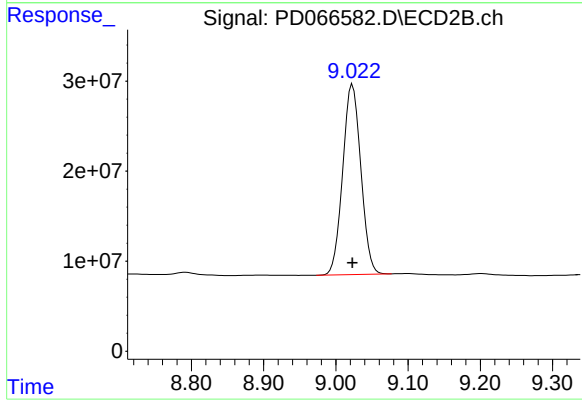

#28 Decachlorobiphenyl

R.T.: 9.023 min
Delta R.T.: 0.000 min
Response: 367084069
Conc: 68.02 ng/ml