

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102821\
 Data File : PD066583.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Oct 2021 22:08
 Operator : AJ\MA
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 01:41:28 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102821.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 28 01:40:01 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.439	3.970	113.9E6	398.6E6	50.000	50.000
28)	SA Decachlor...	8.166	9.023	58911868	269.8E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.302	4.959	36834583	140.9E6	500.000	500.000
24)	Chlordane-2	4.800	5.428	40426805	147.4E6	500.000	500.000
25)	Chlordane-3	5.363	6.073	124.8E6	529.1E6	500.000	500.000
26)	Chlordane-4	5.420	6.145	104.7E6	608.4E6	500.000	500.000
27)	Chlordane-5	6.254	6.954	44295088	142.2E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102821\
Data File : PD066583.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Oct 2021 22:08
Operator : AJ\MA
Sample : PCHLORICC500
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 01:41:28 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102821.M
Quant Title : GC Extractables
QLast Update : Thu Oct 28 01:40:01 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

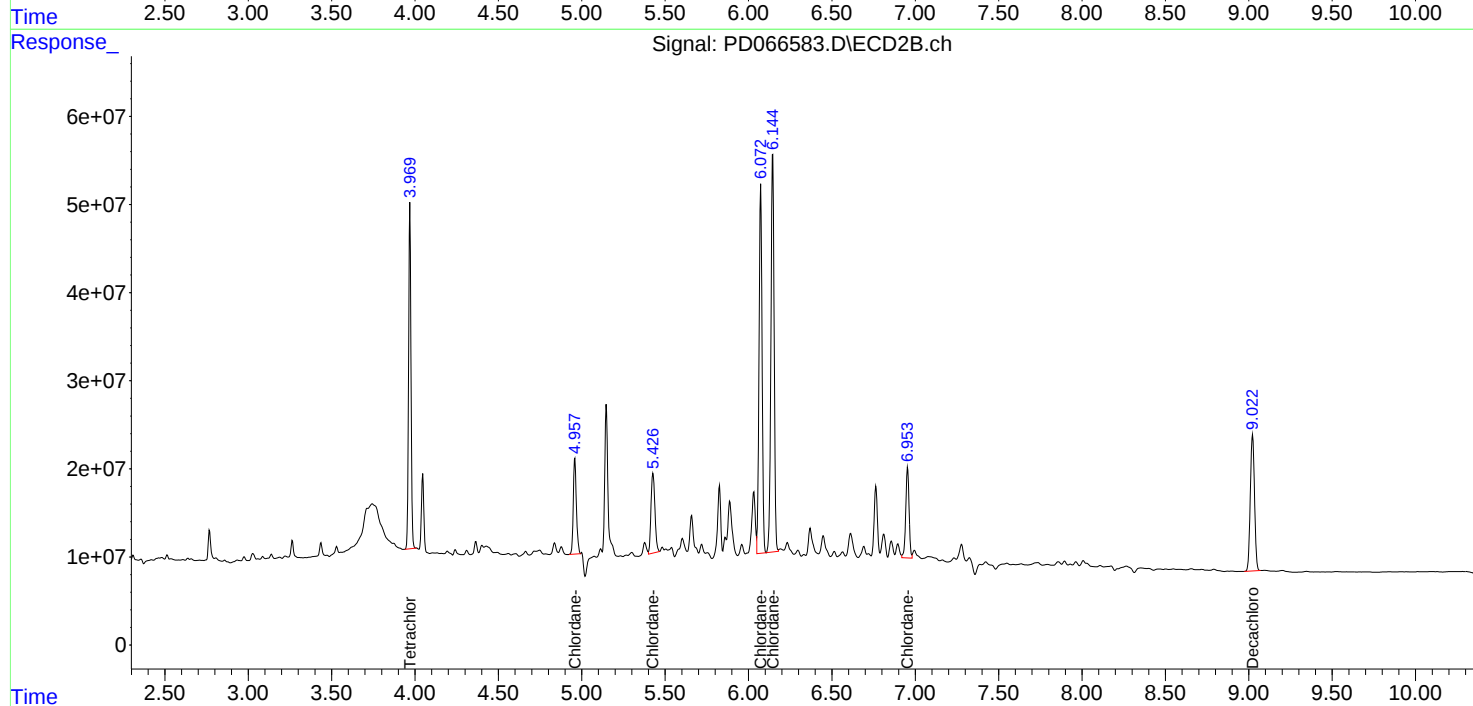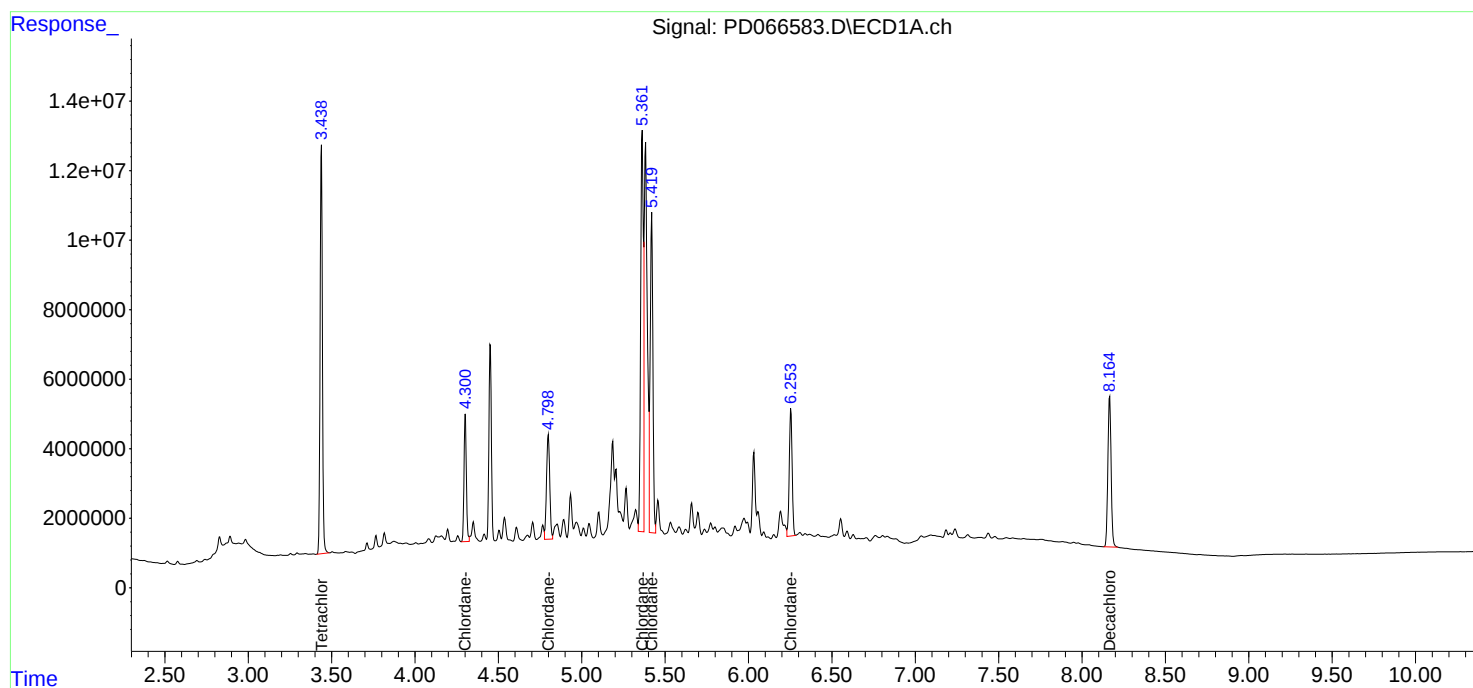


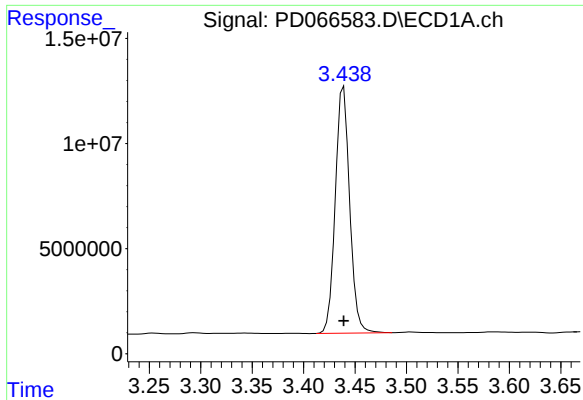

#1 Tetrachloro-m-xylene


R.T.: 3.439 min
Delta R.T.: 0.000 min
Response: 113897218
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

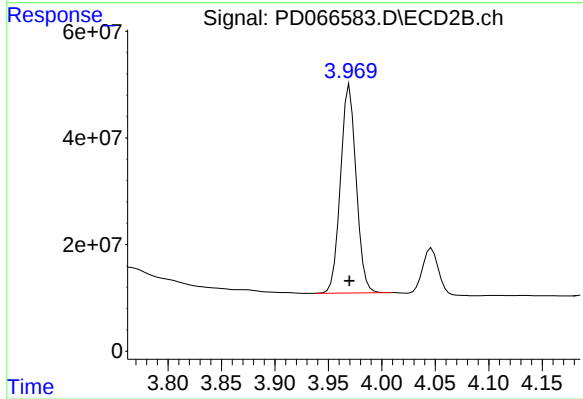


#1 Tetrachloro-m-xylene

R.T.: 3.970 min
Delta R.T.: 0.000 min
Response: 398621037
Conc: 50.00 ng/ml

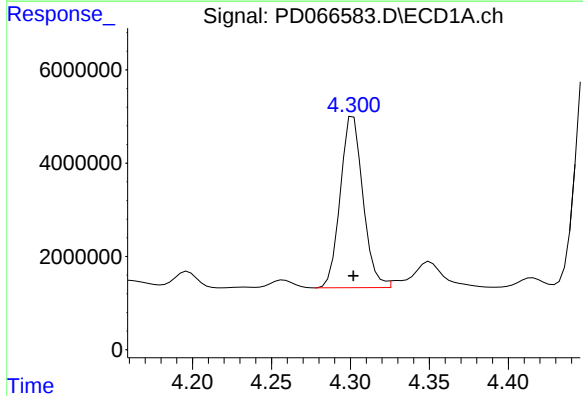


#23 Chlordane-1

R.T.: 4.302 min
Delta R.T.: 0.000 min
Response: 36834583
Conc: 500.00 ng/ml

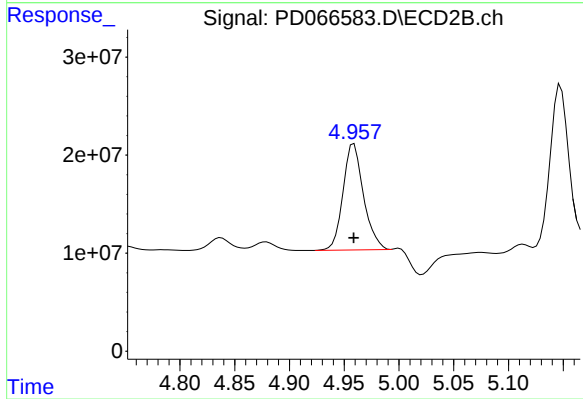

#23 Chlordane-1


R.T.: 4.959 min
Delta R.T.: 0.000 min
Response: 140881693
Conc: 500.00 ng/ml

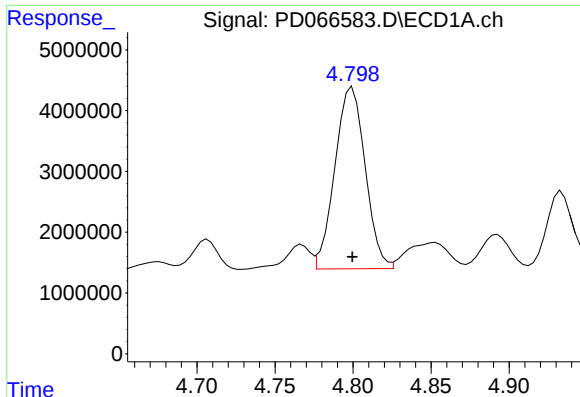

#24 Chlordane-2


R.T.: 4.800 min
Delta R.T.: 0.000 min
Response: 40426805
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

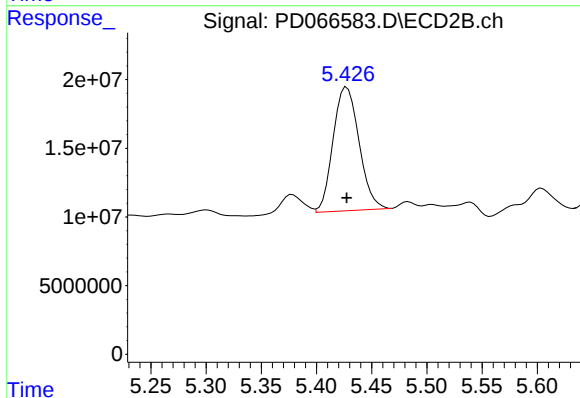


#24 Chlordane-2

R.T.: 5.428 min
Delta R.T.: 0.000 min
Response: 147387633
Conc: 500.00 ng/ml

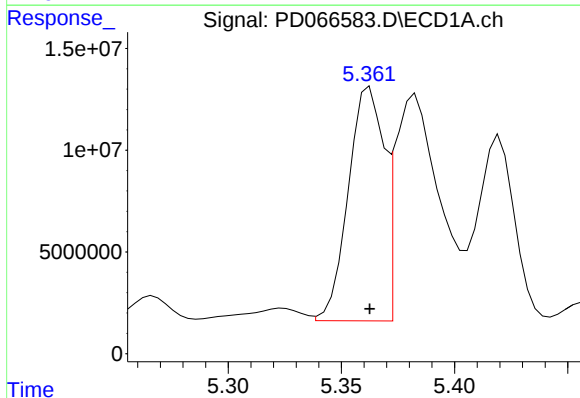


#25 Chlordane-3

R.T.: 5.363 min
Delta R.T.: 0.000 min
Response: 124849304
Conc: 500.00 ng/ml

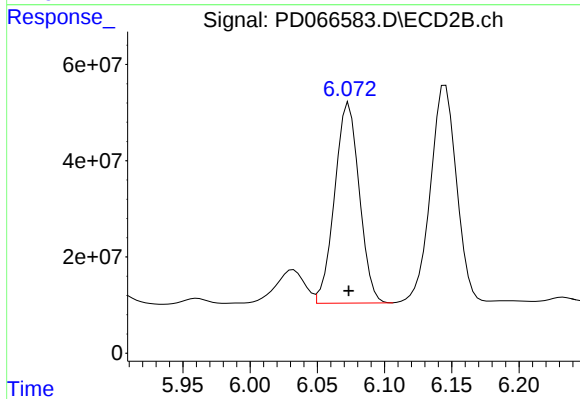

#25 Chlordane-3


R.T.: 6.073 min
Delta R.T.: 0.000 min
Response: 529124585
Conc: 500.00 ng/ml

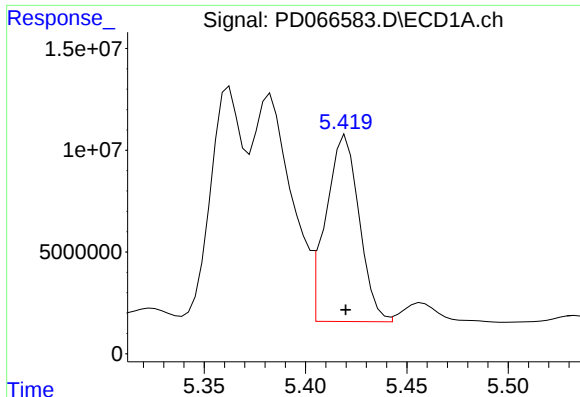

#26 Chlordane-4


R.T.: 5.420 min
Delta R.T.: 0.000 min
Response: 104681732
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

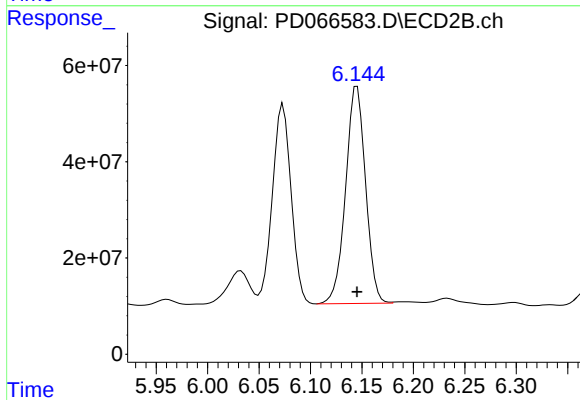


#26 Chlordane-4

R.T.: 6.145 min
Delta R.T.: 0.000 min
Response: 608412543
Conc: 500.00 ng/ml

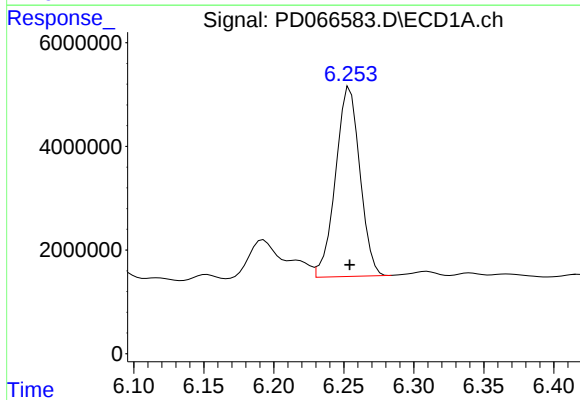


#27 Chlordane-5

R.T.: 6.254 min
Delta R.T.: 0.000 min
Response: 44295088
Conc: 500.00 ng/ml

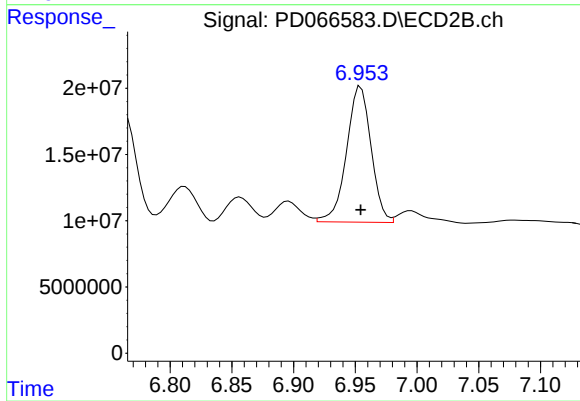

#27 Chlordane-5


R.T.: 6.954 min
Delta R.T.: 0.000 min
Response: 142190366
Conc: 500.00 ng/ml

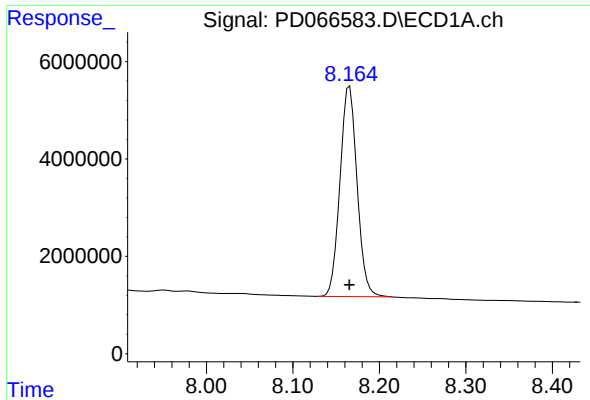

#28 Decachlorobiphenyl

R.T.: 8.166 min
Delta R.T.: 0.000 min
Response: 58911868
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

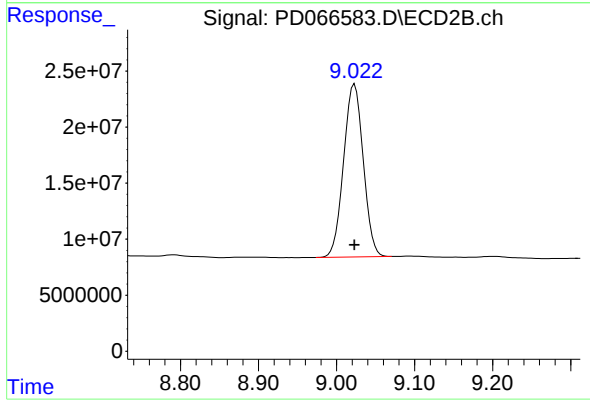

#28 Decachlorobiphenyl

R.T.: 9.023 min
Delta R.T.: 0.000 min
Response: 269829012
Conc: 50.00 ng/ml