

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102821\
 Data File : PD066584.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Oct 2021 22:22
 Operator : AJ\MA
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 01:41:34 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102821.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 28 01:40:01 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.439	3.969	54317125	206.6E6	23.845	25.910
28)	SA Decachlor...	8.166	9.022	29943161	138.1E6	25.414	25.592
Target Compounds							
23)	Chlordane-1	4.302	4.958	18165613	72960677	246.584	258.943
24)	Chlordane-2	4.799	5.427	22207265	76952235	274.660	261.054
25)	Chlordane-3	5.362	6.072	60229617	269.8E6	241.209	254.982
26)	Chlordane-4	5.420	6.145	50479351	318.1E6	241.109	261.390
27)	Chlordane-5	6.252	6.954	20899264	69515070	235.909	244.444



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102821\
Data File : PD066584.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Oct 2021 22:22
Operator : AJ\MA
Sample : PCHLORICC250
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 01:41:34 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102821.M
Quant Title : GC Extractables
QLast Update : Thu Oct 28 01:40:01 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

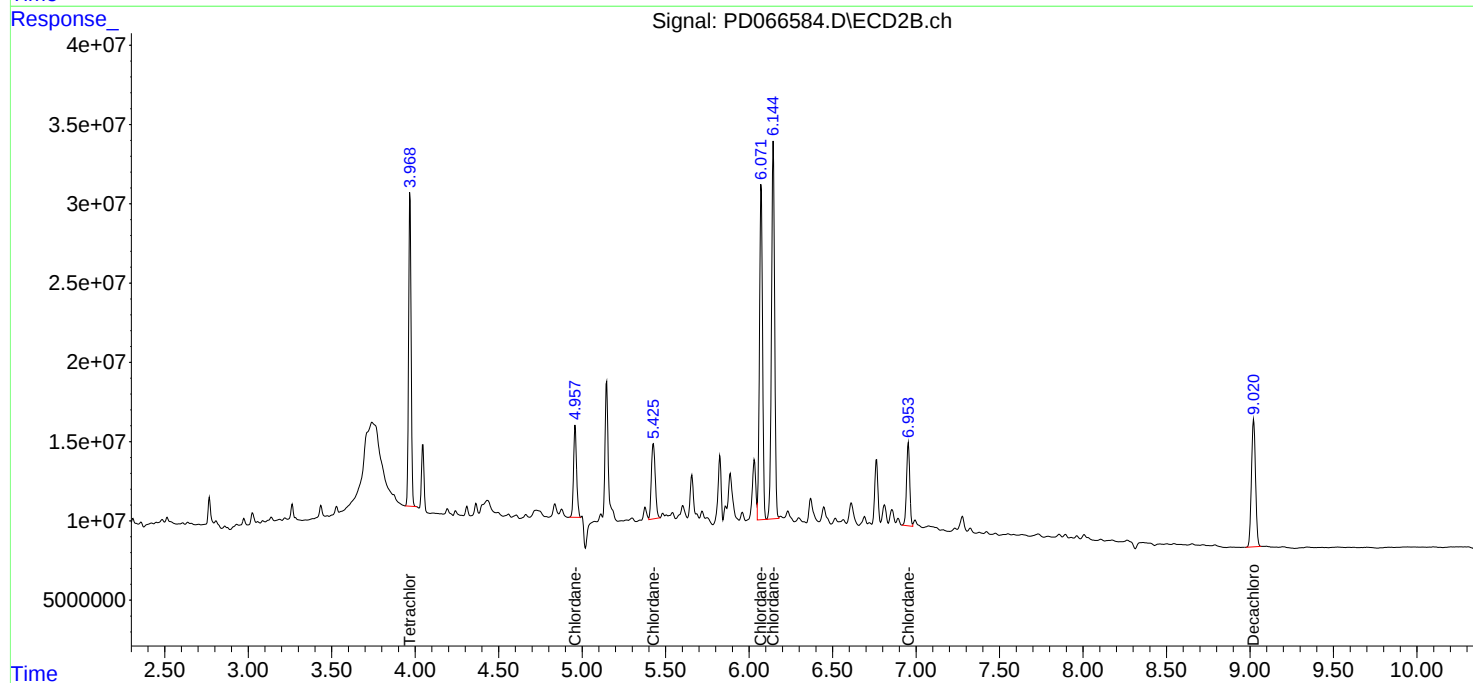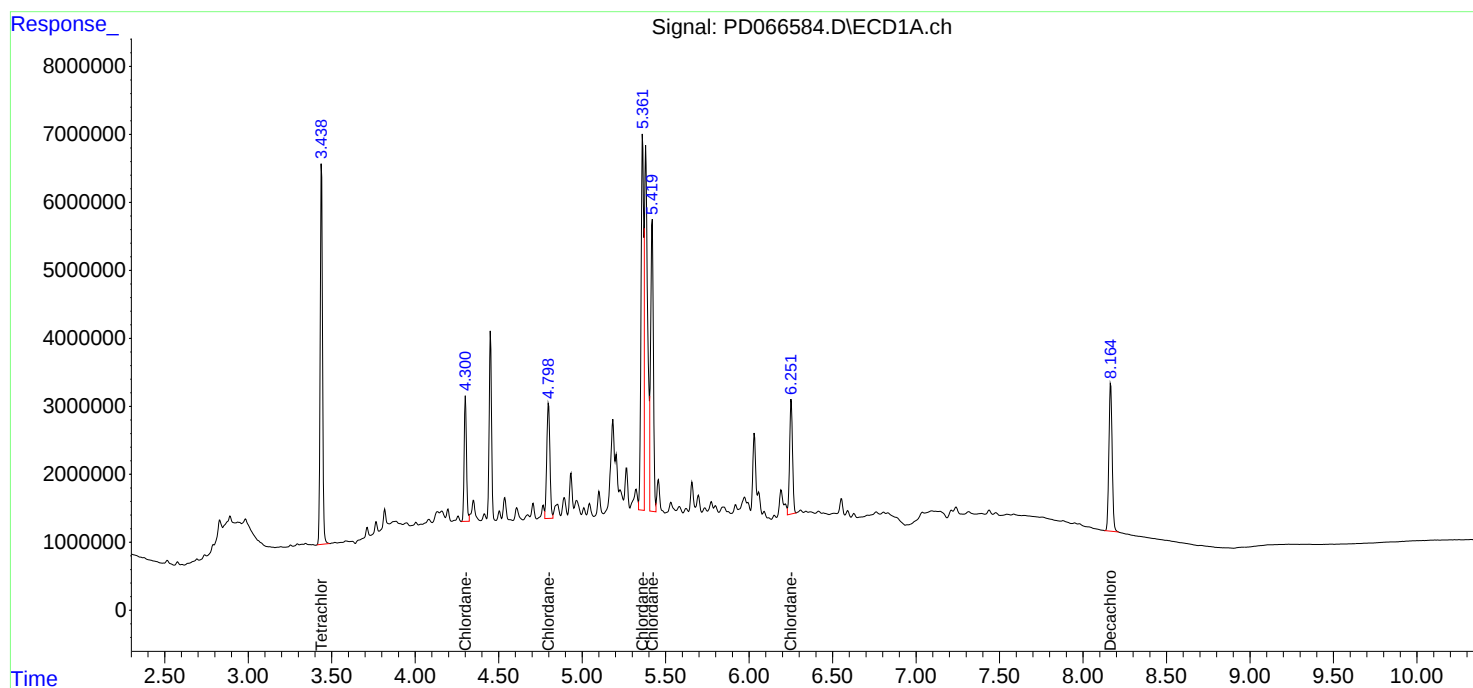


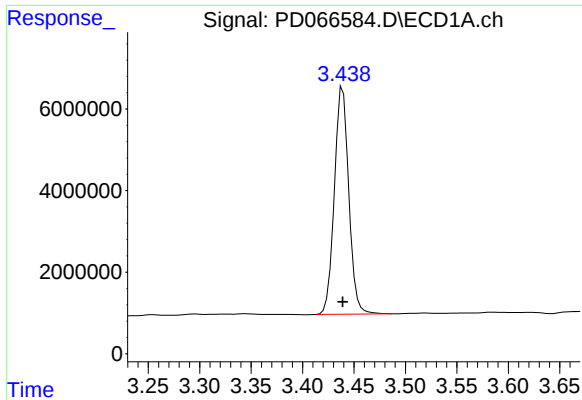

#1 Tetrachloro-m-xylene


R.T.: 3.439 min
Delta R.T.: 0.000 min
Response: 54317125
Conc: 23.84 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

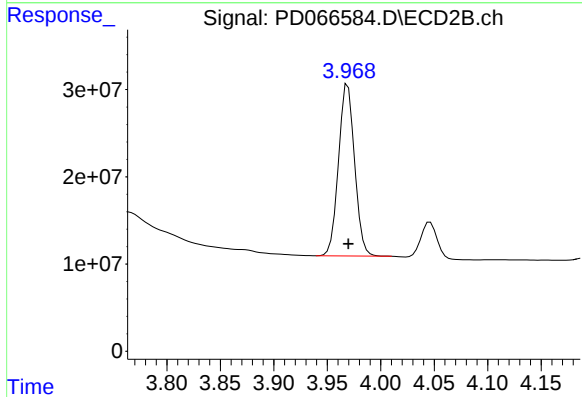


#1 Tetrachloro-m-xylene

R.T.: 3.969 min
Delta R.T.: 0.000 min
Response: 206568833
Conc: 25.91 ng/ml

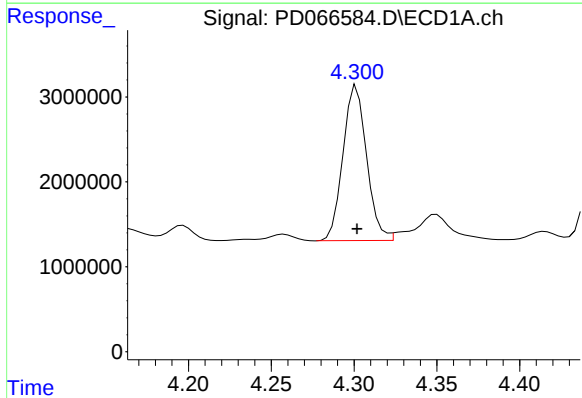


#23 Chlordane-1

R.T.: 4.302 min
Delta R.T.: 0.000 min
Response: 18165613
Conc: 246.58 ng/ml

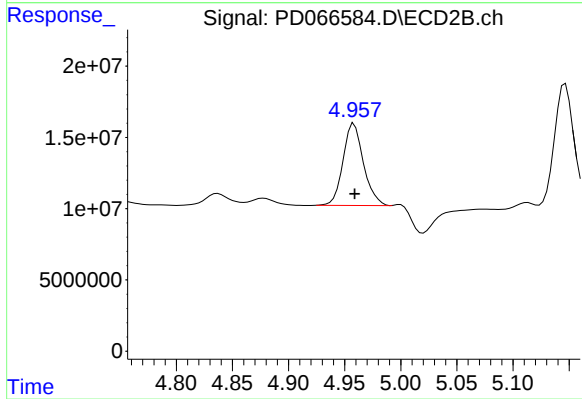

#23 Chlordane-1


R.T.: 4.958 min
Delta R.T.: 0.000 min
Response: 72960677
Conc: 258.94 ng/ml

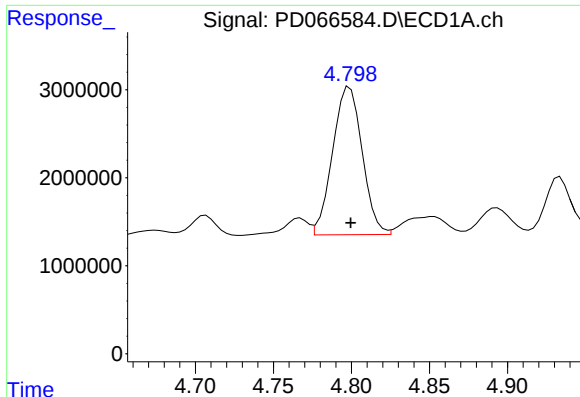

#24 Chlordane-2


R.T.: 4.799 min
Delta R.T.: 0.000 min
Response: 22207265
Conc: 274.66 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

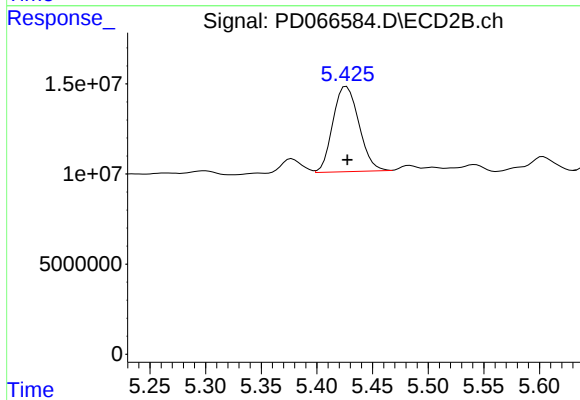


#24 Chlordane-2

R.T.: 5.427 min
Delta R.T.: 0.000 min
Response: 76952235
Conc: 261.05 ng/ml

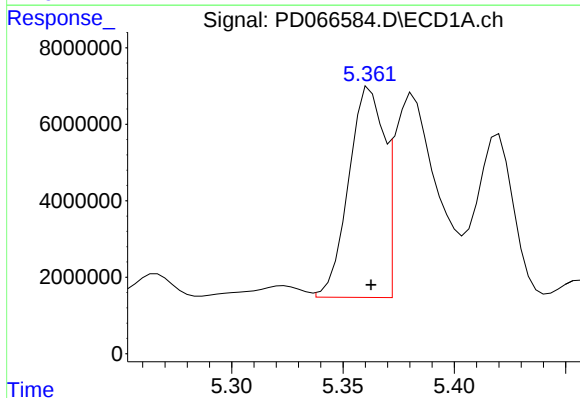


#25 Chlordane-3

R.T.: 5.362 min
Delta R.T.: 0.000 min
Response: 60229617
Conc: 241.21 ng/ml

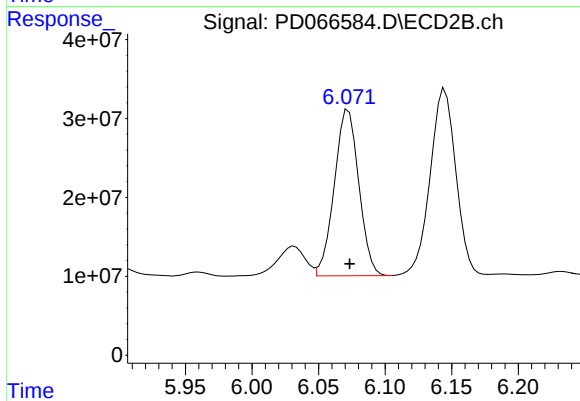

#25 Chlordane-3


R.T.: 6.072 min
Delta R.T.: 0.000 min
Response: 269834861
Conc: 254.98 ng/ml

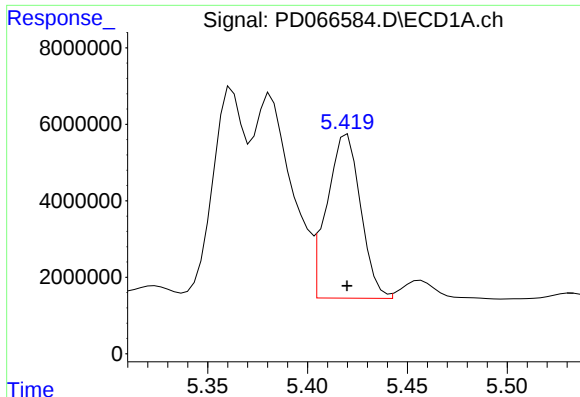

#26 Chlordane-4


R.T.: 5.420 min
Delta R.T.: 0.000 min
Response: 50479351
Conc: 241.11 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

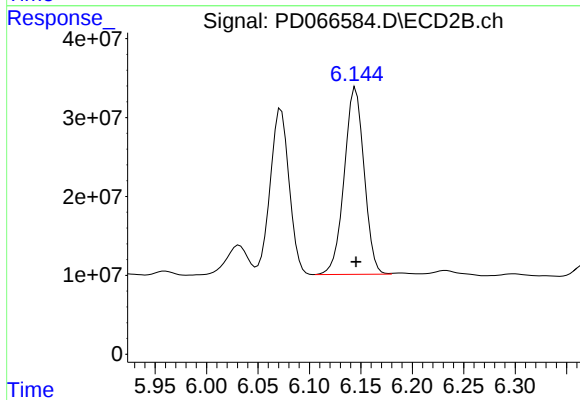


#26 Chlordane-4

R.T.: 6.145 min
Delta R.T.: 0.000 min
Response: 318066449
Conc: 261.39 ng/ml

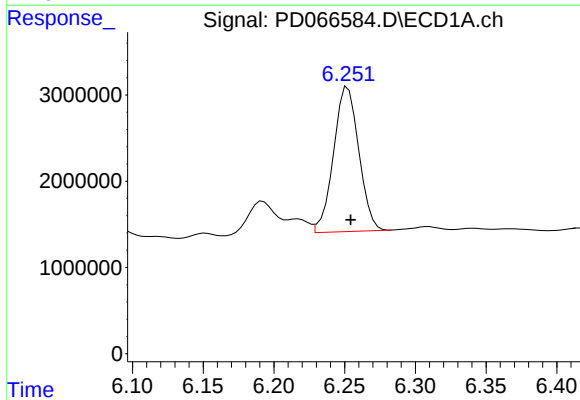


#27 Chlordane-5

R.T.: 6.252 min
Delta R.T.: -0.002 min
Response: 20899264
Conc: 235.91 ng/ml

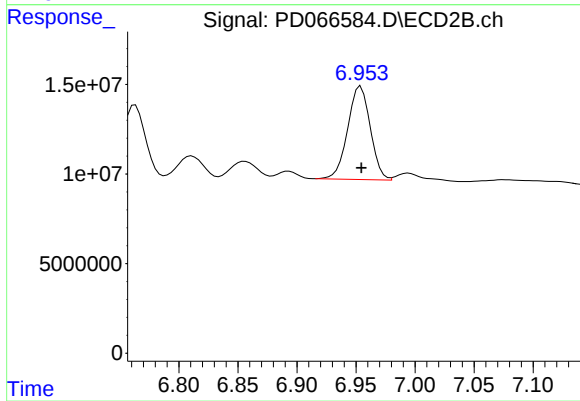

#27 Chlordane-5


R.T.: 6.954 min
Delta R.T.: 0.000 min
Response: 69515070
Conc: 244.44 ng/ml

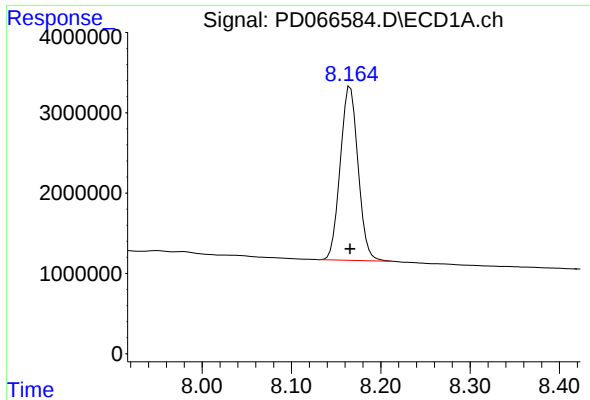

#28 Decachlorobiphenyl

R.T.: 8.166 min
Delta R.T.: 0.000 min
Response: 29943161
Conc: 25.41 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

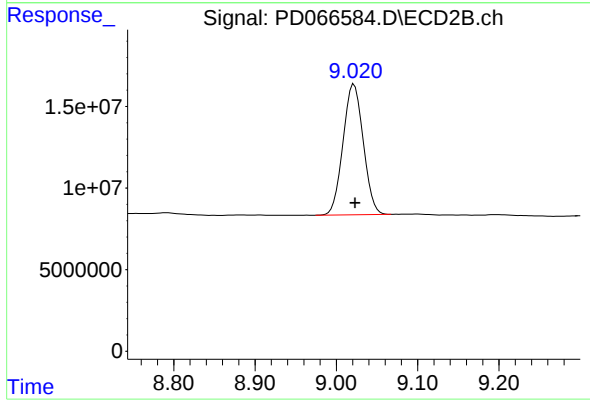

#28 Decachlorobiphenyl

R.T.: 9.022 min
Delta R.T.: -0.001 min
Response: 138110489
Conc: 25.59 ng/ml