

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102821\
 Data File : PD066592.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2021 00:12
 Operator : AJ\MA
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ICVPD102821CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 02:01:25 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102821.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 28 02:00:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.439	3.970	117.3E6	415.4E6	52.710	51.333
28)	SA Decachlor...	8.167	9.023	60177021	275.7E6	50.793	50.707
Target Compounds							
23)	Chlordane-1	4.302	4.959	38491100	148.1E6	520.171	533.507
24)	Chlordane-2	4.799	5.427	44812907	152.3E6	528.241	513.294
25)	Chlordane-3	5.363	6.073	129.8E6	548.6E6	530.121	508.782
26)	Chlordane-4	5.420	6.145	107.6E6	642.1E6	528.091	509.510
27)	Chlordane-5	6.254	6.955	43592674	141.6E6	515.456	519.578



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102821\
Data File : PD066592.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2021 00:12
Operator : AJ\MA
Sample : PCHLORICV500
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
ICVPD102821CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 02:01:25 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102821.M
Quant Title : GC Extractables
QLast Update : Thu Oct 28 02:00:45 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

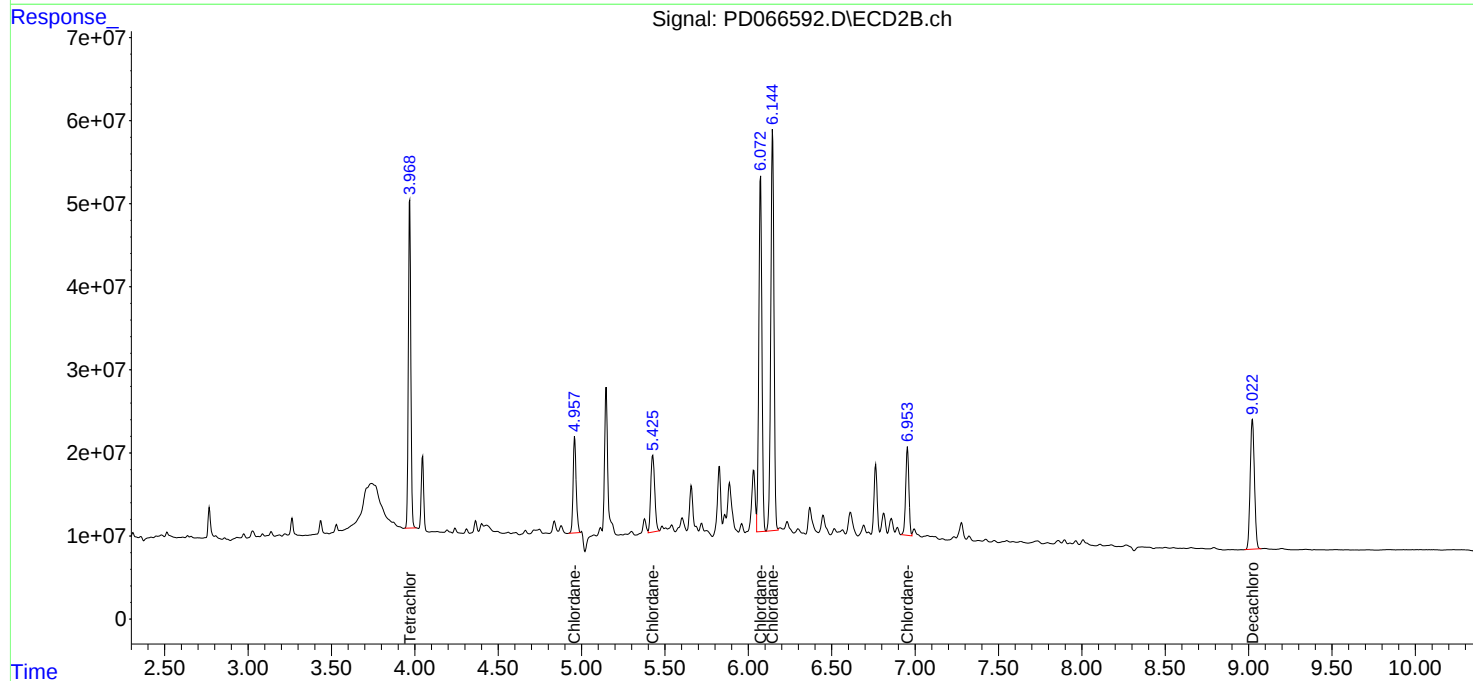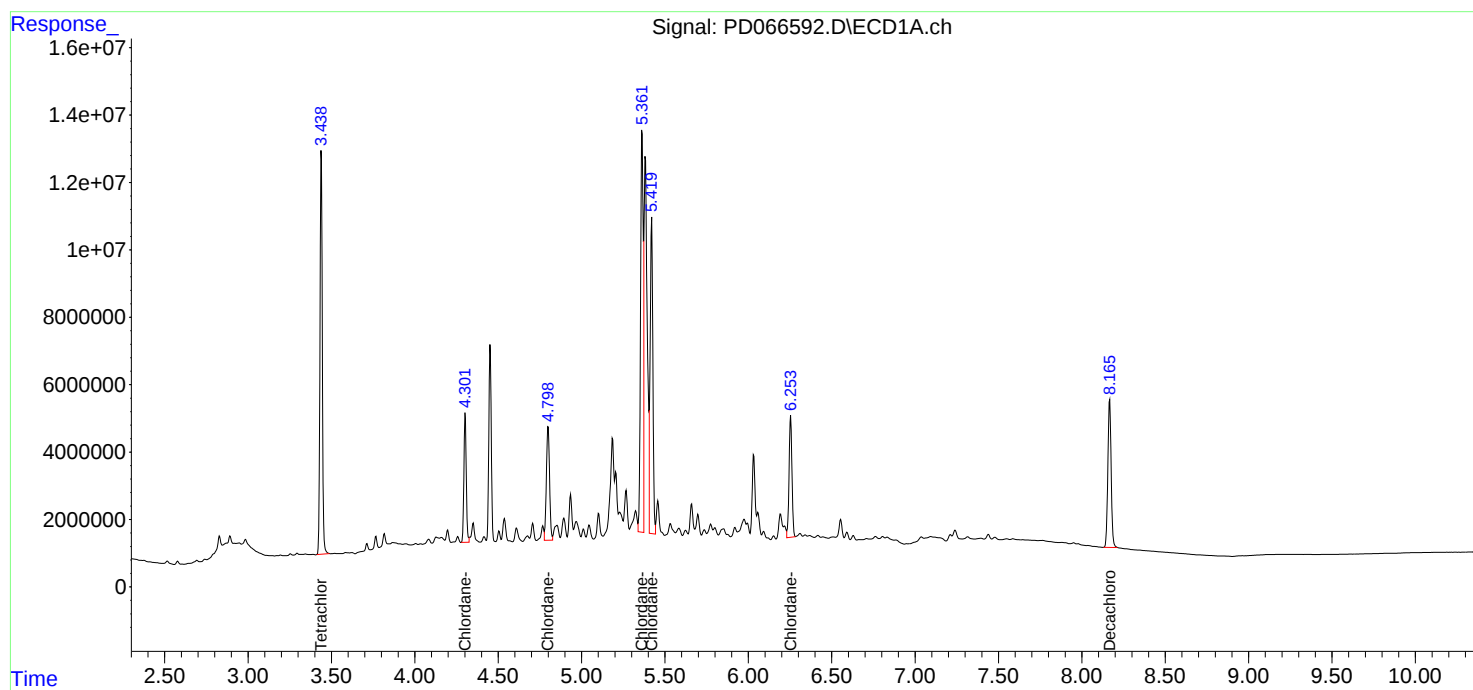


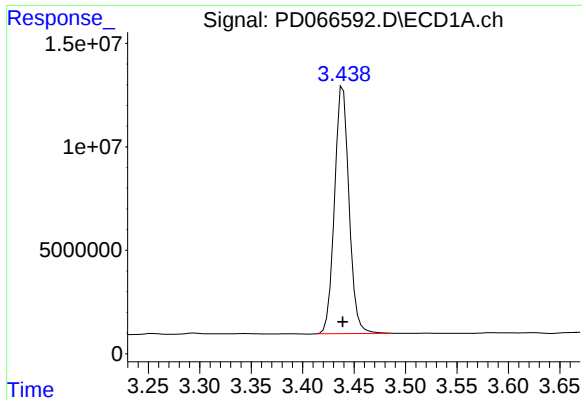

#1 Tetrachloro-m-xylene


R.T.: 3.439 min
Delta R.T.: 0.000 min
Response: 117320760
Conc: 52.71 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD102821CHLOR

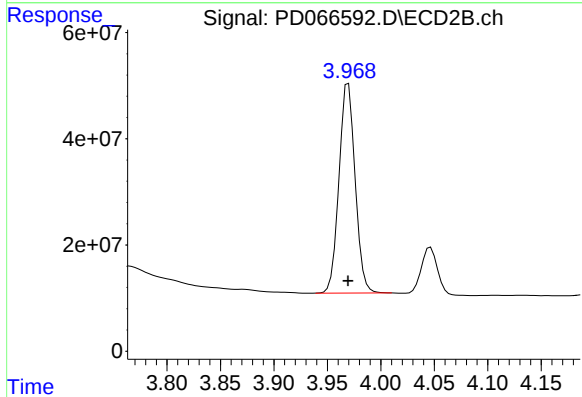


#1 Tetrachloro-m-xylene

R.T.: 3.970 min
Delta R.T.: 0.000 min
Response: 415376870
Conc: 51.33 ng/ml

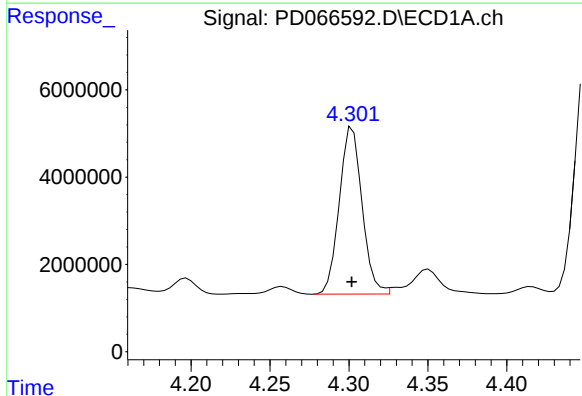


#23 Chlordane-1

R.T.: 4.302 min
Delta R.T.: 0.000 min
Response: 38491100
Conc: 520.17 ng/ml

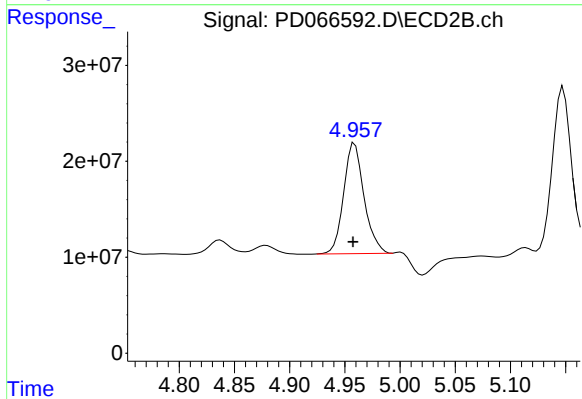

#23 Chlordane-1


R.T.: 4.959 min
Delta R.T.: 0.001 min
Response: 148119825
Conc: 533.51 ng/ml

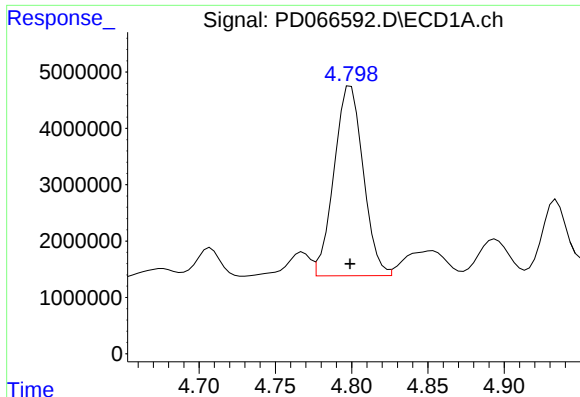

#24 Chlordane-2


R.T.: 4.799 min
Delta R.T.: 0.000 min
Response: 44812907
Conc: 528.24 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD102821CHLOR

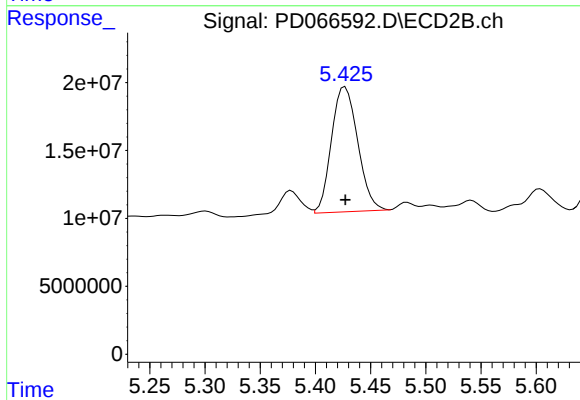


#24 Chlordane-2

R.T.: 5.427 min
Delta R.T.: 0.000 min
Response: 152252767
Conc: 513.29 ng/ml

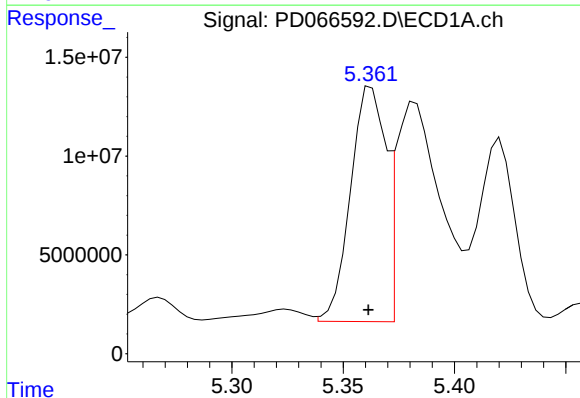


#25 Chlordane-3

R.T.: 5.363 min
Delta R.T.: 0.001 min
Response: 129797718
Conc: 530.12 ng/ml

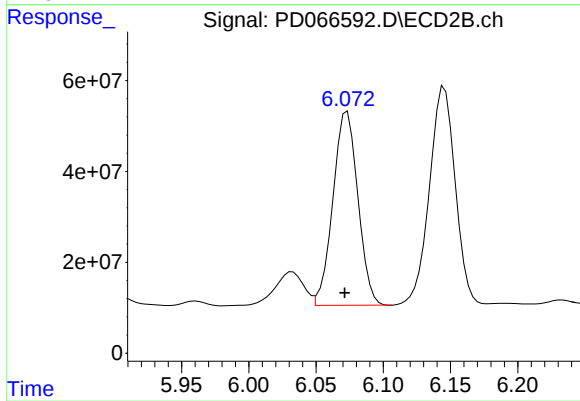

#25 Chlordane-3


R.T.: 6.073 min
Delta R.T.: 0.002 min
Response: 548554946
Conc: 508.78 ng/ml

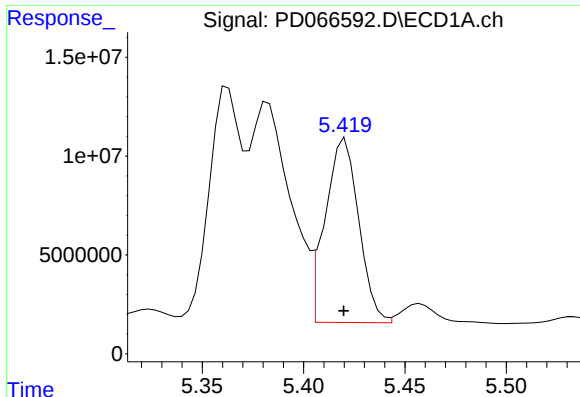

#26 Chlordane-4


R.T.: 5.420 min
Delta R.T.: 0.000 min
Response: 107572116
Conc: 528.09 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD102821CHLOR

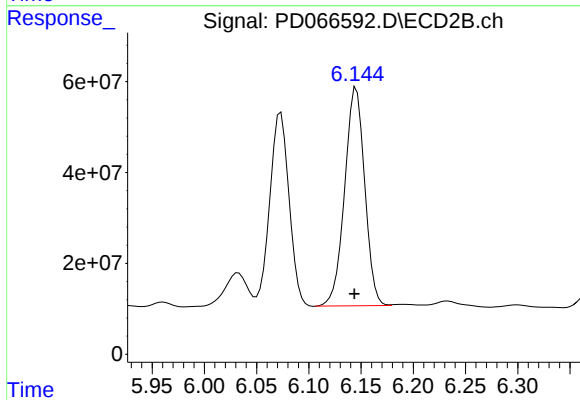


#26 Chlordane-4

R.T.: 6.145 min
Delta R.T.: 0.002 min
Response: 642097249
Conc: 509.51 ng/ml

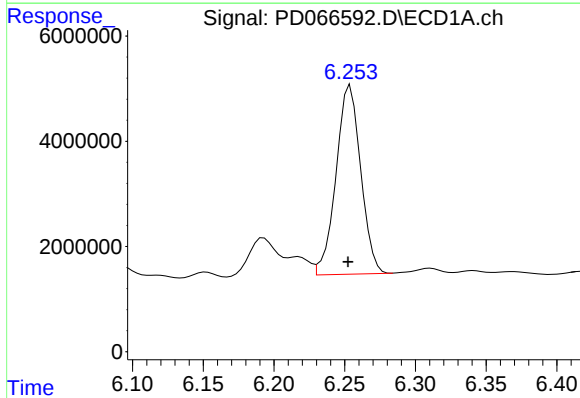


#27 Chlordane-5

R.T.: 6.254 min
Delta R.T.: 0.002 min
Response: 43592674
Conc: 515.46 ng/ml

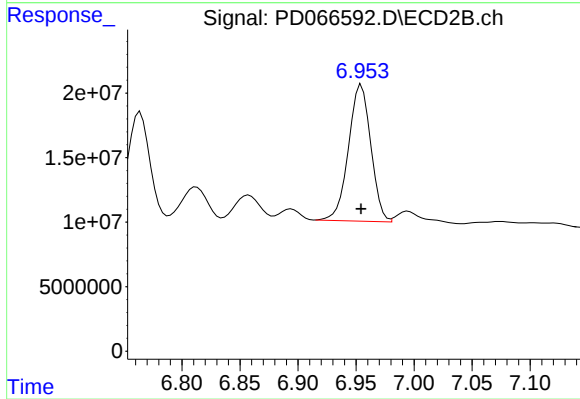

#27 Chlordane-5


R.T.: 6.955 min
Delta R.T.: 0.000 min
Response: 141602004
Conc: 519.58 ng/ml

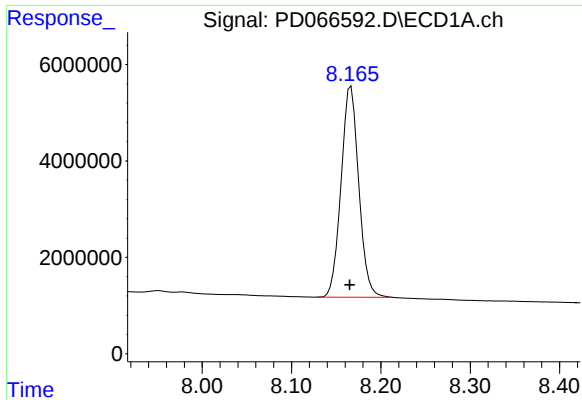

#28 Decachlorobiphenyl

R.T.: 8.167 min
Delta R.T.: 0.001 min
Response: 60177021
Conc: 50.79 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD102821CHLOR

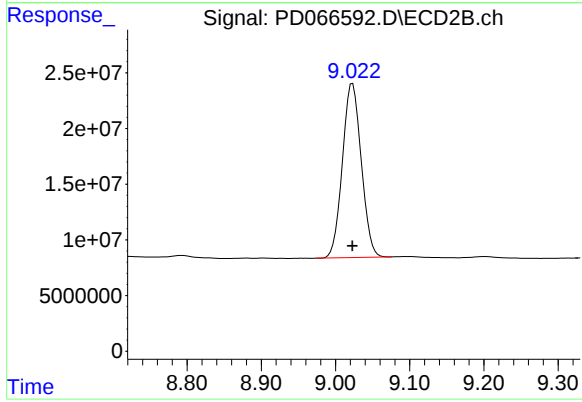

#28 Decachlorobiphenyl

R.T.: 9.023 min
Delta R.T.: 0.000 min
Response: 275718308
Conc: 50.71 ng/ml