

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102822\
 Data File : PD072661.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2022 14:52
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 15:30:36 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102822.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 28 15:28:32 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.703	3.464	122.6E6	1659.5E6	49.328	47.571
28)	SA Decachlor...	7.835	8.918	95860784	468.6E6	48.598	48.280
Target Compounds							
23)	Chlordane-1	3.696	4.614	39590807	476.8E6	463.813	478.370
24)	Chlordane-2	4.273	5.146	46048398	347.4E6	470.658	465.766
25)	Chlordane-3	4.904	5.853	132.8E6	1157.1E6	497.617	475.451
26)	Chlordane-4	4.966	5.930	132.5E6	1318.8E6	487.505	476.483
27)	Chlordane-5	5.863	6.787	45855967	253.3E6	483.471	494.258



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102822\
Data File : PD072661.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2022 14:52
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 15:30:36 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102822.M
Quant Title : GC Extractables
QLast Update : Fri Oct 28 15:28:32 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

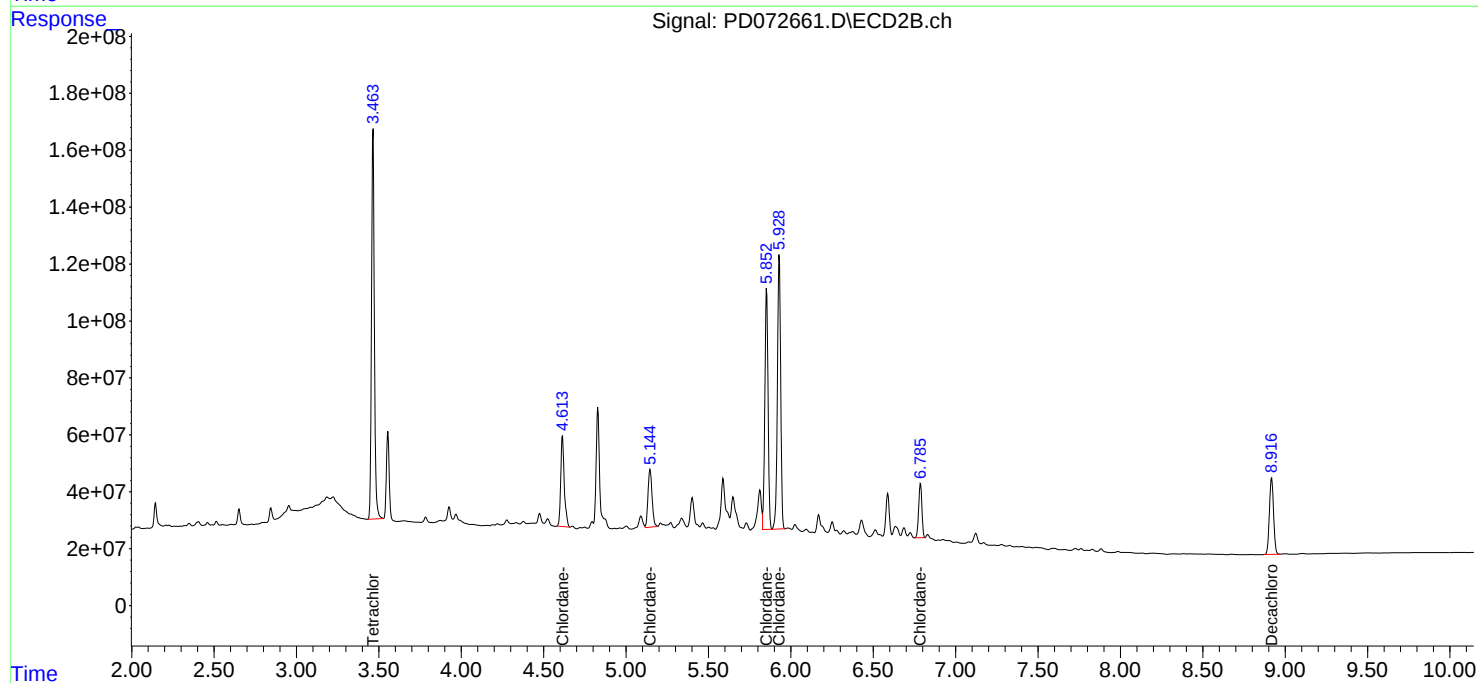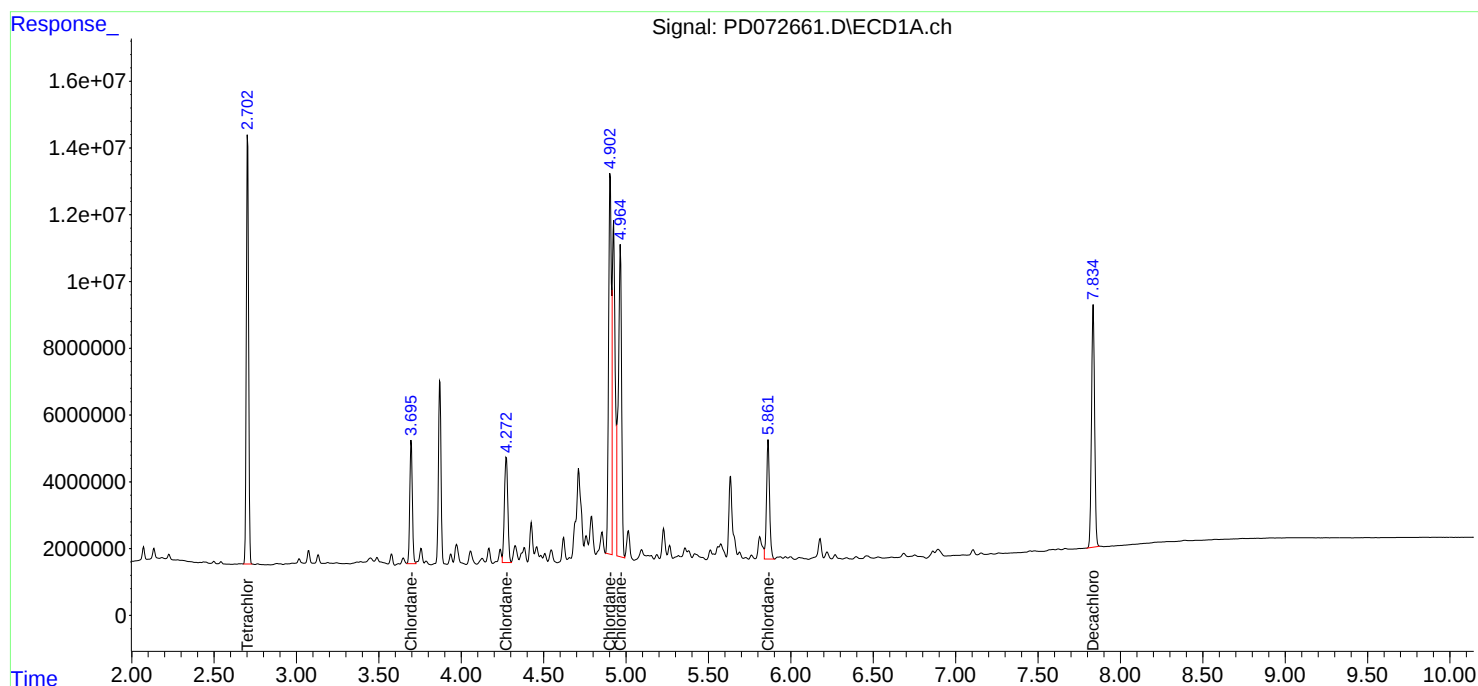


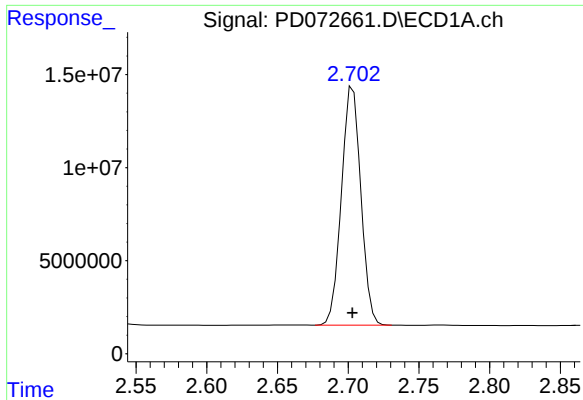

#1 Tetrachloro-m-xylene


R.T.: 2.703 min
Delta R.T.: 0.000 min
Response: 122644876
Conc: 49.33 ng/ml

Instrument :
ECD_D
ClientSampleId :

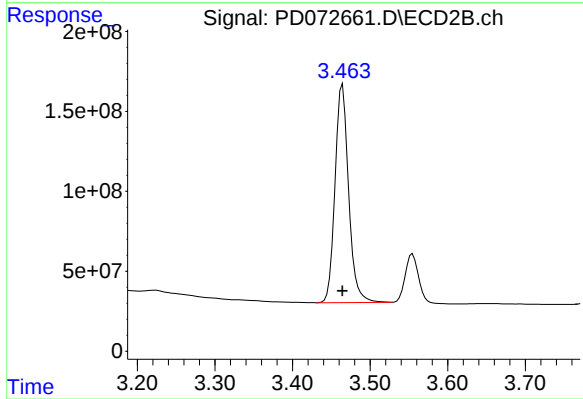


#1 Tetrachloro-m-xylene

R.T.: 3.464 min
Delta R.T.: 0.000 min
Response: 1659487355
Conc: 47.57 ng/ml

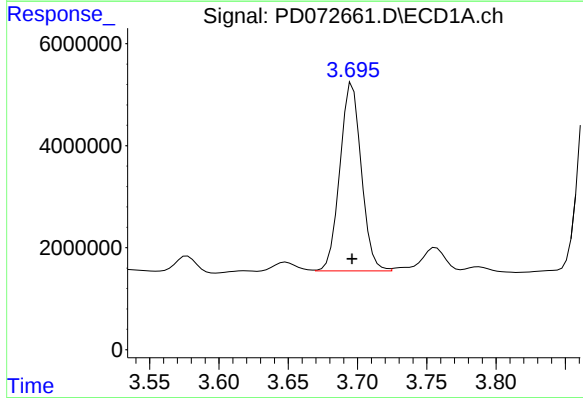


#23 Chlordane-1

R.T.: 3.696 min
Delta R.T.: 0.000 min
Response: 39590807
Conc: 463.81 ng/ml

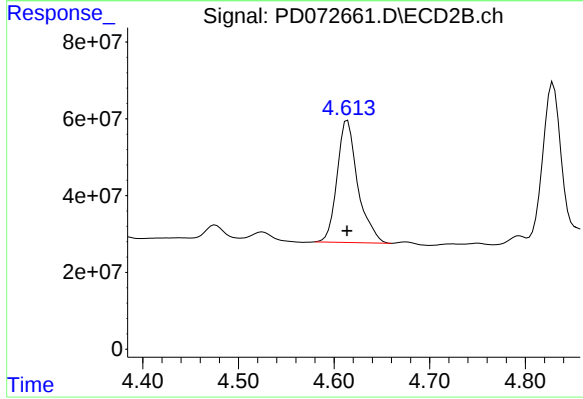

#23 Chlordane-1


R.T.: 4.614 min
Delta R.T.: 0.000 min
Response: 476843424
Conc: 478.37 ng/ml

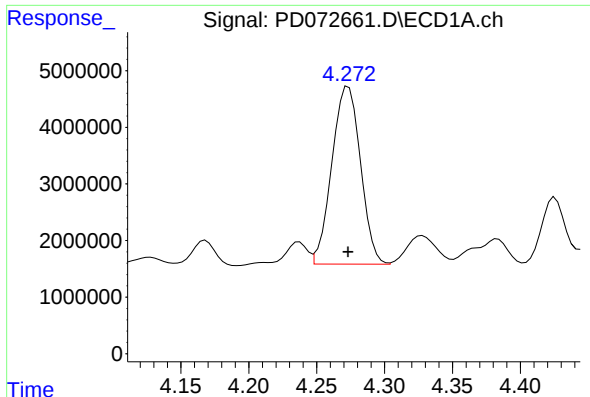

#24 Chlordane-2


R.T.: 4.273 min
Delta R.T.: 0.000 min
Response: 46048398
Conc: 470.66 ng/ml

Instrument :
ECD_D
ClientSampleId :

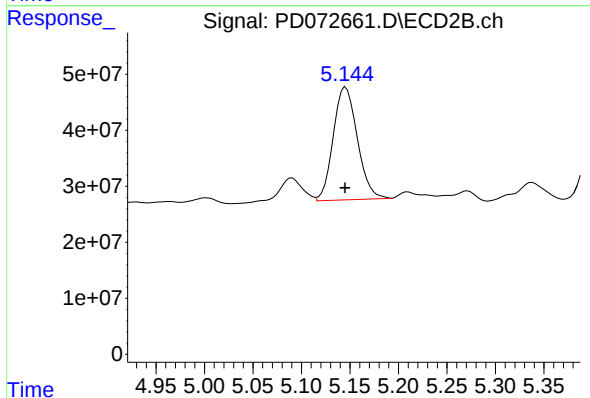


#24 Chlordane-2

R.T.: 5.146 min
Delta R.T.: 0.000 min
Response: 347442627
Conc: 465.77 ng/ml

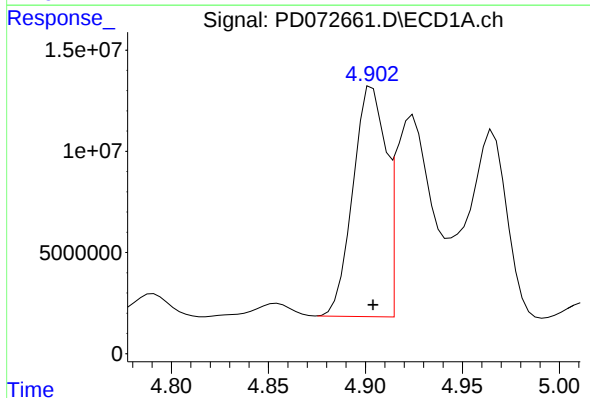


#25 Chlordane-3

R.T.: 4.904 min
Delta R.T.: 0.000 min
Response: 132843924
Conc: 497.62 ng/ml

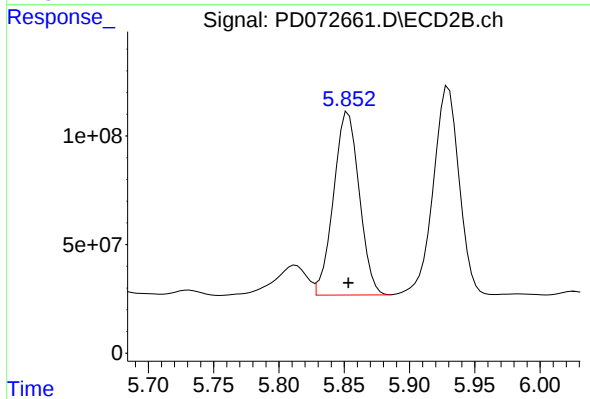

#25 Chlordane-3


R.T.: 5.853 min
Delta R.T.: 0.000 min
Response: 1157059995
Conc: 475.45 ng/ml

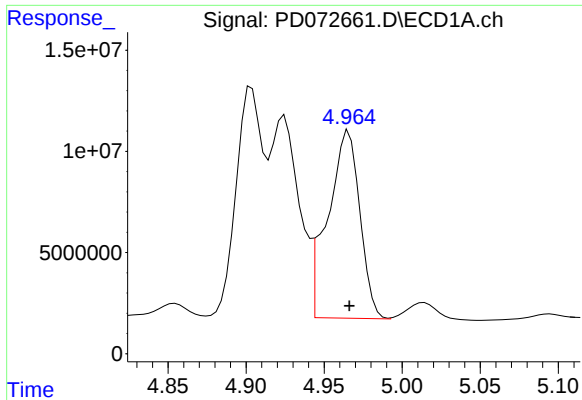

#26 Chlordane-4


R.T.: 4.966 min
Delta R.T.: 0.000 min
Response: 132502760
Conc: 487.51 ng/ml

Instrument :
ECD_D
ClientSampleId :

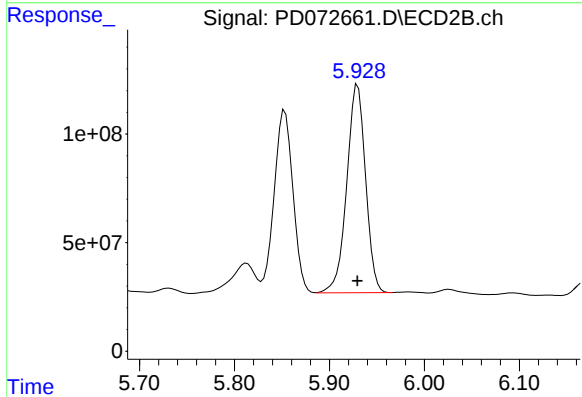


#26 Chlordane-4

R.T.: 5.930 min
Delta R.T.: 0.000 min
Response: 1318772129
Conc: 476.48 ng/ml

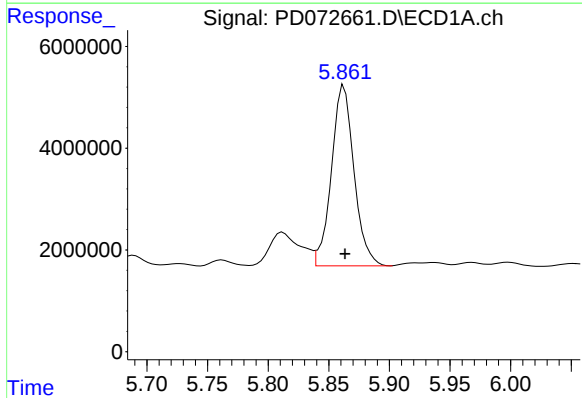


#27 Chlordane-5

R.T.: 5.863 min
Delta R.T.: 0.000 min
Response: 45855967
Conc: 483.47 ng/ml

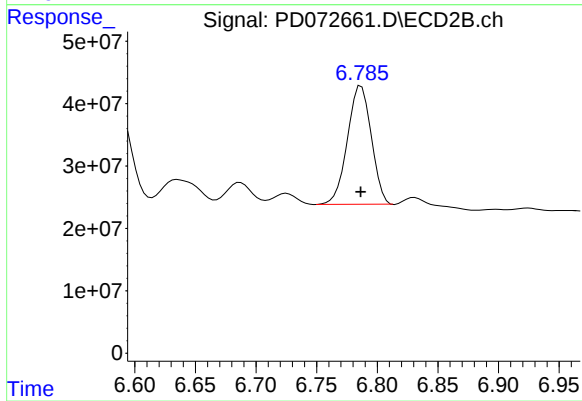

#27 Chlordane-5


R.T.: 6.787 min
Delta R.T.: 0.000 min
Response: 253292240
Conc: 494.26 ng/ml

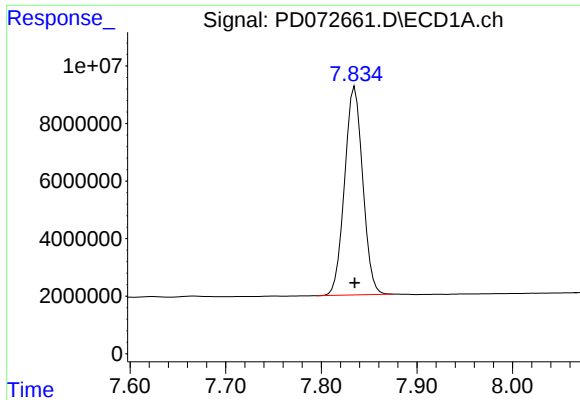

#28 Decachlorobiphenyl

R.T.: 7.835 min
Delta R.T.: 0.000 min
Response: 95860784
Conc: 48.60 ng/ml

Instrument :
ECD_D
ClientSampleId :

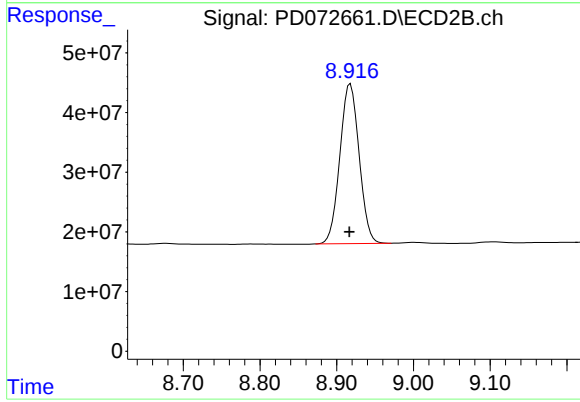

#28 Decachlorobiphenyl

R.T.: 8.918 min
Delta R.T.: 0.001 min
Response: 468649995
Conc: 48.28 ng/ml