

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102822\
 Data File : PD072644.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2022 11:06
 Operator : AR\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 15:46:56 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102822.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 28 15:29:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.704	3.464	49023928	868.5E6	23.903	25.160
28)	SA Decachlor...	7.836	8.918	46468501	236.5E6	24.169	24.686
Target Compounds							
9)	A Endosulfan I	5.025	5.984	28293972	211.8E6	11.786	12.971
10)	B gamma-Chl...	4.904	5.853	30311218	232.1E6	11.465	13.319
12)	B 4,4'-DDE	5.156	6.102	56040982	403.5E6	22.877	24.325
13)	MA Dieldrin	5.291	6.261	59735524	422.4E6	23.550	24.776
19)	B Endosulfa...	6.271	7.086	46845226	289.2E6	22.468	23.087
20)	A Methoxychlor	6.547	7.415	129.3E6	720.8E6	114.493	111.339
21)	B Endrin ke...	6.781	7.575	58028800	338.9E6	23.232	23.956



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102822\
Data File : PD072644.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2022 11:06
Operator : AR\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 15:46:56 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102822.M
Quant Title : GC Extractables
QLast Update : Fri Oct 28 15:29:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

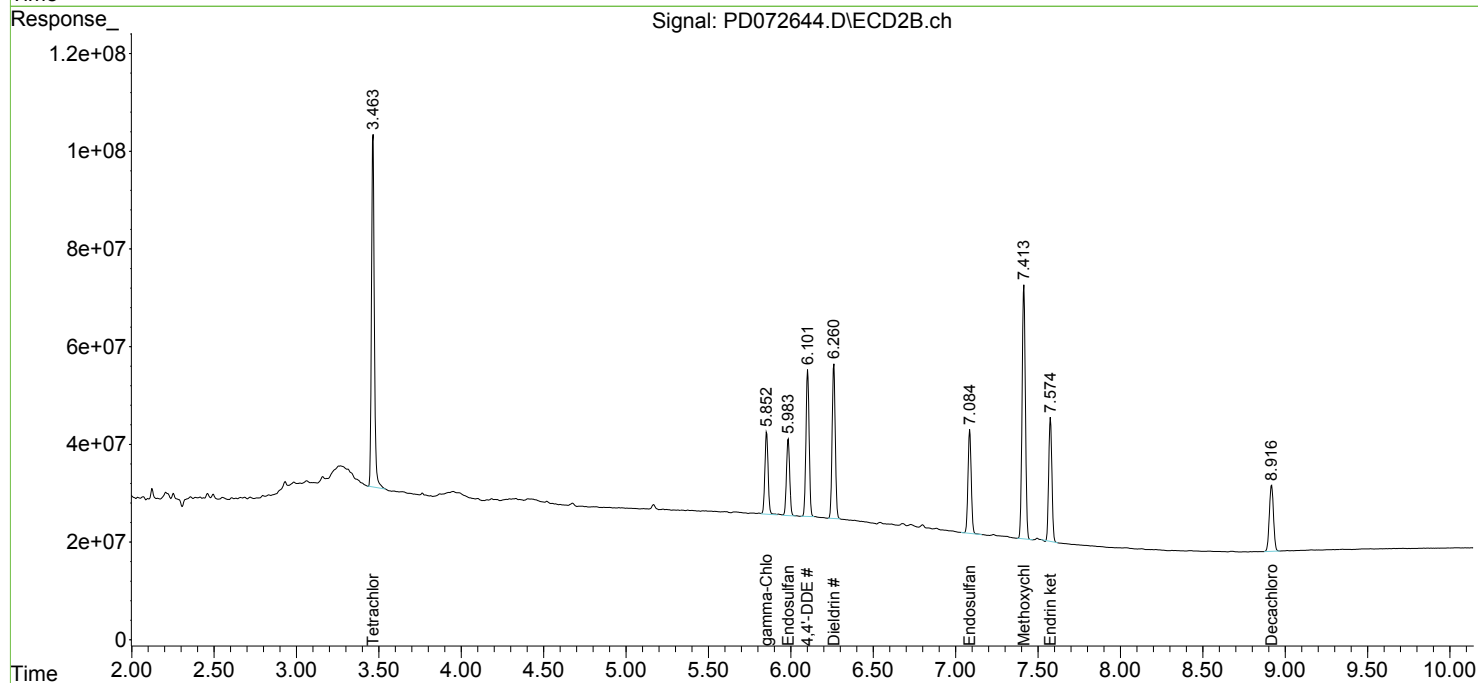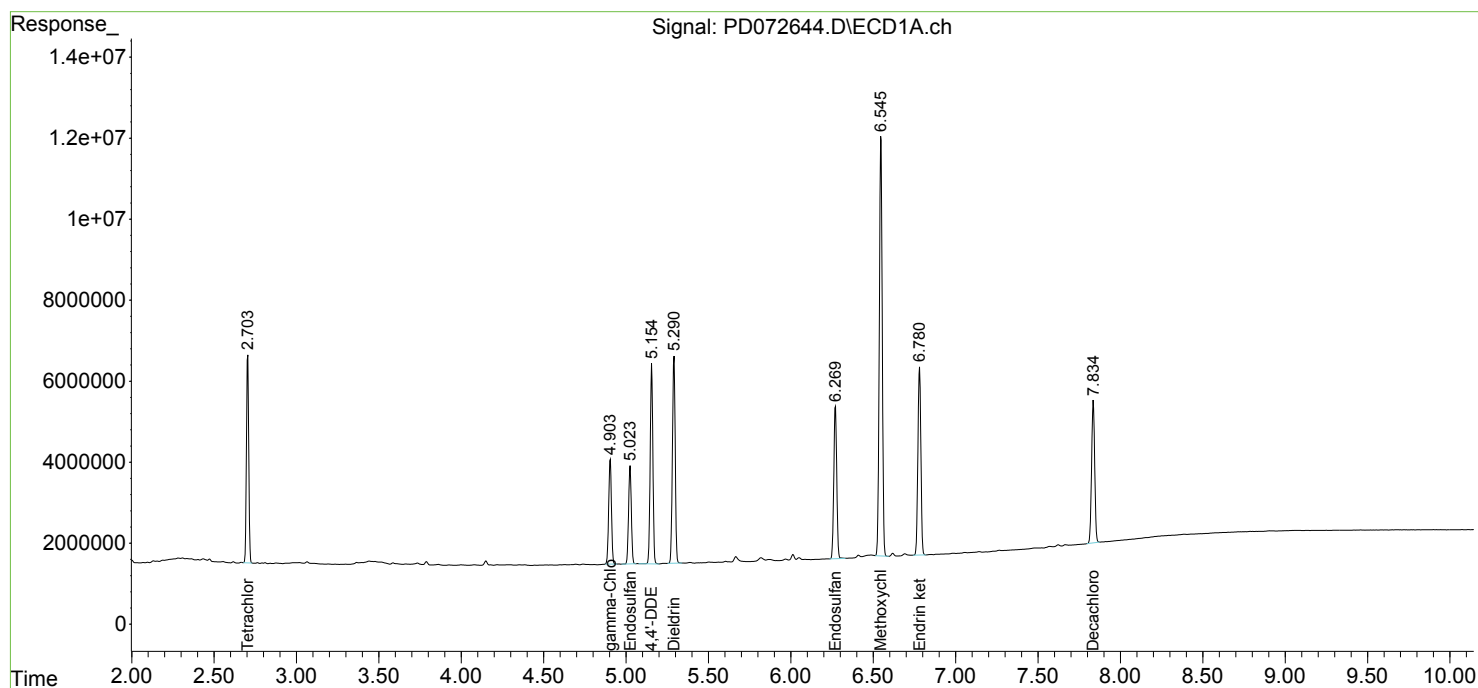


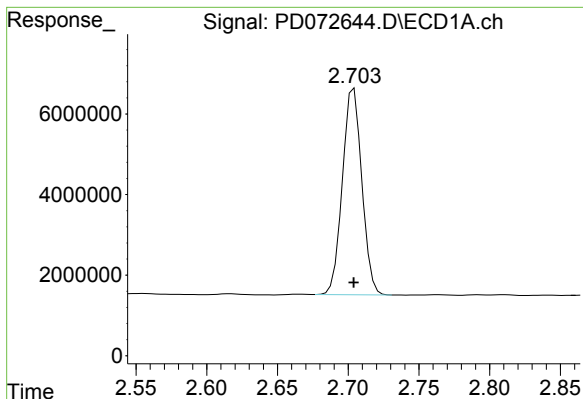

#1 Tetrachloro-m-xylene


R.T.: 2.704 min
Delta R.T.: 0.000 min
Response: 49023928
Conc: 23.90 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

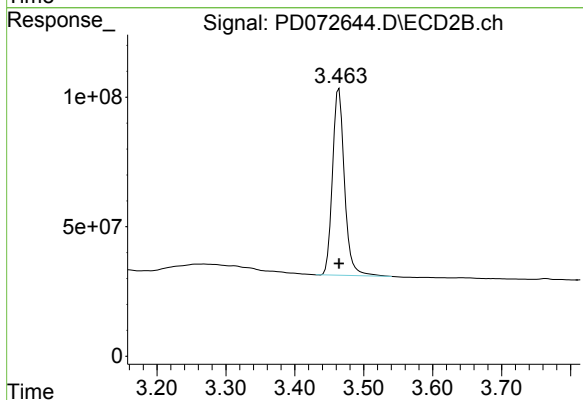


#1 Tetrachloro-m-xylene

R.T.: 3.464 min
Delta R.T.: 0.000 min
Response: 868466339
Conc: 25.16 ng/ml

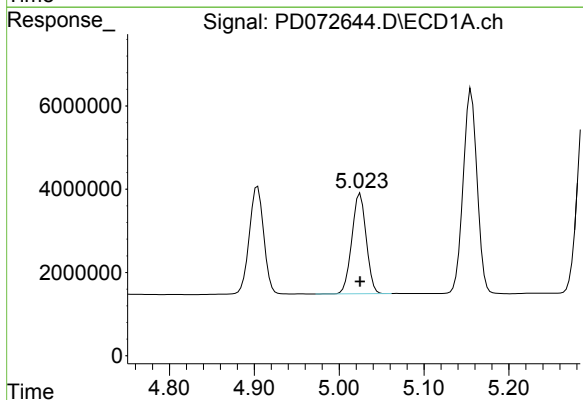


#9 Endosulfan I

R.T.: 5.025 min
Delta R.T.: 0.000 min
Response: 28293972
Conc: 11.79 ng/ml

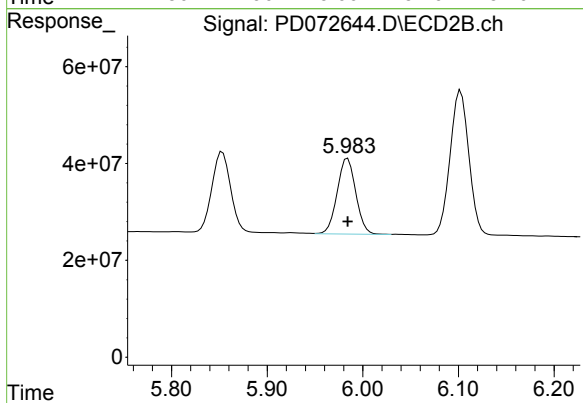

#9 Endosulfan I


R.T.: 5.984 min
Delta R.T.: 0.000 min
Response: 211843915
Conc: 12.97 ng/ml

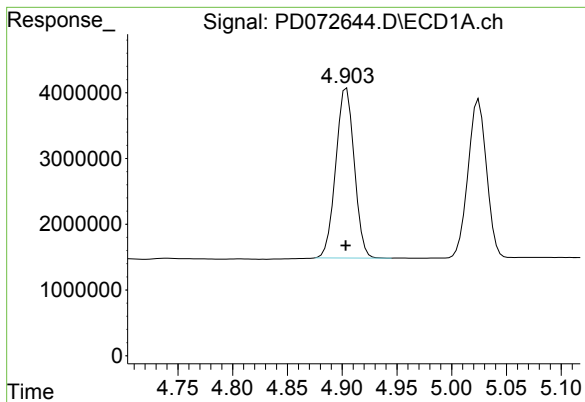

#10 gamma-Chlordane


R.T.: 4.904 min
Delta R.T.: 0.000 min
Response: 30311218
Conc: 11.47 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

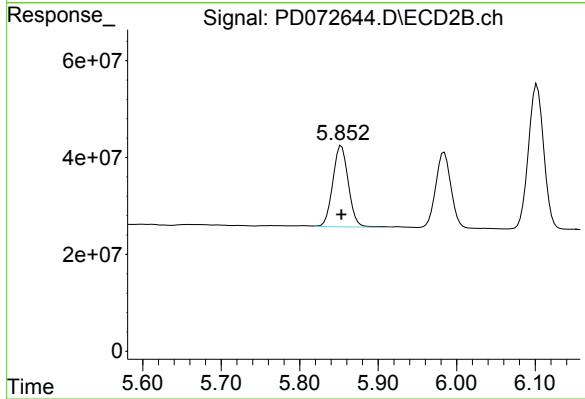


#10 gamma-Chlordane

R.T.: 5.853 min
Delta R.T.: 0.000 min
Response: 232056480
Conc: 13.32 ng/ml

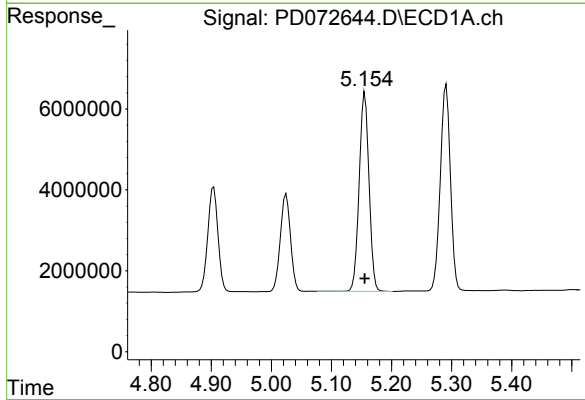


#12 4,4'-DDE

R.T.: 5.156 min
Delta R.T.: 0.000 min
Response: 56040982
Conc: 22.88 ng/ml

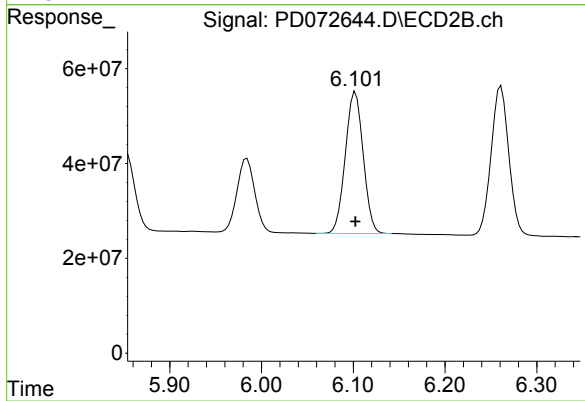

#12 4,4'-DDE


R.T.: 6.102 min
Delta R.T.: 0.000 min
Response: 403535724
Conc: 24.33 ng/ml

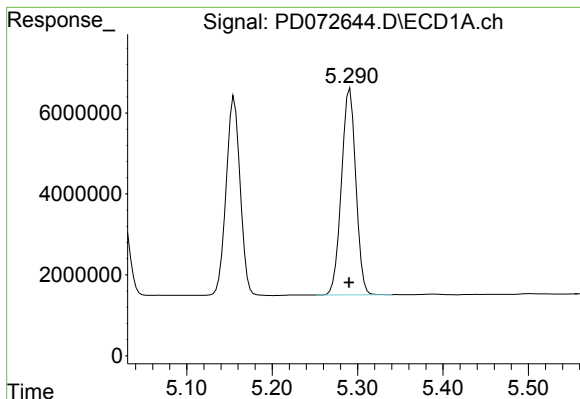

#13 Dieldrin


R.T.: 5.291 min
Delta R.T.: 0.000 min
Response: 59735524
Conc: 23.55 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

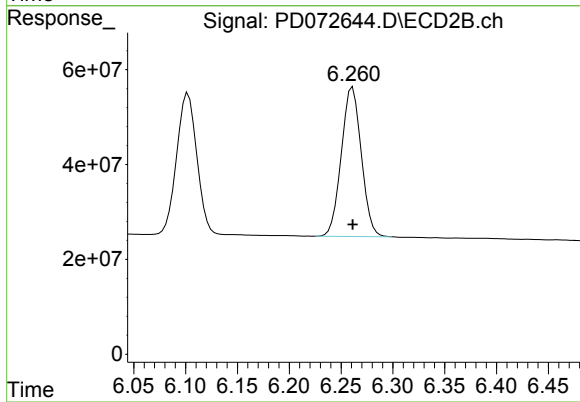


#13 Dieldrin

R.T.: 6.261 min
Delta R.T.: 0.000 min
Response: 422418068
Conc: 24.78 ng/ml

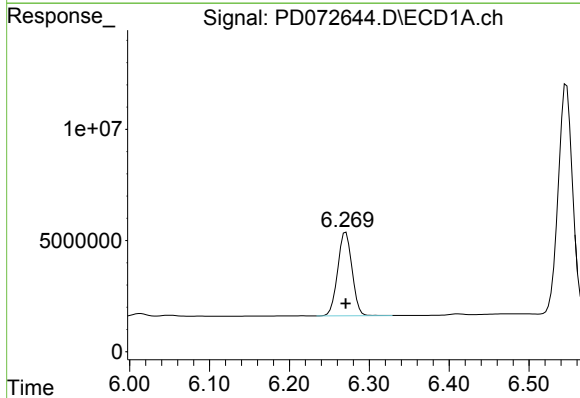


#19 Endosulfan Sulfate

R.T.: 6.271 min
Delta R.T.: 0.000 min
Response: 46845226
Conc: 22.47 ng/ml

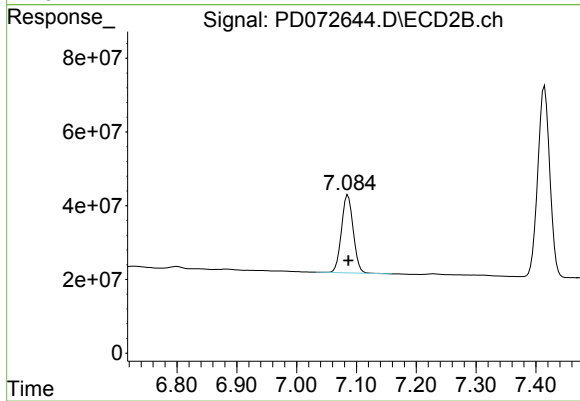

#19 Endosulfan Sulfate


R.T.: 7.086 min
Delta R.T.: 0.000 min
Response: 289164750
Conc: 23.09 ng/ml

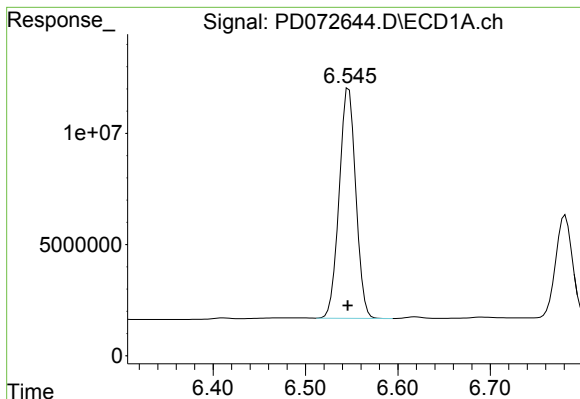

#20 Methoxychlor


R.T.: 6.547 min
Delta R.T.: 0.001 min
Response: 129258580
Conc: 114.49 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

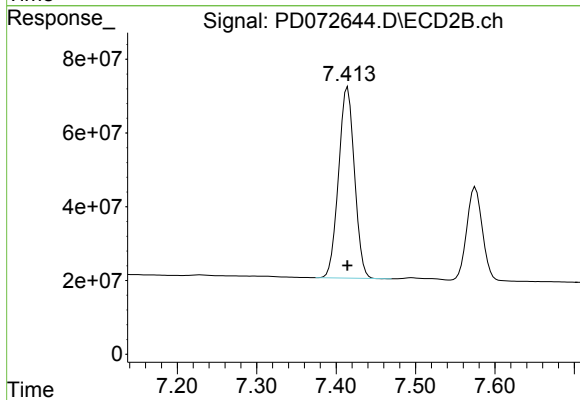


#20 Methoxychlor

R.T.: 7.415 min
Delta R.T.: 0.000 min
Response: 720793964
Conc: 111.34 ng/ml

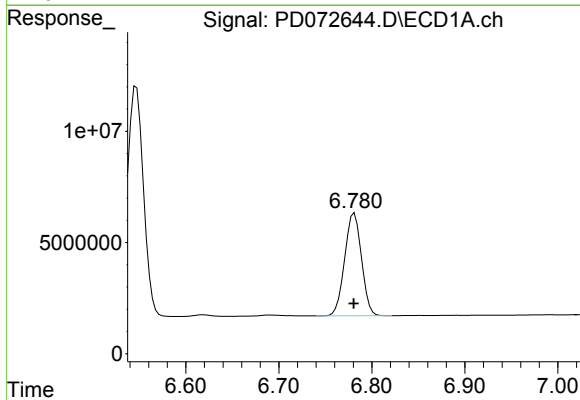


#21 Endrin ketone

R.T.: 6.781 min
Delta R.T.: 0.000 min
Response: 58028800
Conc: 23.23 ng/ml

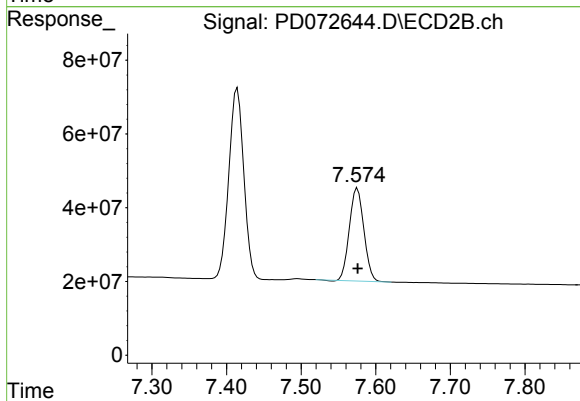

#21 Endrin ketone


R.T.: 7.575 min
Delta R.T.: 0.000 min
Response: 338938773
Conc: 23.96 ng/ml

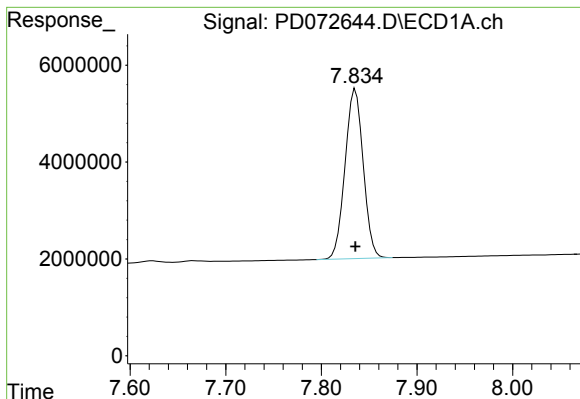

#28 Decachlorobiphenyl

R.T.: 7.836 min
Delta R.T.: 0.000 min
Response: 46468501
Conc: 24.17 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

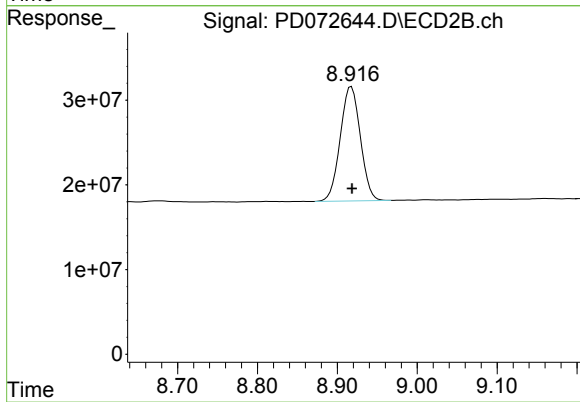

#28 Decachlorobiphenyl

R.T.: 8.918 min
Delta R.T.: 0.000 min
Response: 236547664
Conc: 24.69 ng/ml