

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102822\
 Data File : PD072651.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2022 12:39
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 14:25:25 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102822.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 28 14:24:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.703	3.465	182.5E6	2435.2E6	74.454	72.232
28)	SA Decachlor...	7.835	8.917	135.5E6	674.6E6	71.826	71.755
Target Compounds							
23)	Chlordane-1	3.696	4.614	58096467	687.8E6	732.707	713.752
24)	Chlordane-2	4.273	5.146	65153943	493.3E6	706.682	710.507
25)	Chlordane-3	4.904	5.854	197.7E6	1674.1E6	760.426	724.091
26)	Chlordane-4	4.966	5.930	194.9E6	1901.9E6	741.291	724.128
27)	Chlordane-5	5.863	6.786	66552640	355.0E6	731.600	706.082



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102822\
Data File : PD072651.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2022 12:39
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 14:25:25 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102822.M
Quant Title : GC Extractables
QLast Update : Fri Oct 28 14:24:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

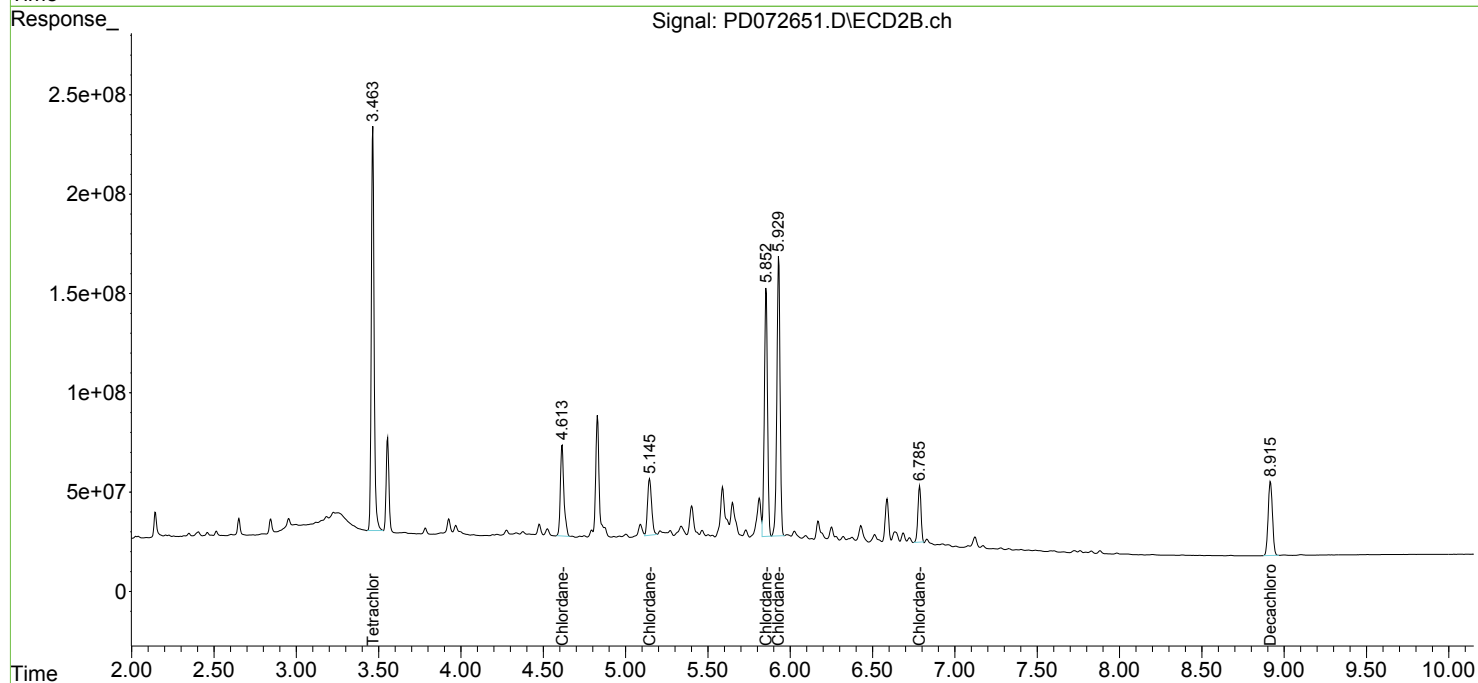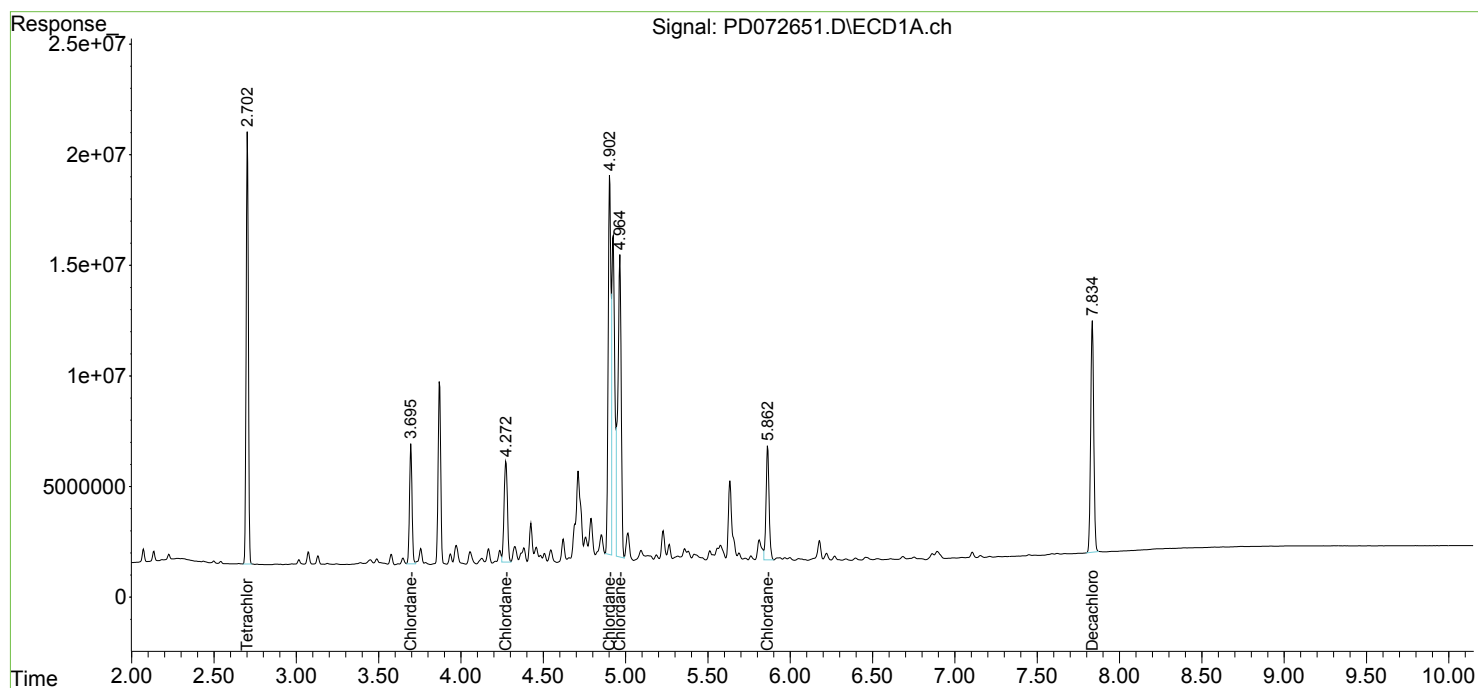


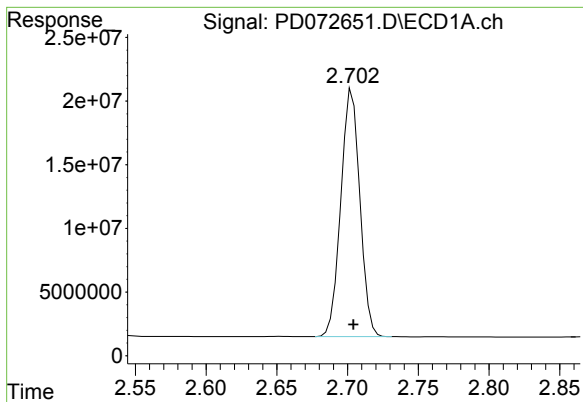

#1 Tetrachloro-m-xylene


R.T.: 2.703 min
Delta R.T.: 0.000 min
Response: 182460074
Conc: 74.45 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

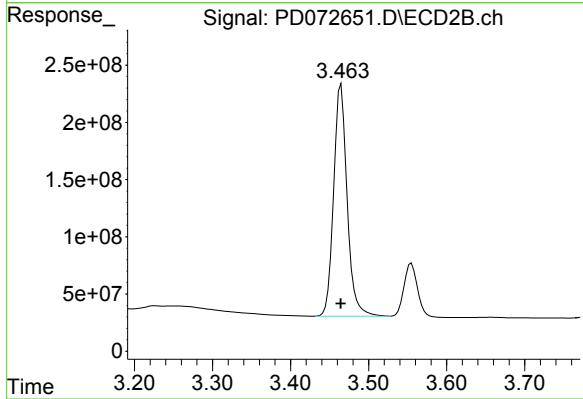


#1 Tetrachloro-m-xylene

R.T.: 3.465 min
Delta R.T.: 0.000 min
Response: 2435179484
Conc: 72.23 ng/ml

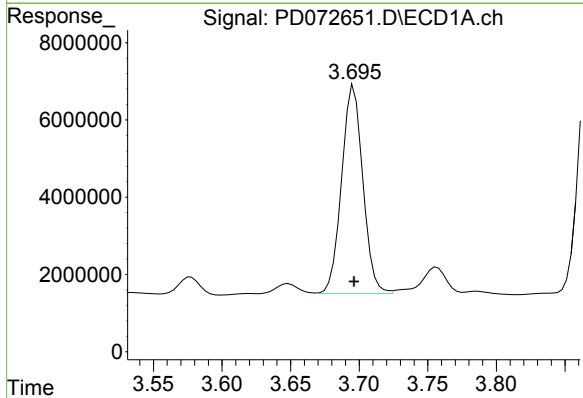


#23 Chlordane-1

R.T.: 3.696 min
Delta R.T.: 0.000 min
Response: 58096467
Conc: 732.71 ng/ml

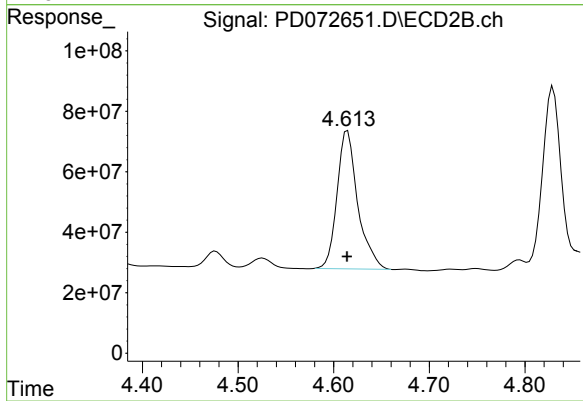

#23 Chlordane-1


R.T.: 4.614 min
Delta R.T.: 0.000 min
Response: 687830328
Conc: 713.75 ng/ml

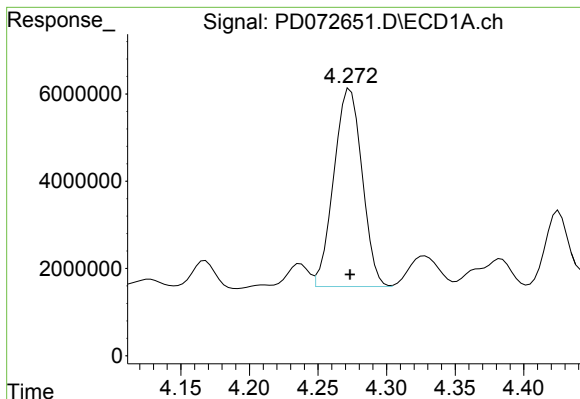

#24 Chlordane-2


R.T.: 4.273 min
Delta R.T.: 0.000 min
Response: 65153943
Conc: 706.68 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

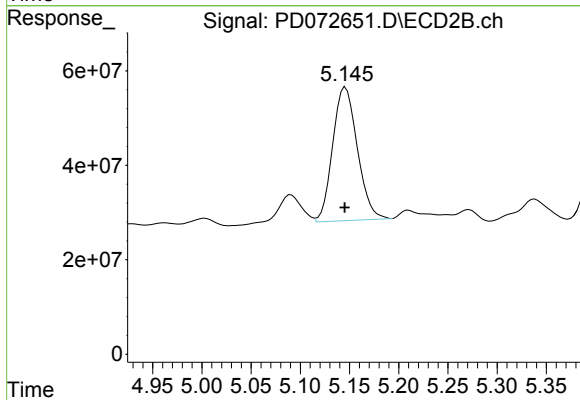


#24 Chlordane-2

R.T.: 5.146 min
Delta R.T.: 0.000 min
Response: 493278497
Conc: 710.51 ng/ml

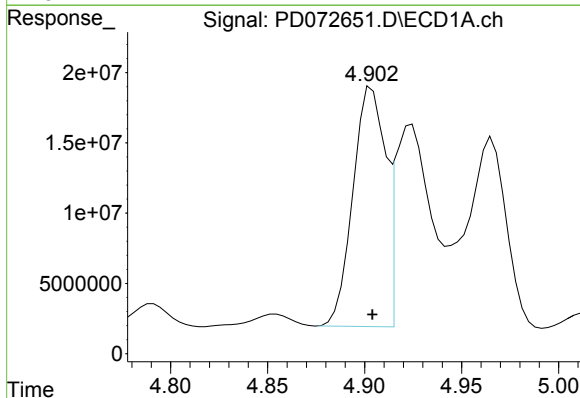


#25 Chlordane-3

R.T.: 4.904 min
Delta R.T.: 0.000 min
Response: 197666653
Conc: 760.43 ng/ml

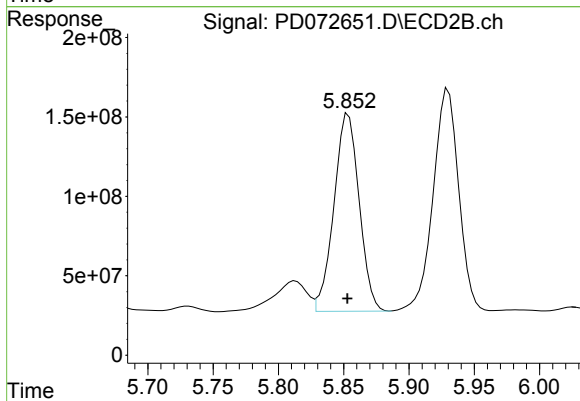

#25 Chlordane-3


R.T.: 5.854 min
Delta R.T.: 0.000 min
Response: 1674094227
Conc: 724.09 ng/ml

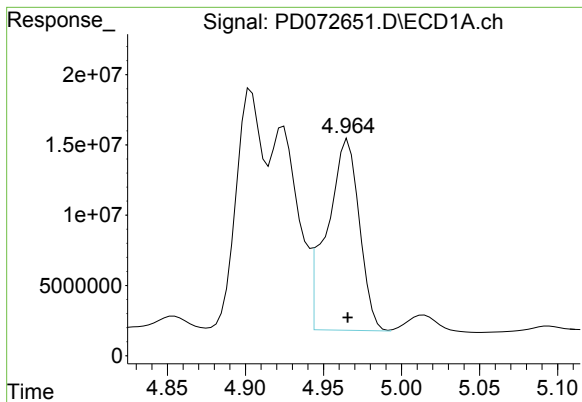

#26 Chlordane-4


R.T.: 4.966 min
Delta R.T.: 0.000 min
Response: 194891418
Conc: 741.29 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

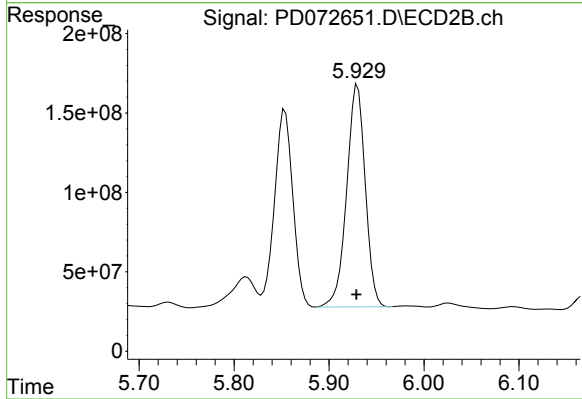


#26 Chlordane-4

R.T.: 5.930 min
Delta R.T.: 0.001 min
Response: 1901941898
Conc: 724.13 ng/ml

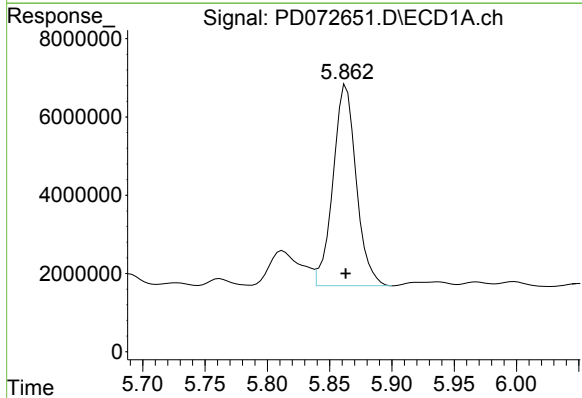


#27 Chlordane-5

R.T.: 5.863 min
Delta R.T.: 0.000 min
Response: 66552640
Conc: 731.60 ng/ml

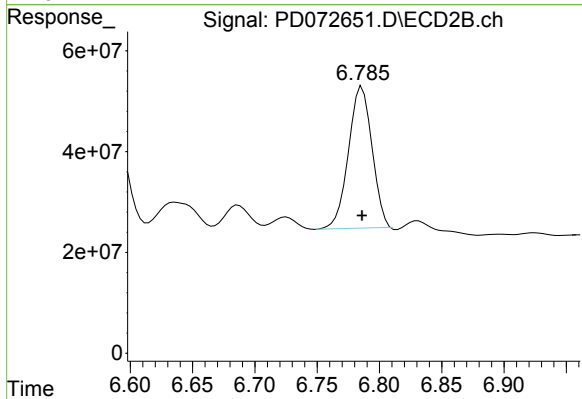

#27 Chlordane-5


R.T.: 6.786 min
Delta R.T.: 0.000 min
Response: 354988664
Conc: 706.08 ng/ml

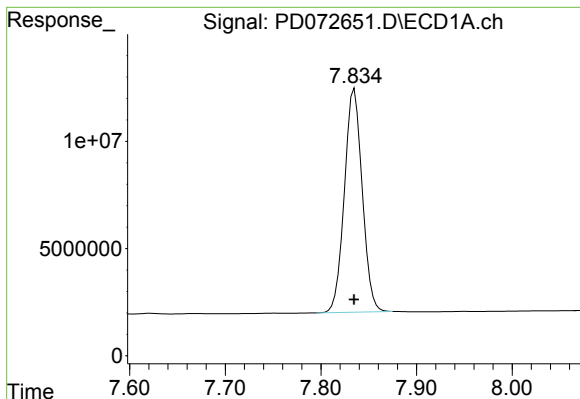

#28 Decachlorobiphenyl

R.T.: 7.835 min
Delta R.T.: 0.000 min
Response: 135508834
Conc: 71.83 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

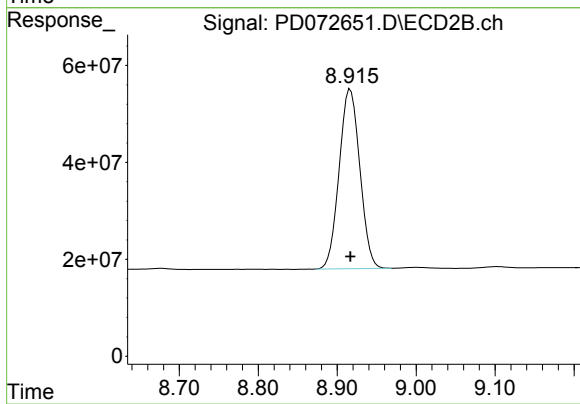

#28 Decachlorobiphenyl

R.T.: 8.917 min
Delta R.T.: 0.000 min
Response: 674604898
Conc: 71.76 ng/ml