

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102822\
 Data File : PD072652.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2022 12:52
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 14:25:37 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102822.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 28 14:24:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.704	3.464	122.5E6	1685.7E6	50.000	50.000
28)	SA Decachlor...	7.835	8.917	94331853	470.1E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	3.696	4.614	39645099	481.8E6	500.000	500.000
24)	Chlordane-2	4.273	5.145	46098471	347.1E6	500.000	500.000
25)	Chlordane-3	4.904	5.853	130.0E6	1156.0E6	500.000	500.000
26)	Chlordane-4	4.966	5.929	131.5E6	1313.3E6	500.000	500.000
27)	Chlordane-5	5.863	6.786	45484332	251.4E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102822\
Data File : PD072652.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2022 12:52
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 14:25:37 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102822.M
Quant Title : GC Extractables
QLast Update : Fri Oct 28 14:24:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

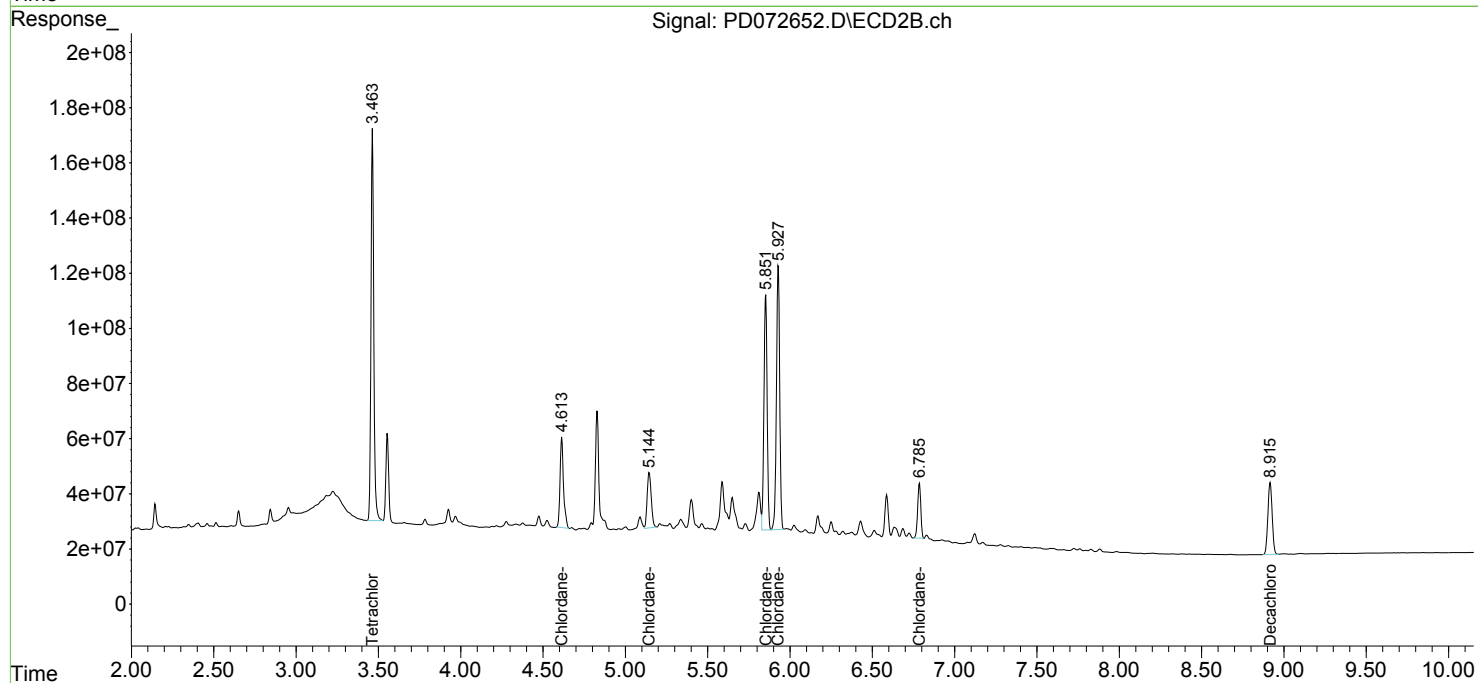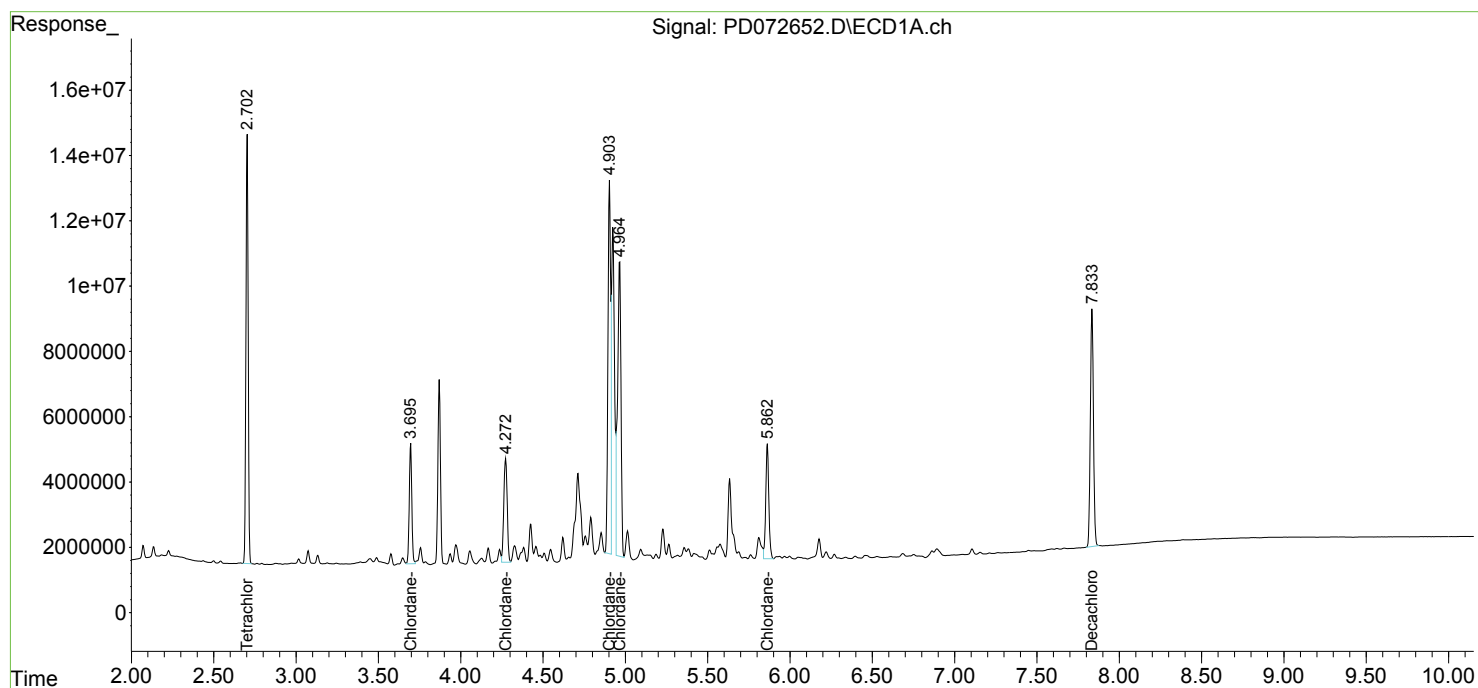


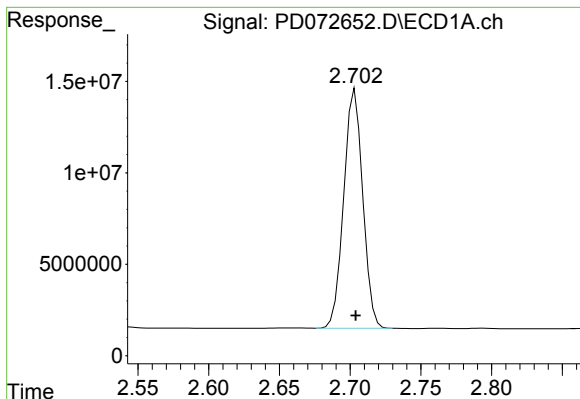

#1 Tetrachloro-m-xylene


R.T.: 2.704 min
Delta R.T.: 0.000 min
Response: 122531943
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

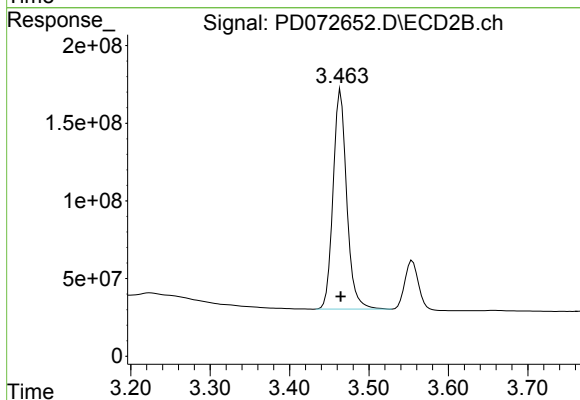


#1 Tetrachloro-m-xylene

R.T.: 3.464 min
Delta R.T.: 0.000 min
Response: 1685655492
Conc: 50.00 ng/ml

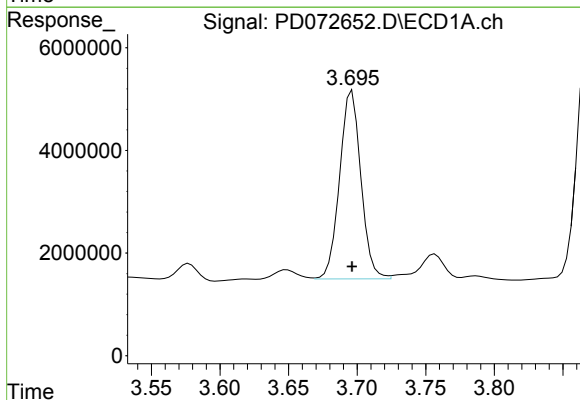


#23 Chlordane-1

R.T.: 3.696 min
Delta R.T.: 0.000 min
Response: 39645099
Conc: 500.00 ng/ml

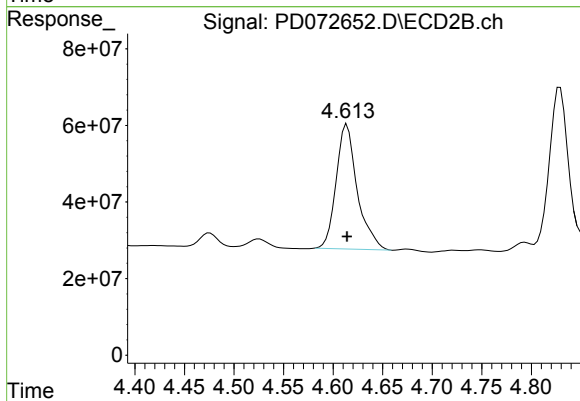

#23 Chlordane-1


R.T.: 4.614 min
Delta R.T.: 0.000 min
Response: 481841257
Conc: 500.00 ng/ml

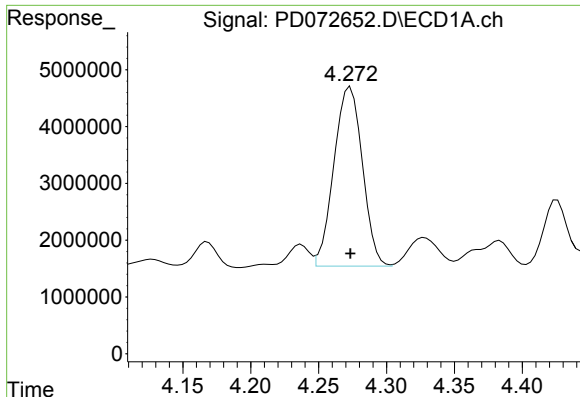

#24 Chlordane-2


R.T.: 4.273 min
Delta R.T.: 0.000 min
Response: 46098471
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

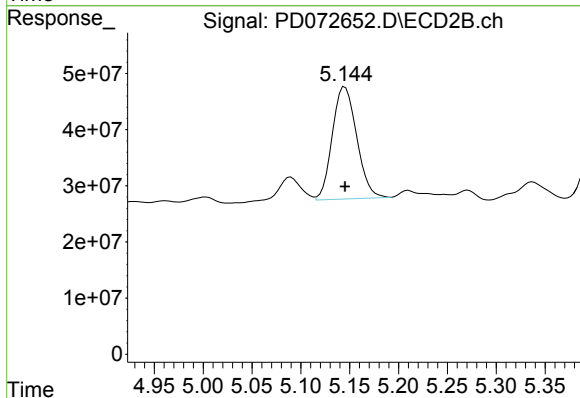


#24 Chlordane-2

R.T.: 5.145 min
Delta R.T.: 0.000 min
Response: 347131363
Conc: 500.00 ng/ml

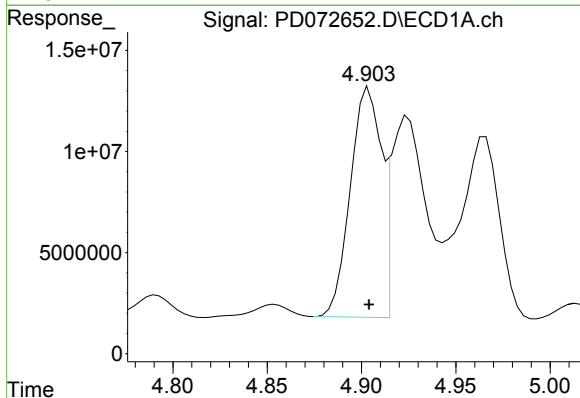


#25 Chlordane-3

R.T.: 4.904 min
Delta R.T.: 0.000 min
Response: 129970953
Conc: 500.00 ng/ml

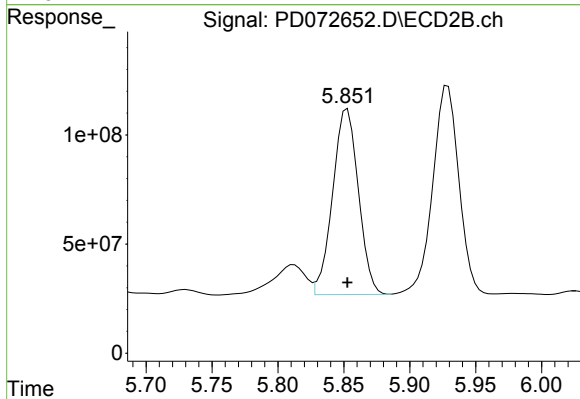

#25 Chlordane-3


R.T.: 5.853 min
Delta R.T.: 0.000 min
Response: 1155997217
Conc: 500.00 ng/ml

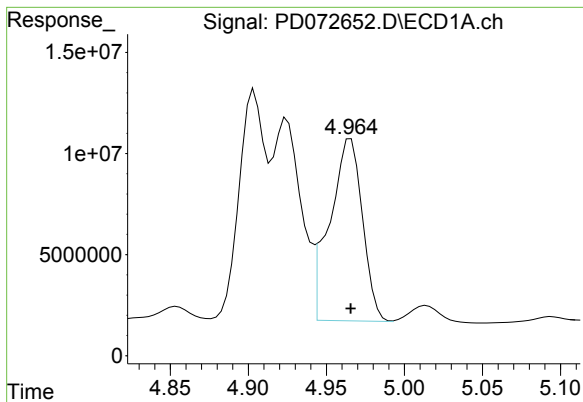

#26 Chlordane-4


R.T.: 4.966 min
Delta R.T.: 0.000 min
Response: 131454033
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

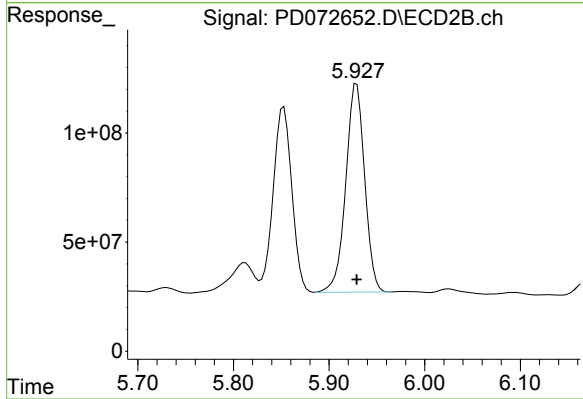


#26 Chlordane-4

R.T.: 5.929 min
Delta R.T.: 0.000 min
Response: 1313263208
Conc: 500.00 ng/ml

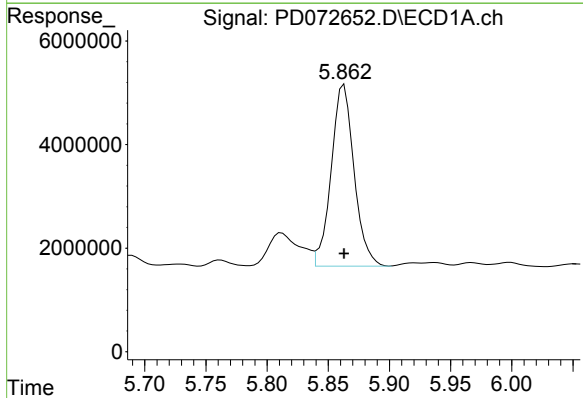


#27 Chlordane-5

R.T.: 5.863 min
Delta R.T.: 0.000 min
Response: 45484332
Conc: 500.00 ng/ml

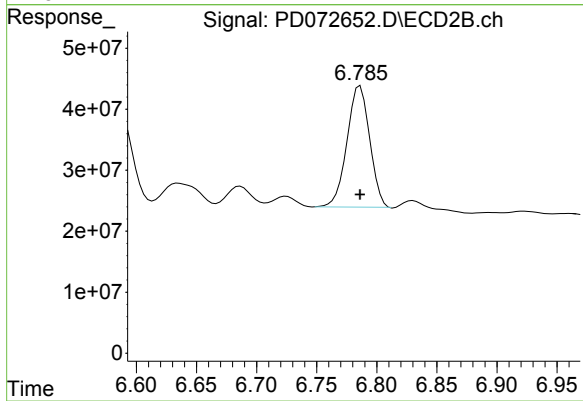

#27 Chlordane-5


R.T.: 6.786 min
Delta R.T.: 0.000 min
Response: 251379112
Conc: 500.00 ng/ml

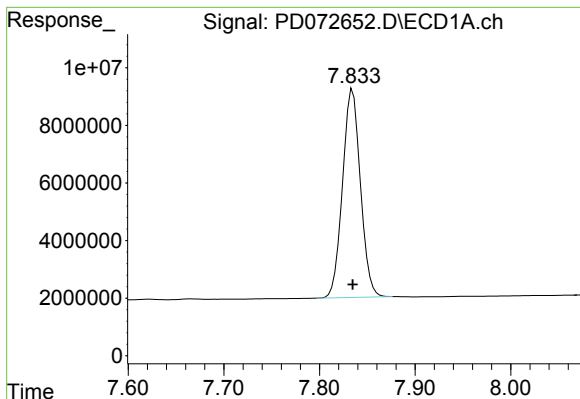

#28 Decachlorobiphenyl

R.T.: 7.835 min
Delta R.T.: 0.000 min
Response: 94331853
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

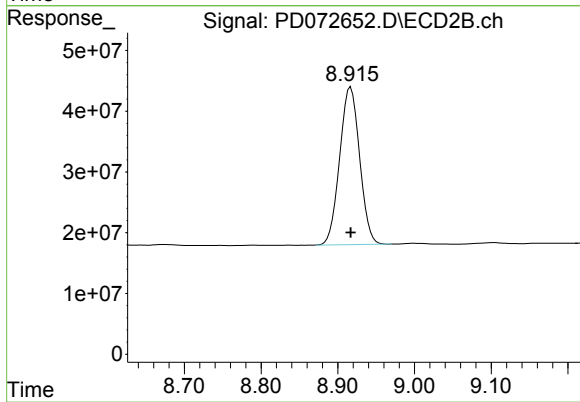

#28 Decachlorobiphenyl

R.T.: 8.917 min
Delta R.T.: 0.000 min
Response: 470074950
Conc: 50.00 ng/ml