

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102822\
 Data File : PD072653.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2022 13:06
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 14:25:48 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102822.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 28 14:24:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.703	3.464	59556033	873.3E6	24.302	25.905
28)	SA Decachlor...	7.835	8.917	48280907	241.7E6	25.591	25.711
Target Compounds							
23)	Chlordane-1	3.696	4.613	20061591	253.7E6	253.015	263.281
24)	Chlordane-2	4.274	5.145	24112639	189.4E6	261.534	272.856
25)	Chlordane-3	4.904	5.853	61598829	597.3E6	236.972	258.331
26)	Chlordane-4	4.966	5.929	64832660	679.2E6	246.598	258.610
27)	Chlordane-5	5.863	6.786	22509550	130.3E6	247.443	259.222



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102822\
Data File : PD072653.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2022 13:06
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 14:25:48 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102822.M
Quant Title : GC Extractables
QLast Update : Fri Oct 28 14:24:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

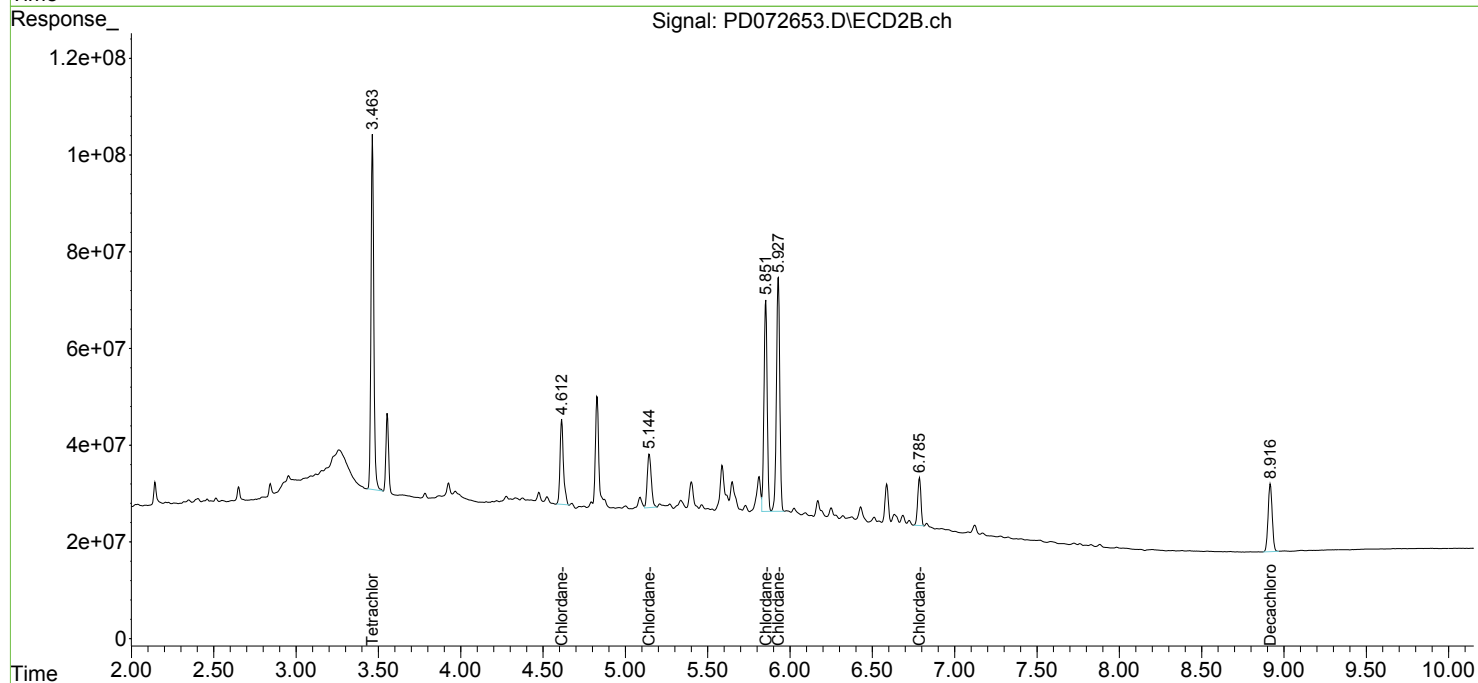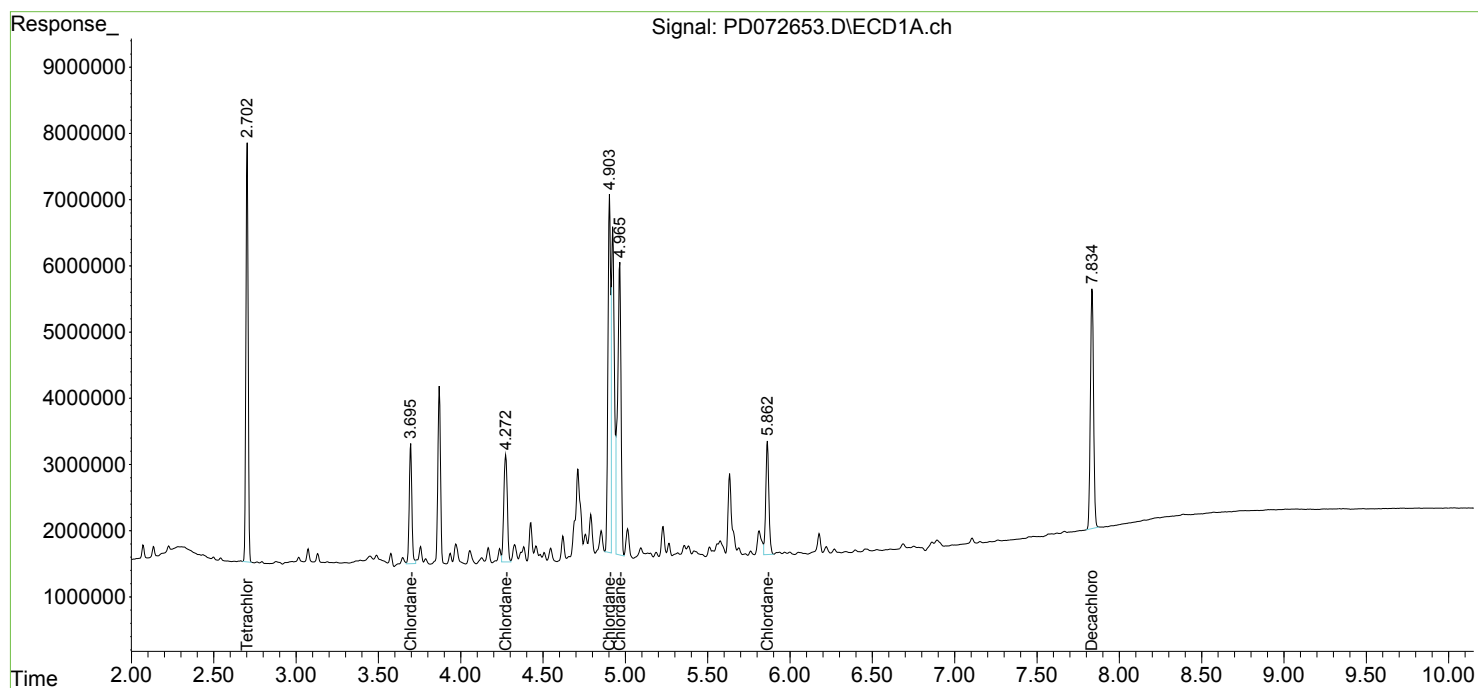


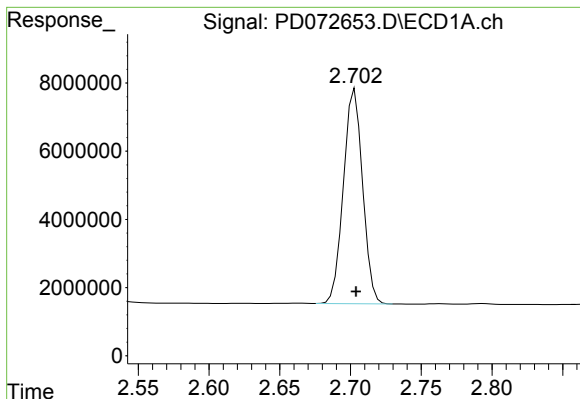

#1 Tetrachloro-m-xylene


R.T.: 2.703 min
Delta R.T.: 0.000 min
Response: 59556033
Conc: 24.30 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

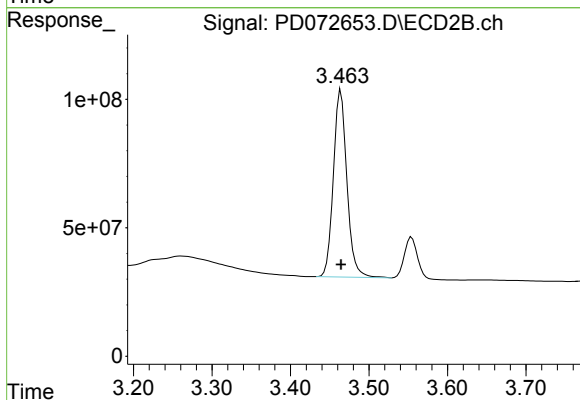


#1 Tetrachloro-m-xylene

R.T.: 3.464 min
Delta R.T.: 0.000 min
Response: 873349604
Conc: 25.91 ng/ml

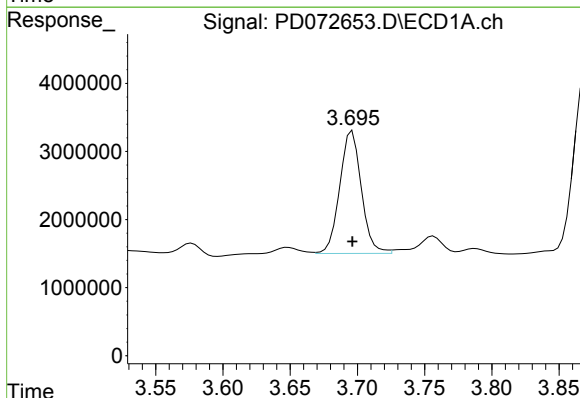


#23 Chlordane-1

R.T.: 3.696 min
Delta R.T.: 0.000 min
Response: 20061591
Conc: 253.01 ng/ml

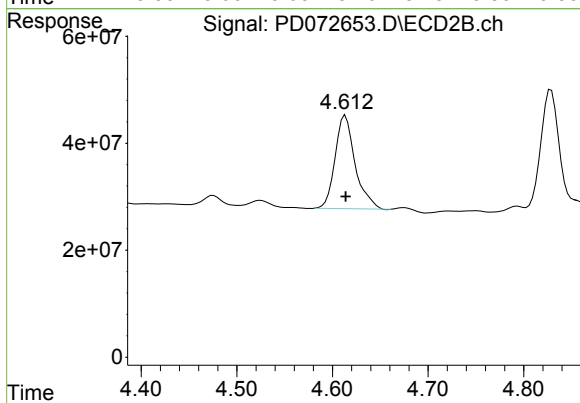

#23 Chlordane-1


R.T.: 4.613 min
Delta R.T.: 0.000 min
Response: 253718827
Conc: 263.28 ng/ml

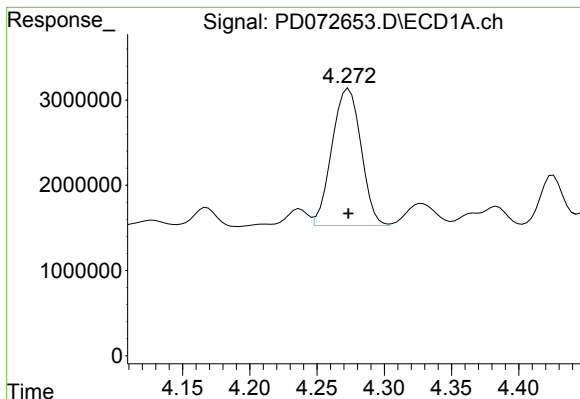

#24 Chlordane-2


R.T.: 4.274 min
Delta R.T.: 0.000 min
Response: 24112639
Conc: 261.53 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

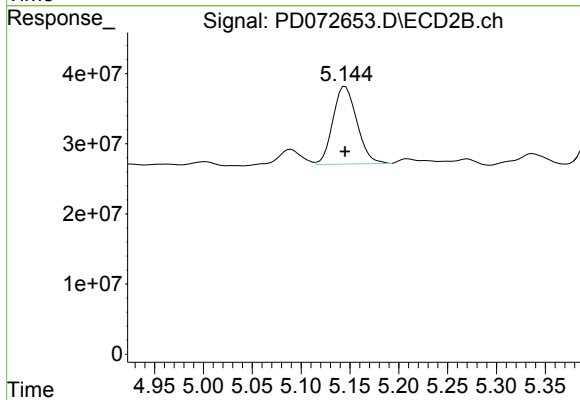


#24 Chlordane-2

R.T.: 5.145 min
Delta R.T.: 0.000 min
Response: 189433441
Conc: 272.86 ng/ml

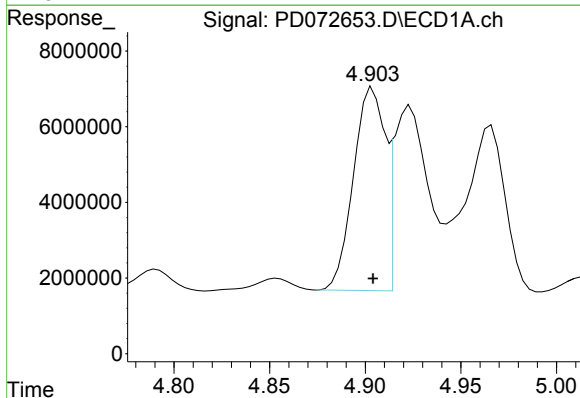


#25 Chlordane-3

R.T.: 4.904 min
Delta R.T.: 0.000 min
Response: 61598829
Conc: 236.97 ng/ml

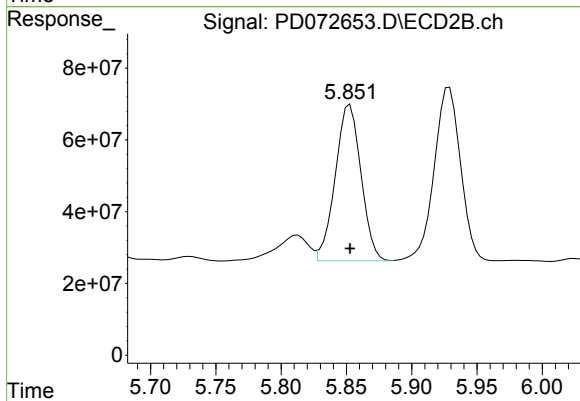

#25 Chlordane-3


R.T.: 5.853 min
Delta R.T.: 0.000 min
Response: 597259282
Conc: 258.33 ng/ml

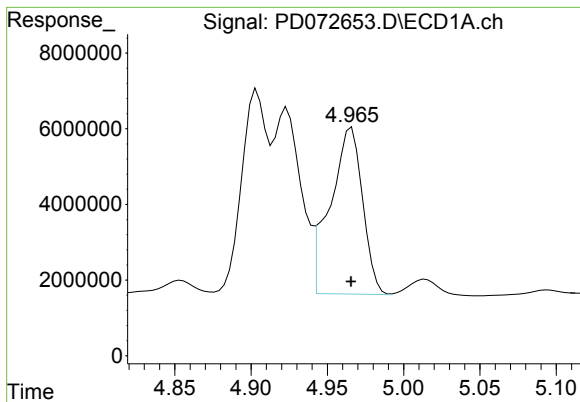

#26 Chlordane-4


R.T.: 4.966 min
Delta R.T.: 0.000 min
Response: 64832660
Conc: 246.60 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

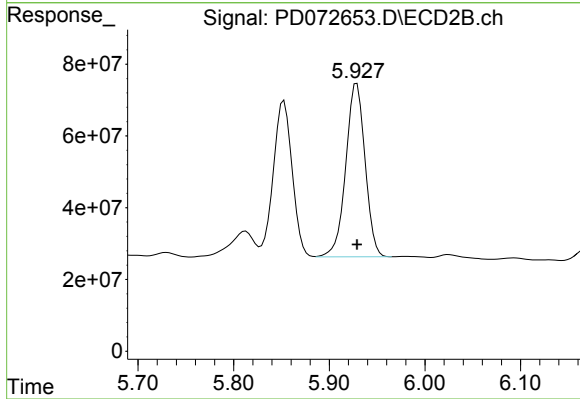


#26 Chlordane-4

R.T.: 5.929 min
Delta R.T.: 0.000 min
Response: 679246439
Conc: 258.61 ng/ml

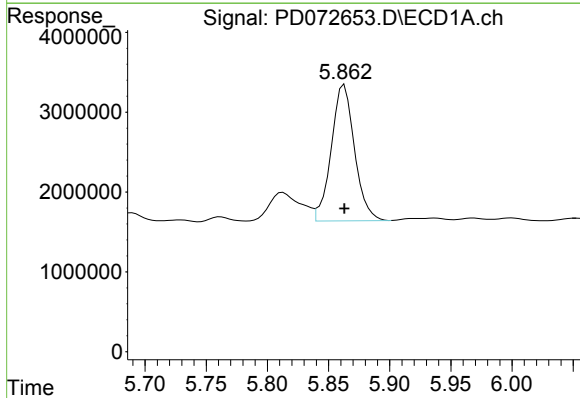


#27 Chlordane-5

R.T.: 5.863 min
Delta R.T.: 0.000 min
Response: 22509550
Conc: 247.44 ng/ml

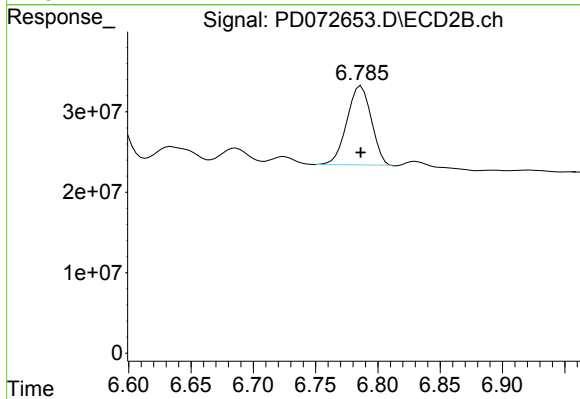

#27 Chlordane-5


R.T.: 6.786 min
Delta R.T.: 0.000 min
Response: 130326204
Conc: 259.22 ng/ml

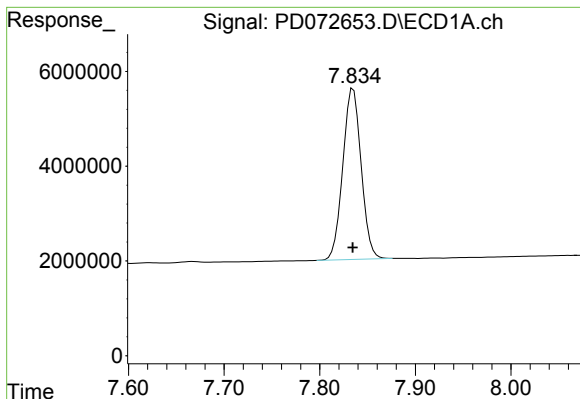

#28 Decachlorobiphenyl

R.T.: 7.835 min
Delta R.T.: 0.000 min
Response: 48280907
Conc: 25.59 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

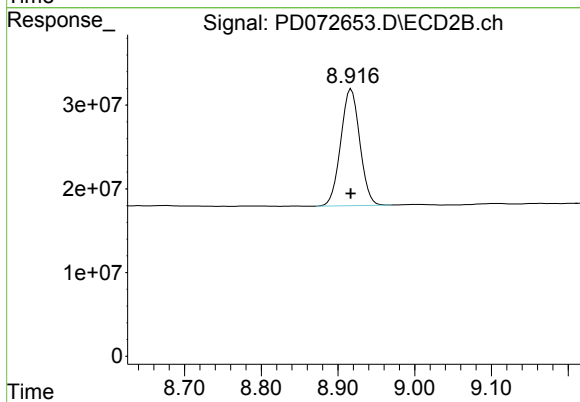

#28 Decachlorobiphenyl

R.T.: 8.917 min
Delta R.T.: 0.000 min
Response: 241725288
Conc: 25.71 ng/ml