

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102822\
 Data File : PD072654.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2022 13:19
 Operator : AR\AJ
 Sample : PCHLORICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 14:26:02 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102822.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 28 14:24:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.703	3.464	13317370	207.5E6	5.434	6.156
28)	SA Decachlor...	7.835	8.918	11943411	57123183	6.331	6.076
Target Compounds							
23)	Chlordane-1	3.696	4.614	5520548	59606498	69.625	61.853
24)	Chlordane-2	4.274	5.145	6279607	48927869	68.111	70.475
25)	Chlordane-3	4.904	5.853	14466026	148.8E6	55.651	64.347
26)	Chlordane-4	4.966	5.929	15066725	169.4E6	57.308	64.513
27)	Chlordane-5	5.863	6.786	5635414	28876837	61.949	57.437



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102822\
Data File : PD072654.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2022 13:19
Operator : AR\AJ
Sample : PCHLORICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 14:26:02 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102822.M
Quant Title : GC Extractables
QLast Update : Fri Oct 28 14:24:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

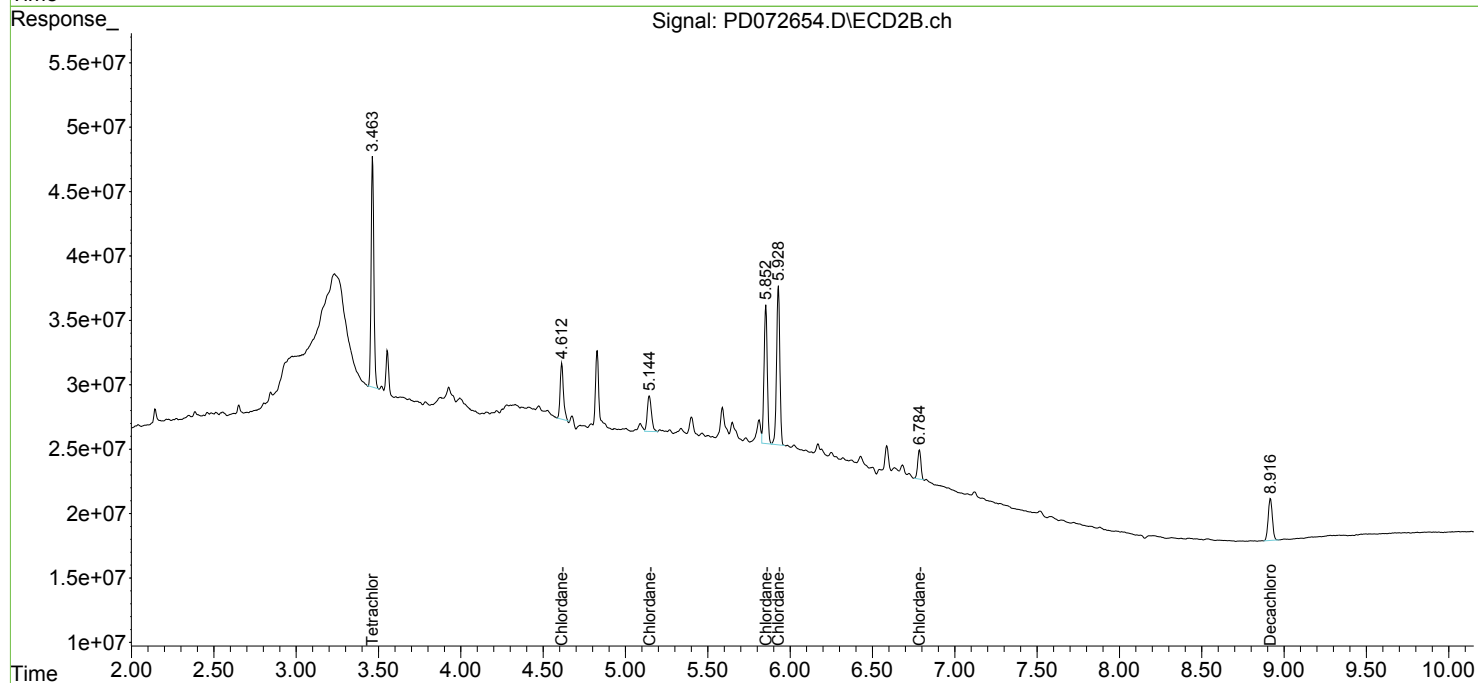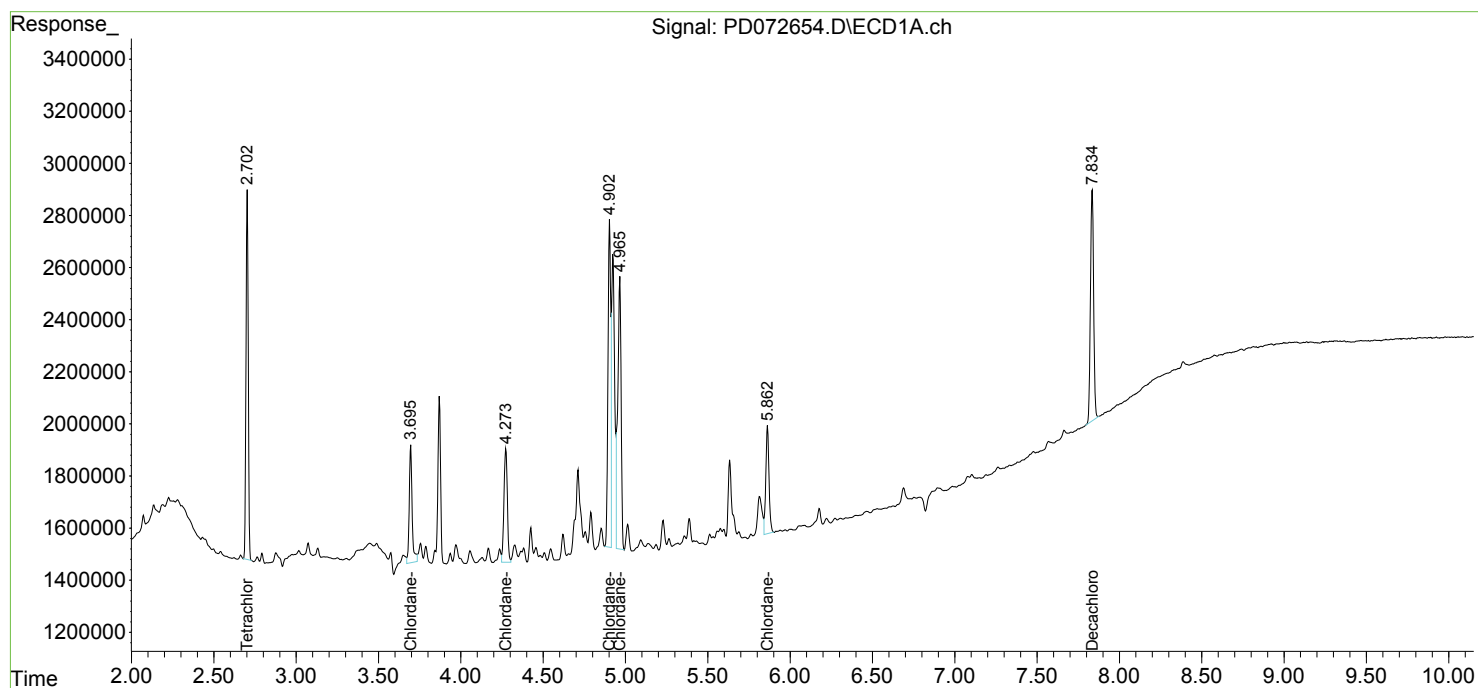


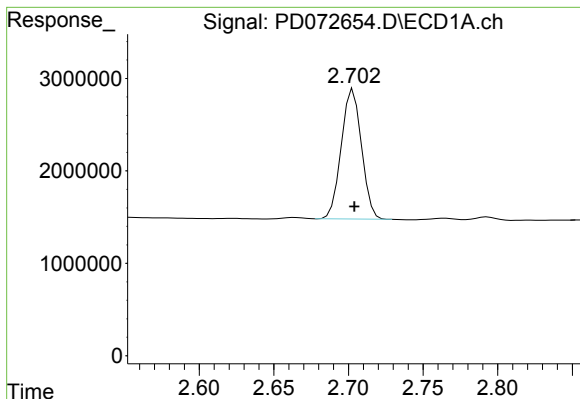

#1 Tetrachloro-m-xylene


R.T.: 2.703 min
Delta R.T.: 0.000 min
Response: 13317370
Conc: 5.43 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

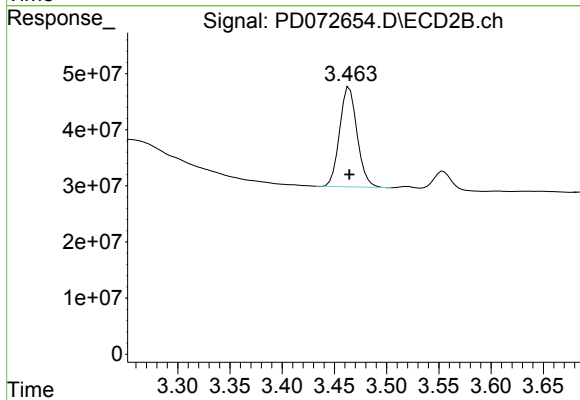


#1 Tetrachloro-m-xylene

R.T.: 3.464 min
Delta R.T.: 0.000 min
Response: 207521813
Conc: 6.16 ng/ml

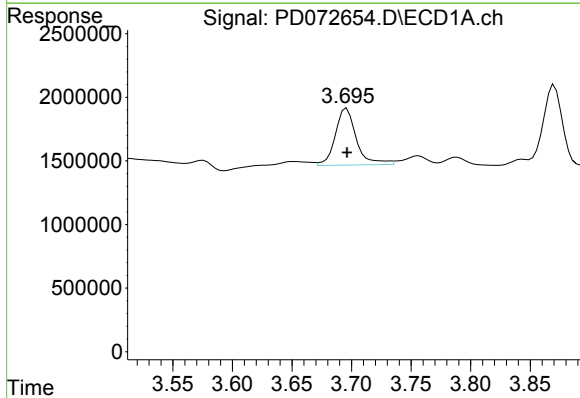


#23 Chlordane-1

R.T.: 3.696 min
Delta R.T.: 0.000 min
Response: 5520548
Conc: 69.62 ng/ml

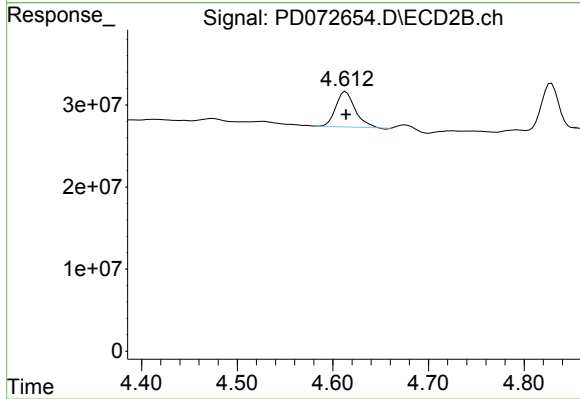

#23 Chlordane-1


R.T.: 4.614 min
Delta R.T.: 0.000 min
Response: 59606498
Conc: 61.85 ng/ml

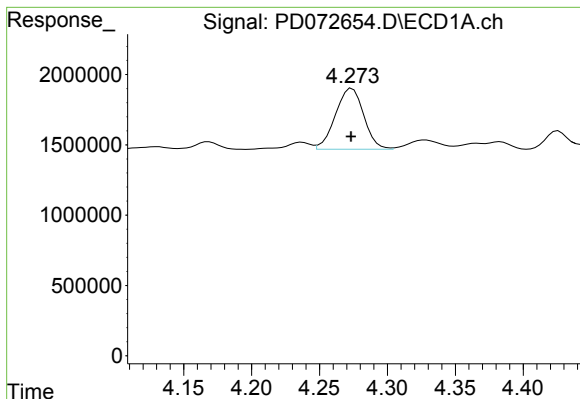

#24 Chlordane-2


R.T.: 4.274 min
Delta R.T.: 0.000 min
Response: 6279607
Conc: 68.11 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

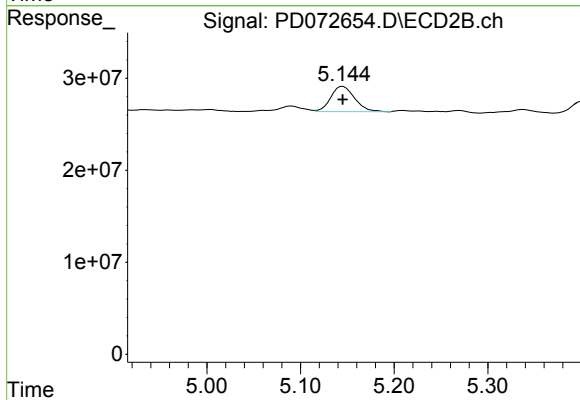


#24 Chlordane-2

R.T.: 5.145 min
Delta R.T.: 0.000 min
Response: 48927869
Conc: 70.47 ng/ml

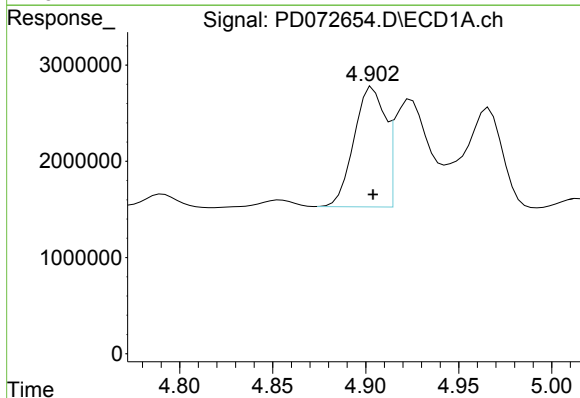


#25 Chlordane-3

R.T.: 4.904 min
Delta R.T.: 0.000 min
Response: 14466026
Conc: 55.65 ng/ml

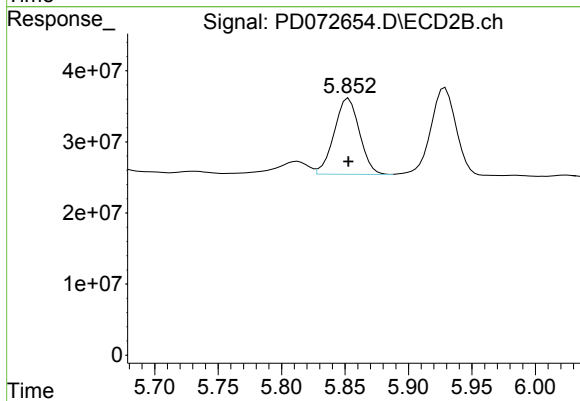

#25 Chlordane-3


R.T.: 5.853 min
Delta R.T.: 0.000 min
Response: 148770266
Conc: 64.35 ng/ml

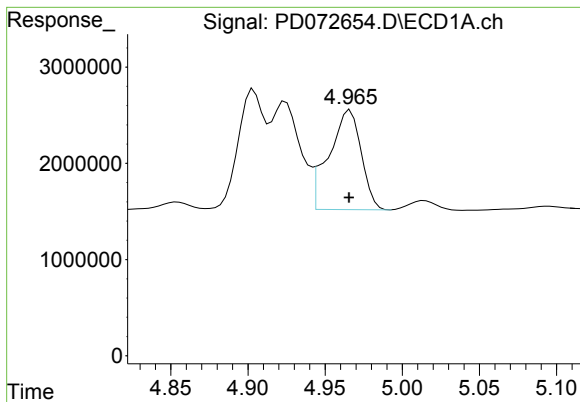

#26 Chlordane-4


R.T.: 4.966 min
Delta R.T.: 0.000 min
Response: 15066725
Conc: 57.31 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

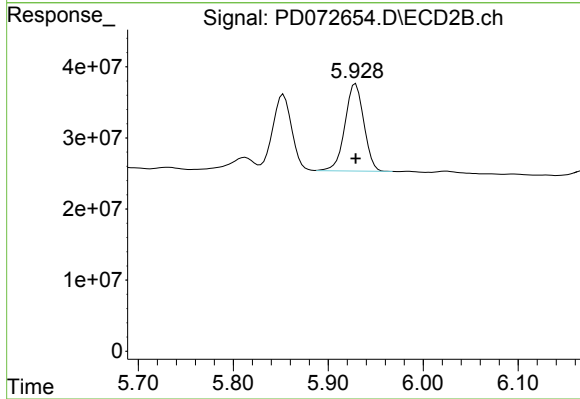


#26 Chlordane-4

R.T.: 5.929 min
Delta R.T.: 0.000 min
Response: 169445317
Conc: 64.51 ng/ml

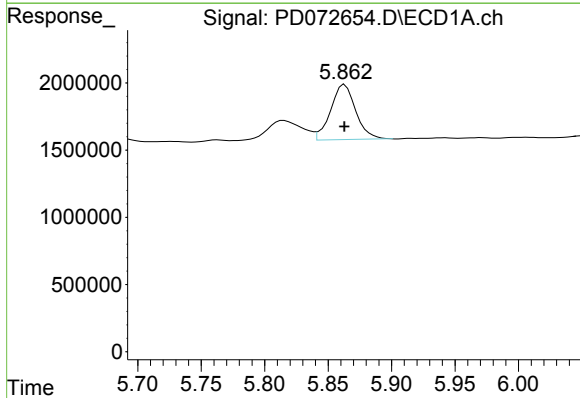


#27 Chlordane-5

R.T.: 5.863 min
Delta R.T.: 0.000 min
Response: 5635414
Conc: 61.95 ng/ml

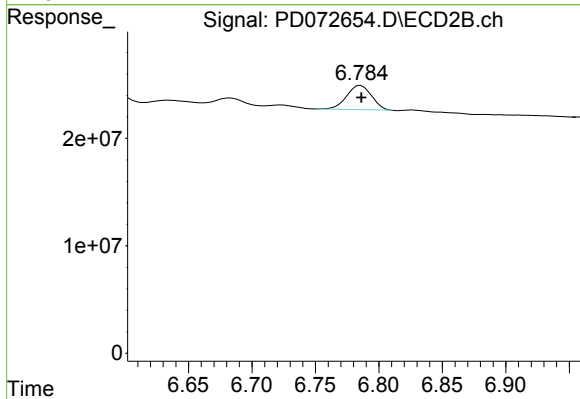

#27 Chlordane-5


R.T.: 6.786 min
Delta R.T.: 0.000 min
Response: 28876837
Conc: 57.44 ng/ml

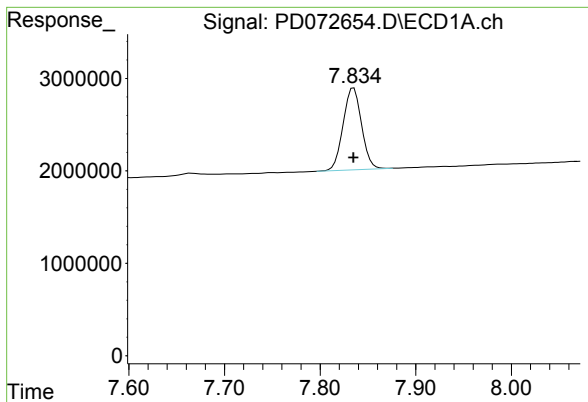

#28 Decachlorobiphenyl

R.T.: 7.835 min
Delta R.T.: 0.000 min
Response: 11943411
Conc: 6.33 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

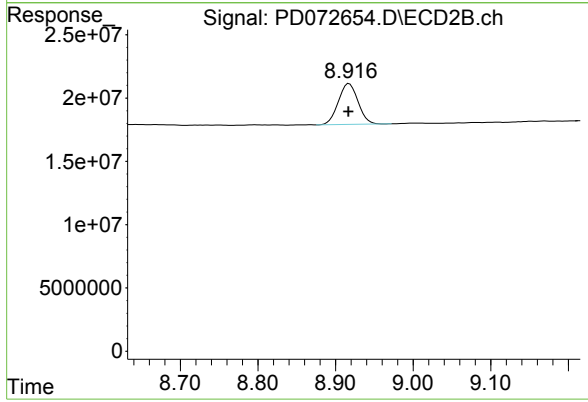

#28 Decachlorobiphenyl

R.T.: 8.918 min
Delta R.T.: 0.000 min
Response: 57123183
Conc: 6.08 ng/ml