

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102822\
 Data File : PD072671.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2022 18:27
 Operator : AR\AJ
 Sample : N5266-03
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 20221100-204.1-SITE-WATER

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 29 01:39:44 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102822.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 28 15:29:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.704	3.464	38277887	681.8E6	18.664	19.751
28)	SA Decachlor...	7.834	8.916	29106386	142.7E6	15.139	14.896

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102822\
Data File : PD072671.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2022 18:27
Operator : AR\AJ
Sample : N5266-03
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
20221100-204.1-SITE-WATER

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 01:39:44 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102822.M
Quant Title : GC Extractables
QLast Update : Fri Oct 28 15:29:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

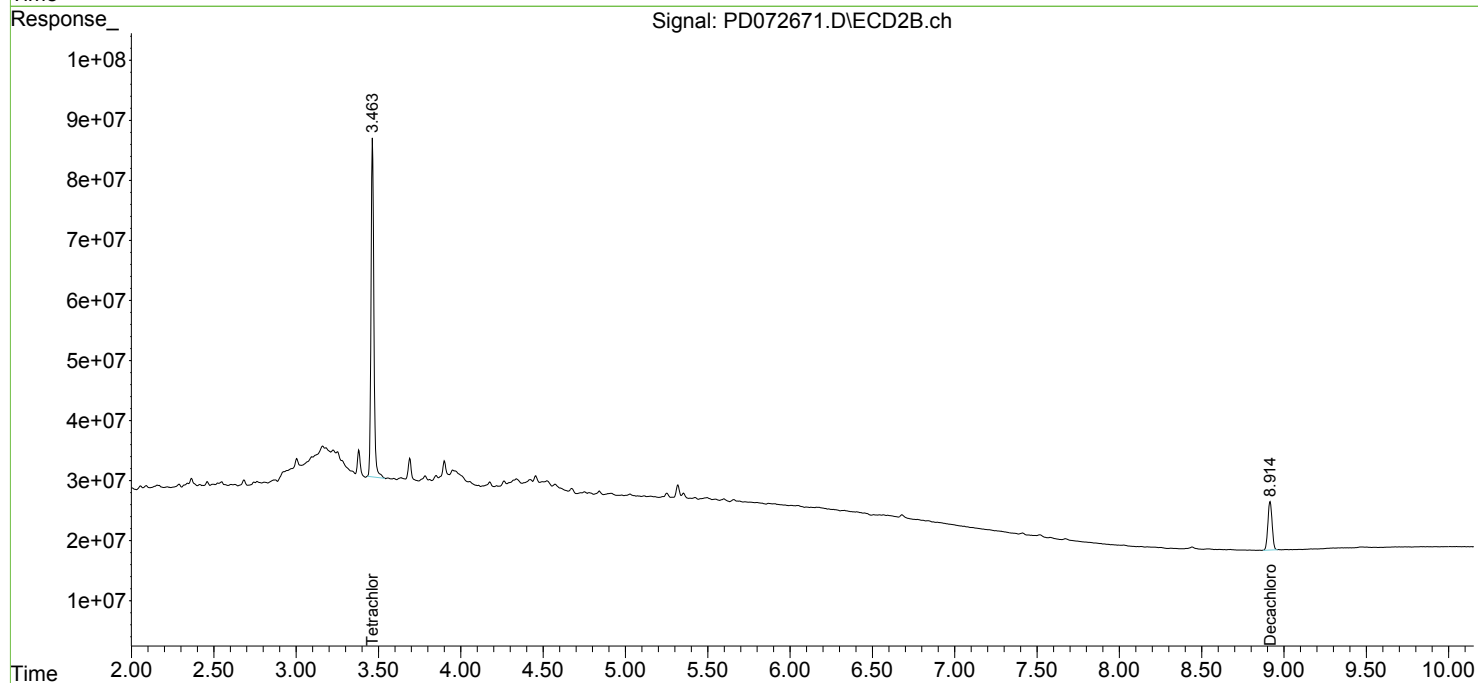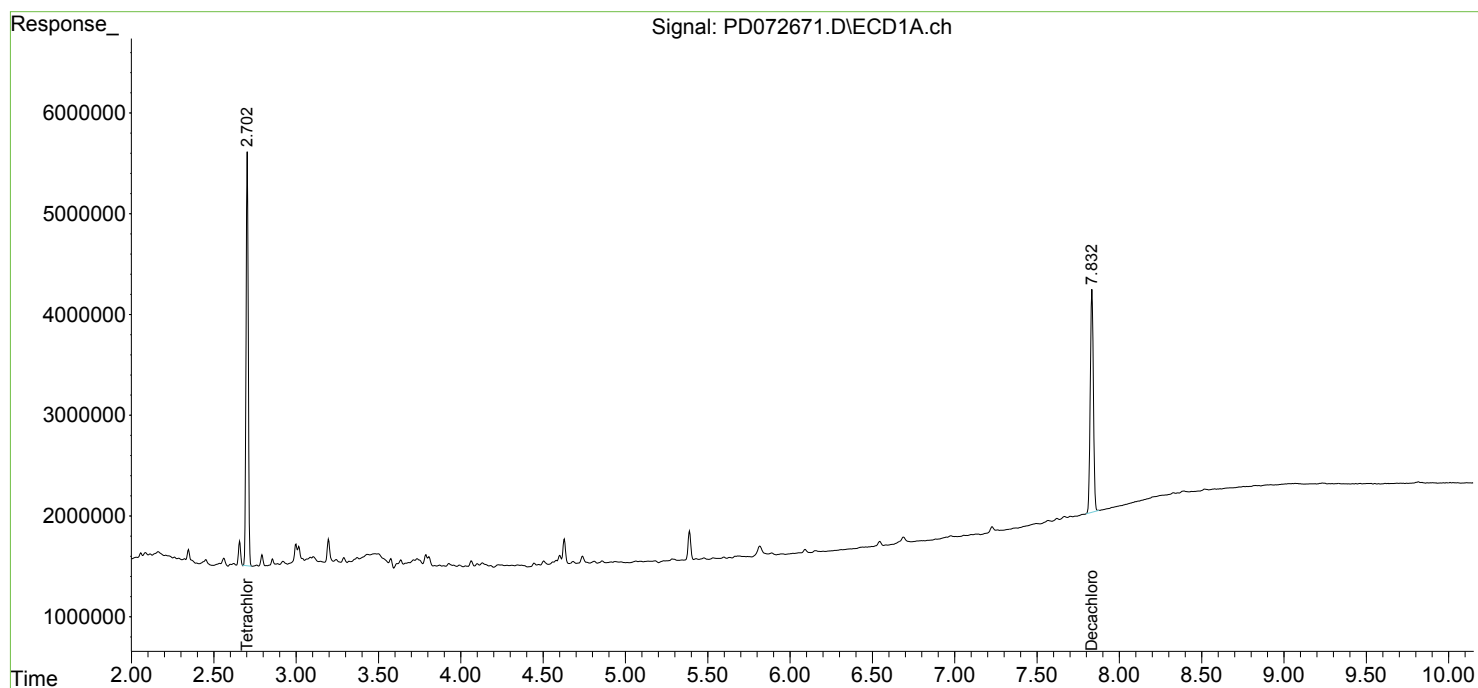


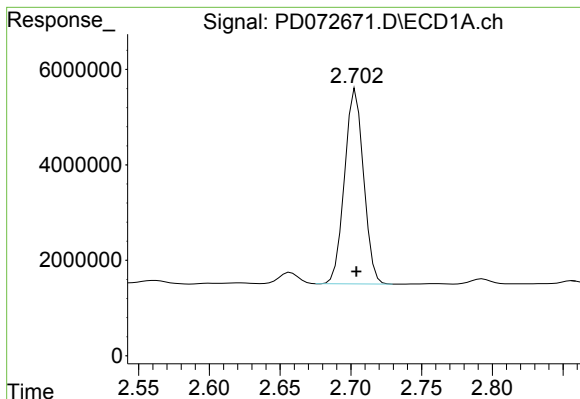

#1 Tetrachloro-m-xylene


R.T.: 2.704 min
Delta R.T.: 0.000 min
Response: 38277887
Conc: 18.66 ng/ml

Instrument :
ECD_D
ClientSampleId :
20221100-204.1-SITE-WATER

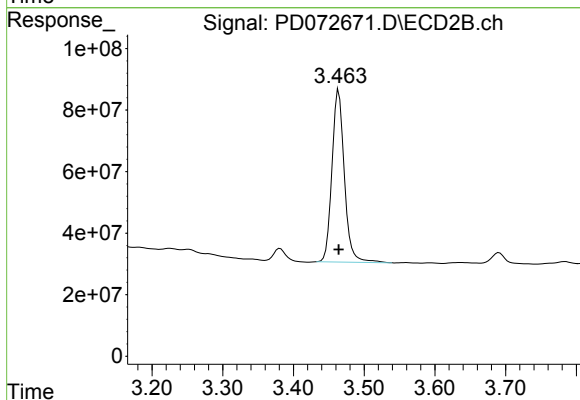


#1 Tetrachloro-m-xylene

R.T.: 3.464 min
Delta R.T.: 0.000 min
Response: 681780177
Conc: 19.75 ng/ml

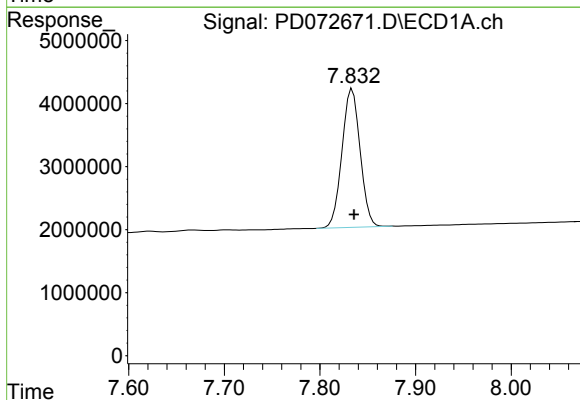

#28 Decachlorobiphenyl

R.T.: 7.834 min
Delta R.T.: -0.002 min
Response: 29106386
Conc: 15.14 ng/ml

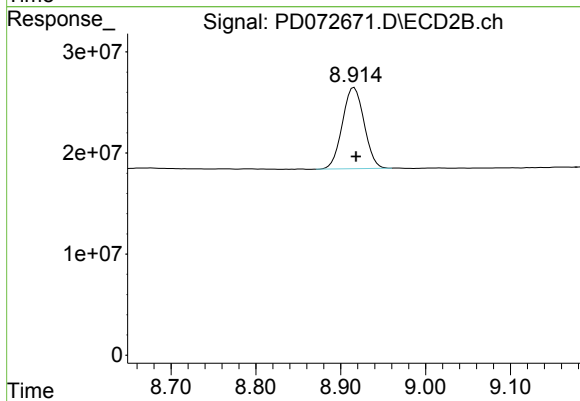

#28 Decachlorobiphenyl

R.T.: 8.916 min
Delta R.T.: -0.002 min
Response: 142741270
Conc: 14.90 ng/ml