

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102824\
 Data File : PD086228.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2024 13:30
 Operator : AR\AJ
 Sample : P4476-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 XA102

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 10/29/2024
 Supervised By :Ankita Jodhani 10/29/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 29 02:30:20 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102524CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 25 14:36:38 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.560	2.892	28195471	206.8E6	21.416	22.289
27)	SA Decachlor...	9.092	8.098	39780179	234.9E6	22.189	24.840
Target Compounds							
2)	A alpha-BHC	4.011	3.406	2227.3E6	7463.0E6	894.724	519.436 #
3)	MA gamma-BHC...	4.343	3.742	2654.5E6	8631.9E6	1066.918	639.985 #
4)	MA Heptachlor	4.944	4.099	1179.8E6	4169.0E6	477.239	305.153 #
5)	MB Aldrin	5.286	4.386	1311.2E6	4551.0E6	540.976	335.453 #
6)	B beta-BHC	4.525	4.037	1140.2E6	4328.7E6	1026.652m	690.396 #
7)	B delta-BHC	4.775	4.275	802.4E6	2888.2E6	309.958	205.830 #
8)	B Heptachlo...	5.704	4.890	603.7E6	2383.2E6	264.167m	190.048 #
9)	A Endosulfan I	6.087	5.264	803.1E6	2810.6E6	396.482m	244.790m#
10)	B trans-Chl...	5.959	5.144	2990.0E6	10122.0E6	1355.075m	769.460 #
11)	B cis-Chlor...	6.040	5.209	2916.2E6	9915.9E6	1318.882m	780.704 #
12)	B 4,4'-DDE	6.210	5.395	3115.7E6	10398.5E6	1458.719	848.074 #
13)	MA Dieldrin	6.362	5.531	1532.0E6	5406.6E6	671.649	438.229 #
14)	MA Endrin	6.589	5.807	465.7E6	1982.5E6	247.752	176.413 #
15)	B Endosulfa...	6.799	6.099	400.1E6	1754.2E6	199.558	158.999
16)	A 4,4'-DDD	6.719	5.949	2362.4E6	7990.5E6	1457.880	814.010 #
17)	MA 4,4'-DDT	7.033	6.204	2209.3E6	7640.6E6	1325.130m	744.570 #
18)	B Endrin al...	6.928	6.277	698.2E6	2746.7E6	468.065	330.887 #
19)	B Endosulfa...	7.161	6.501	1320.1E6	4861.0E6	716.125m	461.133 #
20)	A Methoxychlor	7.506	6.777	900.9E6	3204.4E6	957.257	674.144 #
21)	B Endrin ke...	7.642	7.010	2102.1E6	6877.1E6	1020.043m	600.998 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102824\
Data File : PD086228.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2024 13:30
Operator : AR\AJ
Sample : P4476-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 02:30:20 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102524CLP.M
Quant Title : GC Extractables
QLast Update : Fri Oct 25 14:36:38 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

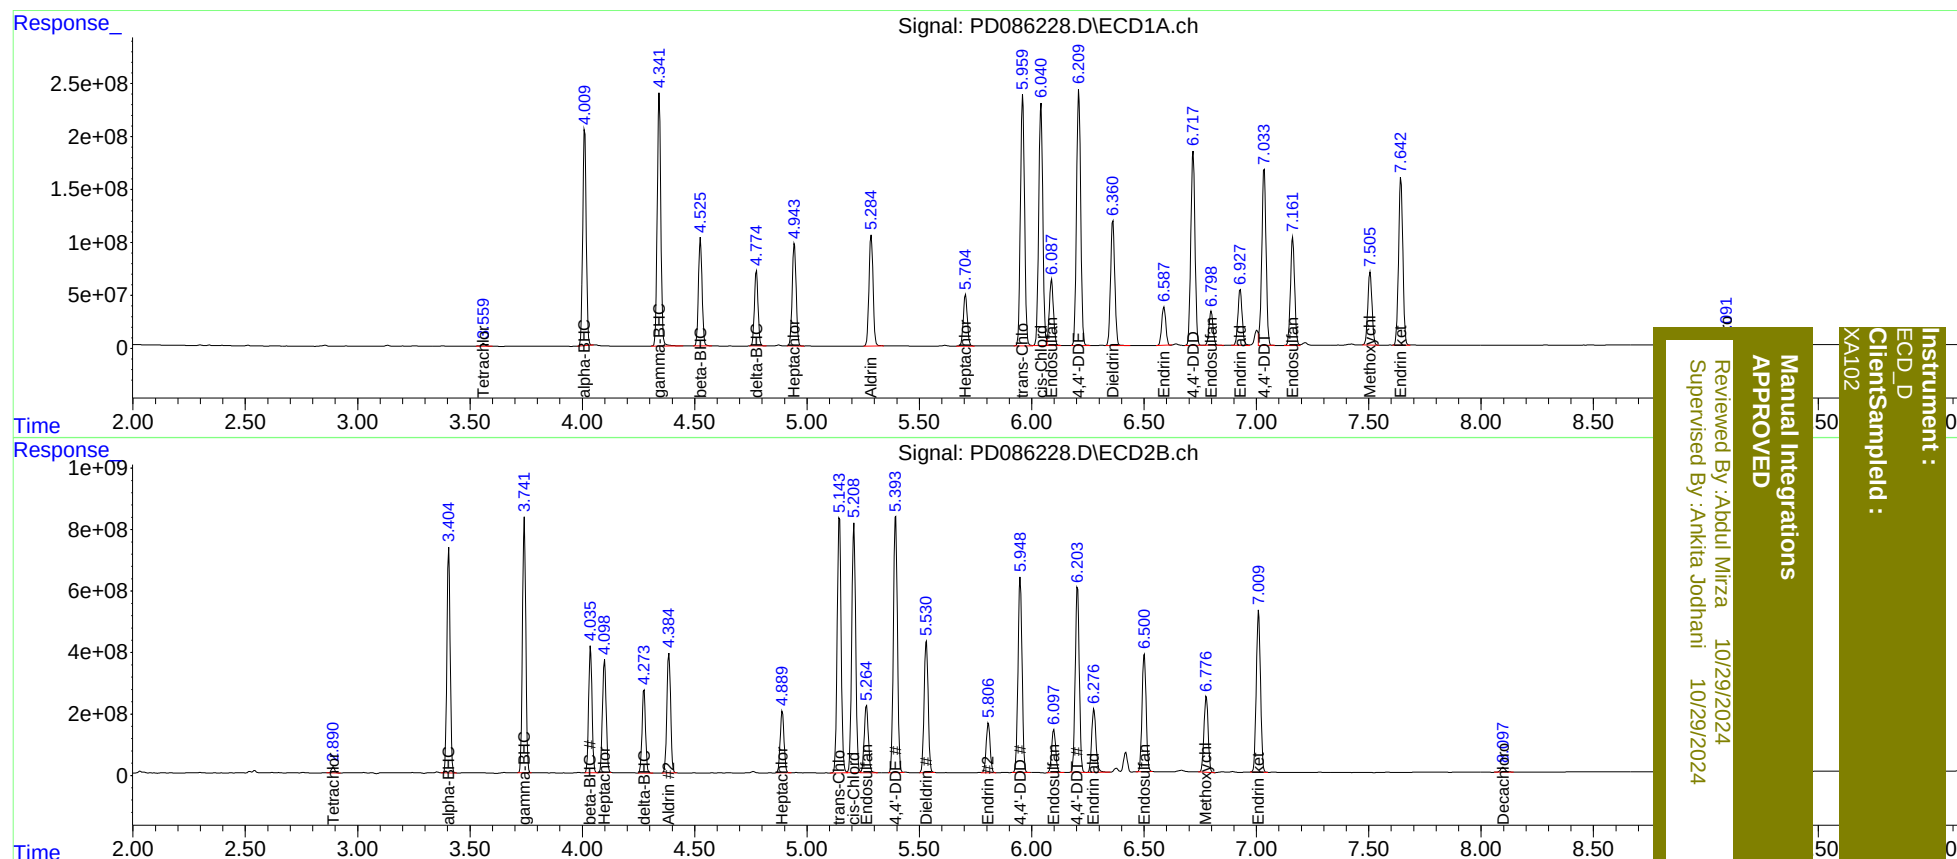

160
Reviewed By: Abdul Mirza 10/29/2024
Supervised By: Ankita Jodhani 10/29/2024

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
XA102