

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102825\
 Data File : PD090899.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2025 20:08
 Operator : AR\AJ
 Sample : Q3472-16 10X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 142

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/29/2025
 Supervised By : Sohil Jodhani 10/29/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 29 01:47:28 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101725.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 17 17:43:28 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.542	2.874	6109998	65828410	1.962m	2.211
28) SA Decachlor...	9.061	8.059	10354286	33385720	2.213m	1.102 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102825\
Data File : PD090899.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2025 20:08
Operator : AR\AJ
Sample : Q3472-16 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
142


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 10/29/2025
Supervised By : Sohil Jodhani 10/29/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 01:47:28 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101725.M
Quant Title : GC Extractables
QLast Update : Fri Oct 17 17:43:28 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

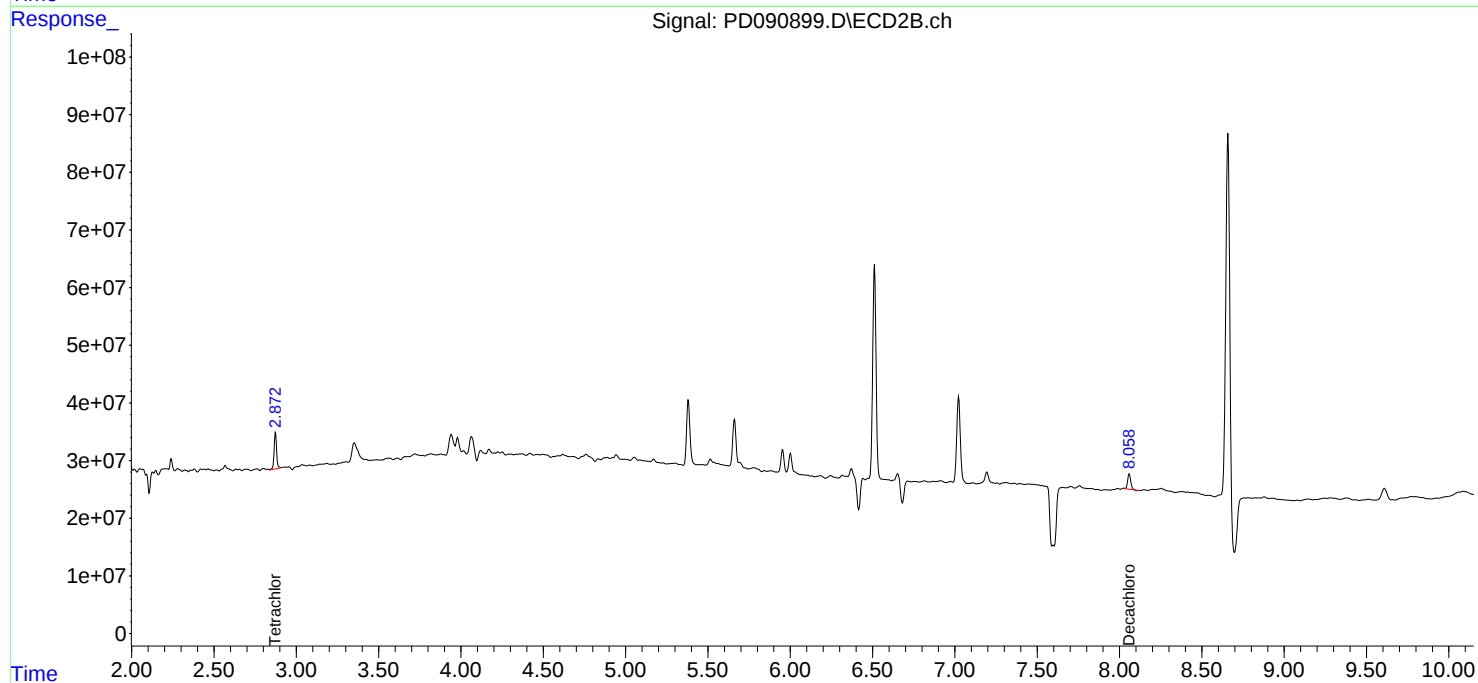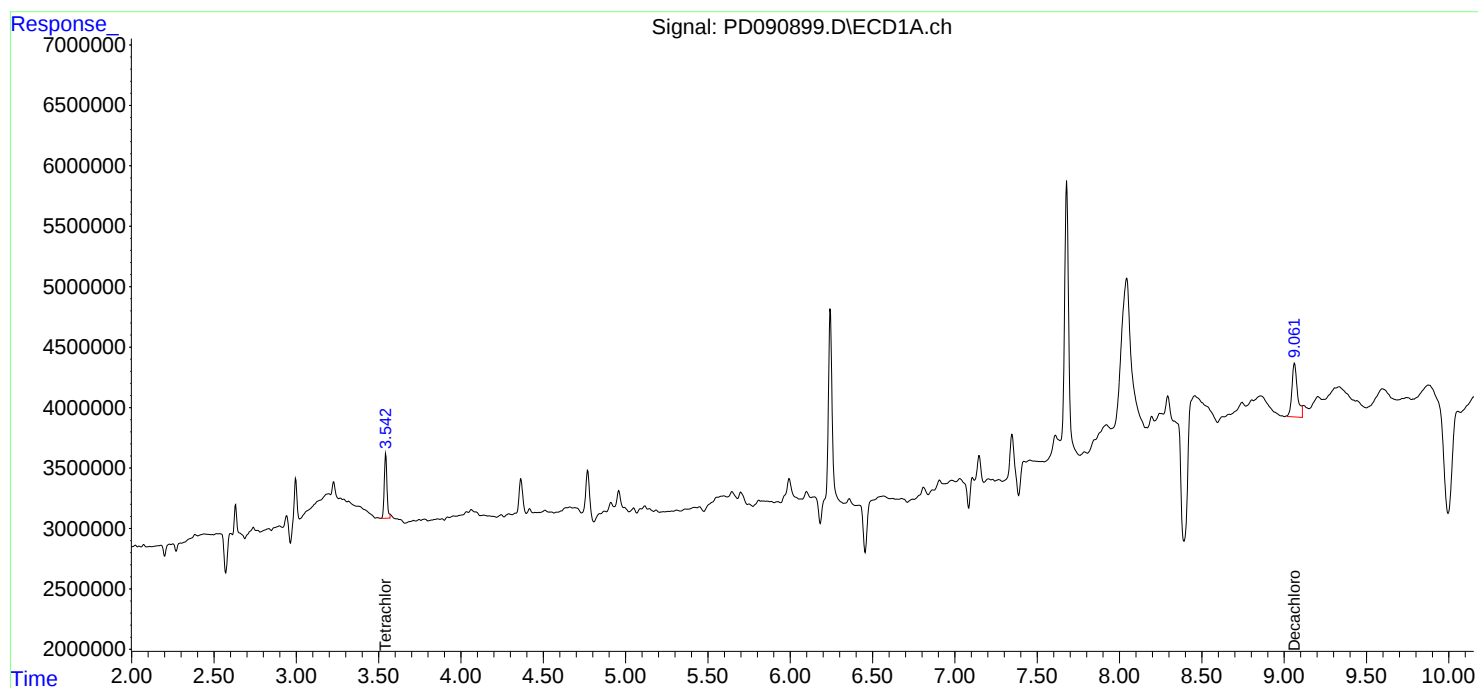

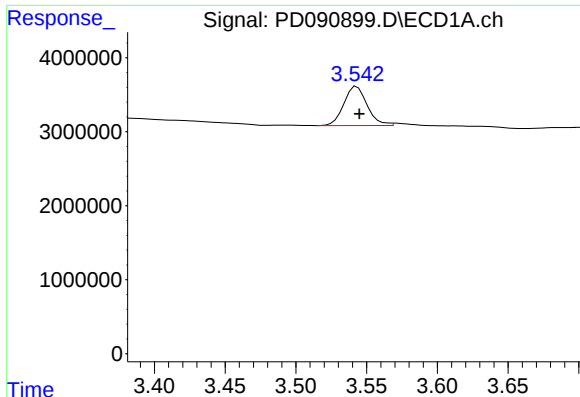


#1 Tetrachloro-m-xylene

R.T.: 3.542 min
Delta R.T.: -0.003 min
Response: 6109998
Conc: 1.96 ng/ml

Instrument :
ECD_D
ClientSampleId :
142


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/29/2025
Supervised By :Sohil Jodhani 10/29/2025

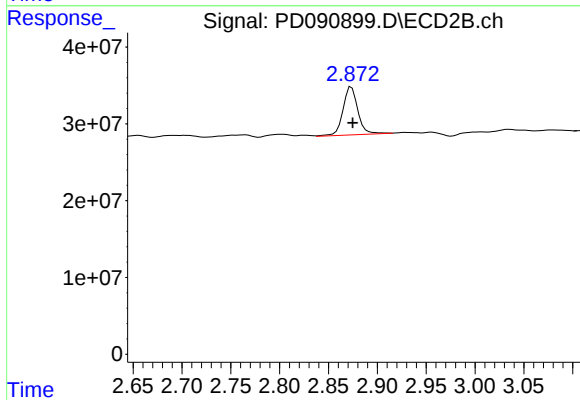


#1 Tetrachloro-m-xylene

R.T.: 2.874 min
Delta R.T.: -0.001 min
Response: 65828410
Conc: 2.21 ng/ml

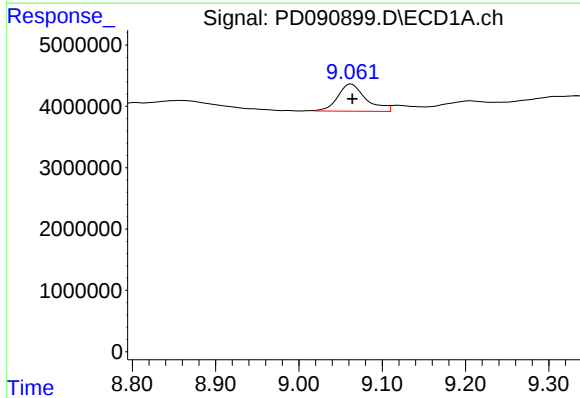

#28 Decachlorobiphenyl

R.T.: 9.061 min
Delta R.T.: -0.003 min
Response: 10354286
Conc: 2.21 ng/ml m

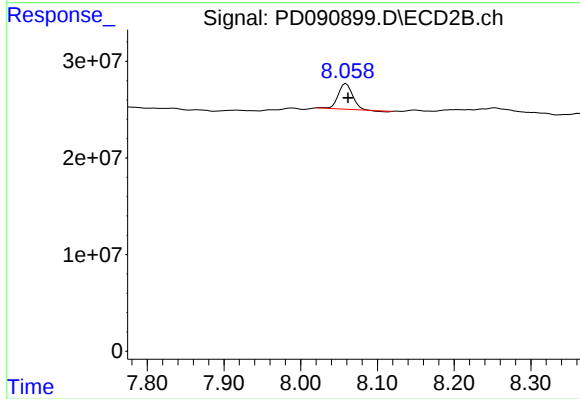

#28 Decachlorobiphenyl

R.T.: 8.059 min
Delta R.T.: -0.003 min
Response: 33385720
Conc: 1.10 ng/ml