

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102920\
 Data File : PD059998.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Oct 2020 00:53
 Operator : DD\AJ
 Sample : PB132705BL
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 08:57:08 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102920.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 30 04:34:44 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	3.507	4.025	18406658	58367612	19.793	20.172
28)	SA Decachlor...	8.308	9.114	23338562	50881474	19.746	21.945
Target Compounds							
5)	MB Aldrin	0.000	5.533	0	814637	N.D.	0.215 #
9)	A Endosulfan I	0.000	6.247f	0	480943	N.D.	0.148 #
10)	B gamma-Chl...	0.000	6.149	0	2477293	N.D.	0.701 #
11)	B alpha-Chl...	0.000	6.208	0	375806	N.D.	0.107 #
24)	Chlordane-2	0.000	5.484	0	677451	N.D.	5.667 #
25)	Chlordane-3	0.000	6.149	0	2477293	N.D.	5.411 #
26)	Chlordane-4	0.000	6.208	0	375806	N.D.	0.698 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102920\
Data File : PD059998.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2020 00:53
Operator : DD\AJ
Sample : PB132705BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 08:57:08 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102920.M
Quant Title : GC Extractables
QLast Update : Fri Oct 30 04:34:44 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

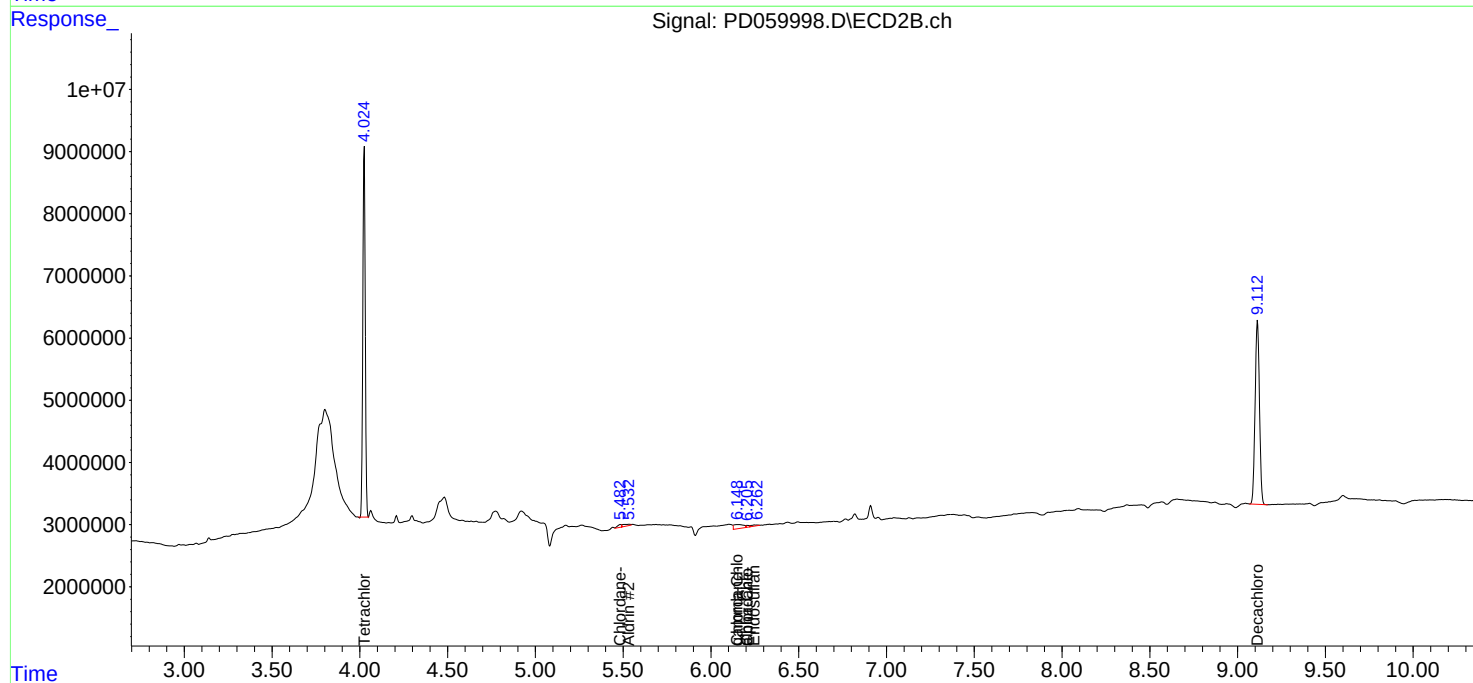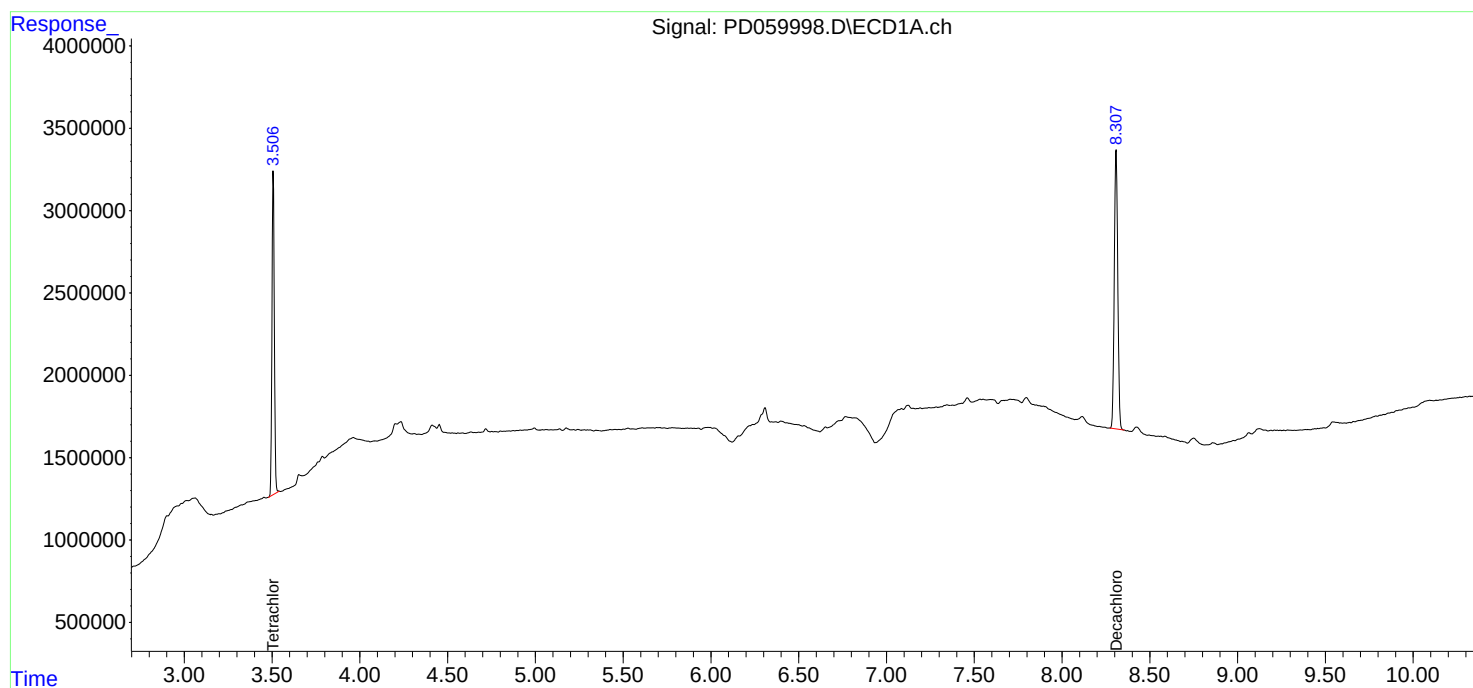

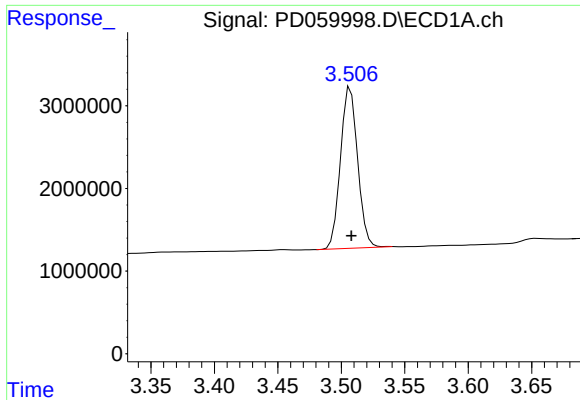


#1 Tetrachloro-m-xylene

R.T.: 3.507 min
Delta R.T.: 0.000 min
Response: 18406658
Conc: 19.79 ng/ml

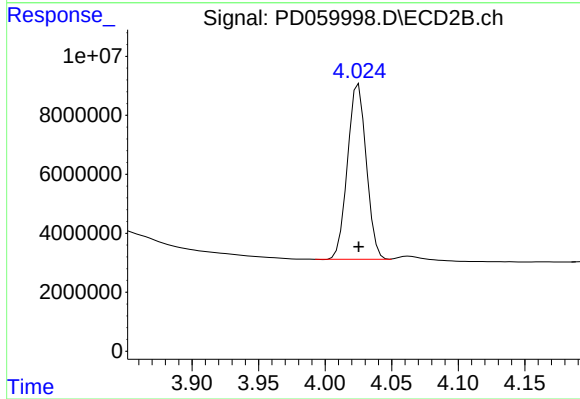


#1 Tetrachloro-m-xylene

R.T.: 4.025 min
Delta R.T.: 0.000 min
Response: 58367612
Conc: 20.17 ng/ml

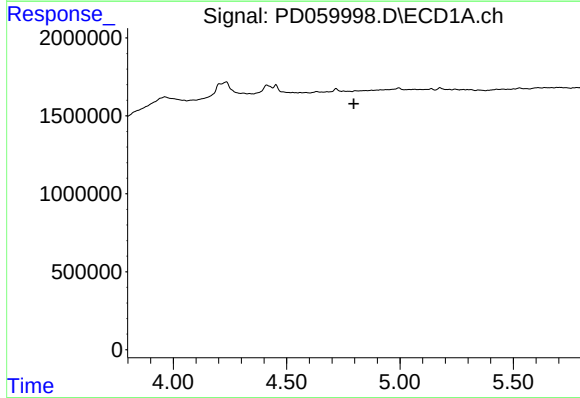


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 4.796 min
Response: 0
Conc: N.D.

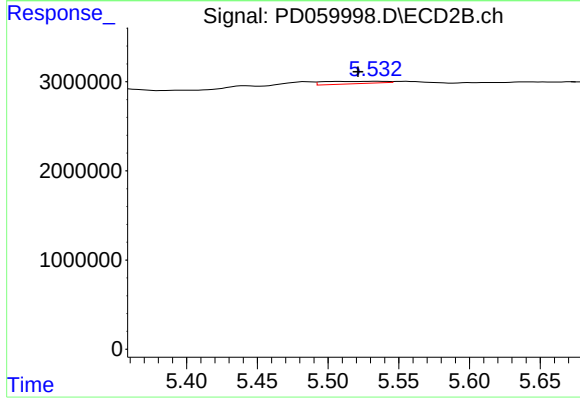


#5 Aldrin

R.T.: 5.533 min
Delta R.T.: 0.012 min
Response: 814637
Conc: 0.21 ng/ml

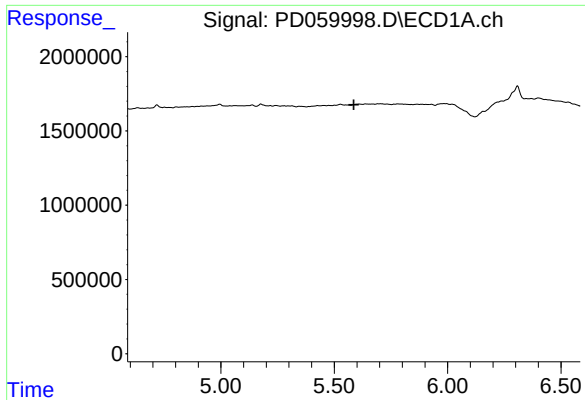


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.586 min
Response: 0
Conc: N.D.

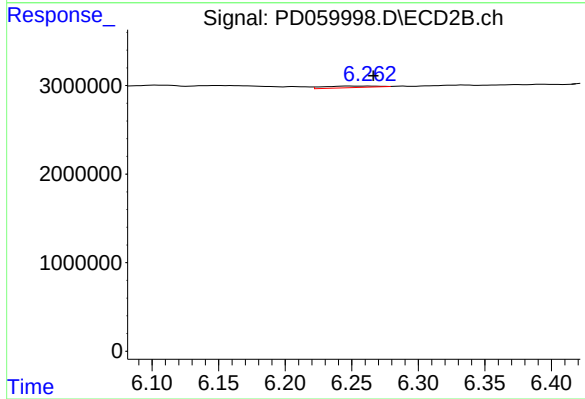


#9 Endosulfan I

R.T.: 6.247 min
Delta R.T.: -0.019 min
Response: 480943
Conc: 0.15 ng/ml

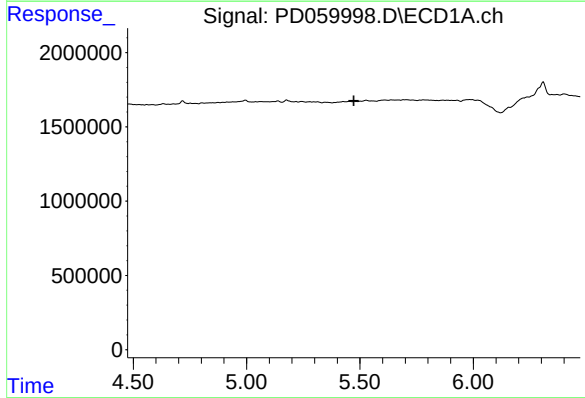


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.472 min
Response: 0
Conc: N.D.

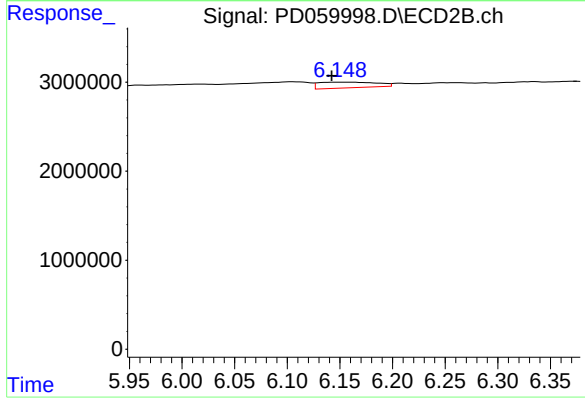


#10 gamma-Chlordane

R.T.: 6.149 min
Delta R.T.: 0.007 min
Response: 2477293
Conc: 0.70 ng/ml

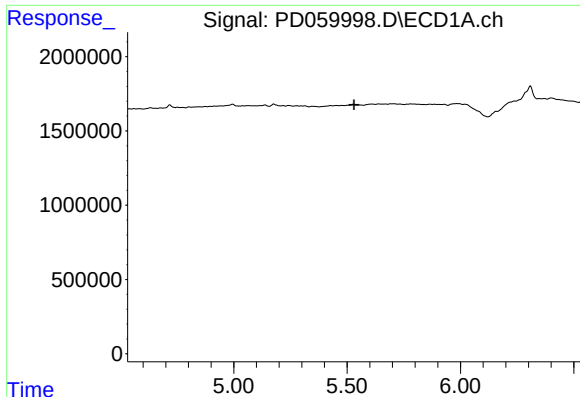


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.532 min
Response: 0
Conc: N.D.

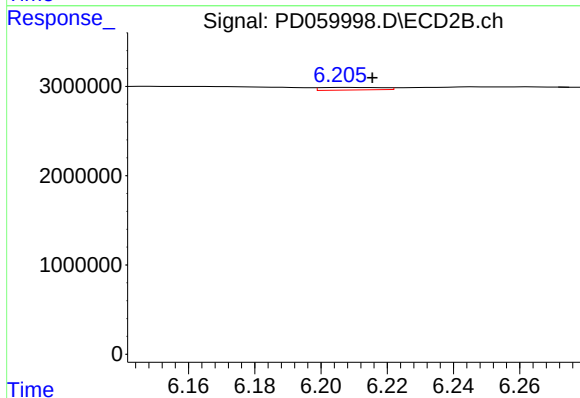


#11 alpha-Chlordane

R.T.: 6.208 min
Delta R.T.: -0.008 min
Response: 375806
Conc: 0.11 ng/ml

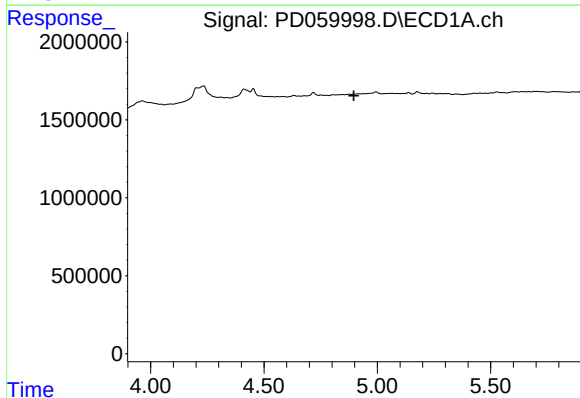


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T.: 4.897 min
Response: 0
Conc: N.D.

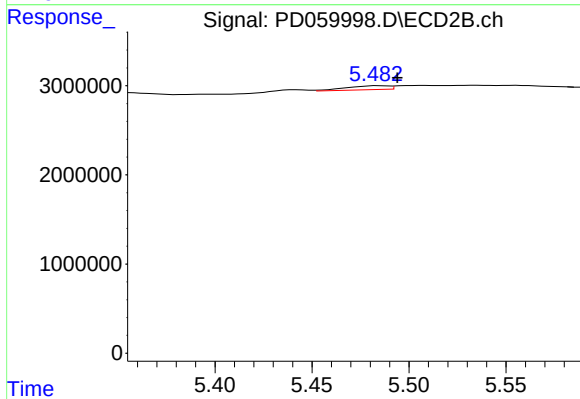


#24 Chlordane-2

R.T.: 5.484 min
Delta R.T.: -0.010 min
Response: 677451
Conc: 5.67 ng/ml

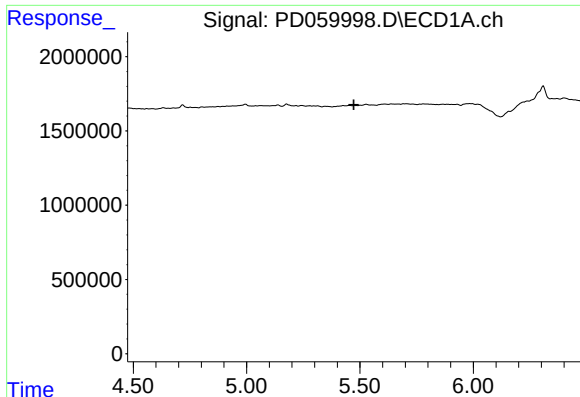


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.472 min
Response: 0
Conc: N.D.

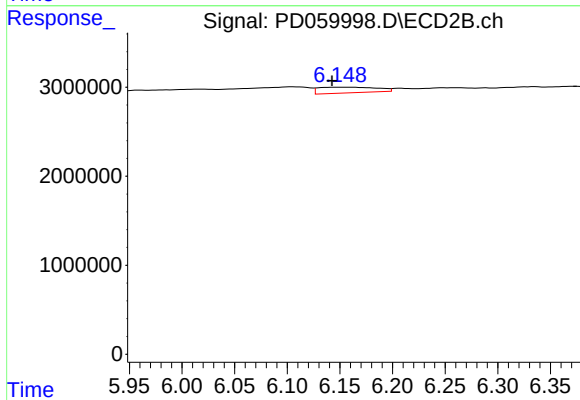


#25 Chlordane-3

R.T.: 6.149 min
Delta R.T.: 0.006 min
Response: 2477293
Conc: 5.41 ng/ml

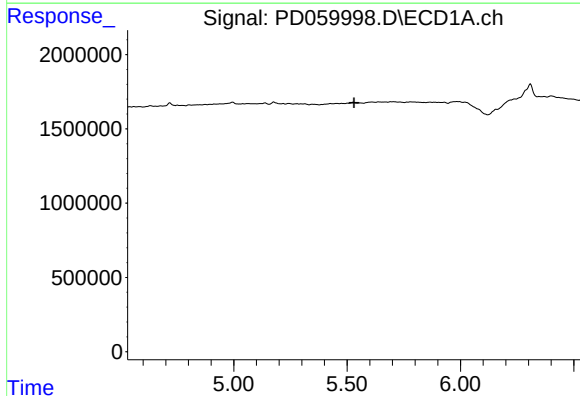


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.531 min
Response: 0
Conc: N.D.

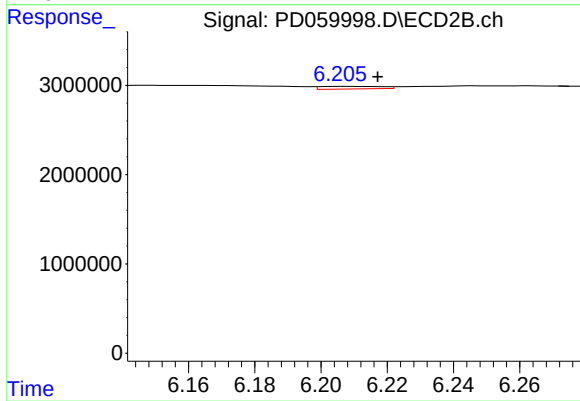


#26 Chlordane-4

R.T.: 6.208 min
Delta R.T.: -0.010 min
Response: 375806
Conc: 0.70 ng/ml

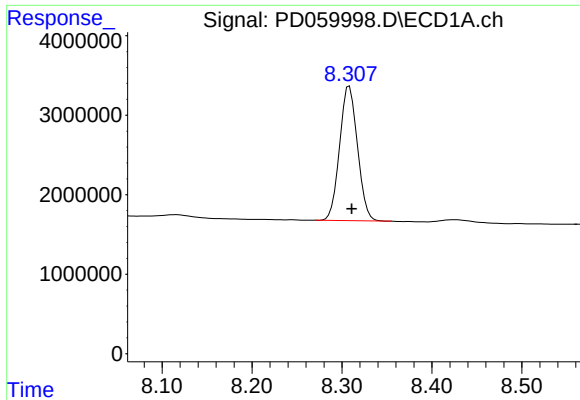

#28 Decachlorobiphenyl

R.T.: 8.308 min
Delta R.T.: -0.003 min
Response: 23338562
Conc: 19.75 ng/ml

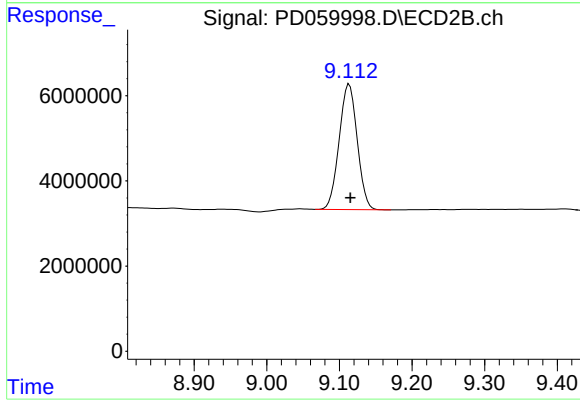

#28 Decachlorobiphenyl

R.T.: 9.114 min
Delta R.T.: -0.002 min
Response: 50881474
Conc: 21.94 ng/ml