

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102920\
 Data File : PD059976.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Oct 2020 19:41
 Operator : DD\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 03:56:17 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102920.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 30 03:55:09 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.507	4.025	82361526	217.6E6	75.636	74.949
28)	SA Decachlor...	8.309	9.115	84887298	169.9E6	74.219	74.358
Target Compounds							
23)	Chlordane-1	4.390	5.025	26003955	83643949	747.896	725.166
24)	Chlordane-2	4.896	5.494	28277356	82651355	740.878	734.511
25)	Chlordane-3	5.472	6.142	88019726	336.2E6	763.870	757.178
26)	Chlordane-4	5.531	6.217	72043953	395.9E6	755.416	753.881
27)	Chlordane-5	6.375	7.024	31119007	73157375	749.035	755.119



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102920\
Data File : PD059976.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Oct 2020 19:41
Operator : DD\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 03:56:17 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102920.M
Quant Title : GC Extractables
QLast Update : Fri Oct 30 03:55:09 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

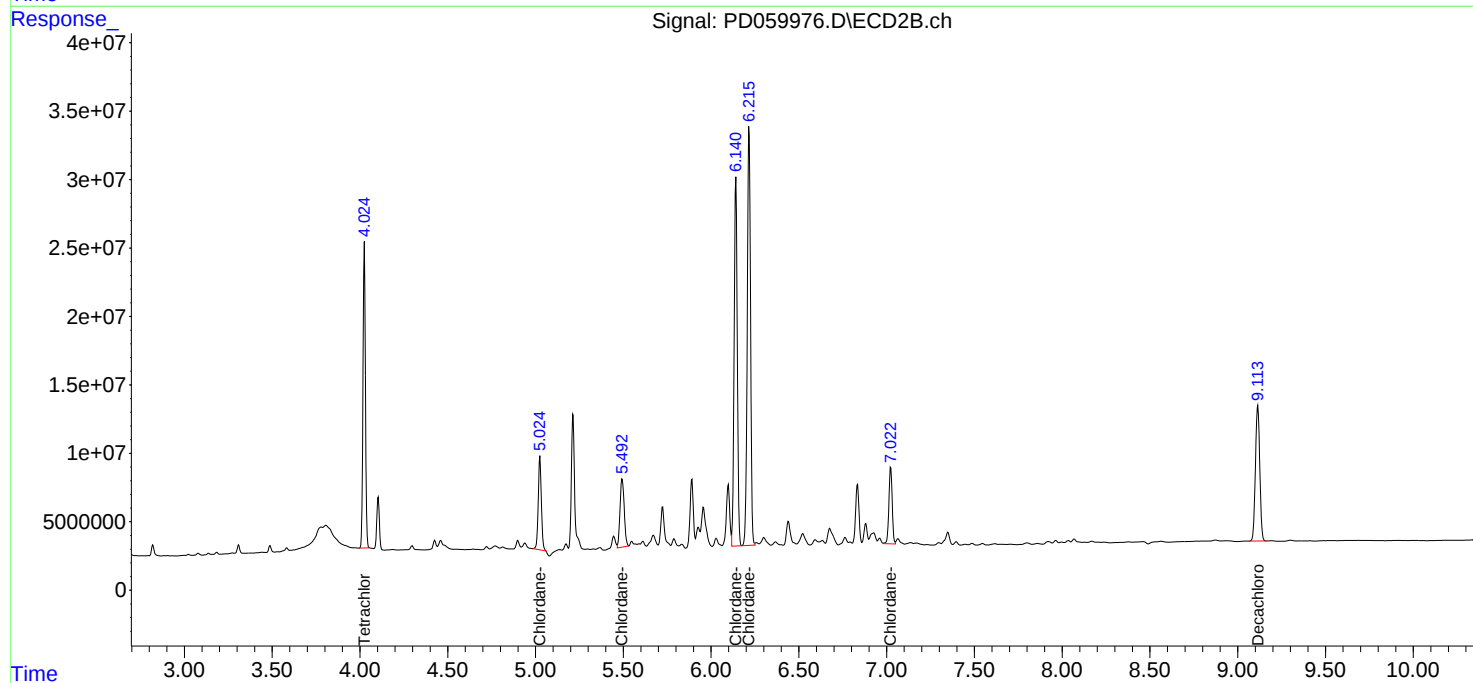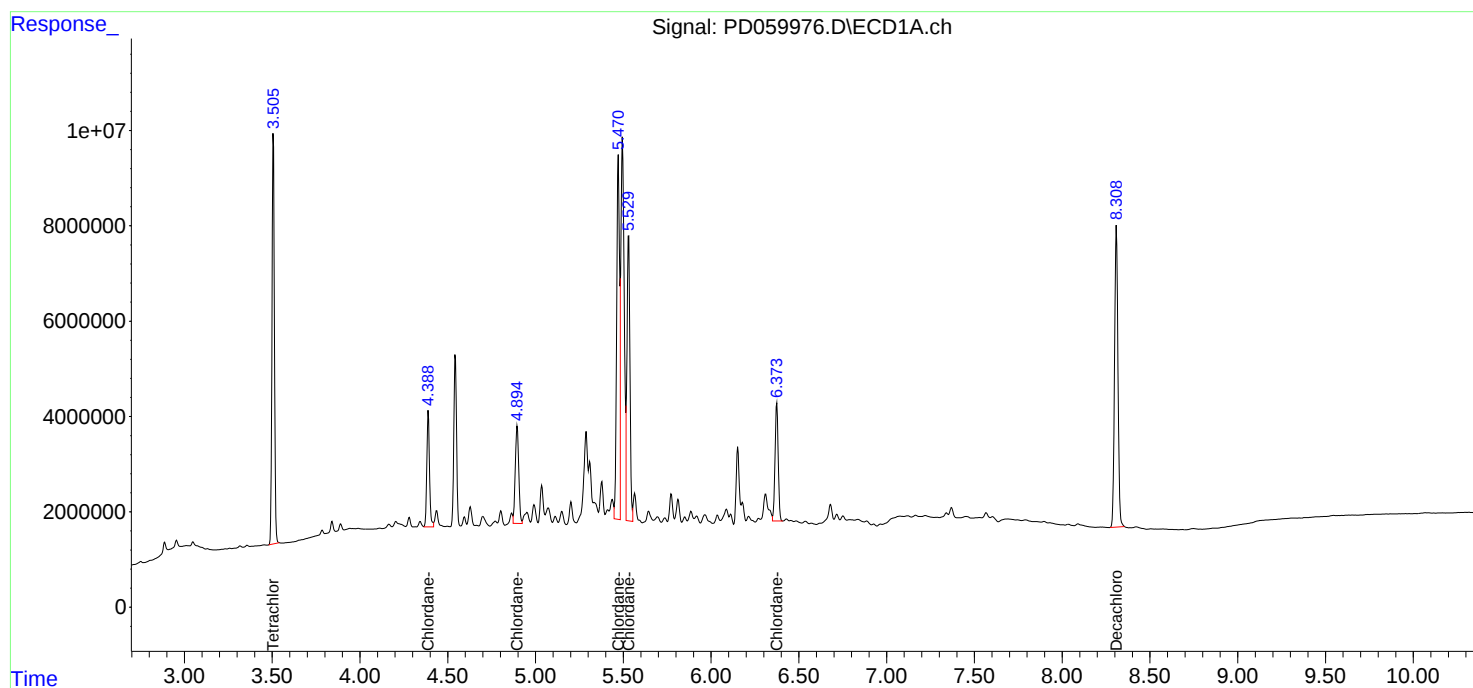


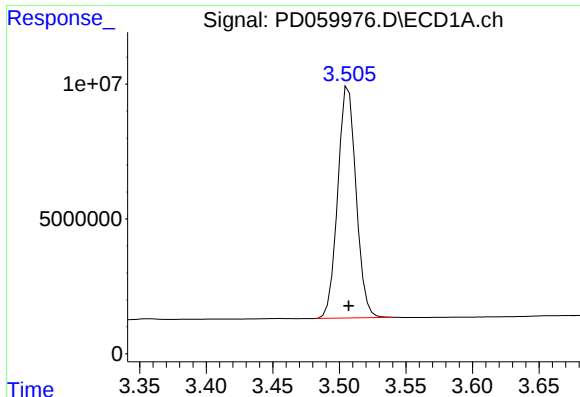

#1 Tetrachloro-m-xylene


R.T.: 3.507 min
Delta R.T.: 0.000 min
Response: 82361526
Conc: 75.64 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

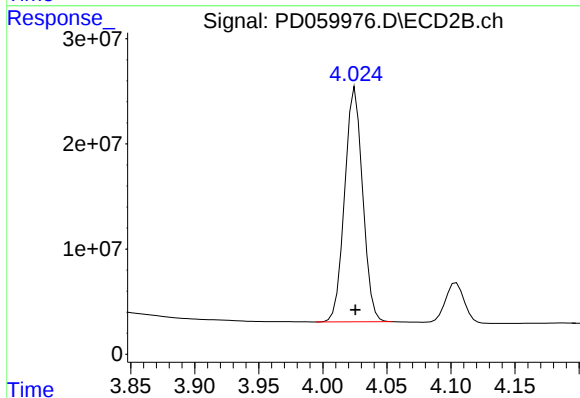


#1 Tetrachloro-m-xylene

R.T.: 4.025 min
Delta R.T.: 0.000 min
Response: 217643279
Conc: 74.95 ng/ml

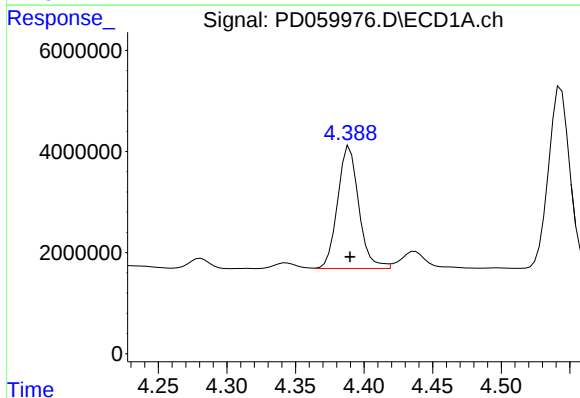


#23 Chlordane-1

R.T.: 4.390 min
Delta R.T.: 0.000 min
Response: 26003955
Conc: 747.90 ng/ml

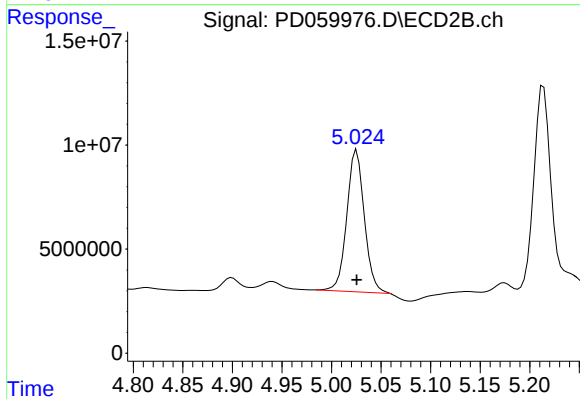

#23 Chlordane-1


R.T.: 5.025 min
Delta R.T.: 0.000 min
Response: 83643949
Conc: 725.17 ng/ml

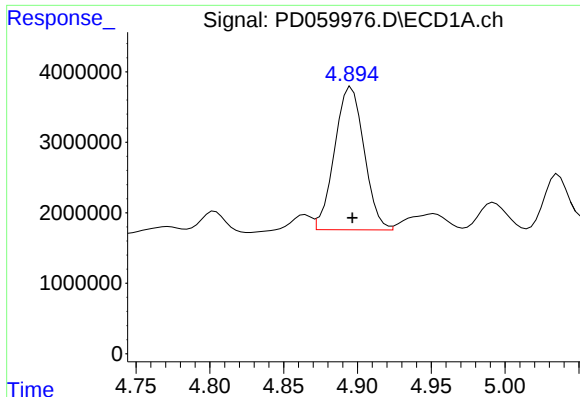

#24 Chlordane-2


R.T.: 4.896 min
Delta R.T.: 0.000 min
Response: 28277356
Conc: 740.88 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

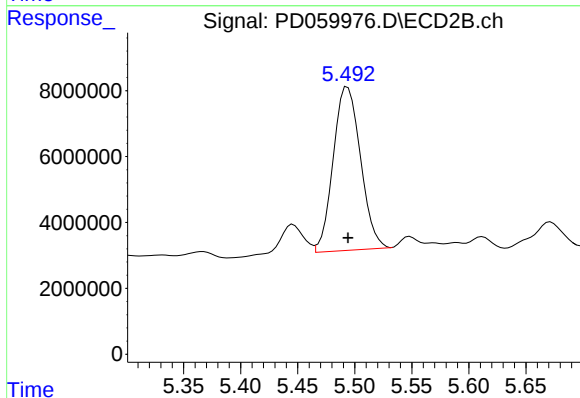


#24 Chlordane-2

R.T.: 5.494 min
Delta R.T.: 0.000 min
Response: 82651355
Conc: 734.51 ng/ml

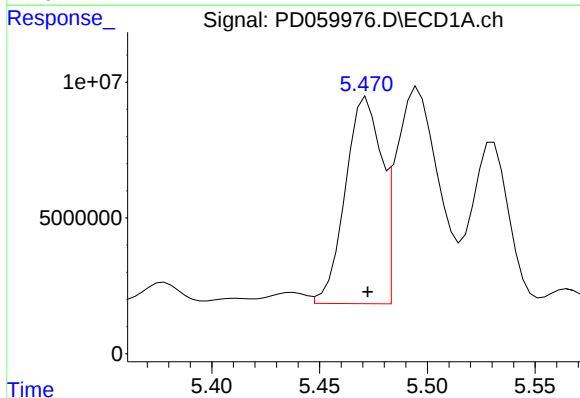


#25 Chlordane-3

R.T.: 5.472 min
Delta R.T.: 0.000 min
Response: 88019726
Conc: 763.87 ng/ml

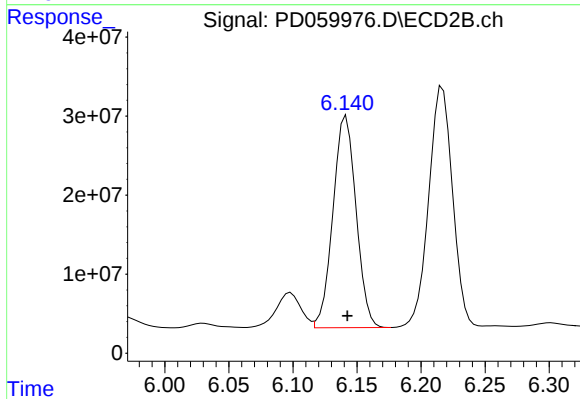

#25 Chlordane-3


R.T.: 6.142 min
Delta R.T.: 0.000 min
Response: 336220336
Conc: 757.18 ng/ml

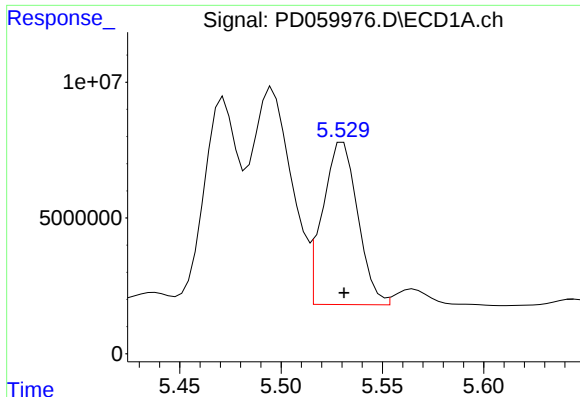

#26 Chlordane-4


R.T.: 5.531 min
Delta R.T.: 0.000 min
Response: 72043953
Conc: 755.42 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

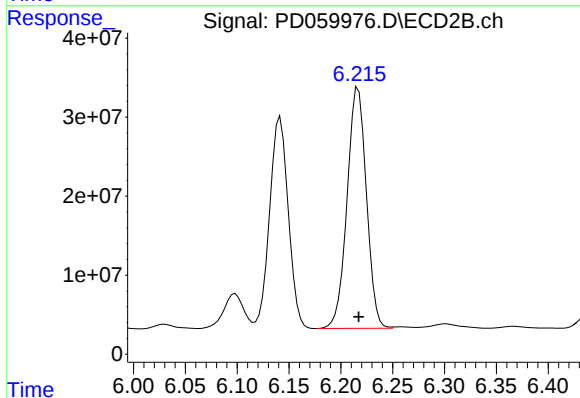


#26 Chlordane-4

R.T.: 6.217 min
Delta R.T.: 0.000 min
Response: 395899561
Conc: 753.88 ng/ml

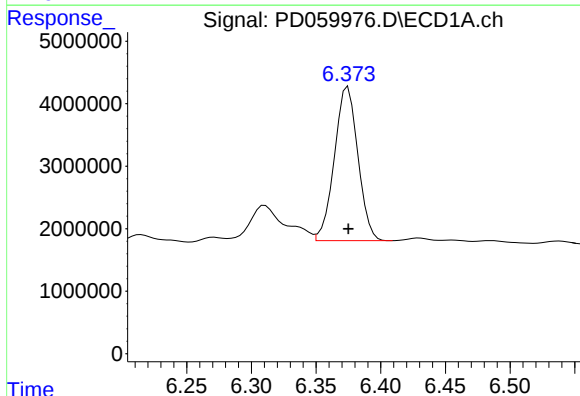


#27 Chlordane-5

R.T.: 6.375 min
Delta R.T.: 0.000 min
Response: 31119007
Conc: 749.03 ng/ml

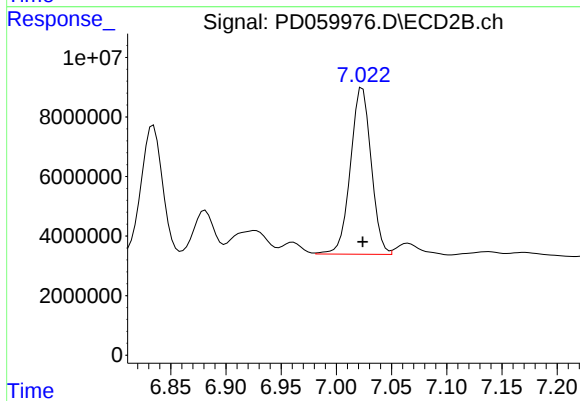

#27 Chlordane-5


R.T.: 7.024 min
Delta R.T.: 0.000 min
Response: 73157375
Conc: 755.12 ng/ml

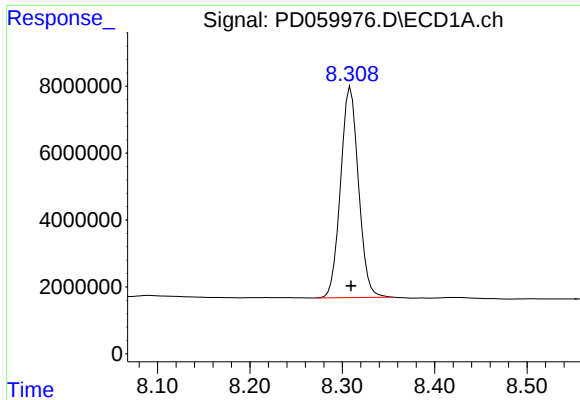

#28 Decachlorobiphenyl

R.T.: 8.309 min
Delta R.T.: 0.000 min
Response: 84887298
Conc: 74.22 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

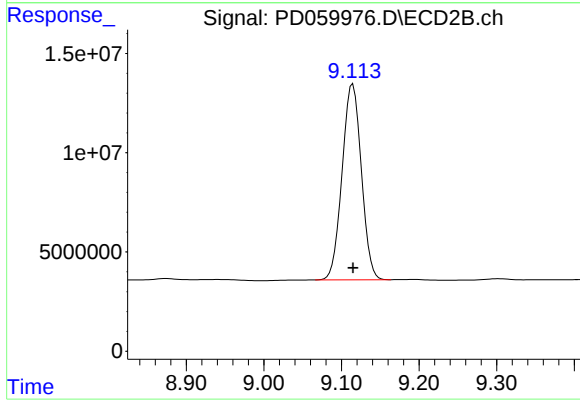

#28 Decachlorobiphenyl

R.T.: 9.115 min
Delta R.T.: 0.000 min
Response: 169897840
Conc: 74.36 ng/ml