

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102920\
 Data File : PD059977.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Oct 2020 19:55
 Operator : DD\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 03:56:28 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102920.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 30 03:55:09 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.507	4.025	54446208	145.2E6	50.000	50.000
28)	SA Decachlor...	8.309	9.115	57186791	114.2E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.390	5.025	17384741	57672273	500.000	500.000
24)	Chlordane-2	4.897	5.494	19083685	56262806	500.000	500.000
25)	Chlordane-3	5.472	6.142	57614367	222.0E6	500.000	500.000
26)	Chlordane-4	5.531	6.217	47684962	262.6E6	500.000	500.000
27)	Chlordane-5	6.375	7.024	20772741	48440965	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102920\
Data File : PD059977.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Oct 2020 19:55
Operator : DD\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 03:56:28 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102920.M
Quant Title : GC Extractables
QLast Update : Fri Oct 30 03:55:09 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

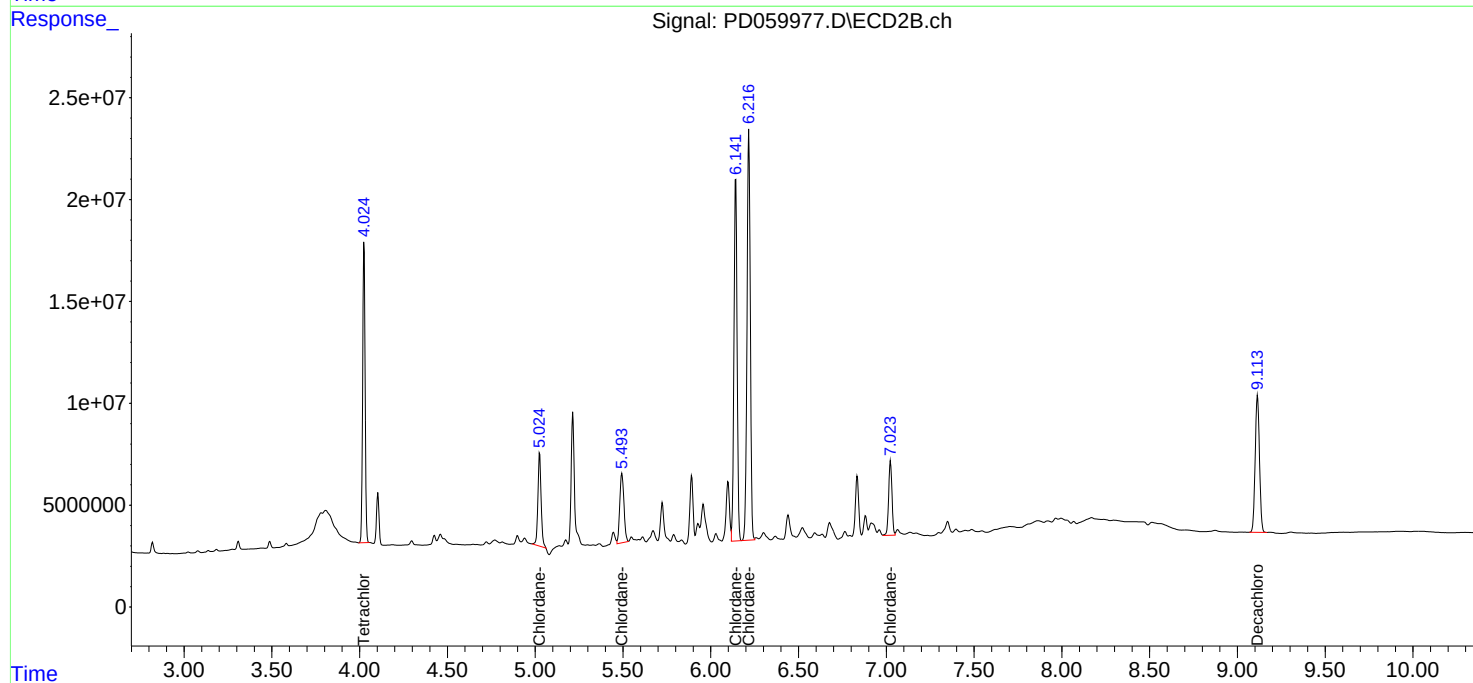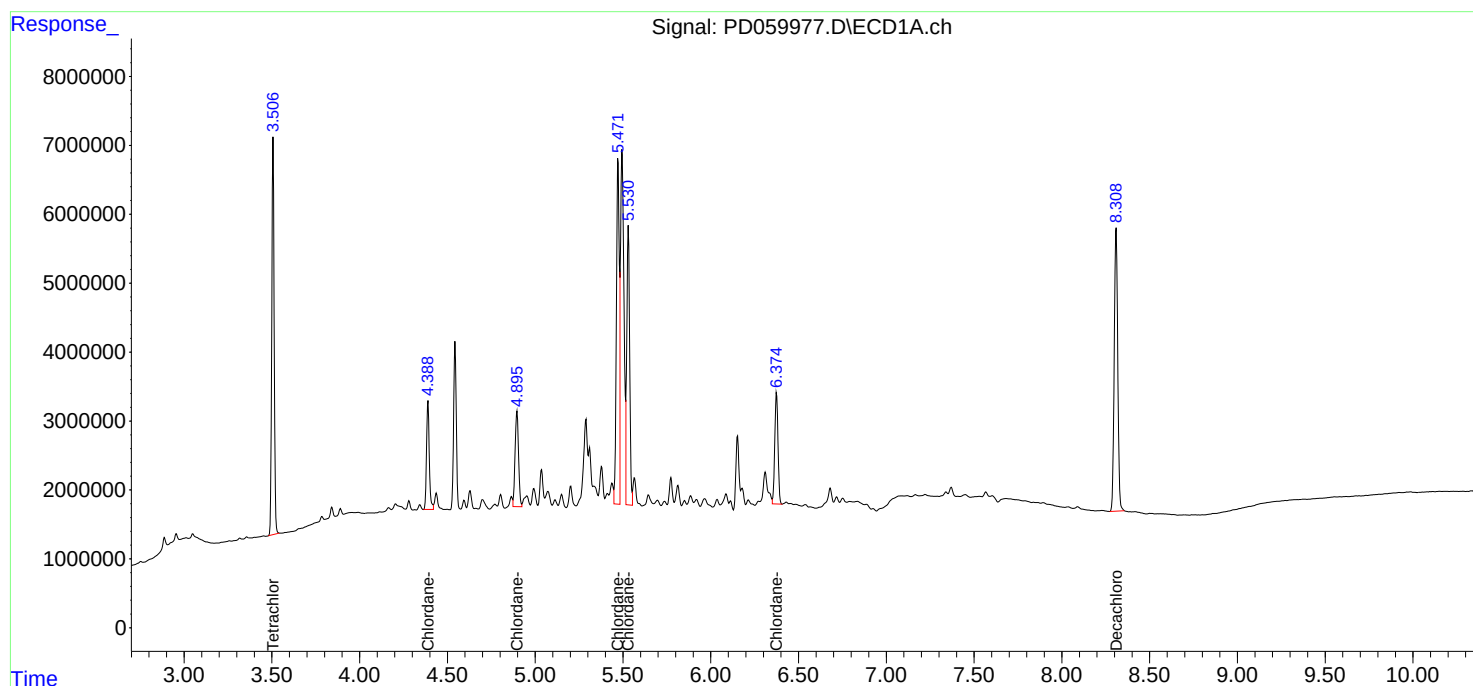


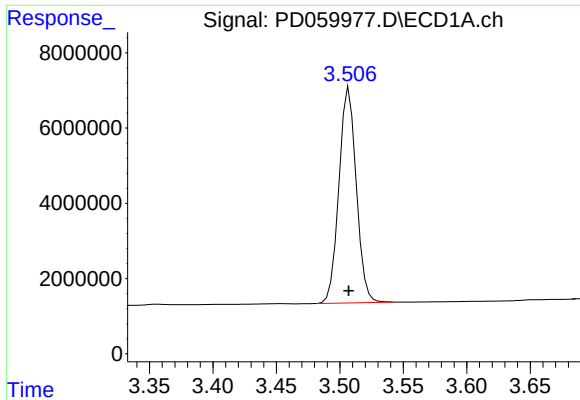

#1 Tetrachloro-m-xylene


R.T.: 3.507 min
Delta R.T.: 0.000 min
Response: 54446208
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

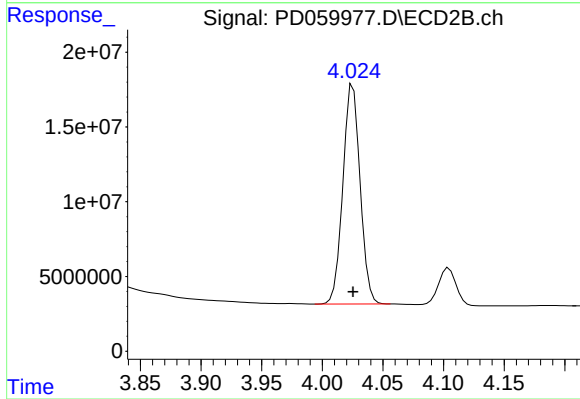


#1 Tetrachloro-m-xylene

R.T.: 4.025 min
Delta R.T.: 0.000 min
Response: 145194986
Conc: 50.00 ng/ml

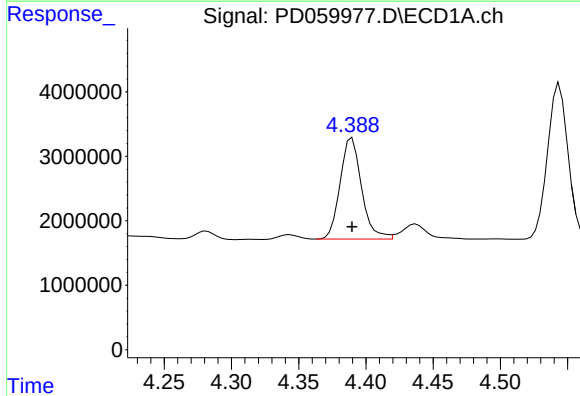


#23 Chlordane-1

R.T.: 4.390 min
Delta R.T.: 0.000 min
Response: 17384741
Conc: 500.00 ng/ml

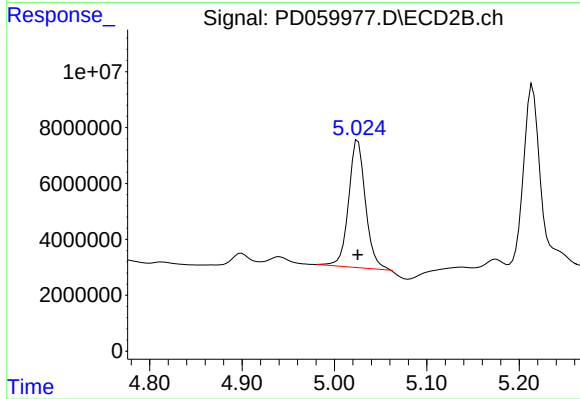

#23 Chlordane-1


R.T.: 5.025 min
Delta R.T.: 0.000 min
Response: 57672273
Conc: 500.00 ng/ml

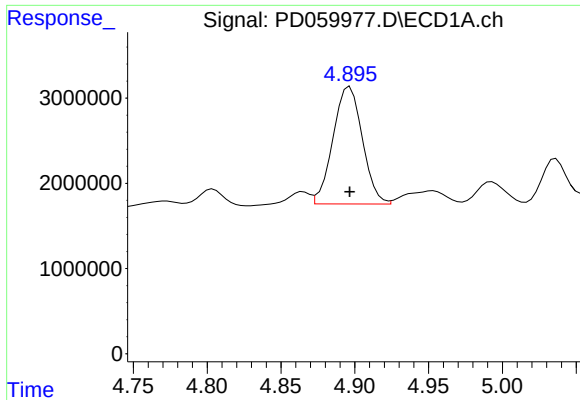

#24 Chlordane-2


R.T.: 4.897 min
Delta R.T.: 0.000 min
Response: 19083685
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

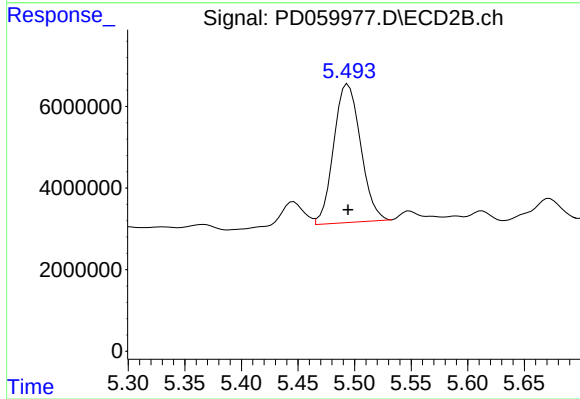


#24 Chlordane-2

R.T.: 5.494 min
Delta R.T.: 0.000 min
Response: 56262806
Conc: 500.00 ng/ml

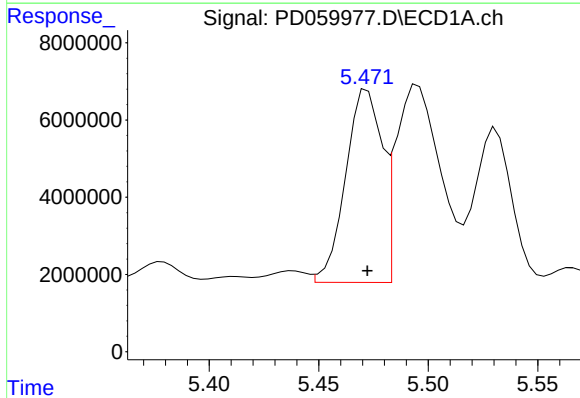


#25 Chlordane-3

R.T.: 5.472 min
Delta R.T.: 0.000 min
Response: 57614367
Conc: 500.00 ng/ml

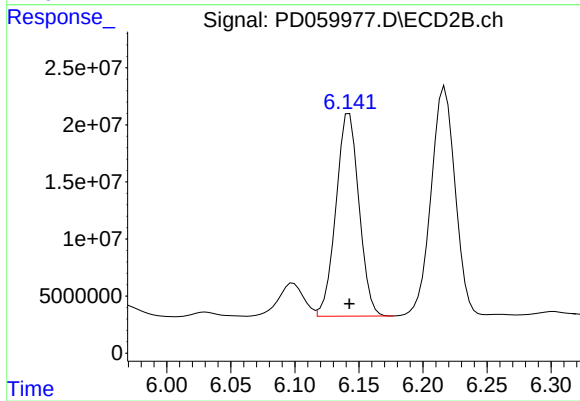

#25 Chlordane-3


R.T.: 6.142 min
Delta R.T.: 0.000 min
Response: 222021958
Conc: 500.00 ng/ml

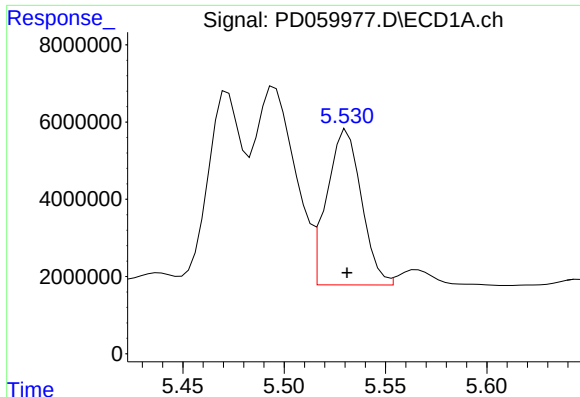

#26 Chlordane-4


R.T.: 5.531 min
Delta R.T.: 0.000 min
Response: 47684962
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

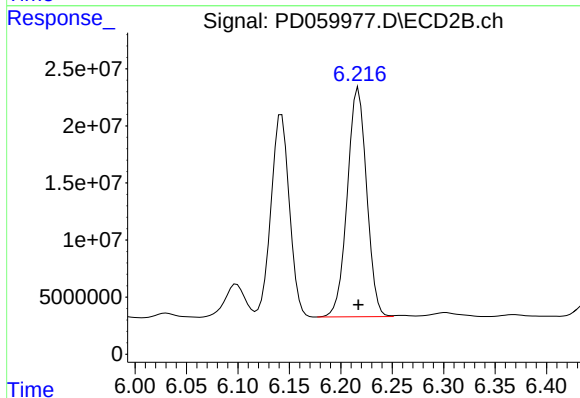


#26 Chlordane-4

R.T.: 6.217 min
Delta R.T.: 0.000 min
Response: 262574243
Conc: 500.00 ng/ml

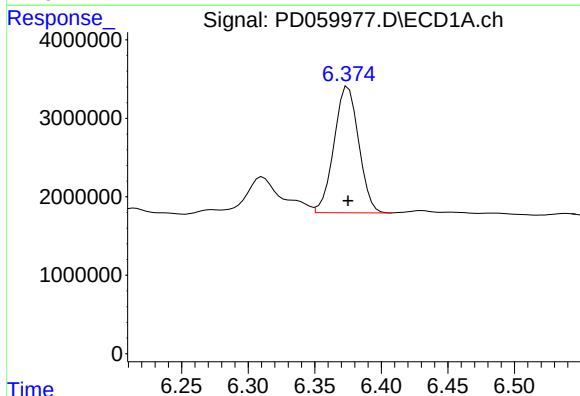


#27 Chlordane-5

R.T.: 6.375 min
Delta R.T.: 0.000 min
Response: 20772741
Conc: 500.00 ng/ml

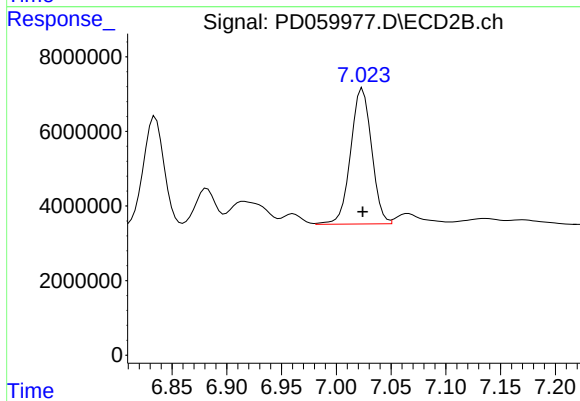

#27 Chlordane-5

R.T.: 7.024 min
Delta R.T.: 0.000 min
Response: 48440965
Conc: 500.00 ng/ml

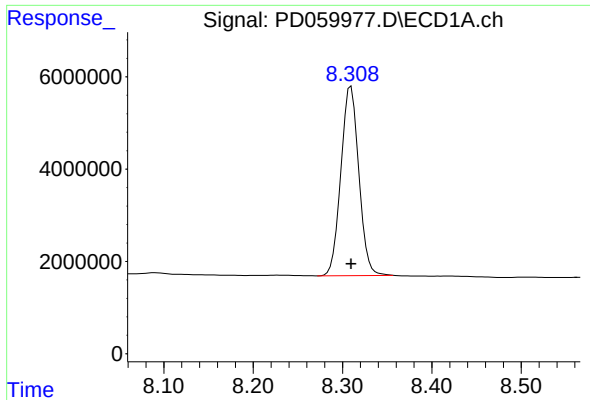

#28 Decachlorobiphenyl


R.T.: 8.309 min

Delta R.T.: 0.000 min

Response: 57186791

Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

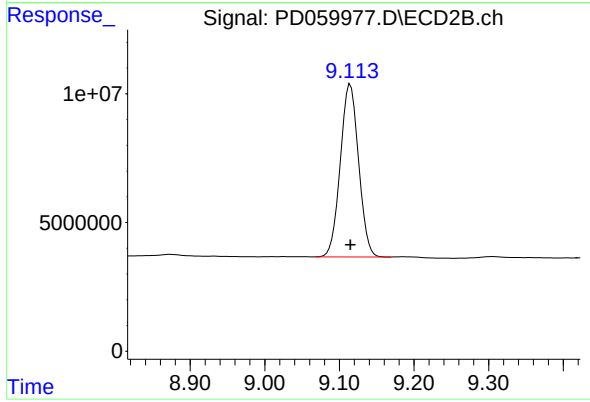

#28 Decachlorobiphenyl

R.T.: 9.115 min

Delta R.T.: 0.000 min

Response: 114242418

Conc: 50.00 ng/ml