

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102920\
 Data File : PD059978.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Oct 2020 20:09
 Operator : DD\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 03:56:38 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102920.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 30 03:55:09 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.507	4.025	26541431	71174885	24.374	24.510
28)	SA Decachlor...	8.309	9.115	29312020	58276124	25.628	25.505
Target Compounds							
23)	Chlordane-1	4.389	5.025	8991094	29461443	258.592	255.421
24)	Chlordane-2	4.896	5.493	9665982	29073692	253.253	258.374
25)	Chlordane-3	5.472	6.142	28248731	108.2E6	245.154	243.672
26)	Chlordane-4	5.531	6.217	23445672	129.3E6	245.839	246.143
27)	Chlordane-5	6.375	7.024	10642450	23936354	256.164	247.067



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102920\
Data File : PD059978.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Oct 2020 20:09
Operator : DD\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 03:56:38 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102920.M
Quant Title : GC Extractables
QLast Update : Fri Oct 30 03:55:09 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

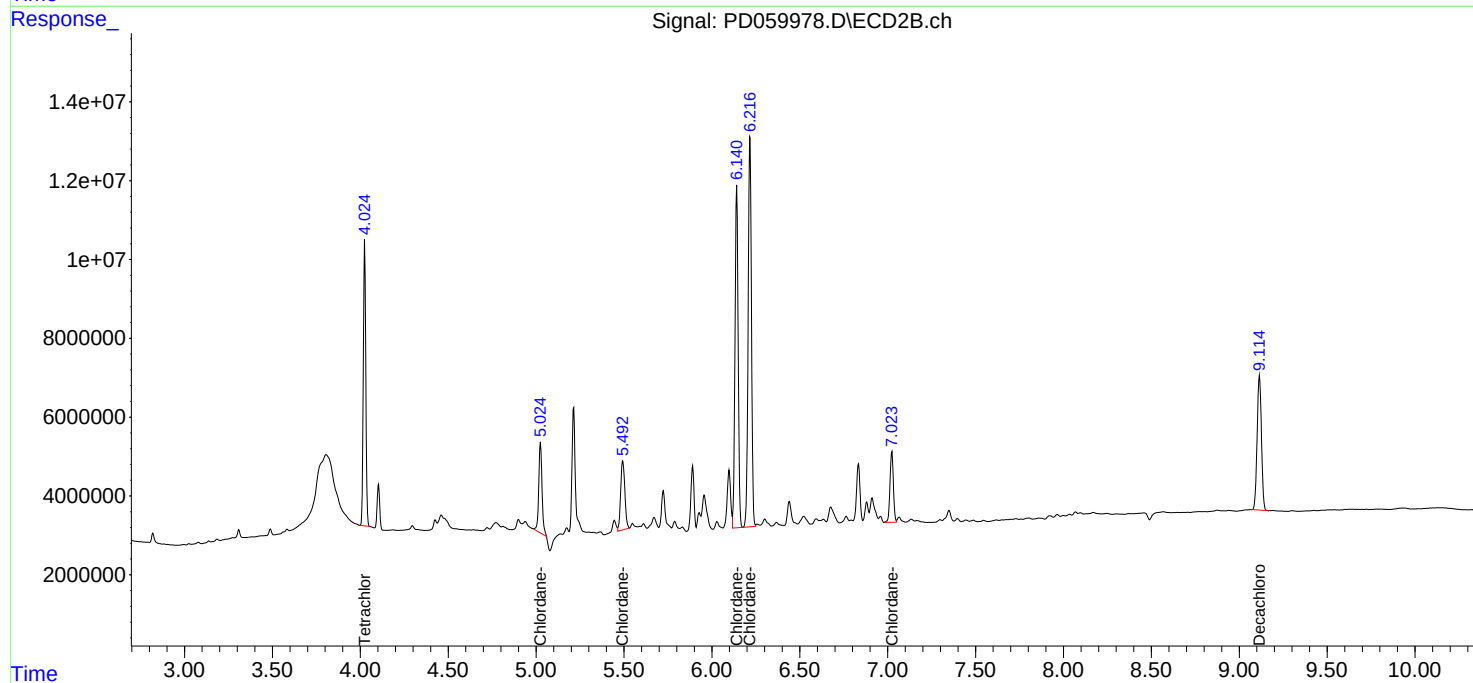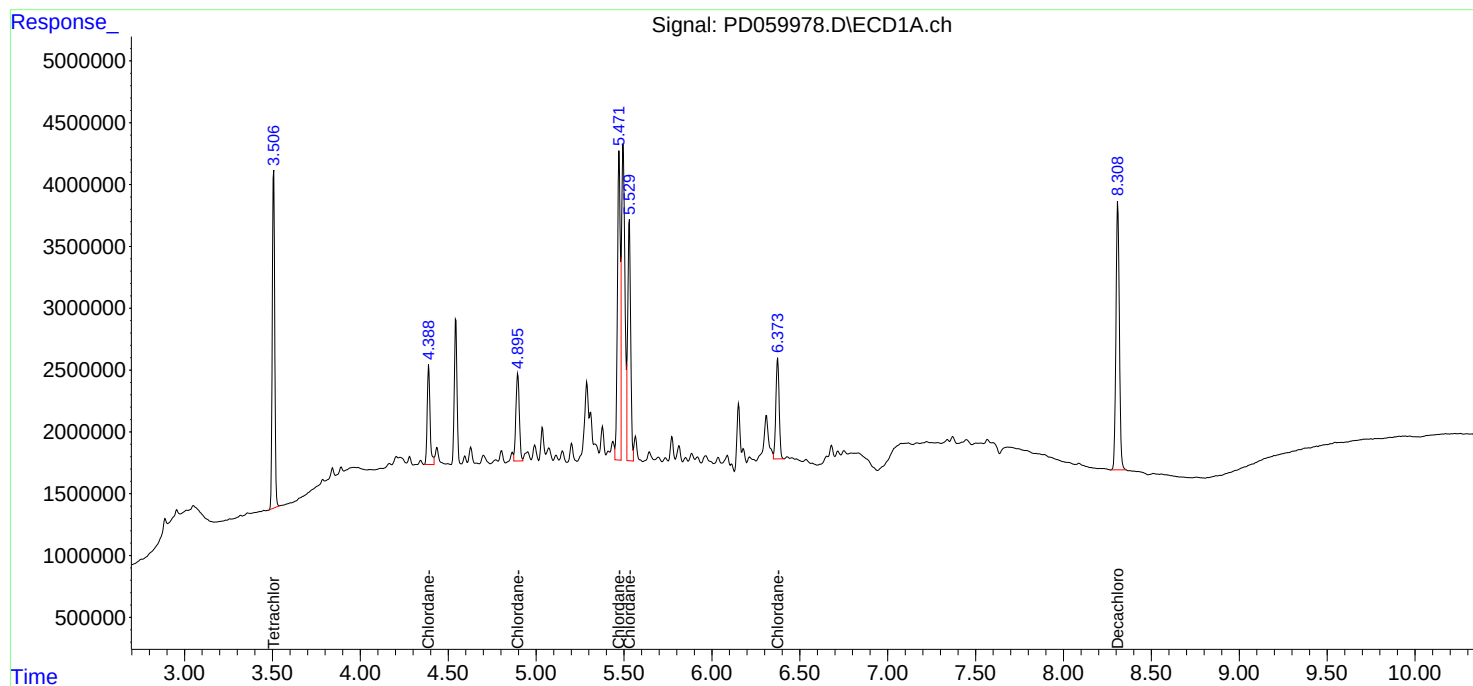


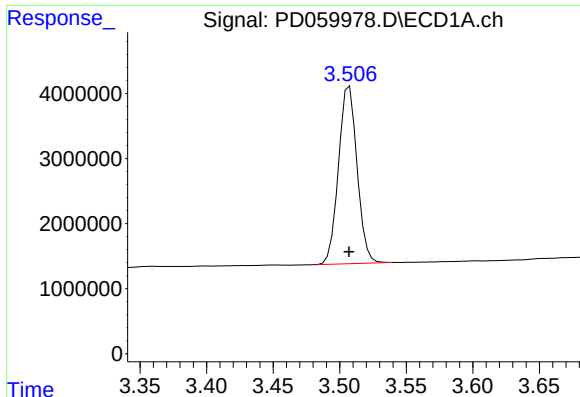

#1 Tetrachloro-m-xylene


R.T.: 3.507 min
Delta R.T.: 0.000 min
Response: 26541431
Conc: 24.37 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

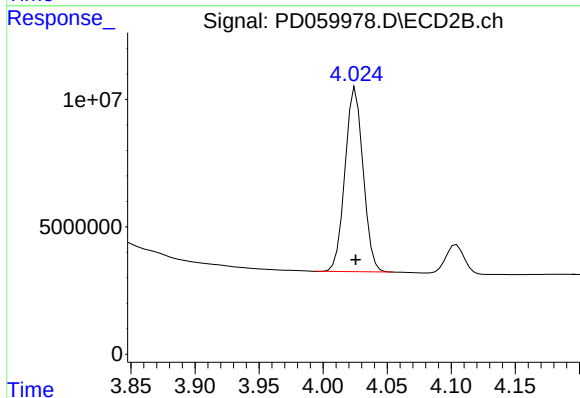


#1 Tetrachloro-m-xylene

R.T.: 4.025 min
Delta R.T.: 0.000 min
Response: 71174885
Conc: 24.51 ng/ml

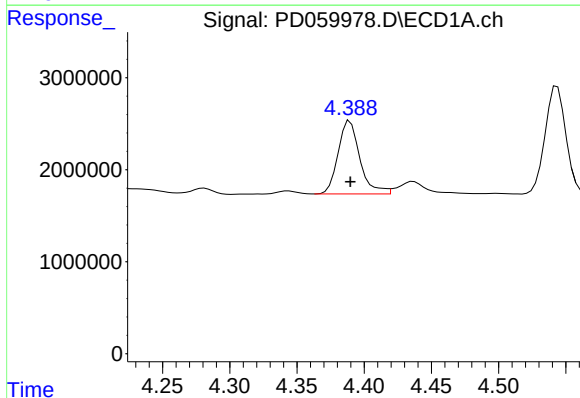


#23 Chlordane-1

R.T.: 4.389 min
Delta R.T.: 0.000 min
Response: 8991094
Conc: 258.59 ng/ml

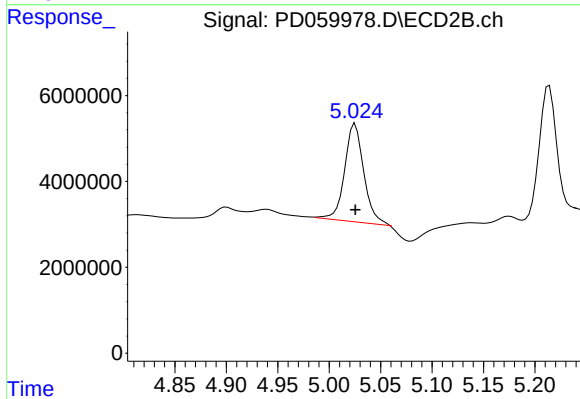

#23 Chlordane-1


R.T.: 5.025 min
Delta R.T.: 0.000 min
Response: 29461443
Conc: 255.42 ng/ml

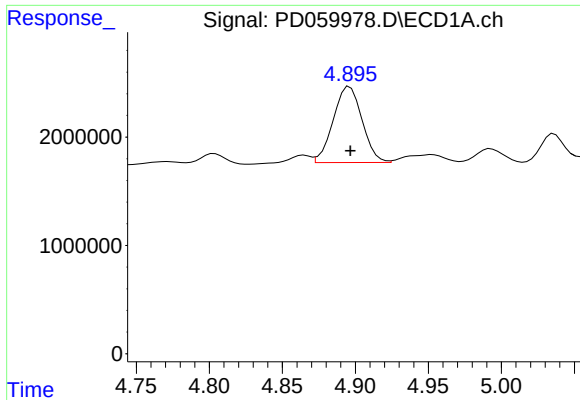

#24 Chlordane-2


R.T.: 4.896 min
Delta R.T.: 0.000 min
Response: 9665982
Conc: 253.25 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

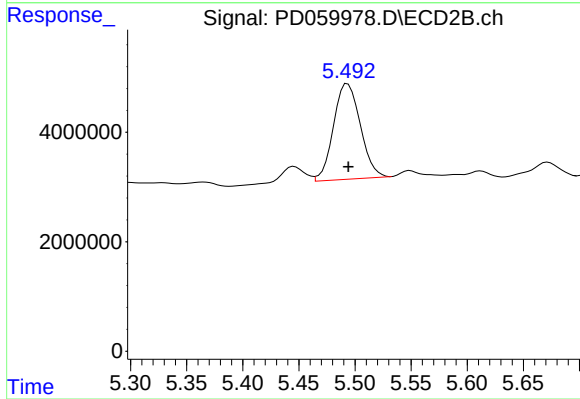


#24 Chlordane-2

R.T.: 5.493 min
Delta R.T.: 0.000 min
Response: 29073692
Conc: 258.37 ng/ml

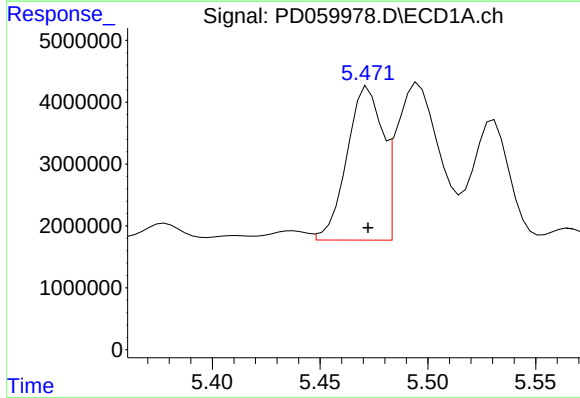


#25 Chlordane-3

R.T.: 5.472 min
Delta R.T.: 0.000 min
Response: 28248731
Conc: 245.15 ng/ml

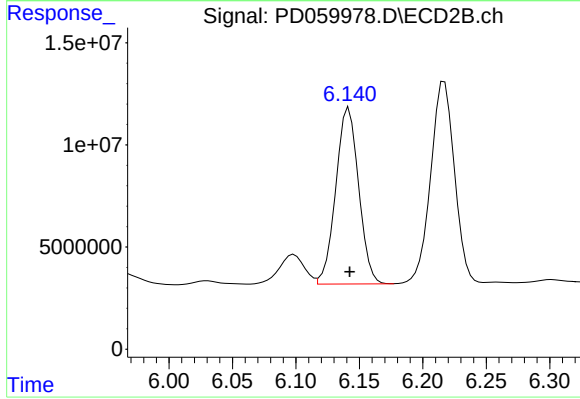

#25 Chlordane-3


R.T.: 6.142 min
Delta R.T.: 0.000 min
Response: 108201040
Conc: 243.67 ng/ml

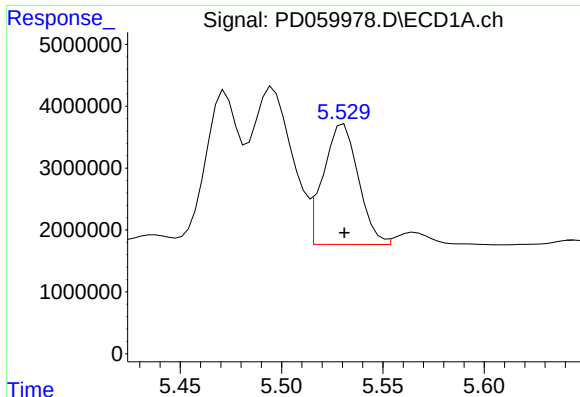

#26 Chlordane-4


R.T.: 5.531 min
Delta R.T.: 0.000 min
Response: 23445672
Conc: 245.84 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

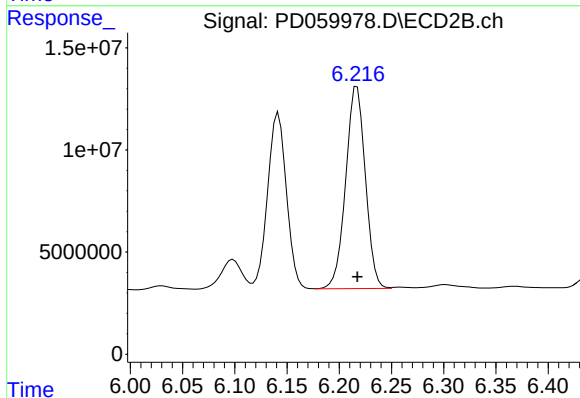


#26 Chlordane-4

R.T.: 6.217 min
Delta R.T.: 0.000 min
Response: 129261440
Conc: 246.14 ng/ml

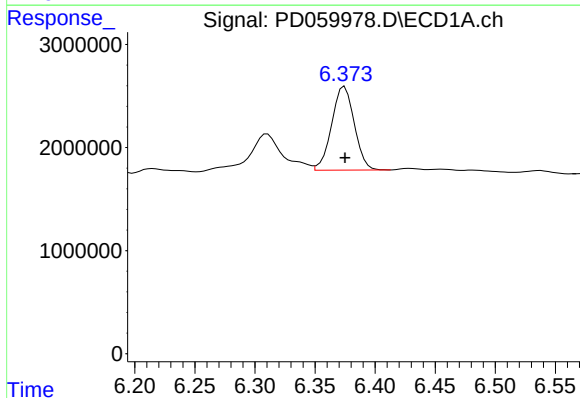


#27 Chlordane-5

R.T.: 6.375 min
Delta R.T.: 0.000 min
Response: 10642450
Conc: 256.16 ng/ml

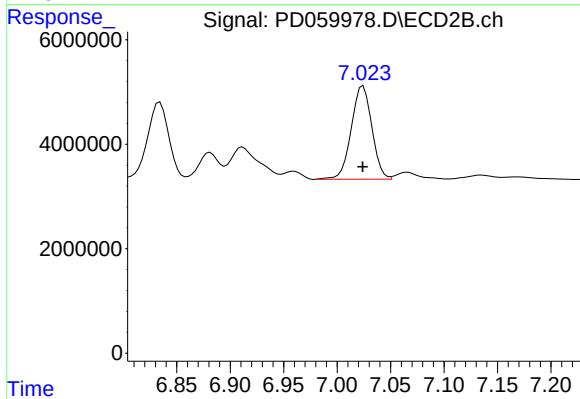

#27 Chlordane-5


R.T.: 7.024 min
Delta R.T.: 0.000 min
Response: 23936354
Conc: 247.07 ng/ml

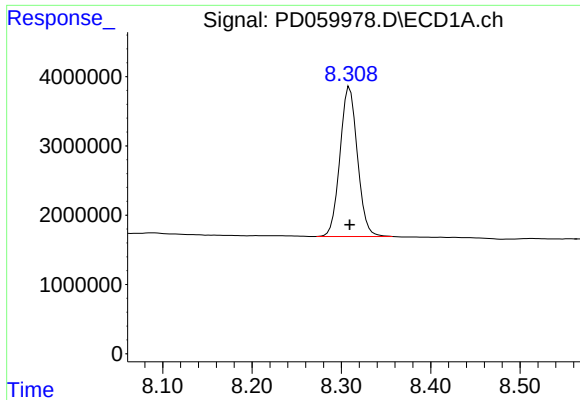

#28 Decachlorobiphenyl

R.T.: 8.309 min
Delta R.T.: 0.000 min
Response: 29312020
Conc: 25.63 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

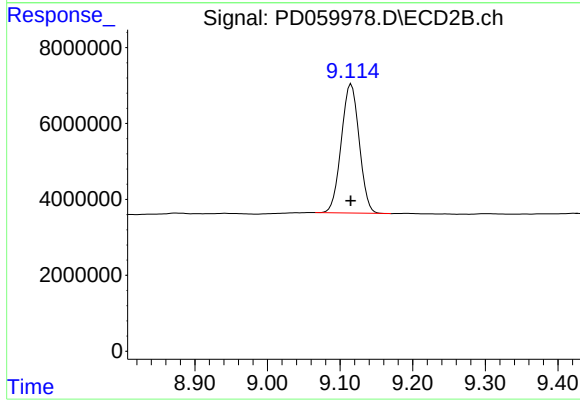

#28 Decachlorobiphenyl

R.T.: 9.115 min
Delta R.T.: 0.000 min
Response: 58276124
Conc: 25.51 ng/ml