

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102920\
 Data File : PD059986.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Oct 2020 22:03
 Operator : DD\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ICVPD102920CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 08:54:00 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102920.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 30 04:34:44 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.507	4.025	52968431	143.6E6	56.956	49.621
28)	SA Decachlor...	8.310	9.114	55419463	114.7E6	46.888	49.480
Target Compounds							
23)	Chlordane-1	4.390	5.024	16933906	56215830	480.812	475.317
24)	Chlordane-2	4.896	5.493	18520676	56038551	477.369	468.790
25)	Chlordane-3	5.472	6.142	56315863	221.5E6	486.742	483.729
26)	Chlordane-4	5.530	6.217	46870514	261.8E6	491.900	486.388
27)	Chlordane-5	6.375	7.024	20354396	49294696	463.236	490.190



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102920\
Data File : PD059986.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Oct 2020 22:03
Operator : DD\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
ICVPD102920CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 08:54:00 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102920.M
Quant Title : GC Extractables
QLast Update : Fri Oct 30 04:34:44 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

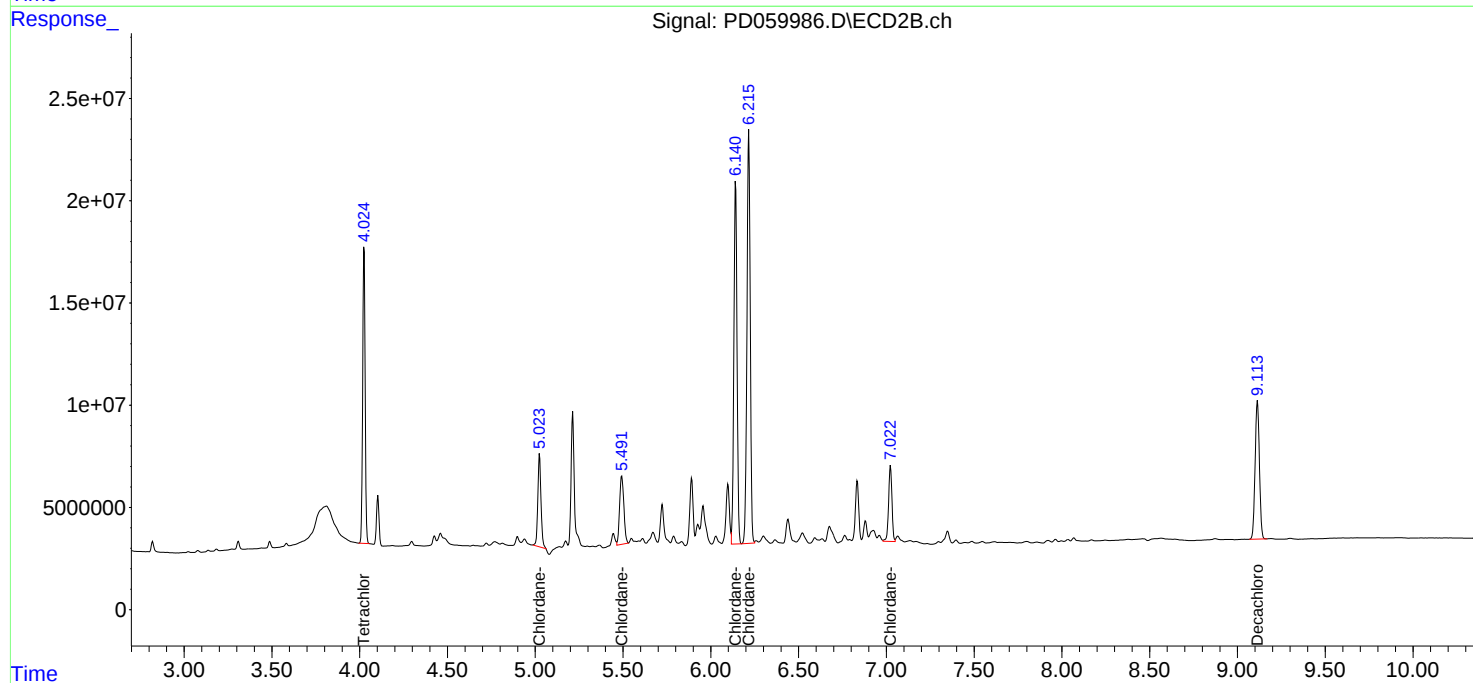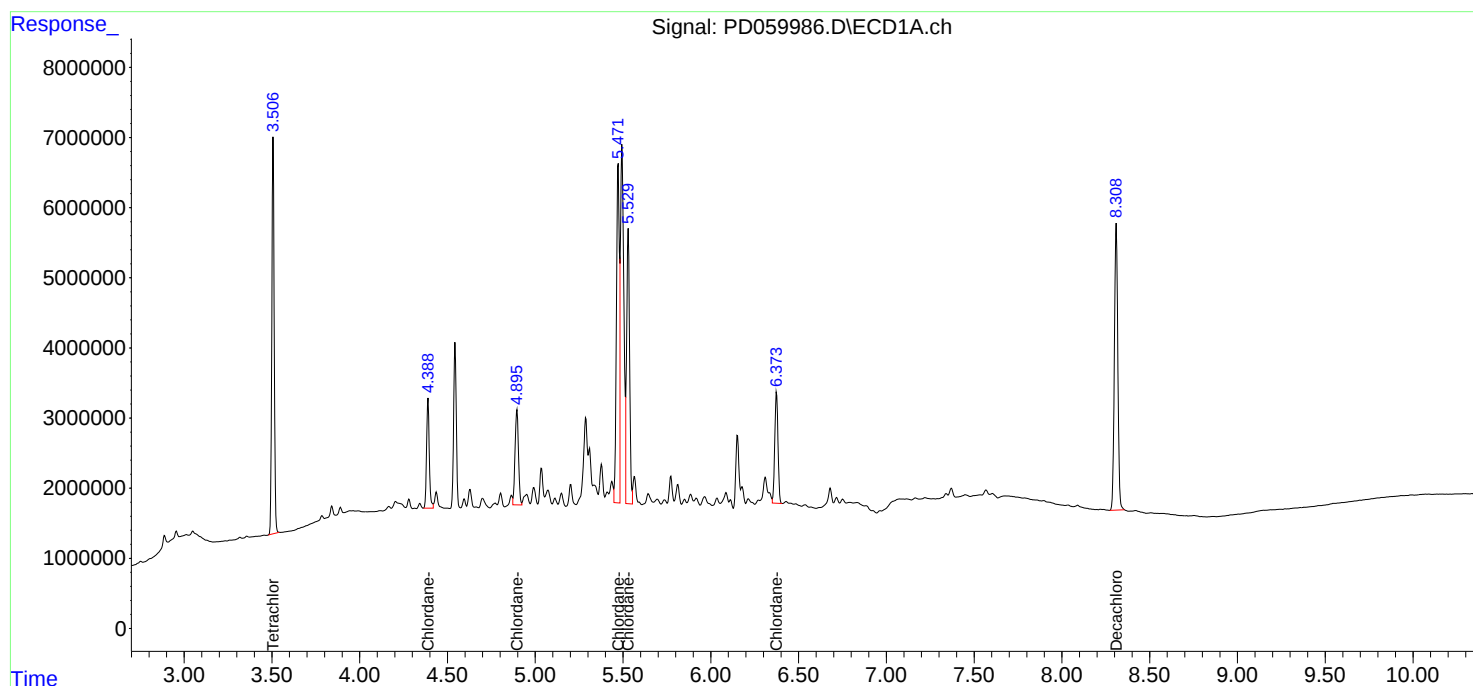


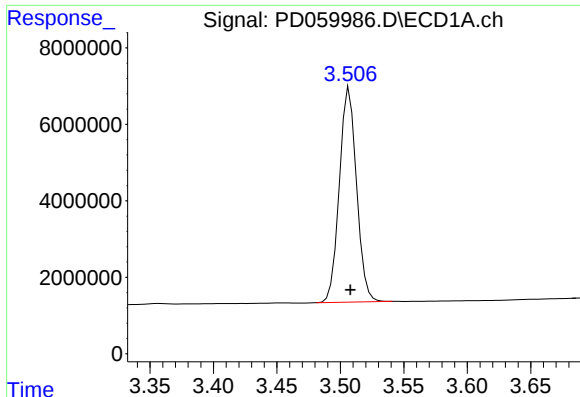

#1 Tetrachloro-m-xylene


R.T.: 3.507 min
Delta R.T.: 0.000 min
Response: 52968431
Conc: 56.96 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD102920CHLOR

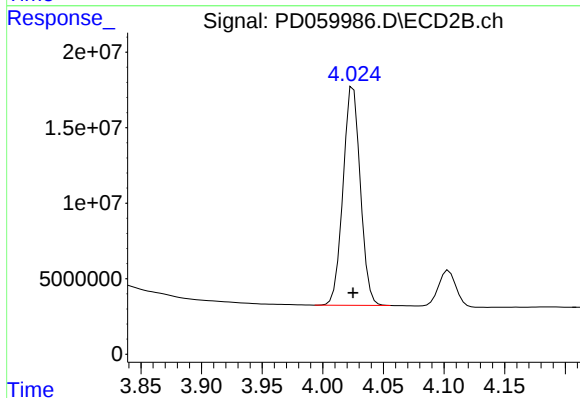


#1 Tetrachloro-m-xylene

R.T.: 4.025 min
Delta R.T.: 0.000 min
Response: 143580353
Conc: 49.62 ng/ml

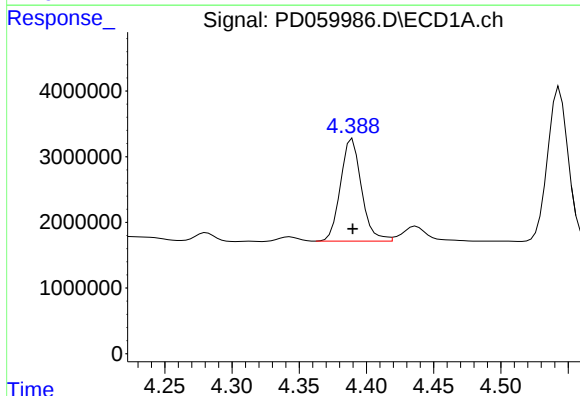


#23 Chlordane-1

R.T.: 4.390 min
Delta R.T.: 0.000 min
Response: 16933906
Conc: 480.81 ng/ml

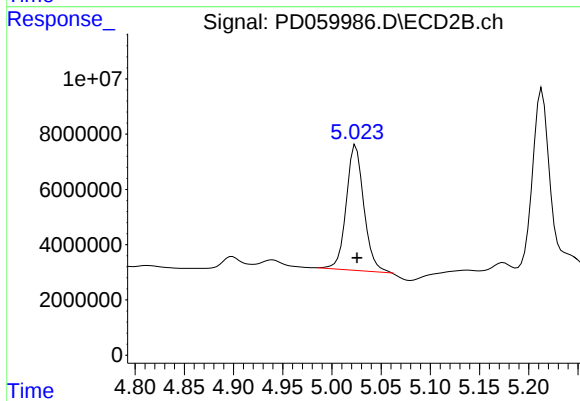

#23 Chlordane-1


R.T.: 5.024 min
Delta R.T.: -0.001 min
Response: 56215830
Conc: 475.32 ng/ml

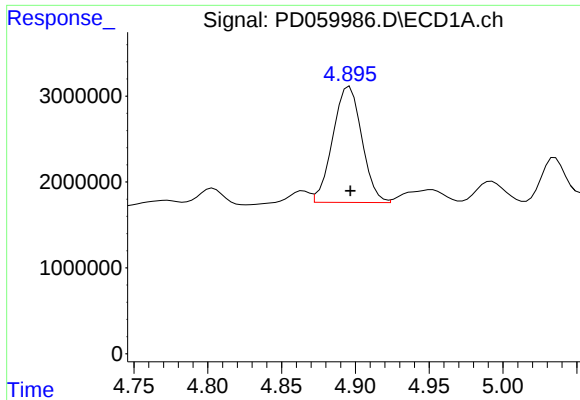

#24 Chlordane-2


R.T.: 4.896 min
Delta R.T.: 0.000 min
Response: 18520676
Conc: 477.37 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD102920CHLOR

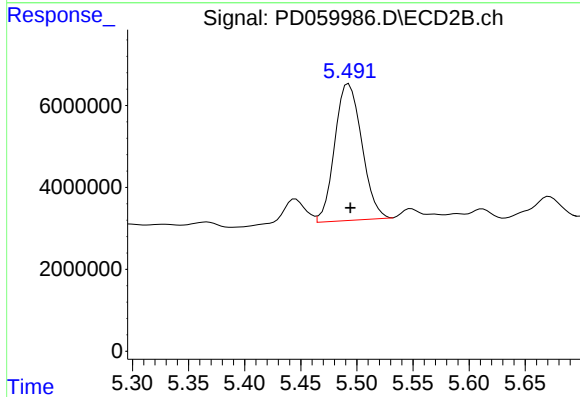


#24 Chlordane-2

R.T.: 5.493 min
Delta R.T.: -0.001 min
Response: 56038551
Conc: 468.79 ng/ml

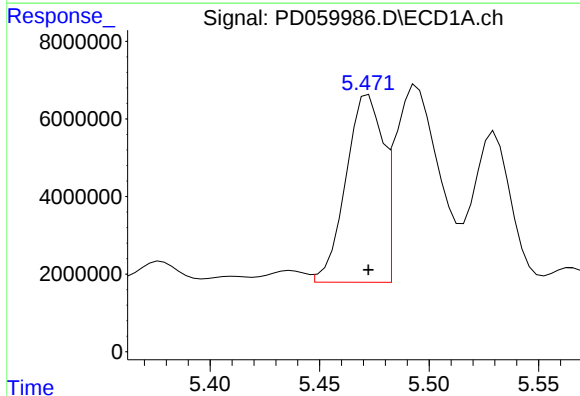


#25 Chlordane-3

R.T.: 5.472 min
Delta R.T.: 0.000 min
Response: 56315863
Conc: 486.74 ng/ml

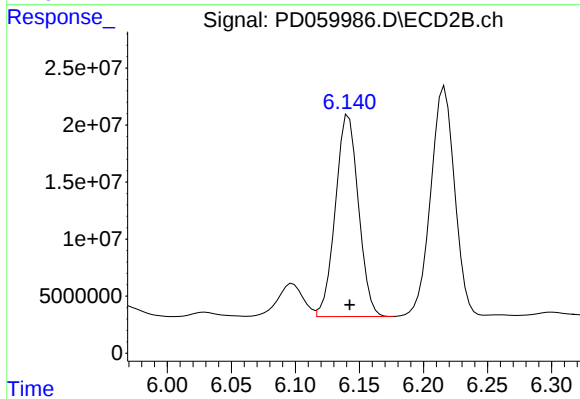

#25 Chlordane-3


R.T.: 6.142 min
Delta R.T.: 0.000 min
Response: 221482092
Conc: 483.73 ng/ml

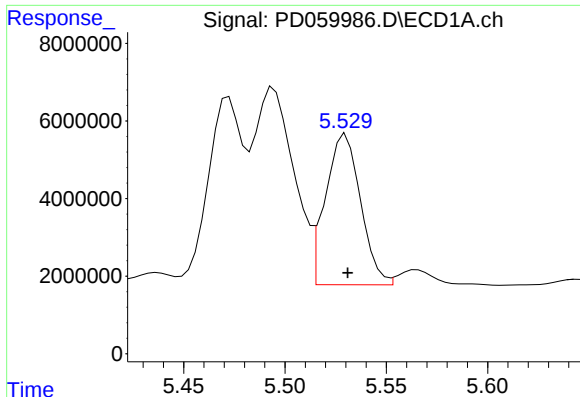

#26 Chlordane-4


R.T.: 5.530 min
Delta R.T.: -0.001 min
Response: 46870514
Conc: 491.90 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD102920CHLOR

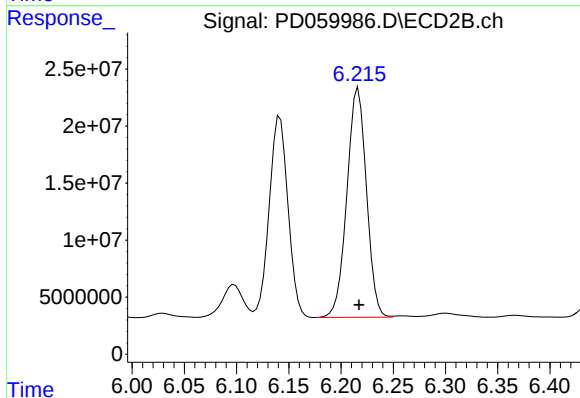


#26 Chlordane-4

R.T.: 6.217 min
Delta R.T.: 0.000 min
Response: 261758935
Conc: 486.39 ng/ml

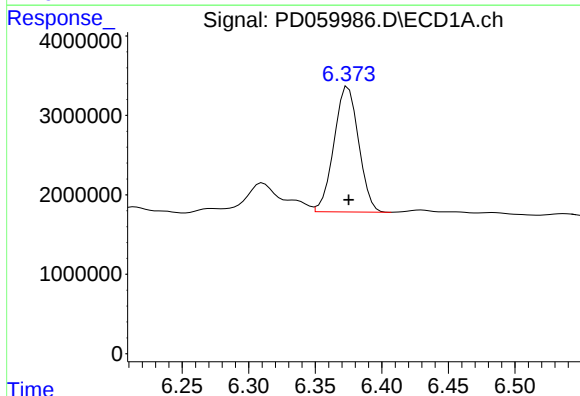


#27 Chlordane-5

R.T.: 6.375 min
Delta R.T.: 0.000 min
Response: 20354396
Conc: 463.24 ng/ml

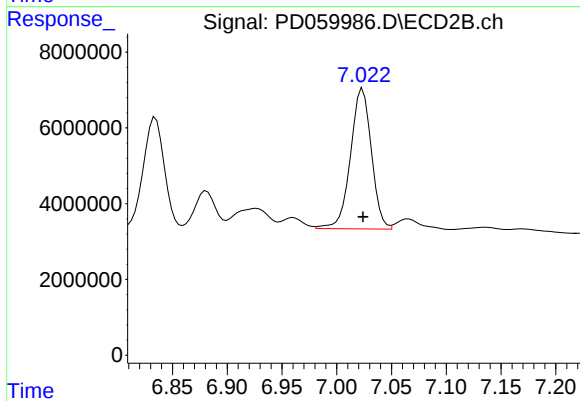

#27 Chlordane-5

R.T.: 7.024 min
Delta R.T.: 0.000 min
Response: 49294696
Conc: 490.19 ng/ml

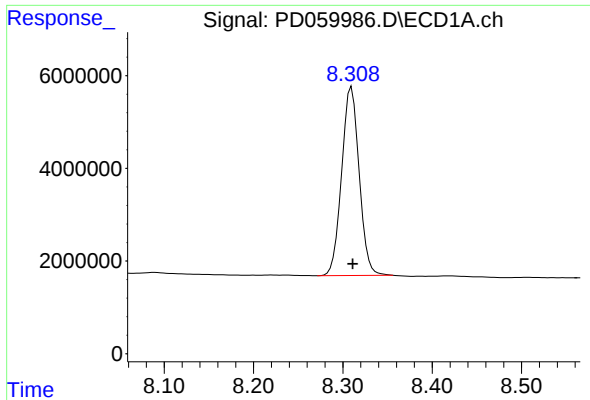

#28 Decachlorobiphenyl


R.T.: 8.310 min

Delta R.T.: -0.001 min

Response: 55419463

Conc: 46.89 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD102920CHLOR

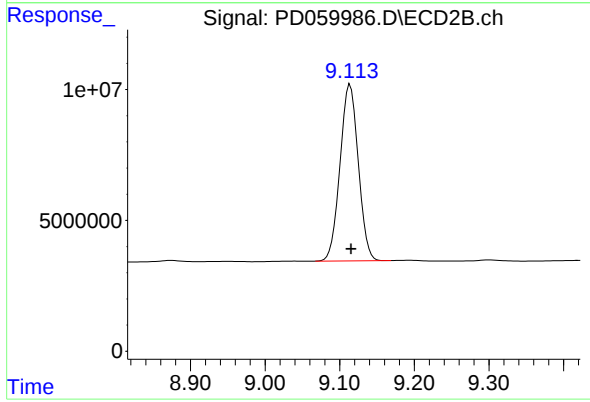

#28 Decachlorobiphenyl

R.T.: 9.114 min

Delta R.T.: -0.001 min

Response: 114724769

Conc: 49.48 ng/ml