

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102920\
 Data File : PD059991.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Oct 2020 23:14
 Operator : DD\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 08:55:07 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102920.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 30 04:34:44 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.507	4.025	50954886	138.8E6	54.791	47.972
28)	SA Decachlor...	8.309	9.113	54344628	113.5E6	45.979	48.965
Target Compounds							
23)	Chlordane-1	4.390	5.025	16494838	54417705	468.346	460.113
24)	Chlordane-2	4.896	5.494	18116844	55005580	466.961	460.149
25)	Chlordane-3	5.472	6.142	55515910	219.3E6	479.828	479.009
26)	Chlordane-4	5.531	6.216	45817705	259.3E6	480.851	481.897
27)	Chlordane-5	6.374	7.024	20072372	47677999	456.818	474.113



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102920\
Data File : PD059991.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Oct 2020 23:14
Operator : DD\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 08:55:07 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102920.M
Quant Title : GC Extractables
QLast Update : Fri Oct 30 04:34:44 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

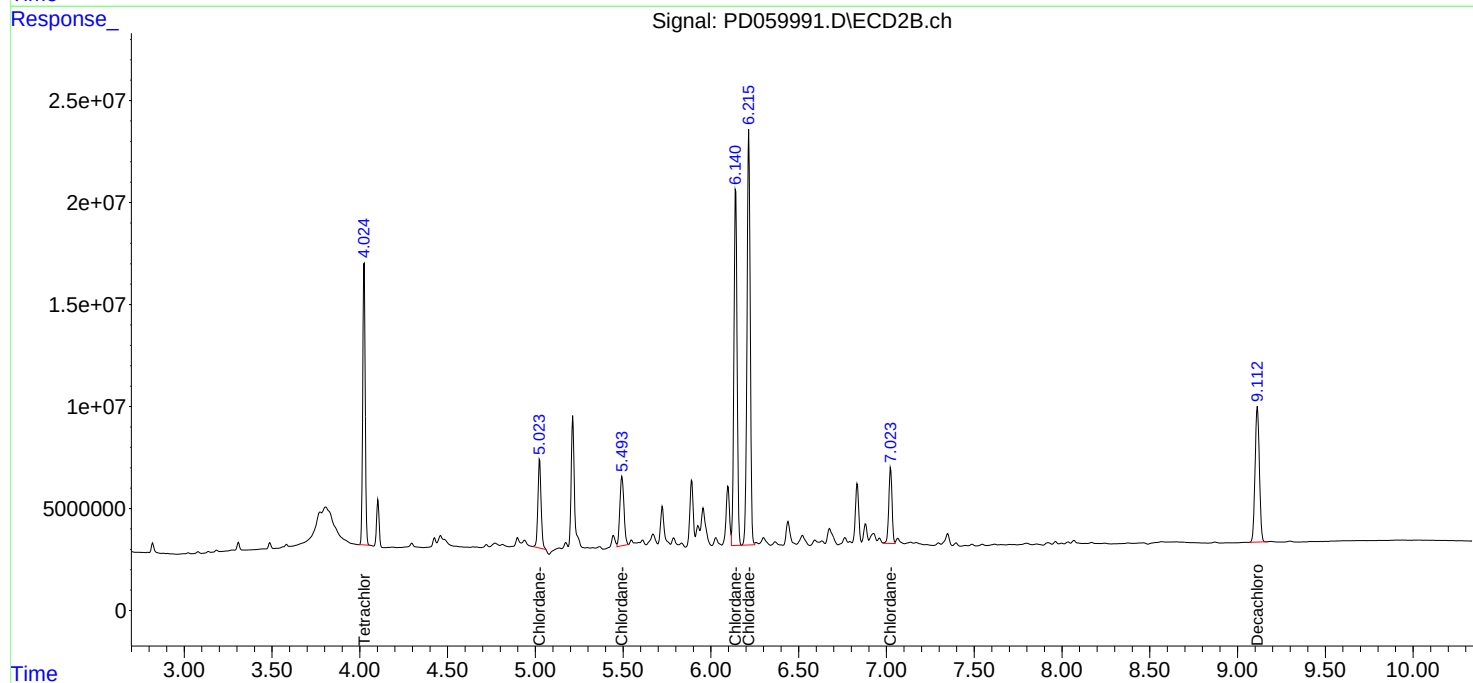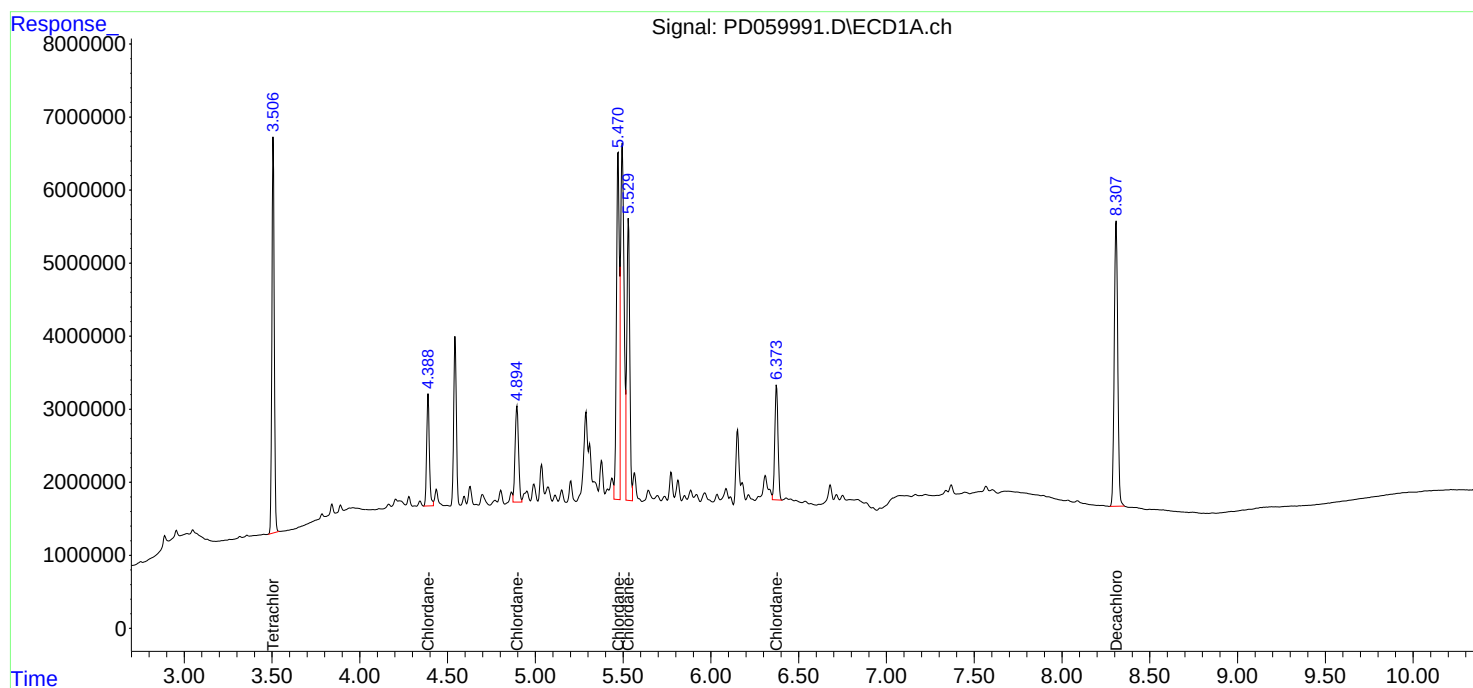


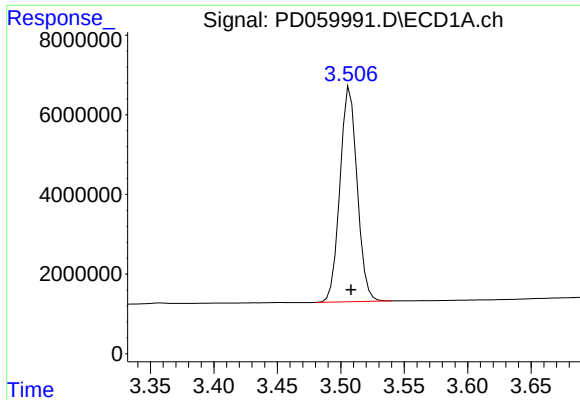

#1 Tetrachloro-m-xylene


R.T.: 3.507 min
Delta R.T.: 0.000 min
Response: 50954886
Conc: 54.79 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

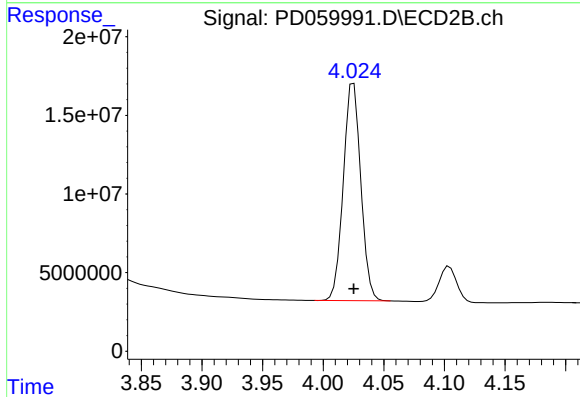


#1 Tetrachloro-m-xylene

R.T.: 4.025 min
Delta R.T.: 0.000 min
Response: 138808870
Conc: 47.97 ng/ml

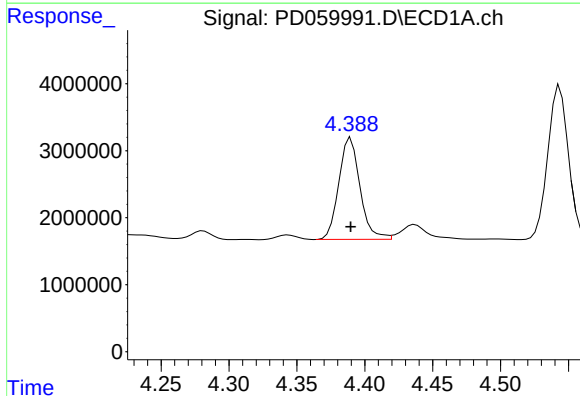


#23 Chlordane-1

R.T.: 4.390 min
Delta R.T.: 0.000 min
Response: 16494838
Conc: 468.35 ng/ml

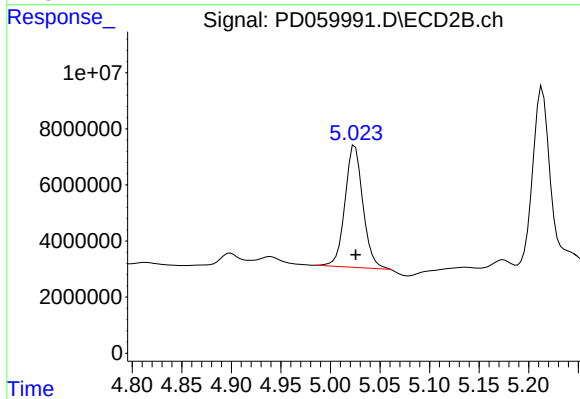

#23 Chlordane-1


R.T.: 5.025 min
Delta R.T.: 0.000 min
Response: 54417705
Conc: 460.11 ng/ml

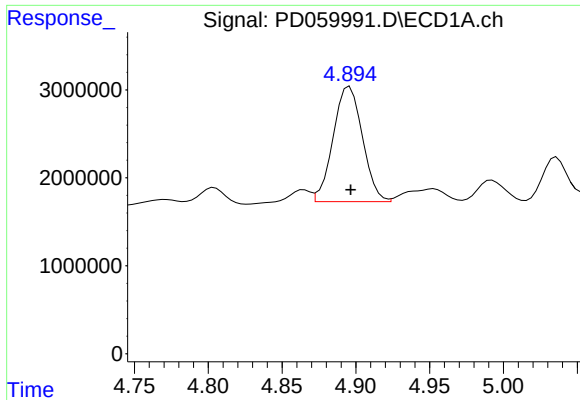

#24 Chlordane-2


R.T.: 4.896 min
Delta R.T.: 0.000 min
Response: 18116844
Conc: 466.96 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

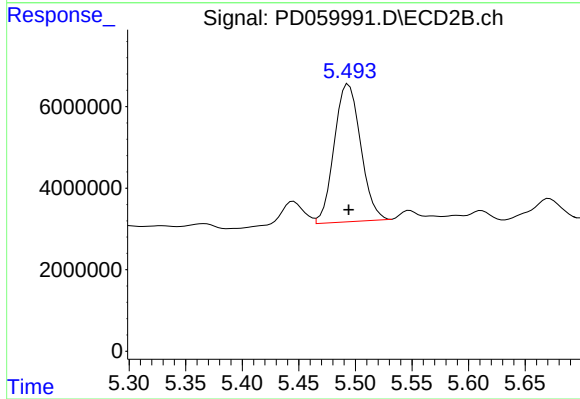


#24 Chlordane-2

R.T.: 5.494 min
Delta R.T.: 0.000 min
Response: 55005580
Conc: 460.15 ng/ml

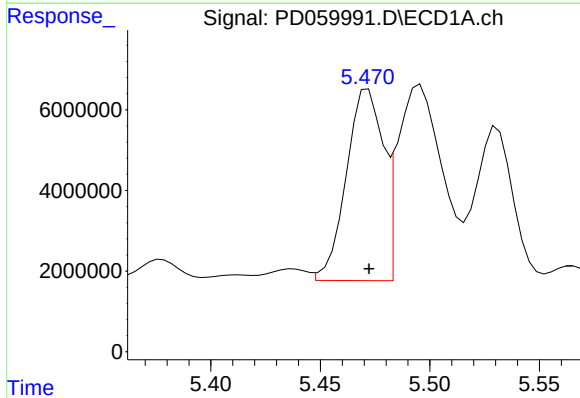


#25 Chlordane-3

R.T.: 5.472 min
Delta R.T.: 0.000 min
Response: 55515910
Conc: 479.83 ng/ml

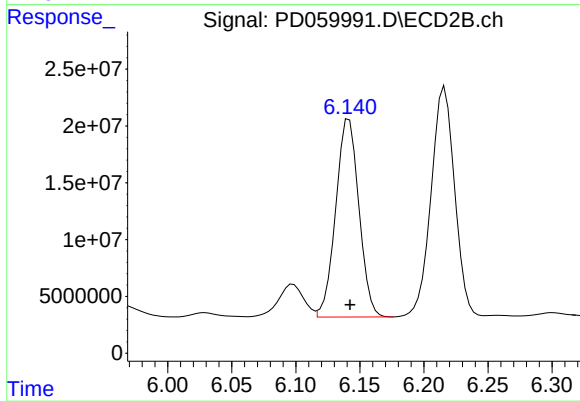

#25 Chlordane-3


R.T.: 6.142 min
Delta R.T.: 0.000 min
Response: 219320823
Conc: 479.01 ng/ml

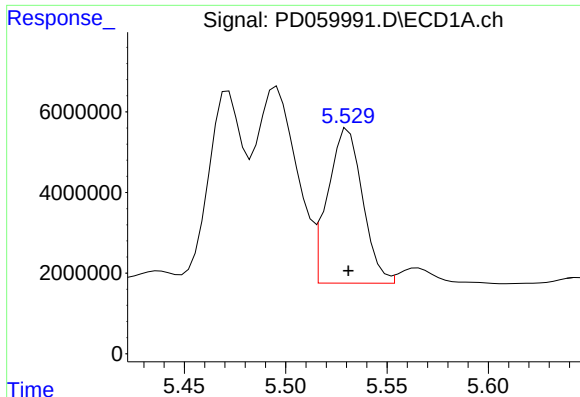

#26 Chlordane-4


R.T.: 5.531 min
Delta R.T.: 0.000 min
Response: 45817705
Conc: 480.85 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

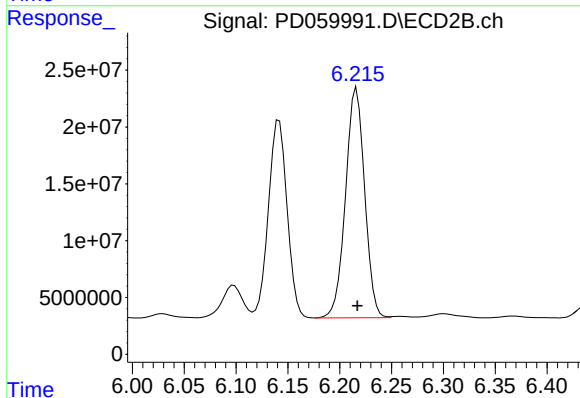


#26 Chlordane-4

R.T.: 6.216 min
Delta R.T.: 0.000 min
Response: 259342102
Conc: 481.90 ng/ml

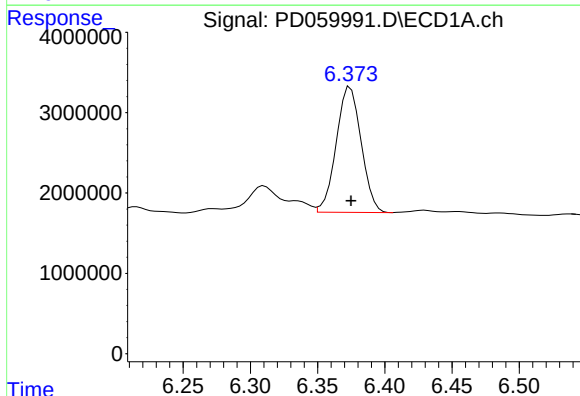


#27 Chlordane-5

R.T.: 6.374 min
Delta R.T.: 0.000 min
Response: 20072372
Conc: 456.82 ng/ml

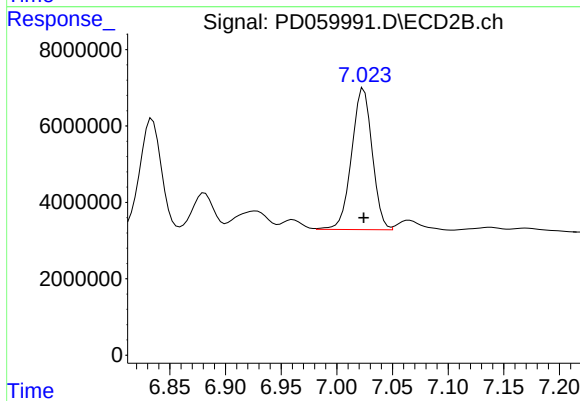

#27 Chlordane-5


R.T.: 7.024 min
Delta R.T.: 0.000 min
Response: 47677999
Conc: 474.11 ng/ml

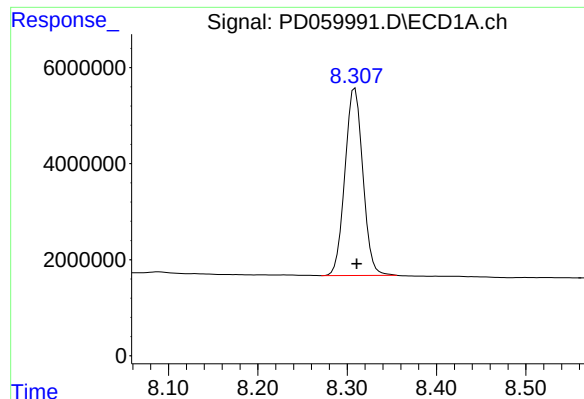

#28 Decachlorobiphenyl

R.T.: 8.309 min
Delta R.T.: -0.002 min
Response: 54344628
Conc: 45.98 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

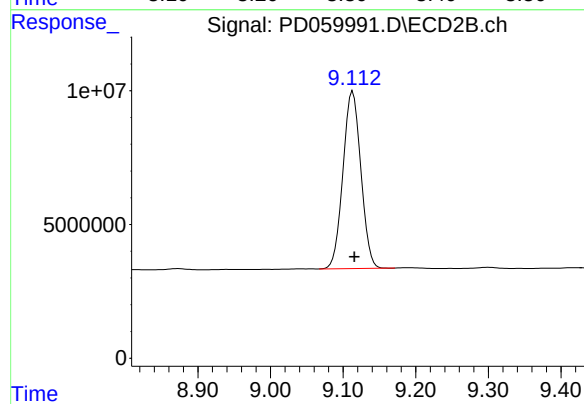

#28 Decachlorobiphenyl

R.T.: 9.113 min
Delta R.T.: -0.002 min
Response: 113530172
Conc: 48.97 ng/ml