

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102920\
 Data File : PD060008.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Oct 2020 03:15
 Operator : DD\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 08:58:51 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102920.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 30 04:34:44 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.507	4.025	49692246	139.5E6	53.434	48.225
28)	SA Decachlor...	8.308	9.114	49419383	113.4E6	41.811	48.911
Target Compounds							
23)	Chlordane-1	4.389	5.024	16186355	54042257	459.587	456.939
24)	Chlordane-2	4.896	5.493	17772260	54717389	458.079	457.738
25)	Chlordane-3	5.472	6.142	53643902	217.6E6	463.648	475.292
26)	Chlordane-4	5.530	6.216	43627305	257.1E6	457.863	477.720
27)	Chlordane-5	6.374	7.023	19113299	47517894	434.991	472.521



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102920\
Data File : PD060008.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2020 03:15
Operator : DD\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 08:58:51 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102920.M
Quant Title : GC Extractables
QLast Update : Fri Oct 30 04:34:44 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

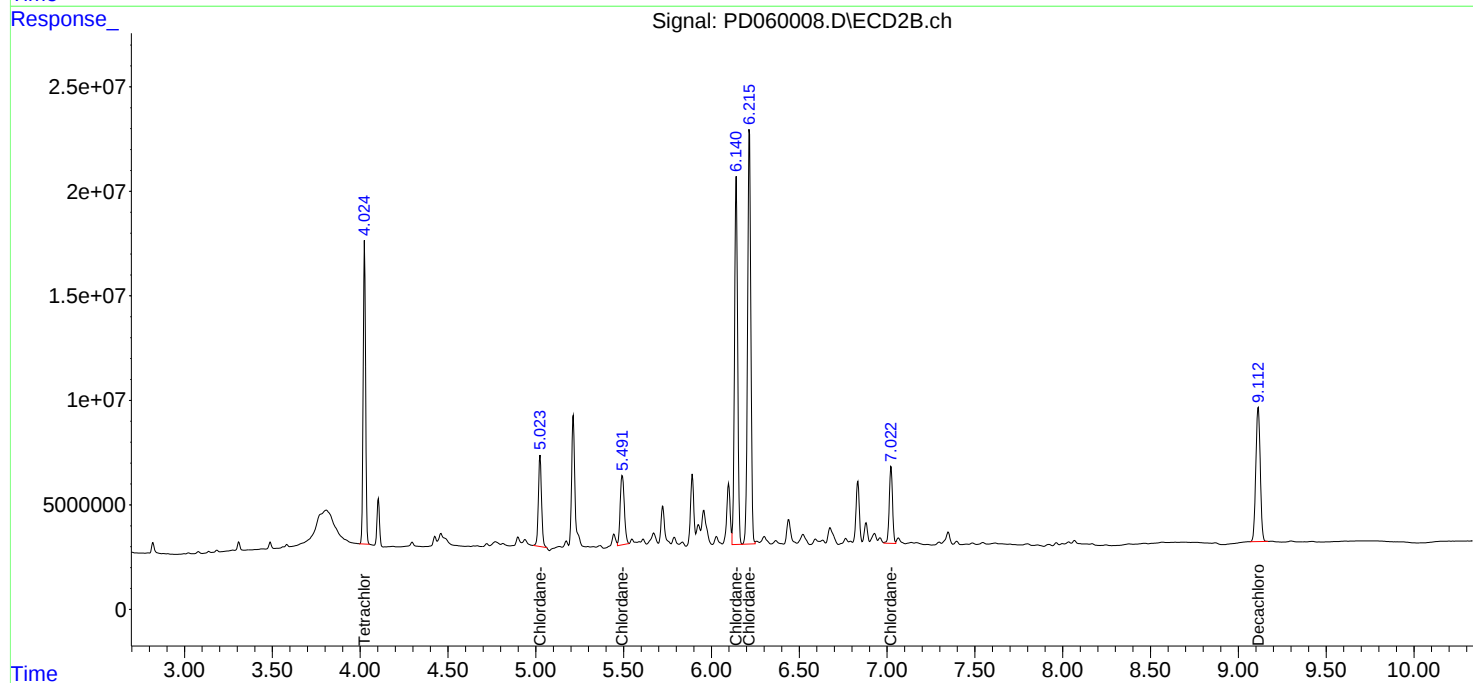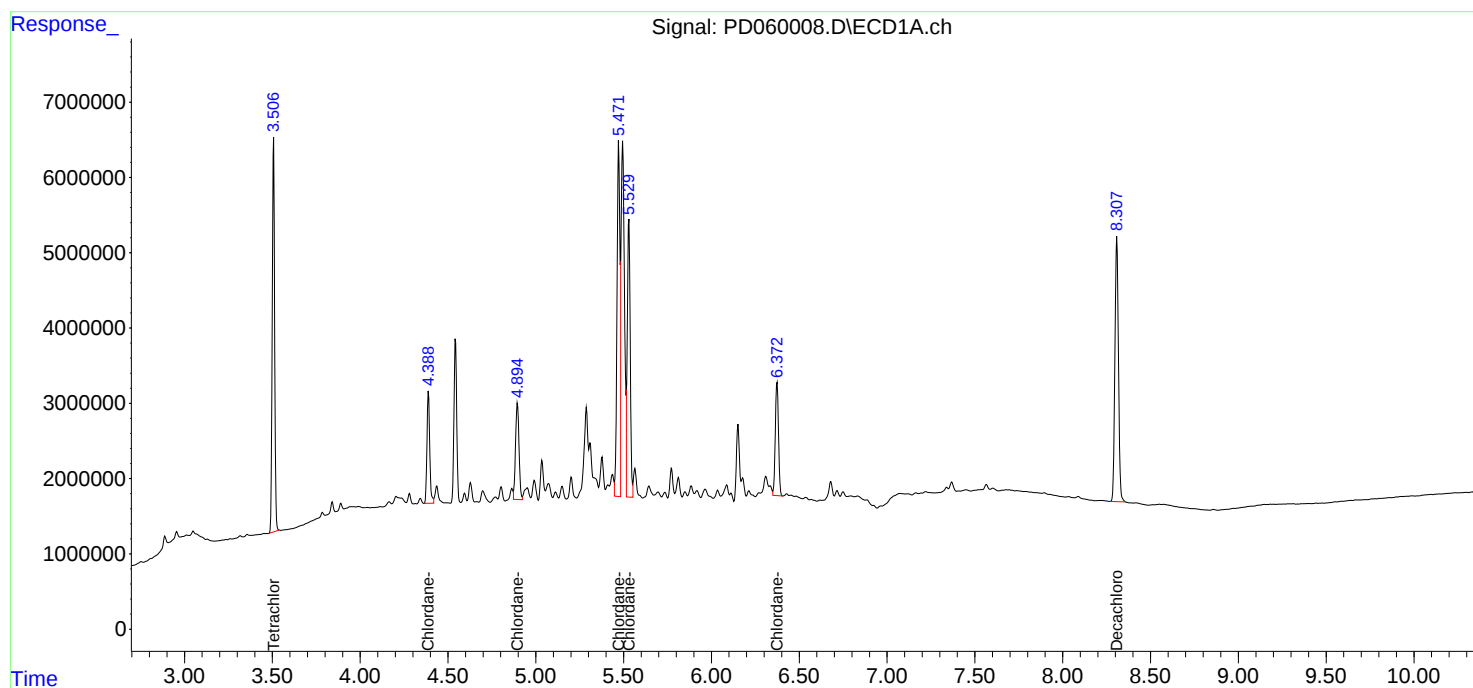


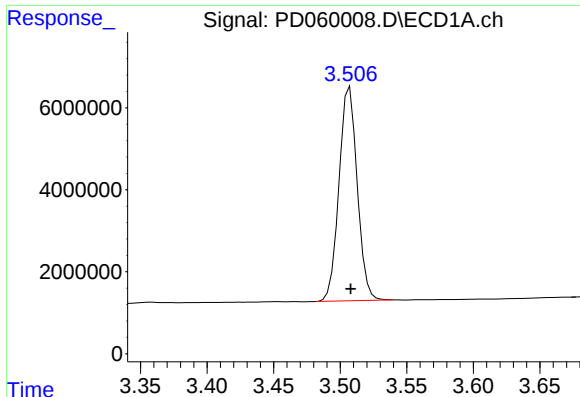

#1 Tetrachloro-m-xylene


R.T.: 3.507 min
Delta R.T.: 0.000 min
Response: 49692246
Conc: 53.43 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

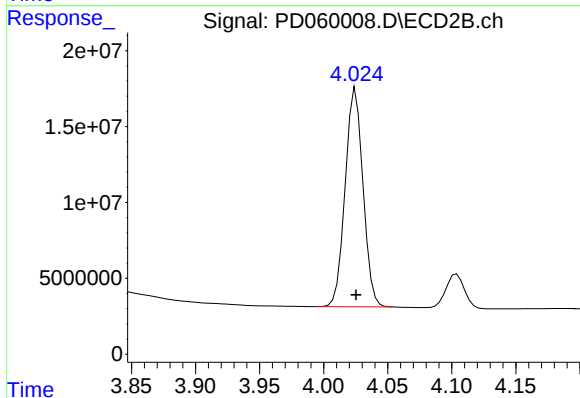


#1 Tetrachloro-m-xylene

R.T.: 4.025 min
Delta R.T.: 0.000 min
Response: 139540614
Conc: 48.23 ng/ml

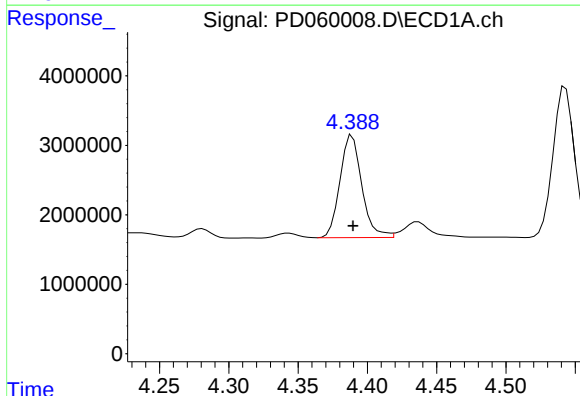


#23 Chlordane-1

R.T.: 4.389 min
Delta R.T.: 0.000 min
Response: 16186355
Conc: 459.59 ng/ml

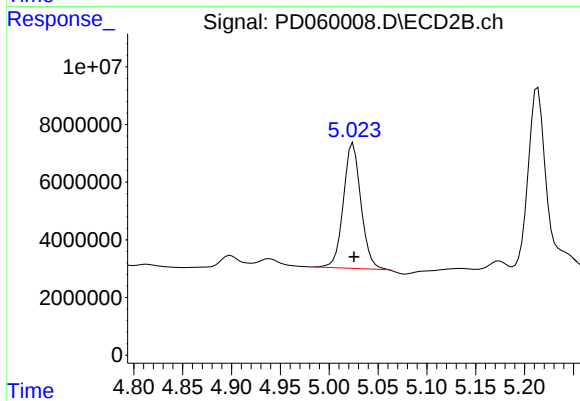

#23 Chlordane-1


R.T.: 5.024 min
Delta R.T.: 0.000 min
Response: 54042257
Conc: 456.94 ng/ml

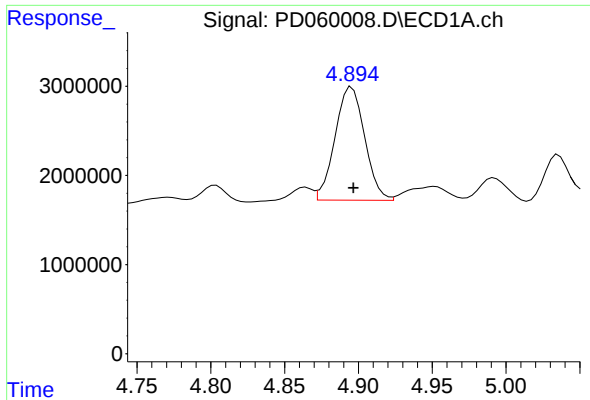

#24 Chlordane-2


R.T.: 4.896 min
Delta R.T.: -0.001 min
Response: 17772260
Conc: 458.08 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

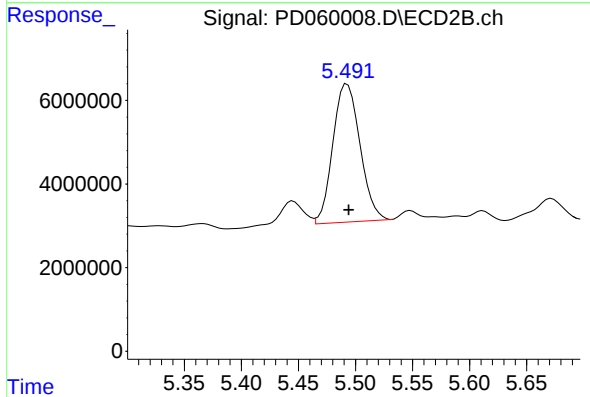


#24 Chlordane-2

R.T.: 5.493 min
Delta R.T.: -0.001 min
Response: 54717389
Conc: 457.74 ng/ml

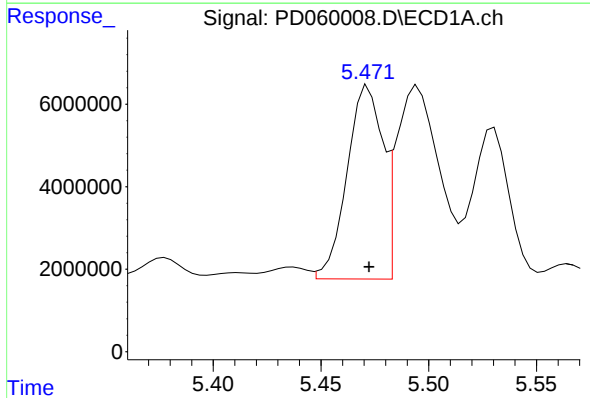


#25 Chlordane-3

R.T.: 5.472 min
Delta R.T.: 0.000 min
Response: 53643902
Conc: 463.65 ng/ml

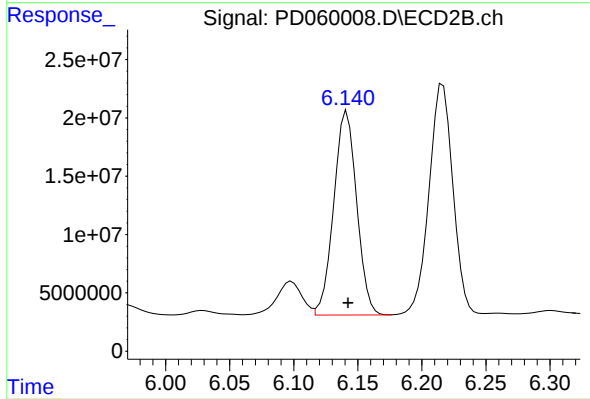

#25 Chlordane-3


R.T.: 6.142 min
Delta R.T.: 0.000 min
Response: 217619114
Conc: 475.29 ng/ml

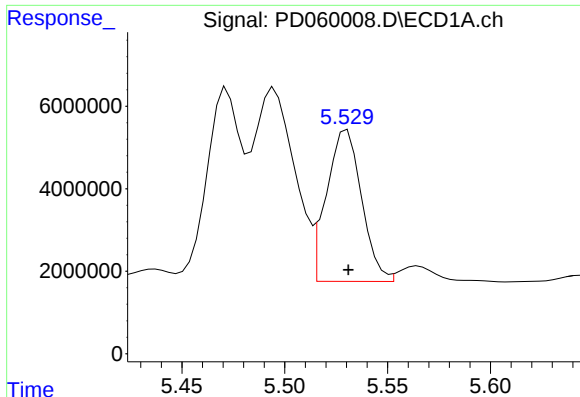

#26 Chlordane-4


R.T.: 5.530 min
Delta R.T.: 0.000 min
Response: 43627305
Conc: 457.86 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

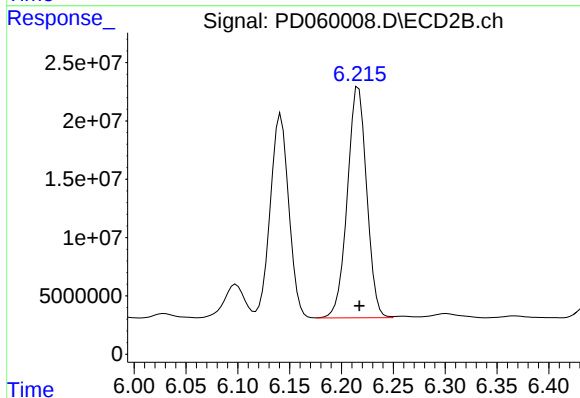


#26 Chlordane-4

R.T.: 6.216 min
Delta R.T.: 0.000 min
Response: 257094114
Conc: 477.72 ng/ml

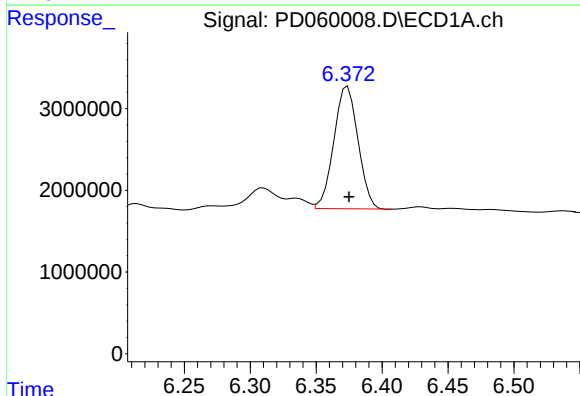


#27 Chlordane-5

R.T.: 6.374 min
Delta R.T.: -0.001 min
Response: 19113299
Conc: 434.99 ng/ml

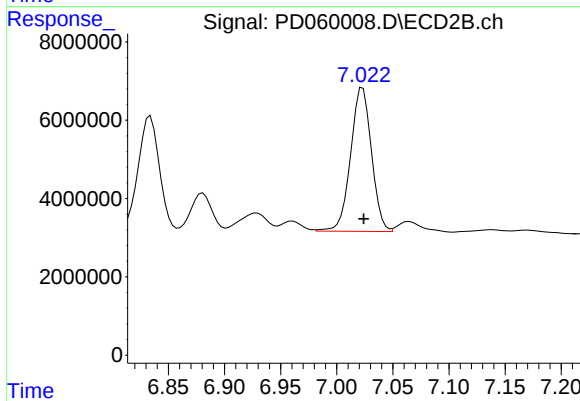

#27 Chlordane-5


R.T.: 7.023 min
Delta R.T.: 0.000 min
Response: 47517894
Conc: 472.52 ng/ml

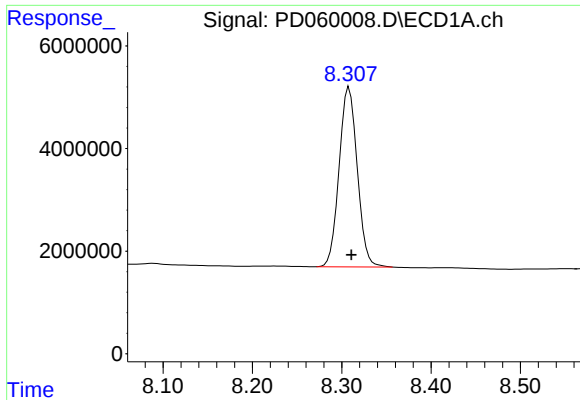

#28 Decachlorobiphenyl

R.T.: 8.308 min
Delta R.T.: -0.003 min
Response: 49419383
Conc: 41.81 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

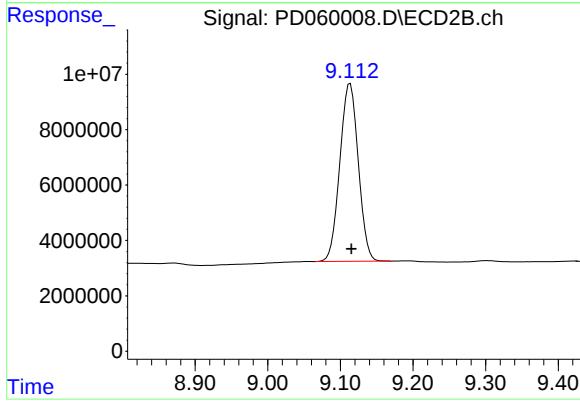

#28 Decachlorobiphenyl

R.T.: 9.114 min
Delta R.T.: -0.002 min
Response: 113405516
Conc: 48.91 ng/ml