

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102921\
 Data File : PD066594.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2021 09:19
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 29 02:02:25 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102821.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 28 02:17:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
28)	SA Decachlor...	0.000	9.037	0	1877057	N.D.	0.348 #
Target Compounds							
2)	A alpha-BHC	0.000	4.367	0	7353331	N.D.	0.667 #
7)	B delta-BHC	0.000	5.056f	0	2879539	N.D.	0.315 #
8)	B Heptachlo...	0.000	5.837	0	25574679	N.D.	3.529 #
9)	A Endosulfan I	0.000	6.207	0	455142	N.D.	0.058 #
14)	MA Endrin	0.000	6.665	0	14962508	N.D.	2.174 #
18)	B Endrin al...	0.000	7.014	0	626305	N.D.	0.110 #
20)	A Methoxychlor	0.000	7.571	0	6993630	N.D.	1.717 #
22)	Mirex	0.000	8.156	0	1673102	N.D.	0.283 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102921\
Data File : PD066594.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2021 09:19
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 02:02:25 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102821.M
Quant Title : GC Extractables
QLast Update : Thu Oct 28 02:17:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

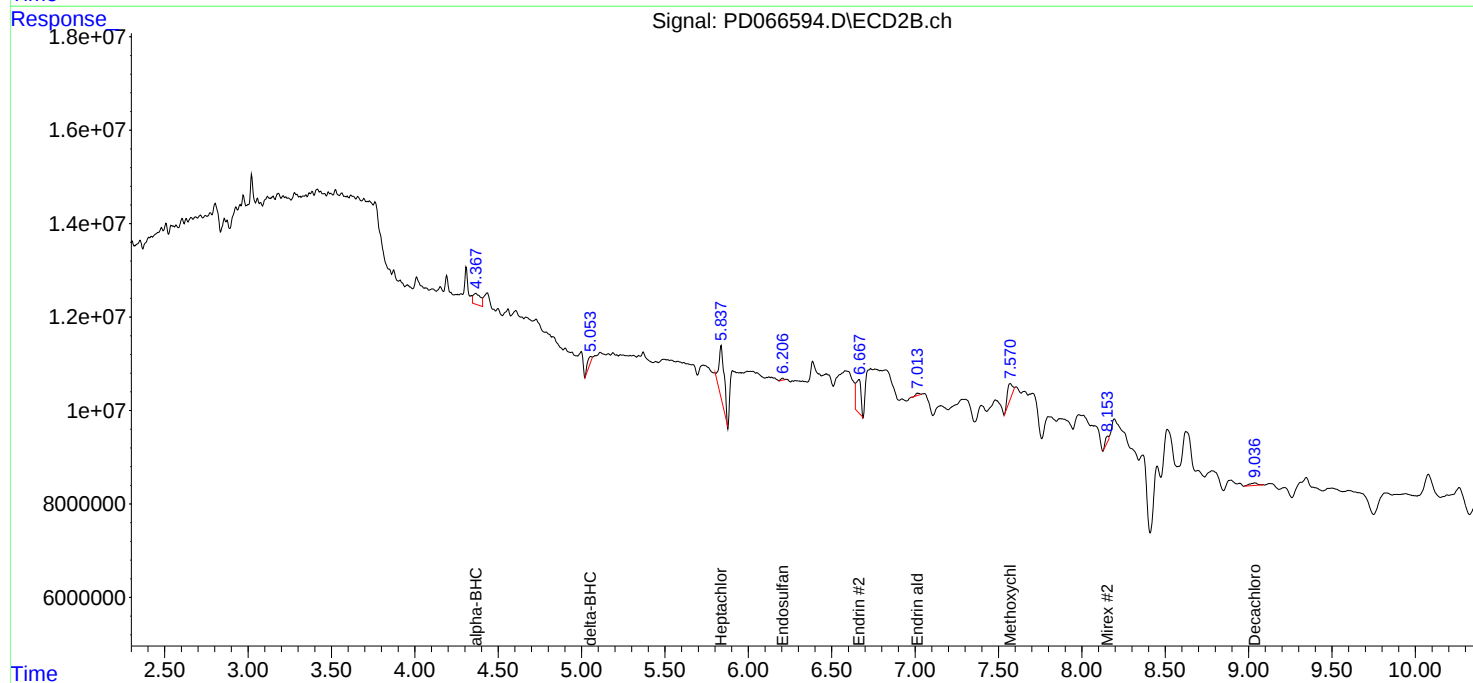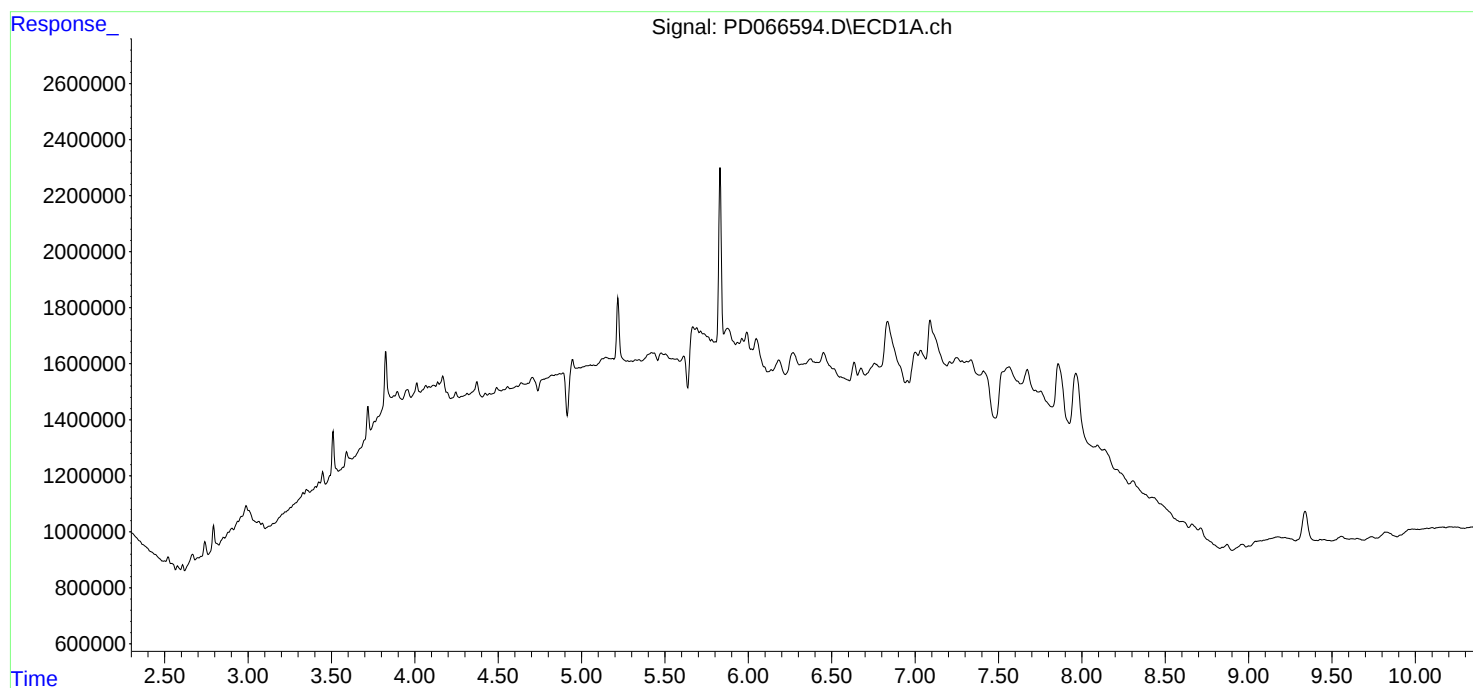


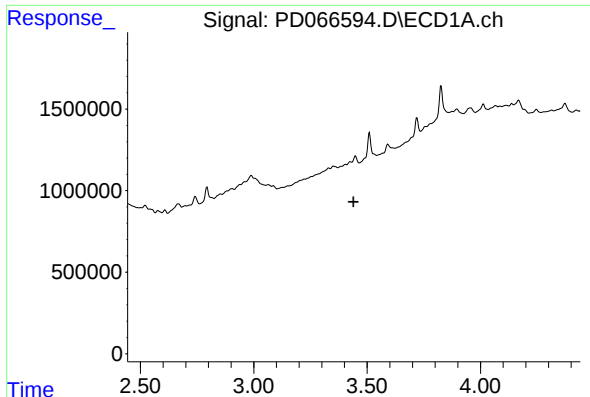

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.440 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

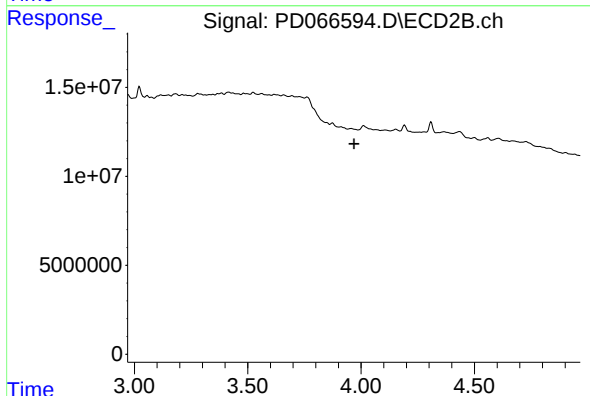


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.970 min
Response: 0
Conc: N.D.

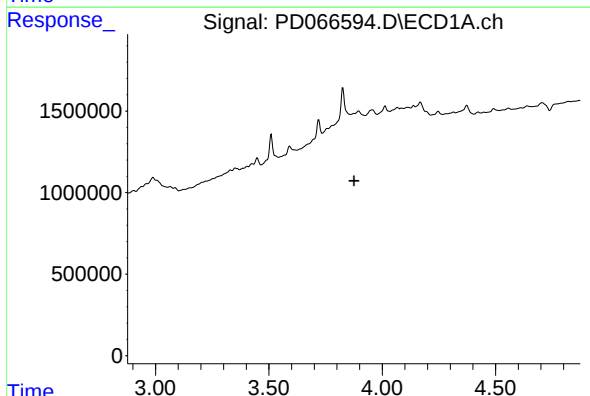


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.876 min
Response: 0
Conc: N.D.

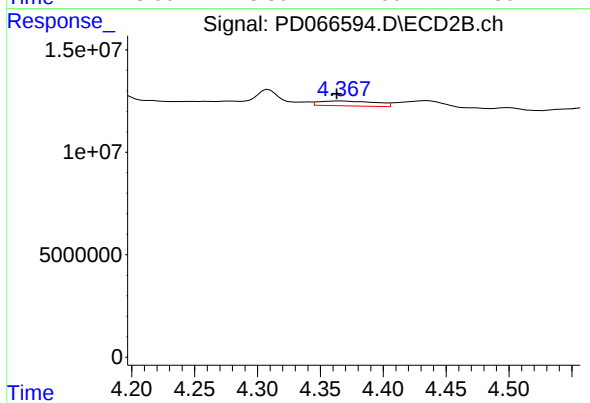

#2 alpha-BHC


R.T.: 4.367 min
Delta R.T.: 0.004 min
Response: 7353331
Conc: 0.67 ng/ml

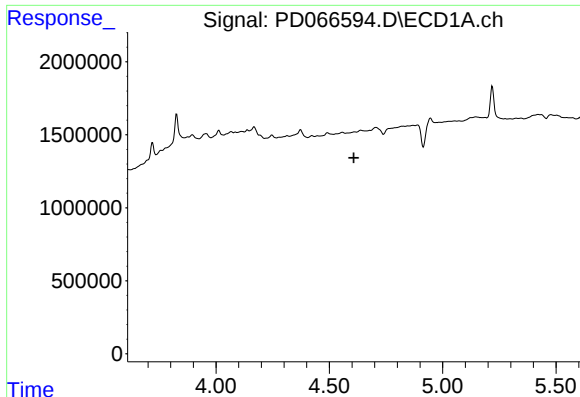

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.608 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

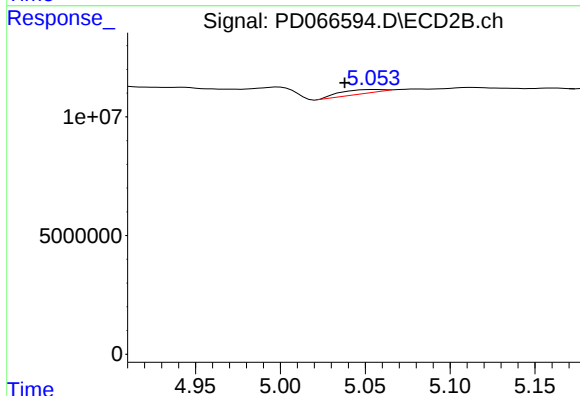


#7 delta-BHC

R.T.: 5.056 min
Delta R.T.: 0.018 min
Response: 2879539
Conc: 0.32 ng/ml

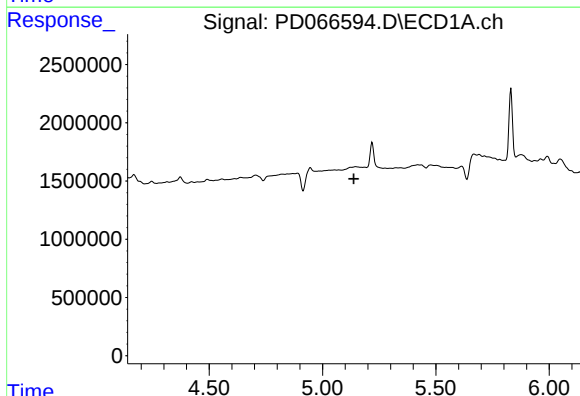


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.138 min
Response: 0
Conc: N.D.

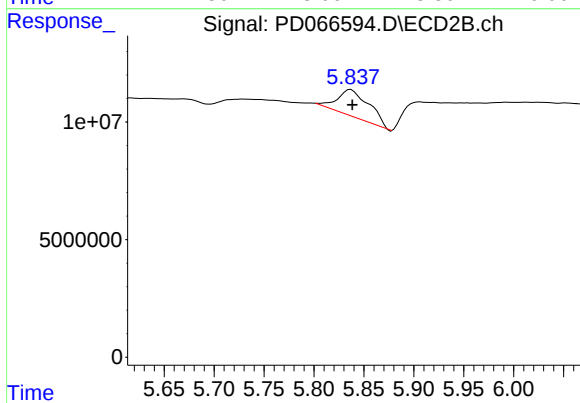

#8 Heptachlor epoxide


R.T.: 5.837 min
Delta R.T.: -0.002 min
Response: 25574679
Conc: 3.53 ng/ml

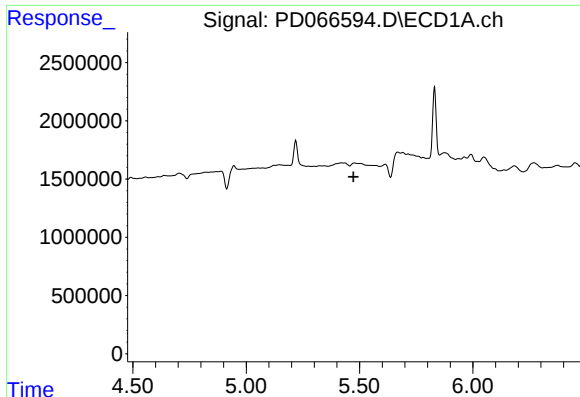

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.474 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

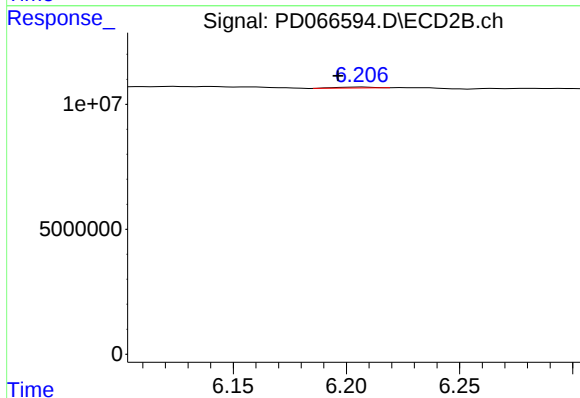


#9 Endosulfan I

R.T.: 6.207 min
Delta R.T.: 0.010 min
Response: 455142
Conc: 0.06 ng/ml

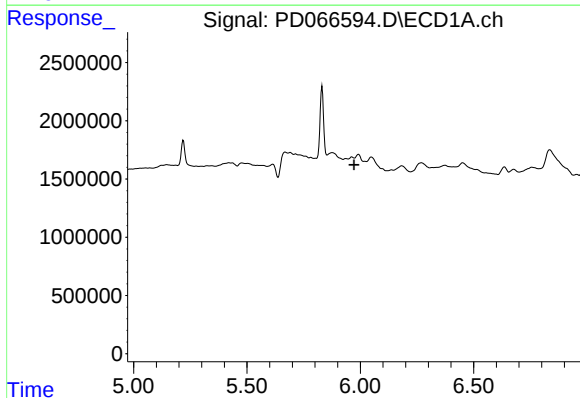


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 5.973 min
Response: 0
Conc: N.D.

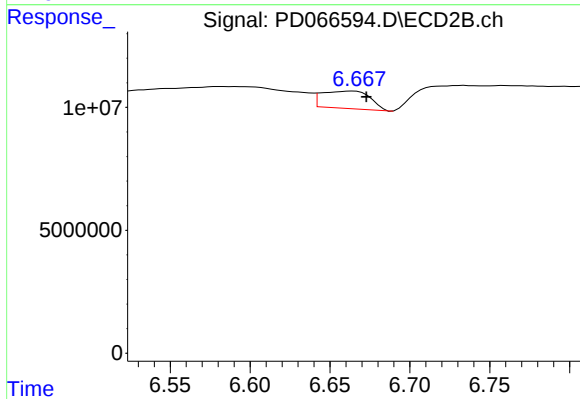

#14 Endrin


R.T.: 6.665 min
Delta R.T.: -0.008 min
Response: 14962508
Conc: 2.17 ng/ml

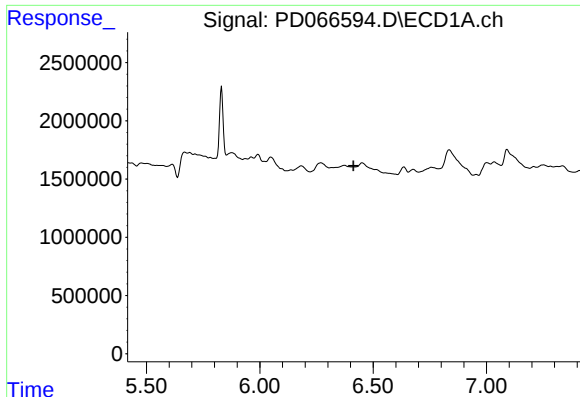

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 6.414 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

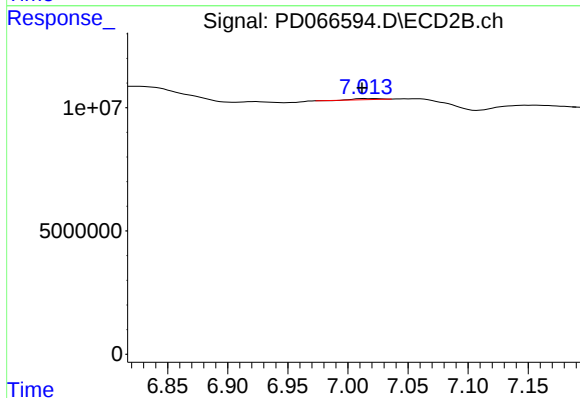


#18 Endrin aldehyde

R.T.: 7.014 min
Delta R.T.: 0.002 min
Response: 626305
Conc: 0.11 ng/ml

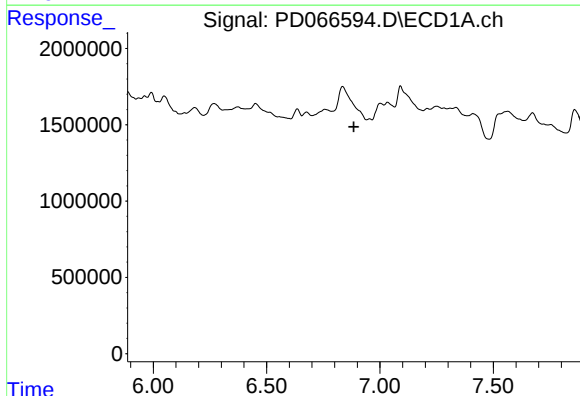


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.884 min
Response: 0
Conc: N.D.

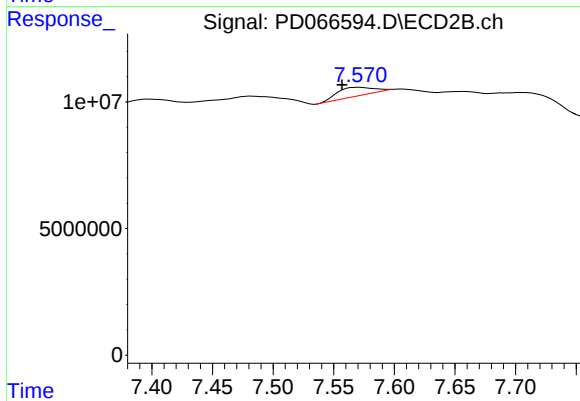

#20 Methoxychlor


R.T.: 7.571 min
Delta R.T.: 0.014 min
Response: 6993630
Conc: 1.72 ng/ml

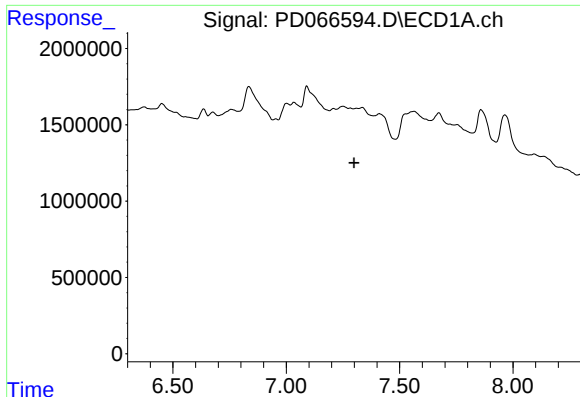

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 7.299 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

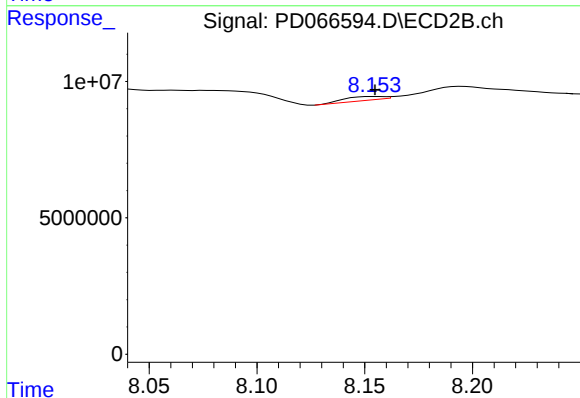


#22 Mirex

R.T.: 8.156 min
Delta R.T.: 0.001 min
Response: 1673102
Conc: 0.28 ng/ml

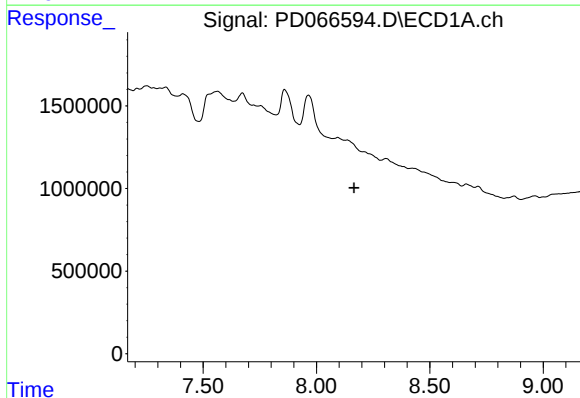

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 8.166 min
Response: 0
Conc: N.D.

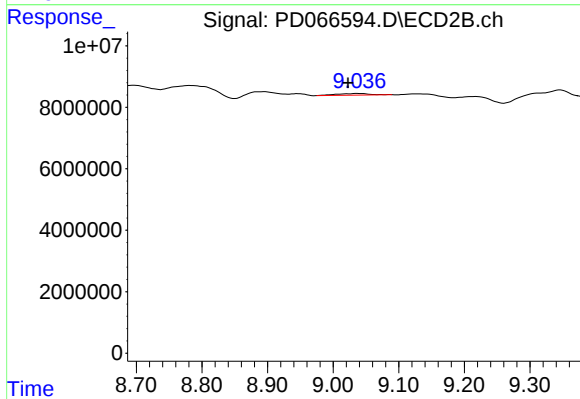

#28 Decachlorobiphenyl

R.T.: 9.037 min
Delta R.T.: 0.014 min
Response: 1877057
Conc: 0.35 ng/ml