

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102921\
 Data File : PD066598.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2021 13:03
 Operator : AJ\MA
 Sample : PB140304BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 29 02:03:01 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102821.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 28 02:17:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.445	3.968	38226721	173.5E6	20.488	21.442
28)	SA Decachlor...	8.175	9.027	24572936	118.5E6	21.268	21.996
Target Compounds							
2)	A alpha-BHC	0.000	4.366	0	2749647	N.D.	0.249 #
9)	A Endosulfan I	0.000	6.216f	0	602689	N.D.	0.076 #
11)	B alpha-Chl...	0.000	6.142	0	1734625	N.D.	0.209 #
16)	A 4,4'-DDD	0.000	6.798	0	5740604	N.D.	0.845 #
18)	B Endrin al...	0.000	7.034f	0	105194	N.D.	0.018 #
20)	A Methoxychlor	0.000	7.580f	0	340244	N.D.	0.084 #
21)	B Endrin ke...	0.000	7.716	0	8785831	N.D.	1.045 #
22)	Mirex	0.000	8.155	0	646426	N.D.	0.109 #
26)	Chlordane-4	0.000	6.142	0	1734625	N.D.	1.376 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102921\
Data File : PD066598.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2021 13:03
Operator : AJ\MA
Sample : PB140304BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 02:03:01 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102821.M
Quant Title : GC Extractables
QLast Update : Thu Oct 28 02:17:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

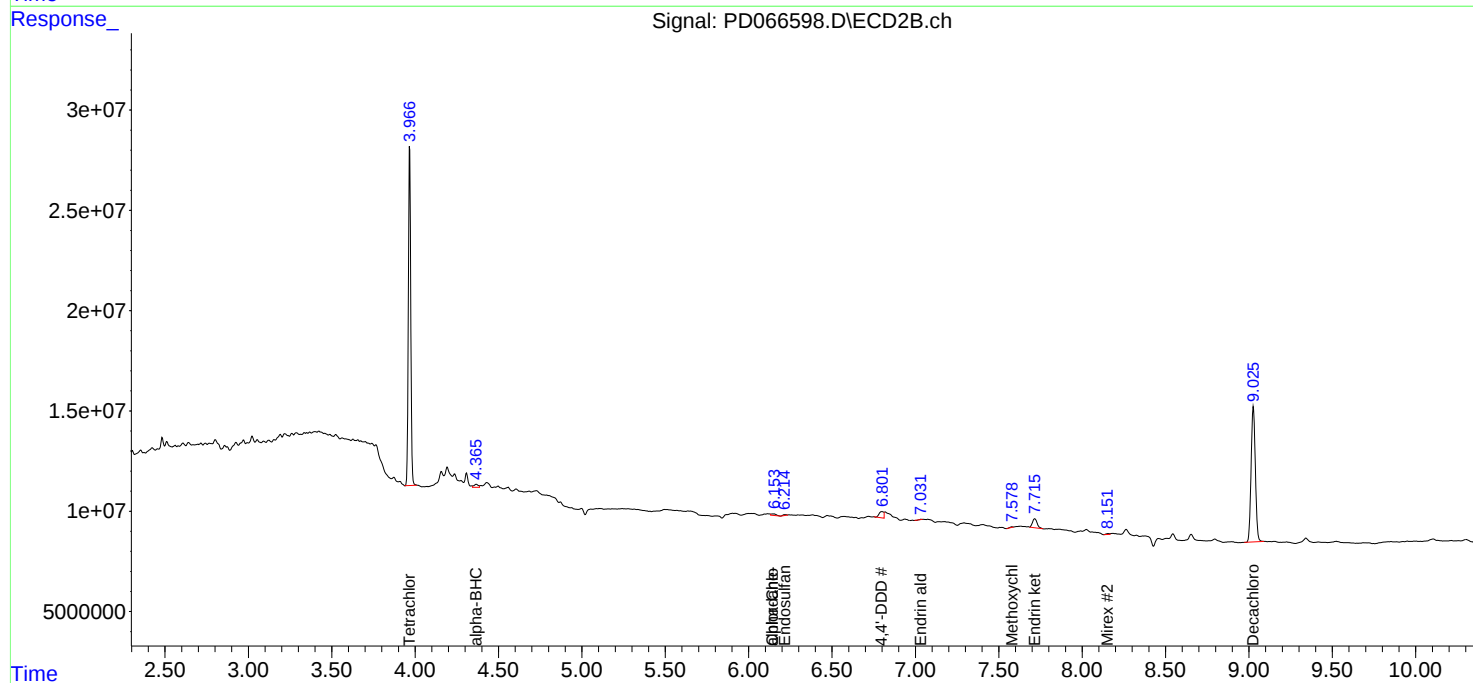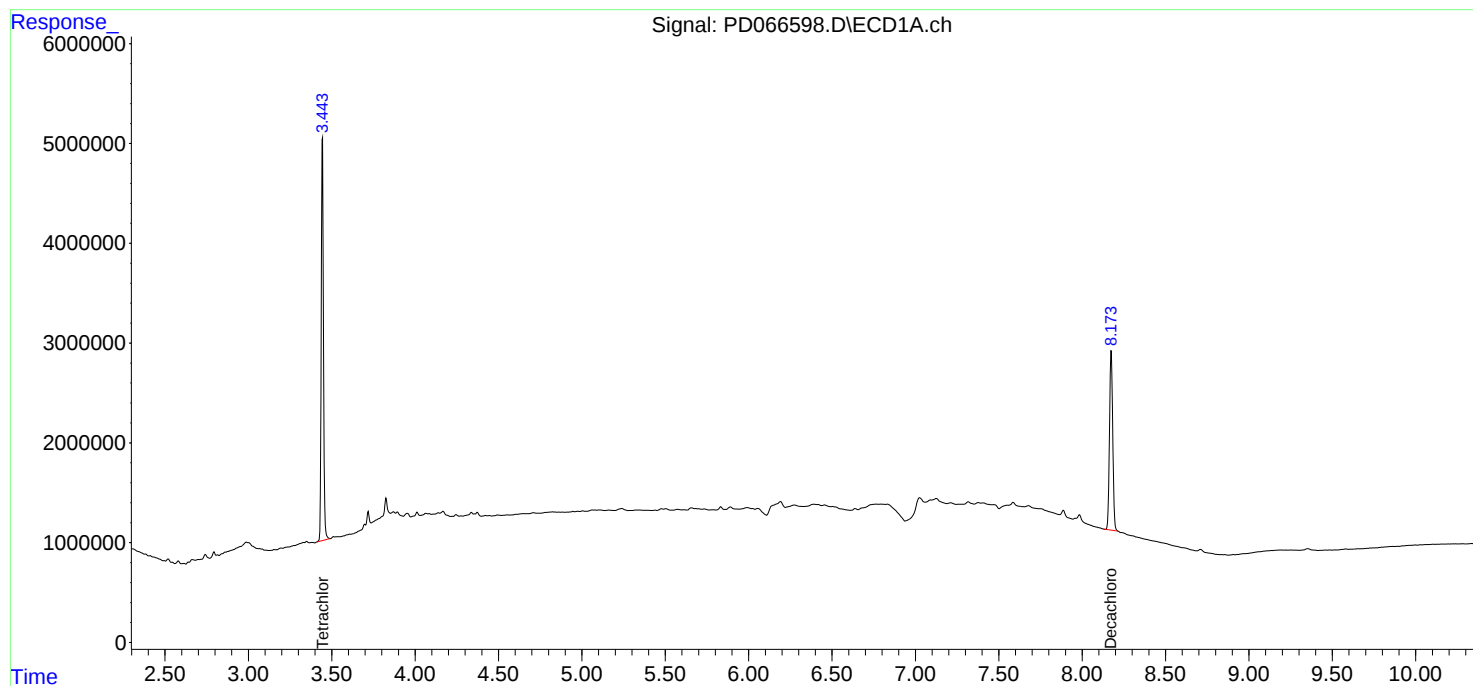


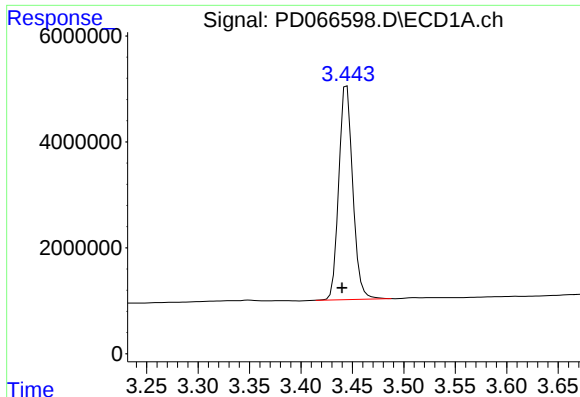

#1 Tetrachloro-m-xylene


R.T.: 3.445 min
Delta R.T.: 0.005 min
Response: 38226721
Conc: 20.49 ng/ml

Instrument :
ECD_D
ClientSampleId :

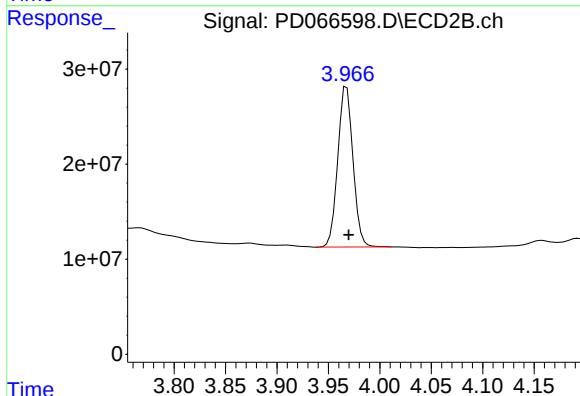


#1 Tetrachloro-m-xylene

R.T.: 3.968 min
Delta R.T.: -0.002 min
Response: 173509035
Conc: 21.44 ng/ml

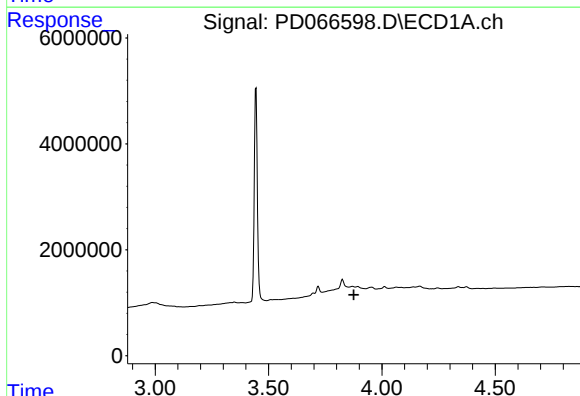


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.876 min
Response: 0
Conc: N.D.

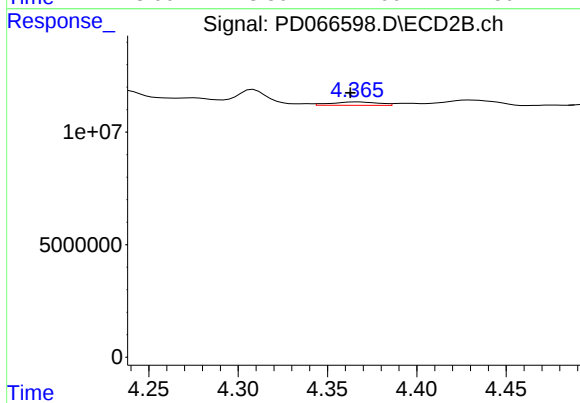

#2 alpha-BHC


R.T.: 4.366 min
Delta R.T.: 0.004 min
Response: 2749647
Conc: 0.25 ng/ml

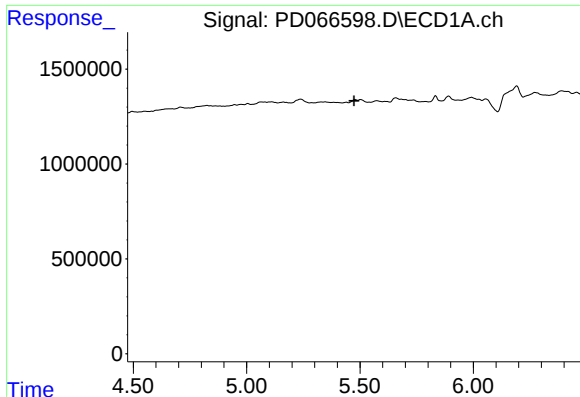

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.474 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

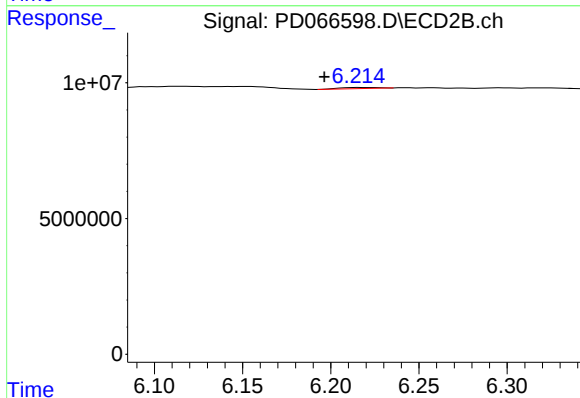


#9 Endosulfan I

R.T.: 6.216 min
Delta R.T.: 0.019 min
Response: 602689
Conc: 0.08 ng/ml

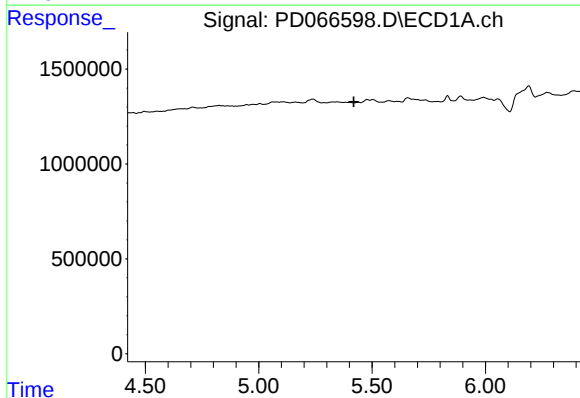


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.420 min
Response: 0
Conc: N.D.

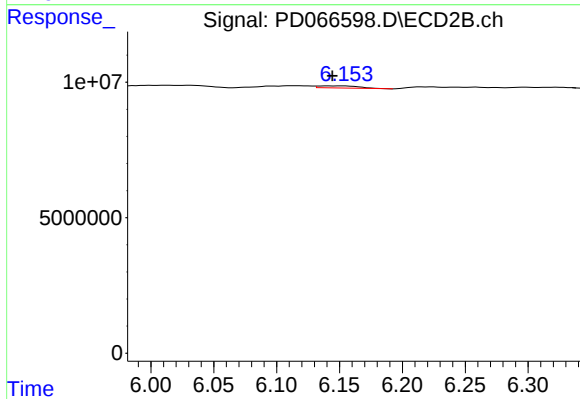

#11 alpha-Chlordane


R.T.: 6.142 min
Delta R.T.: -0.002 min
Response: 1734625
Conc: 0.21 ng/ml

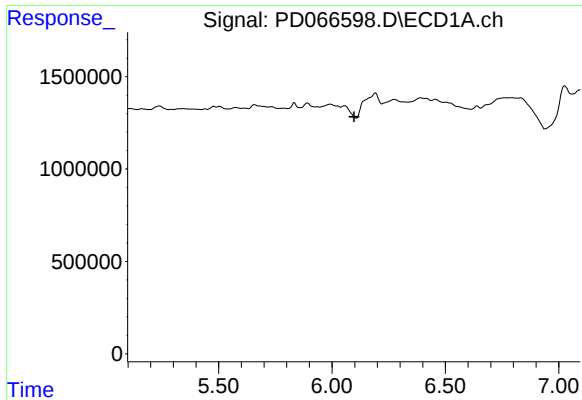

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.097 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

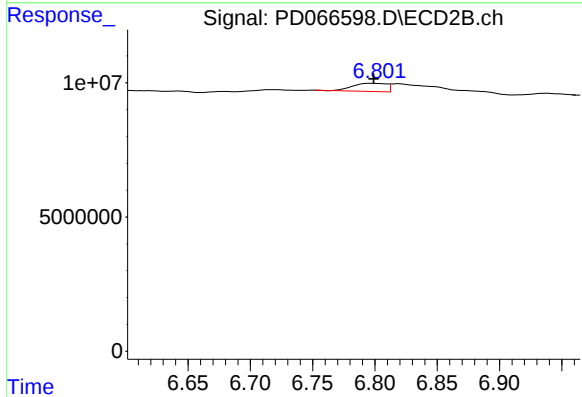


#16 4,4'-DDD

R.T.: 6.798 min
Delta R.T.: -0.001 min
Response: 5740604
Conc: 0.84 ng/ml

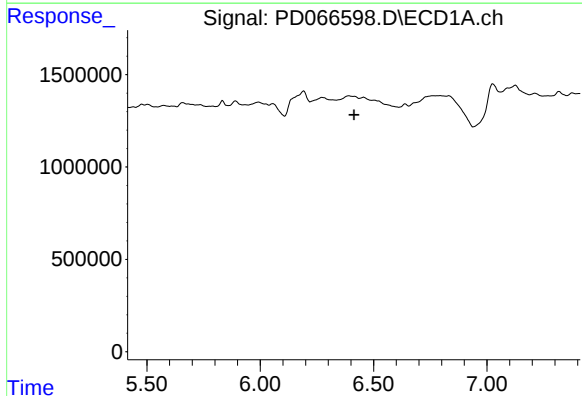


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 6.414 min
Response: 0
Conc: N.D.

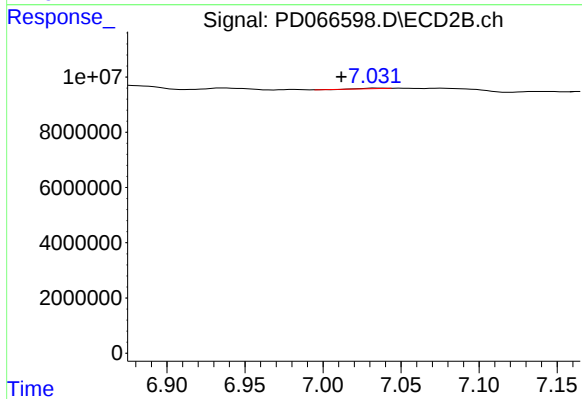

#18 Endrin aldehyde


R.T.: 7.034 min
Delta R.T.: 0.022 min
Response: 105194
Conc: 0.02 ng/ml

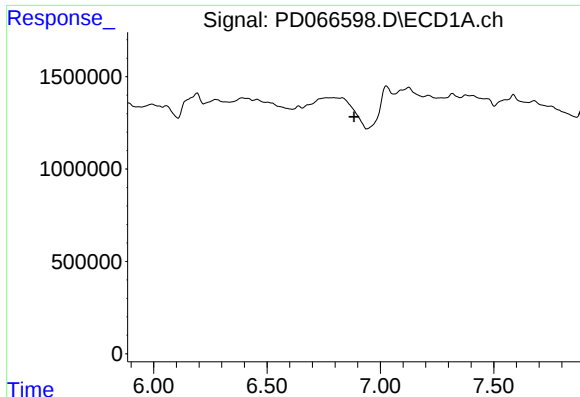

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 6.884 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

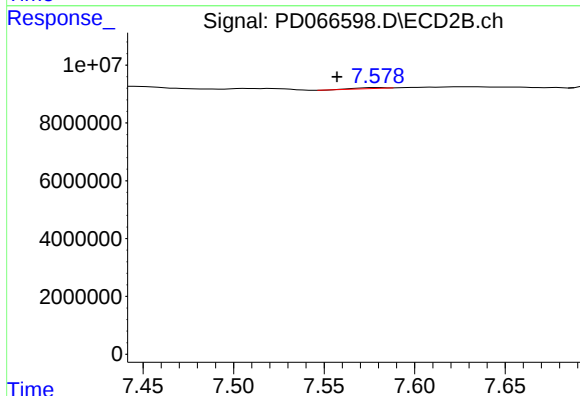


#20 Methoxychlor

R.T.: 7.580 min
Delta R.T.: 0.023 min
Response: 340244
Conc: 0.08 ng/ml

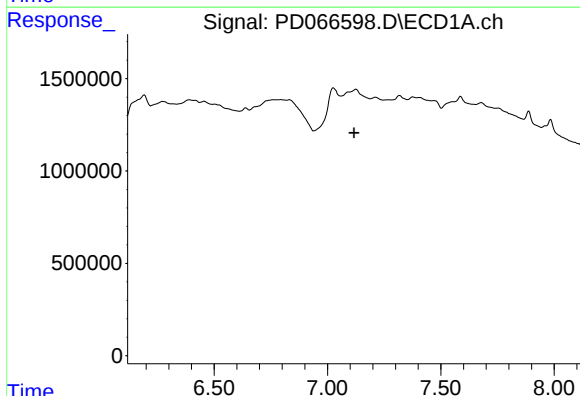


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 7.118 min
Response: 0
Conc: N.D.

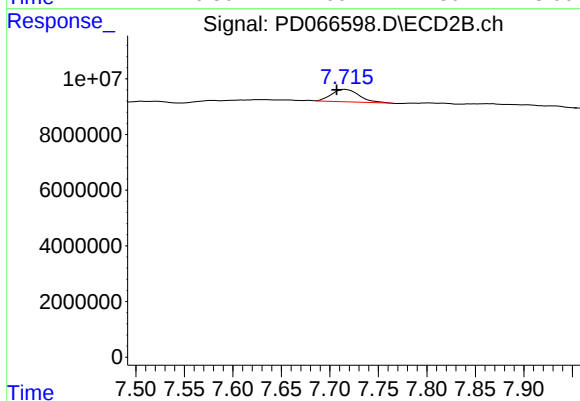

#21 Endrin ketone


R.T.: 7.716 min
Delta R.T.: 0.009 min
Response: 8785831
Conc: 1.04 ng/ml

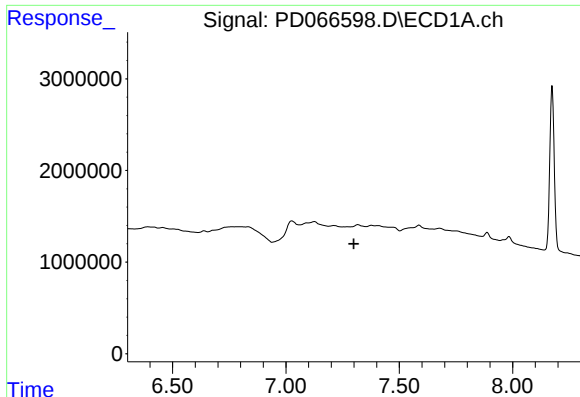

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 7.299 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

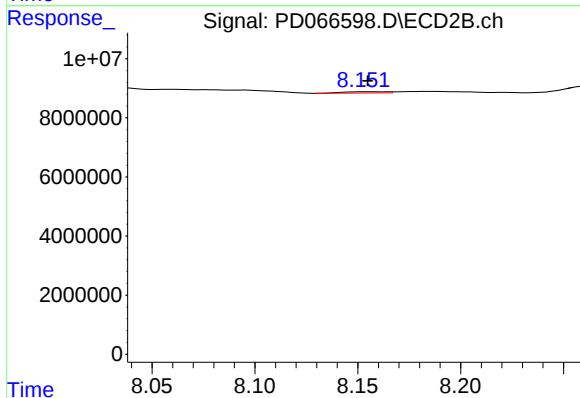


#22 Mirex

R.T.: 8.155 min
Delta R.T.: 0.000 min
Response: 646426
Conc: 0.11 ng/ml

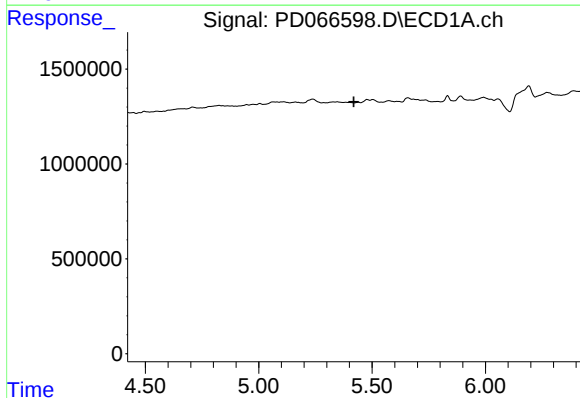


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.420 min
Response: 0
Conc: N.D.

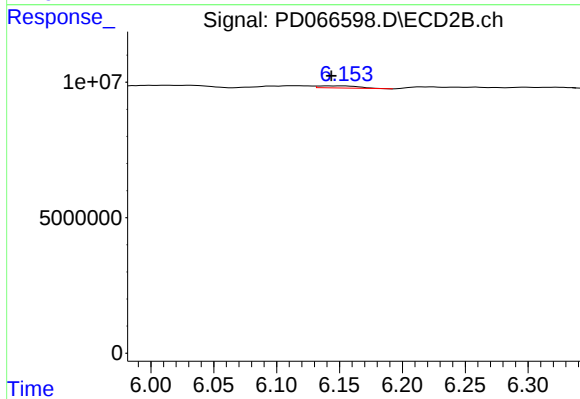

#26 Chlordane-4


R.T.: 6.142 min
Delta R.T.: -0.001 min
Response: 1734625
Conc: 1.38 ng/ml

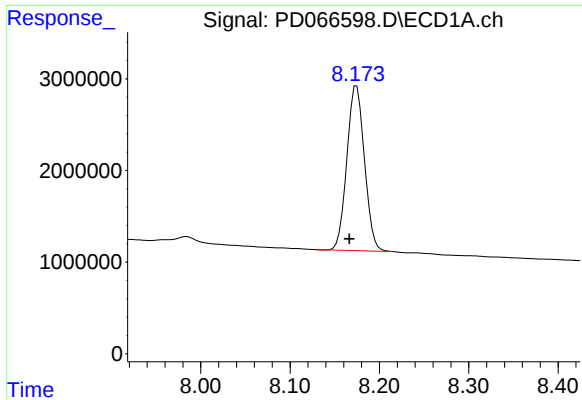

#28 Decachlorobiphenyl

R.T.: 8.175 min
Delta R.T.: 0.008 min
Response: 24572936
Conc: 21.27 ng/ml

Instrument :
ECD_D
ClientSampleId :

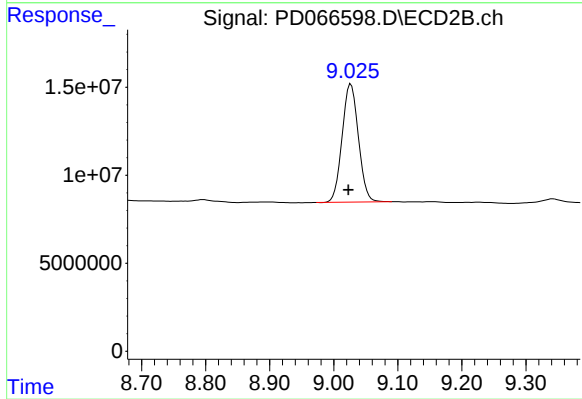

#28 Decachlorobiphenyl

R.T.: 9.027 min
Delta R.T.: 0.004 min
Response: 118479583
Conc: 22.00 ng/ml