

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102921\
 Data File : PD066603.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2021 14:38
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 29 02:03:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102821.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 28 02:17:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.439	3.969	39947674	185.2E6	21.410	22.880
28)	SA Decachlor...	8.166	9.022	26032638	123.2E6	22.531	22.865
Target Compounds							
3)	MA gamma-BHC...	4.160	0.000	5137974	0	1.701	N.D. #
4)	MA Heptachlor	0.000	5.124f	0	526831	N.D.	0.054 #
5)	MB Aldrin	0.000	5.480f	0	80603	N.D.	0.009 #
6)	B beta-BHC	4.415	4.842f	2106033	1981478	1.686	0.426 #
7)	B delta-BHC	0.000	5.062f	0	4871839	N.D.	0.533 #
8)	B Heptachlo...	0.000	5.862f	0	2872262	N.D.	0.396 #
15)	B Endosulfa...	0.000	6.887	0	1678811	N.D.	0.238 #
21)	B Endrin ke...	0.000	7.730f	0	12787172	N.D.	1.521 #
27)	Chlordane-5	0.000	6.936f	0	20334	N.D.	0.075 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102921\
Data File : PD066603.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2021 14:38
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 02:03:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102821.M
Quant Title : GC Extractables
QLast Update : Thu Oct 28 02:17:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

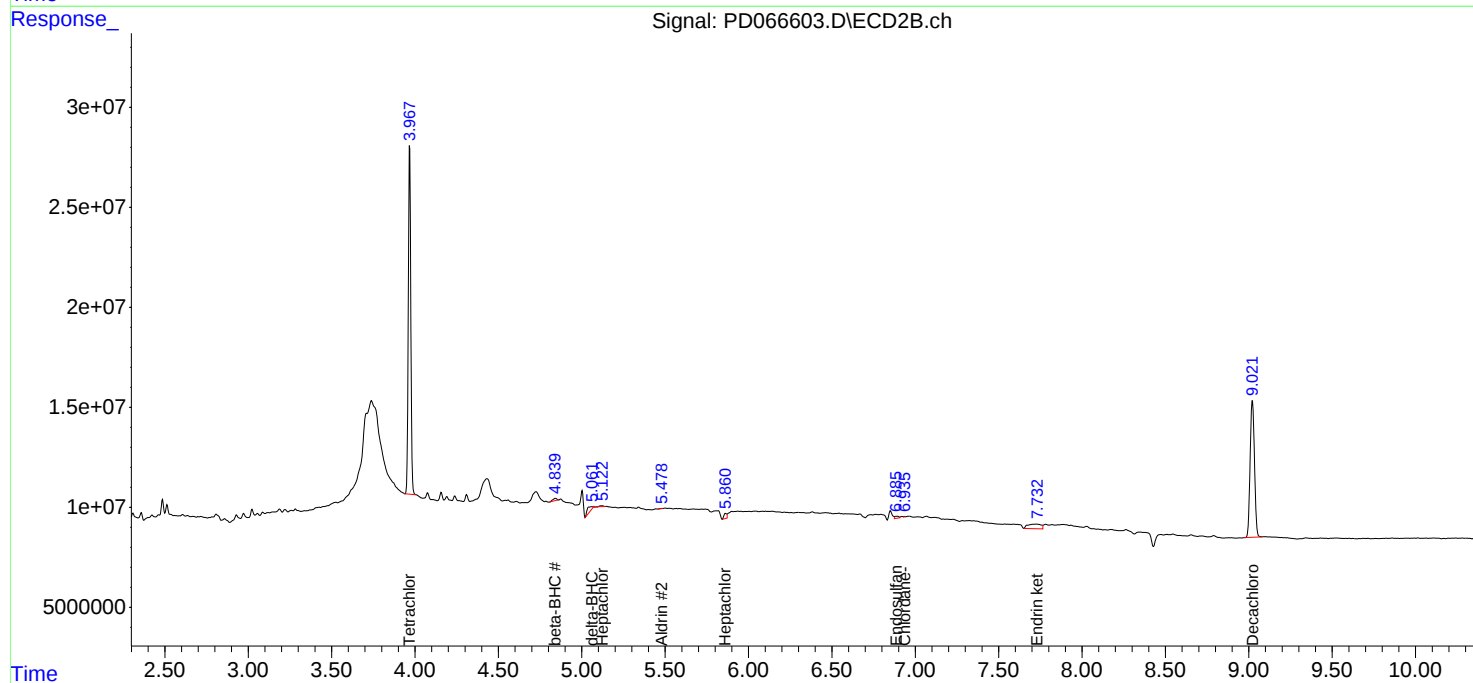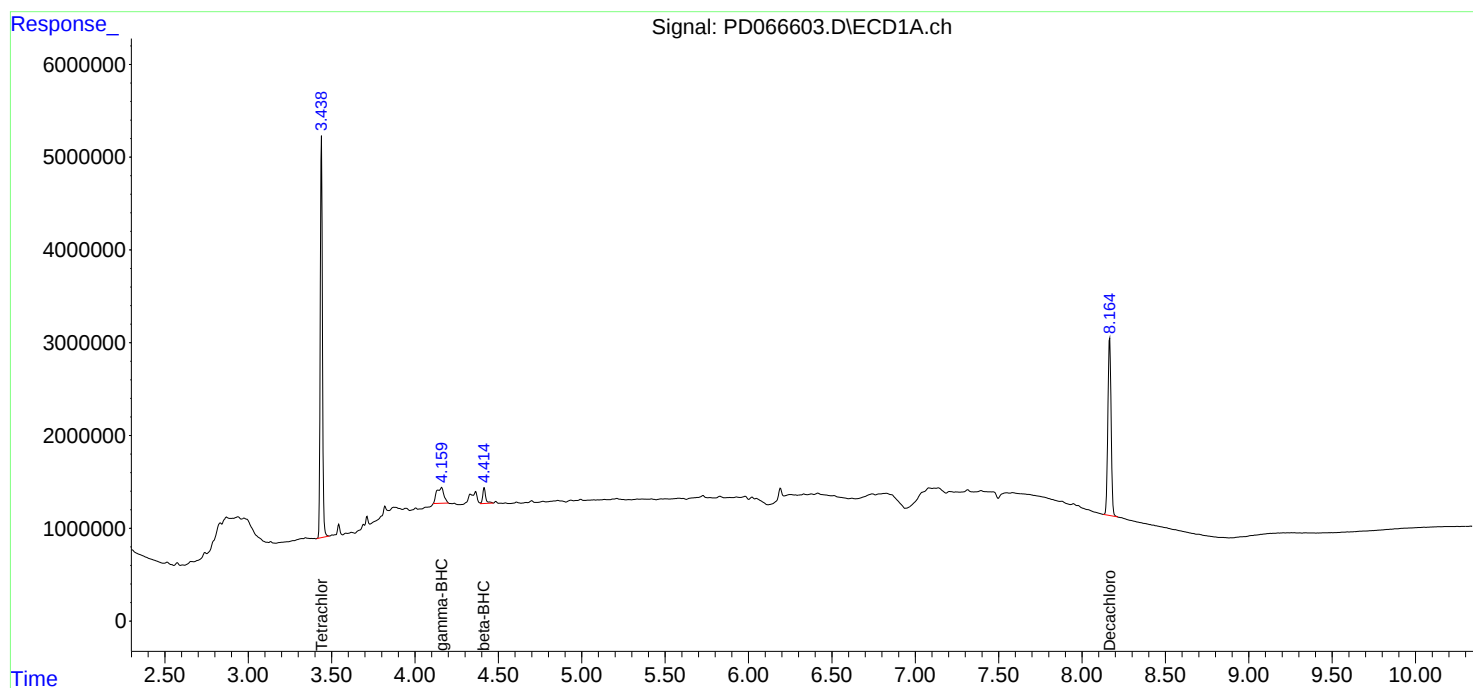


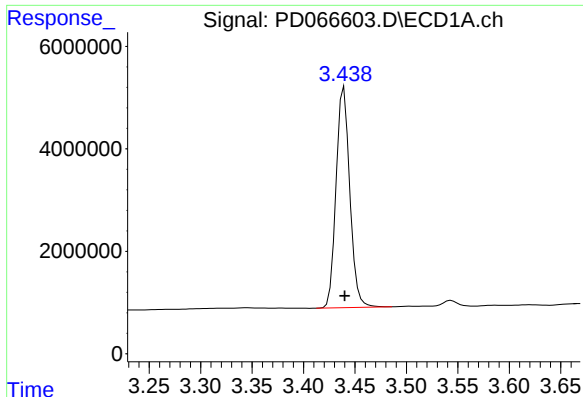

#1 Tetrachloro-m-xylene


R.T.: 3.439 min
Delta R.T.: 0.000 min
Response: 39947674
Conc: 21.41 ng/ml

Instrument :
ECD_D
ClientSampleId :

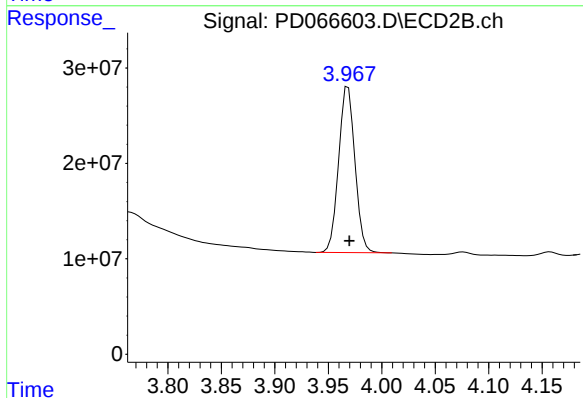


#1 Tetrachloro-m-xylene

R.T.: 3.969 min
Delta R.T.: -0.001 min
Response: 185151861
Conc: 22.88 ng/ml

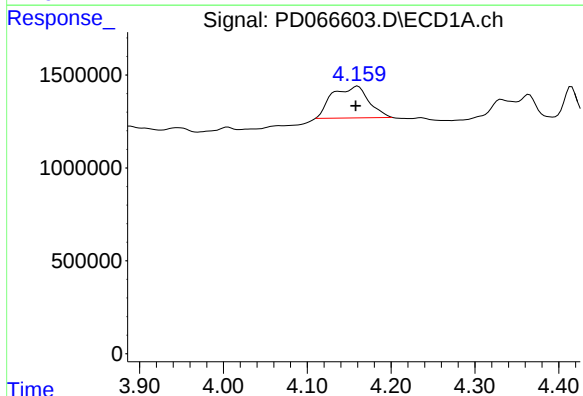


#3 gamma-BHC (Lindane)

R.T.: 4.160 min
Delta R.T.: 0.003 min
Response: 5137974
Conc: 1.70 ng/ml

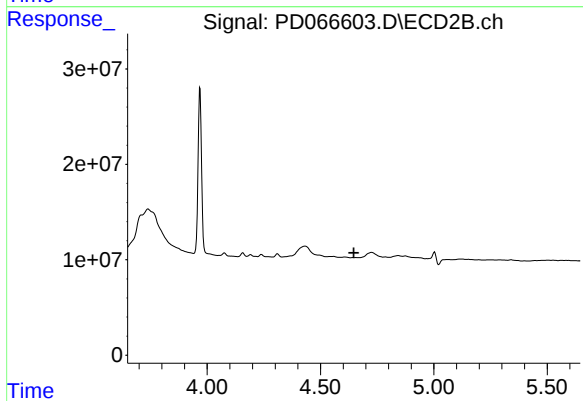

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.647 min
Response: 0
Conc: N.D.

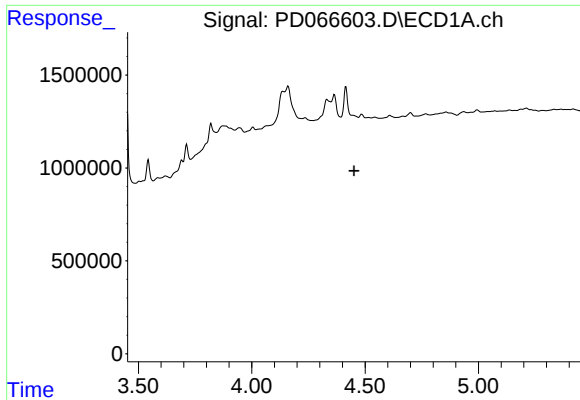

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.452 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

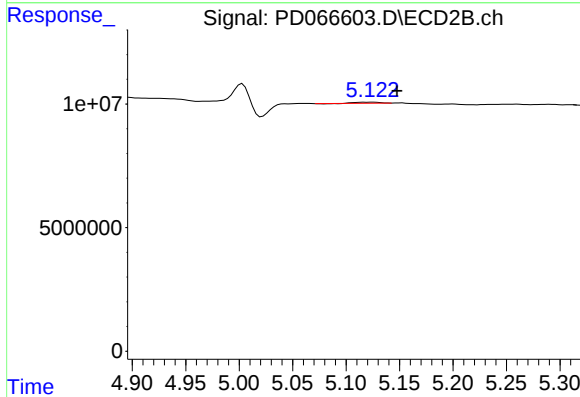


#4 Heptachlor

R.T.: 5.124 min
Delta R.T.: -0.024 min
Response: 526831
Conc: 0.05 ng/ml

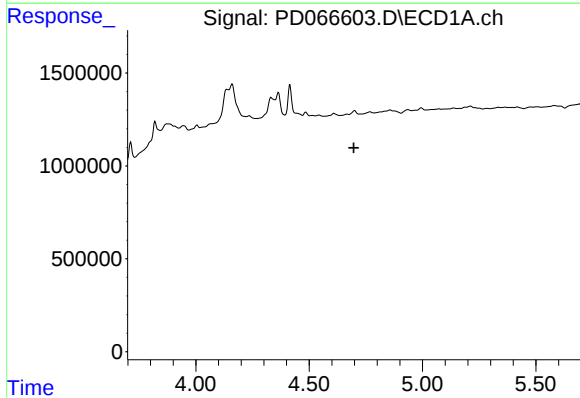


#5 Aldrin

R.T.: 0.000 min
Exp R.T.: 4.697 min
Response: 0
Conc: N.D.

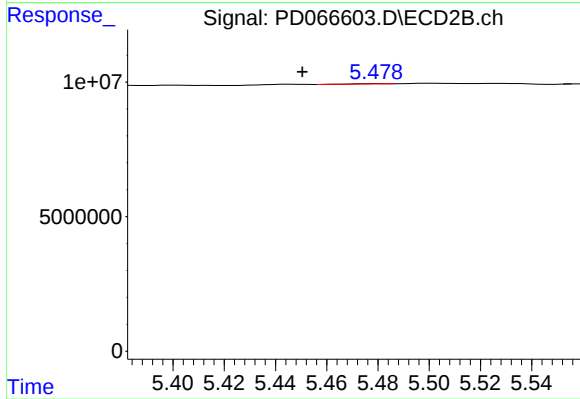

#5 Aldrin


R.T.: 5.480 min
Delta R.T.: 0.029 min
Response: 80603
Conc: 0.01 ng/ml

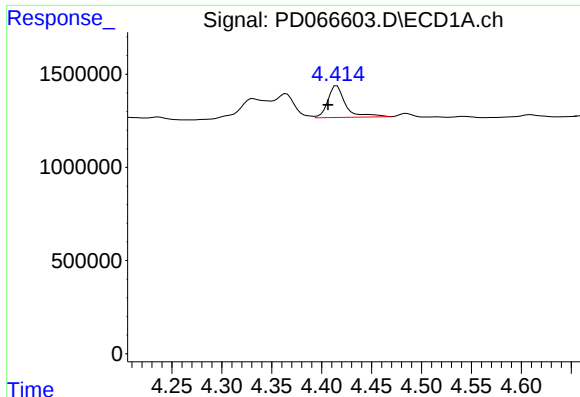

#6 beta-BHC


R.T.: 4.415 min
Delta R.T.: 0.009 min
Response: 2106033
Conc: 1.69 ng/ml

Instrument :
ECD_D
ClientSampleId :

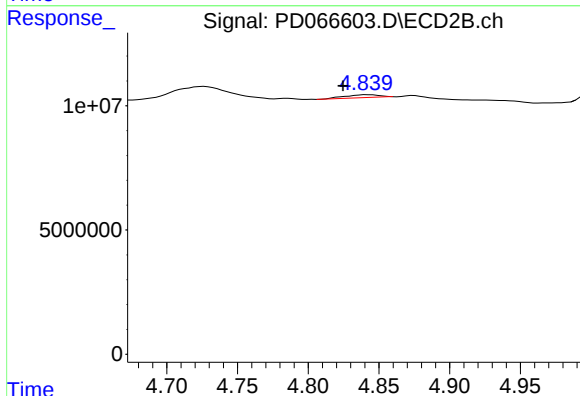


#6 beta-BHC

R.T.: 4.842 min
Delta R.T.: 0.017 min
Response: 1981478
Conc: 0.43 ng/ml

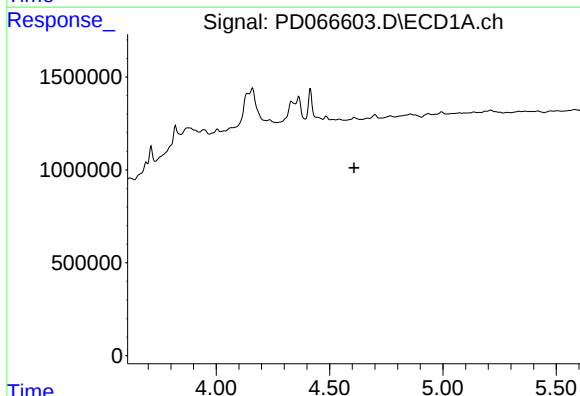


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.608 min
Response: 0
Conc: N.D.

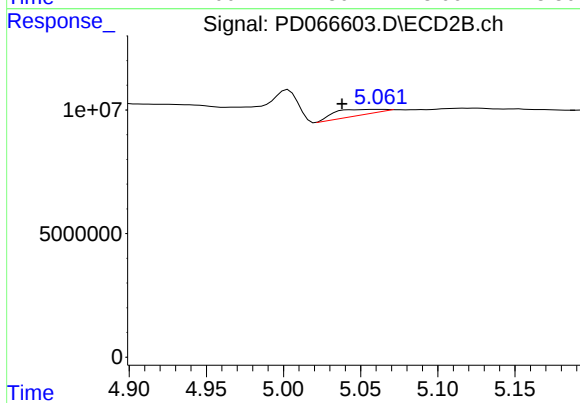

#7 delta-BHC


R.T.: 5.062 min
Delta R.T.: 0.024 min
Response: 4871839
Conc: 0.53 ng/ml

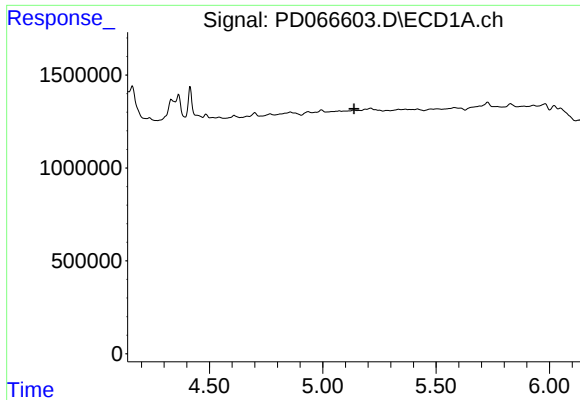

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.138 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

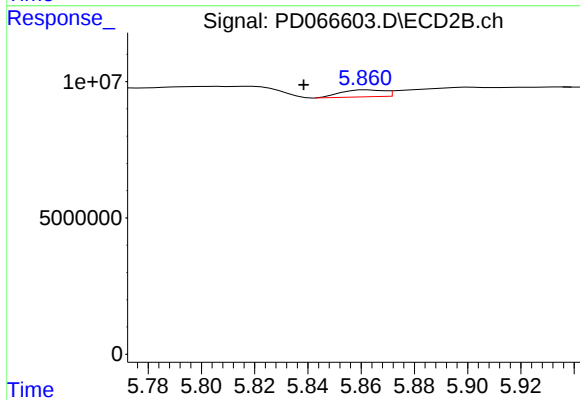


#8 Heptachlor epoxide

R.T.: 5.862 min
Delta R.T.: 0.024 min
Response: 2872262
Conc: 0.40 ng/ml

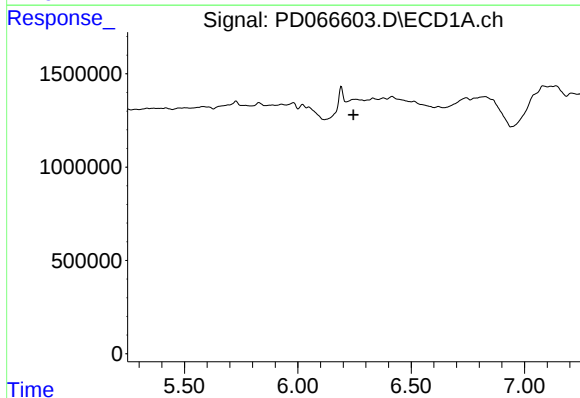


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.246 min
Response: 0
Conc: N.D.

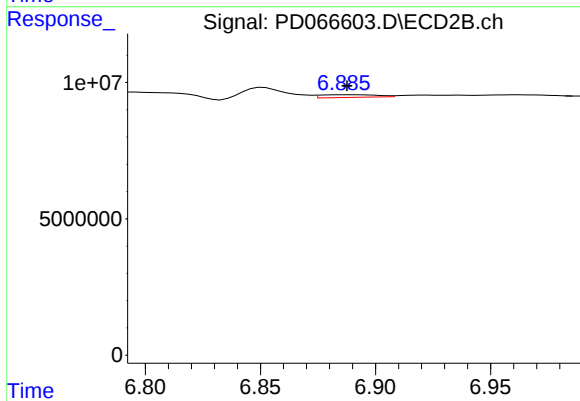

#15 Endosulfan II


R.T.: 6.887 min
Delta R.T.: -0.001 min
Response: 1678811
Conc: 0.24 ng/ml

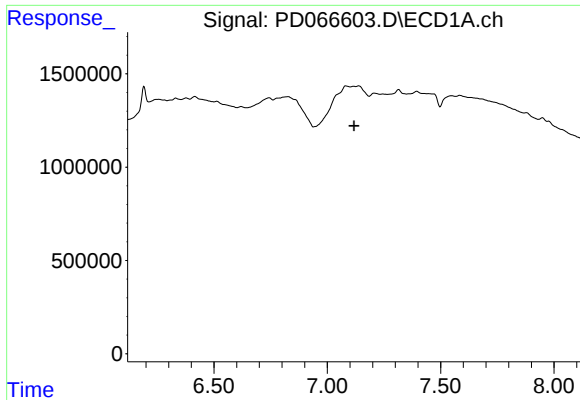

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.118 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

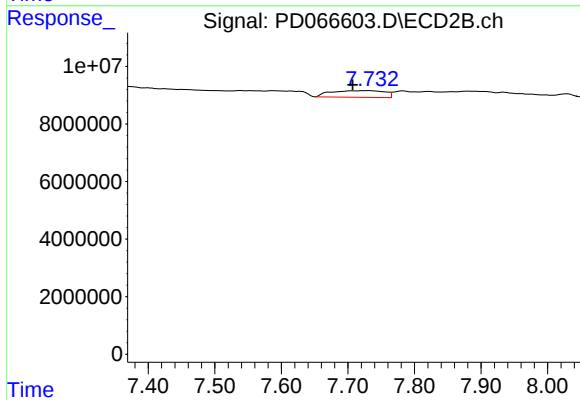


#21 Endrin ketone

R.T.: 7.730 min
Delta R.T.: 0.023 min
Response: 12787172
Conc: 1.52 ng/ml

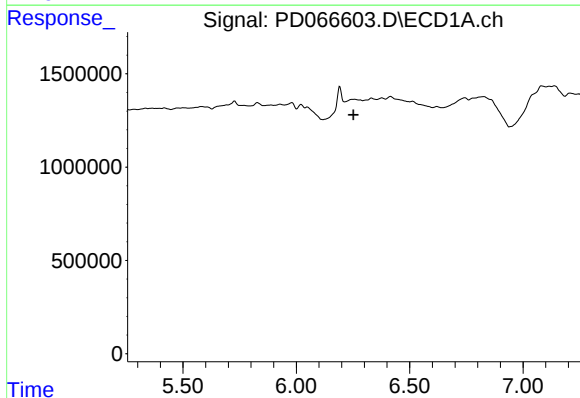


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.252 min
Response: 0
Conc: N.D.

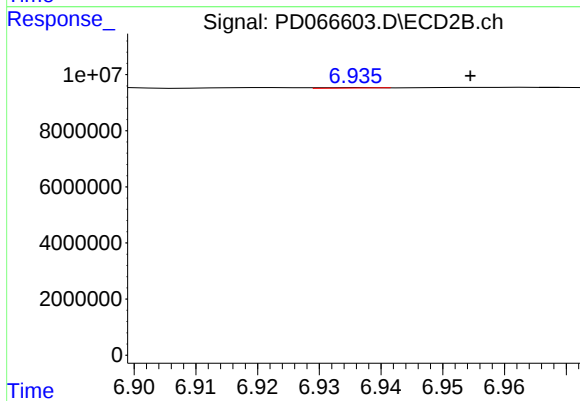

#27 Chlordane-5


R.T.: 6.936 min
Delta R.T.: -0.018 min
Response: 20334
Conc: 0.07 ng/ml

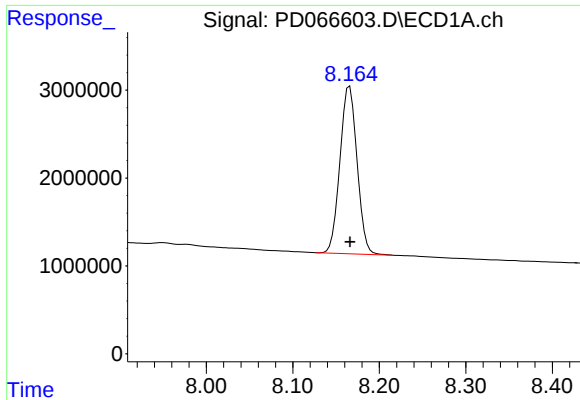

#28 Decachlorobiphenyl

R.T.: 8.166 min
Delta R.T.: 0.000 min
Response: 26032638
Conc: 22.53 ng/ml

Instrument :
ECD_D
ClientSampleId :

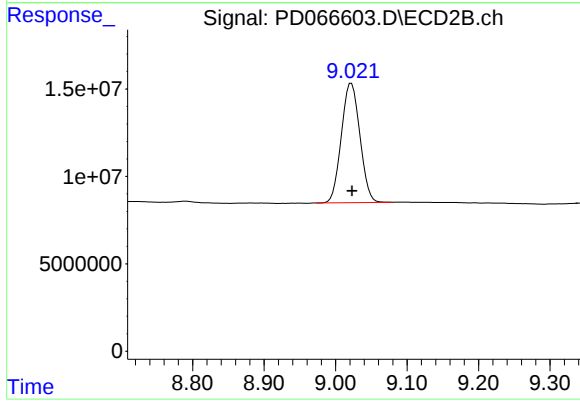

#28 Decachlorobiphenyl

R.T.: 9.022 min
Delta R.T.: 0.000 min
Response: 123157245
Conc: 22.86 ng/ml