

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102921\
 Data File : PD066616.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2021 17:40
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 29 02:04:41 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102821.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 28 02:17:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.440	3.969	40124115	181.0E6	21.505	22.372
28)	SA Decachlor...	8.165	9.022	25749273	121.9E6	22.286	22.624
Target Compounds							
3)	MA gamma-BHC...	4.161	0.000	3970120	0	1.315	N.D. #
4)	MA Heptachlor	0.000	5.125f	0	1111723	N.D.	0.113 #
5)	MB Aldrin	0.000	5.455	0	245825	N.D.	0.027 #
6)	B beta-BHC	4.415	4.844f	2116335	2714780	1.694	0.583 #
7)	B delta-BHC	0.000	5.058f	0	4722518	N.D.	0.517 #
15)	B Endosulfa...	0.000	6.893	0	1526097	N.D.	0.216 #
21)	B Endrin ke...	0.000	7.701	0	1709482	N.D.	0.203 #
24)	Chlordane-2	0.000	5.455f	0	245825	N.D.	0.829 #
27)	Chlordane-5	0.000	6.931f	0	164987	N.D.	0.605 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102921\
Data File : PD066616.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2021 17:40
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 02:04:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102821.M
Quant Title : GC Extractables
QLast Update : Thu Oct 28 02:17:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

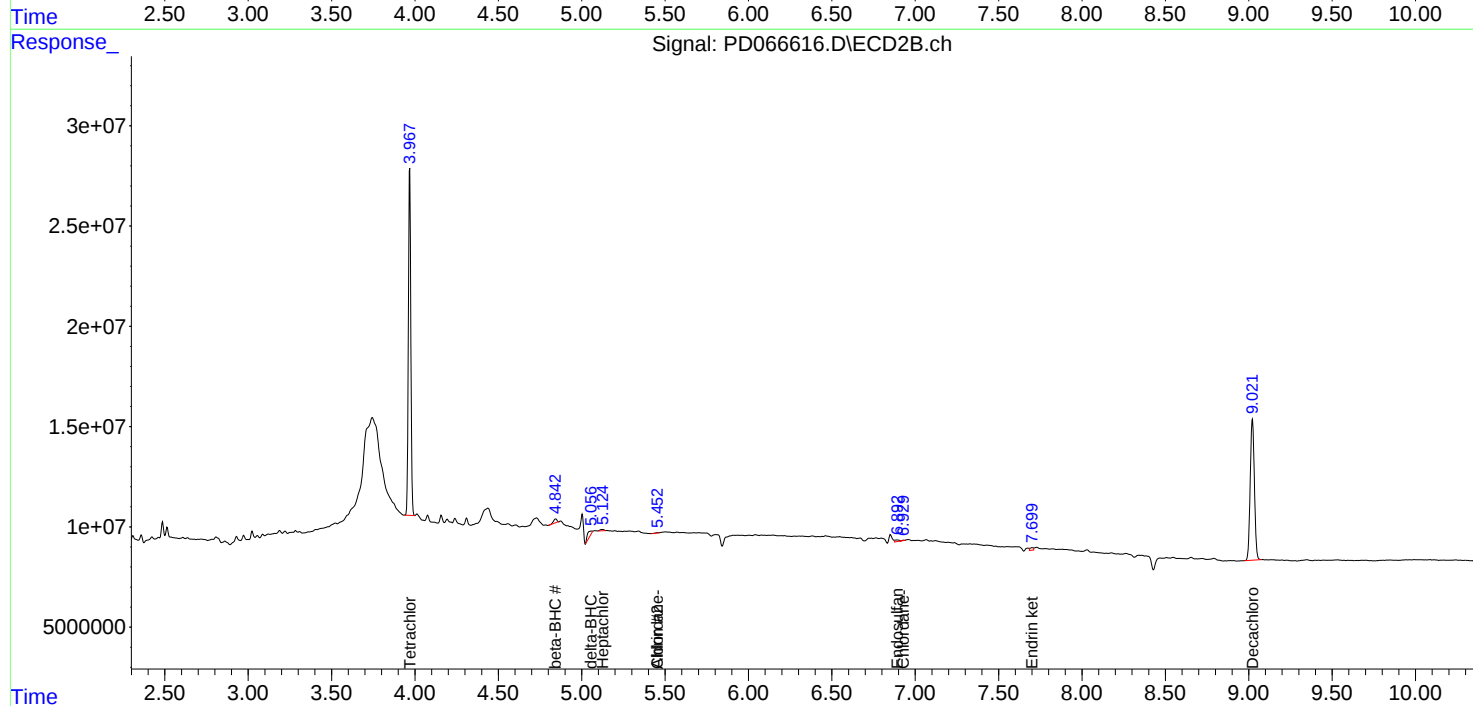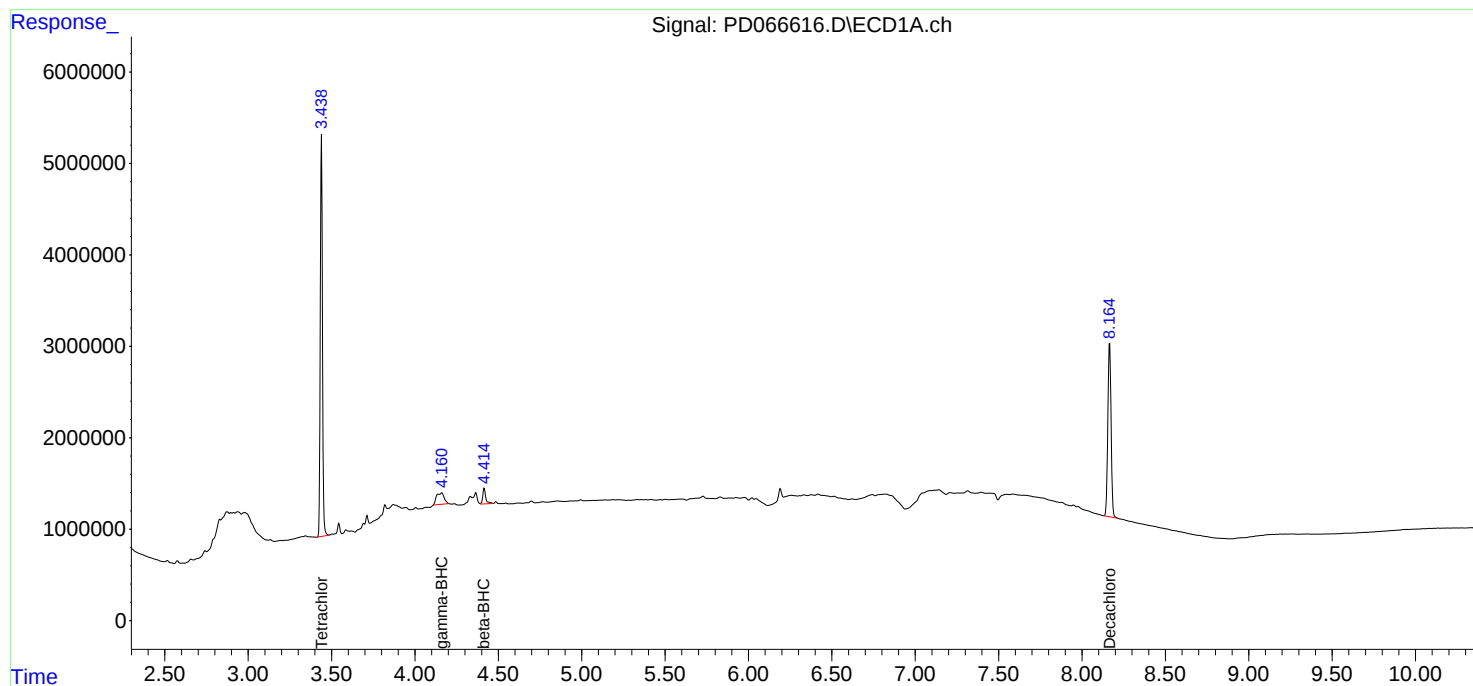


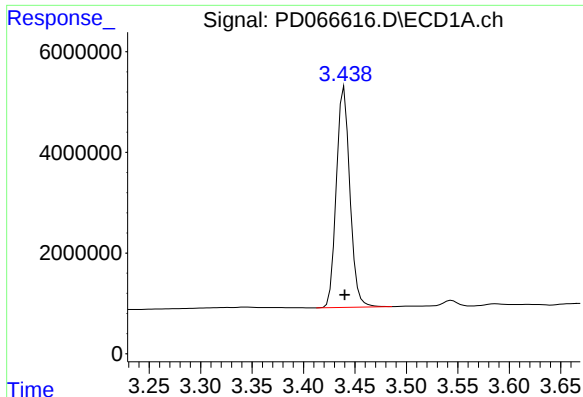

#1 Tetrachloro-m-xylene


R.T.: 3.440 min
Delta R.T.: 0.000 min
Response: 40124115
Conc: 21.50 ng/ml

Instrument :
ECD_D
ClientSampleId :

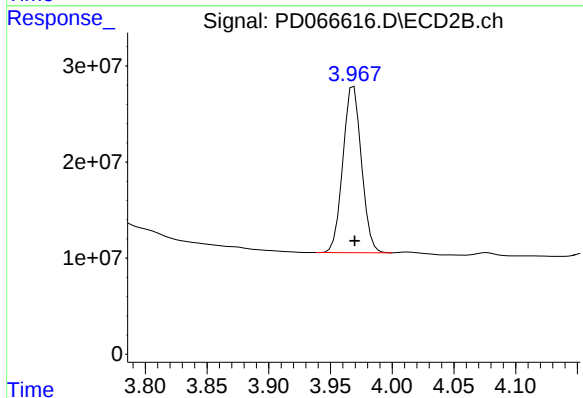


#1 Tetrachloro-m-xylene

R.T.: 3.969 min
Delta R.T.: -0.001 min
Response: 181035663
Conc: 22.37 ng/ml

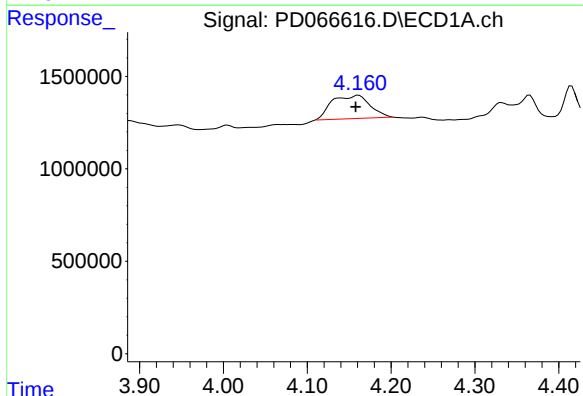


#3 gamma-BHC (Lindane)

R.T.: 4.161 min
Delta R.T.: 0.004 min
Response: 3970120
Conc: 1.31 ng/ml

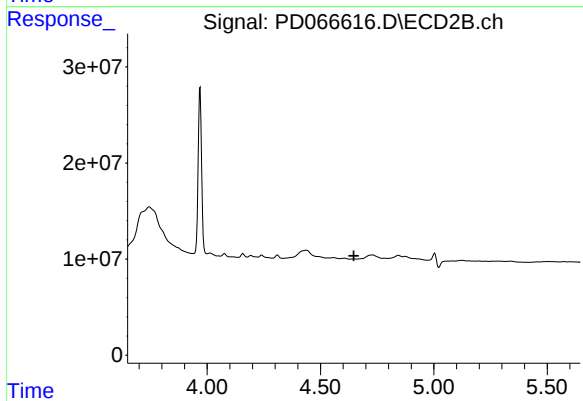

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.647 min
Response: 0
Conc: N.D.

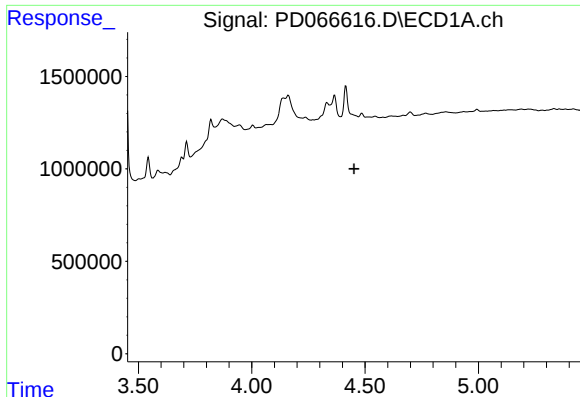

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.452 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

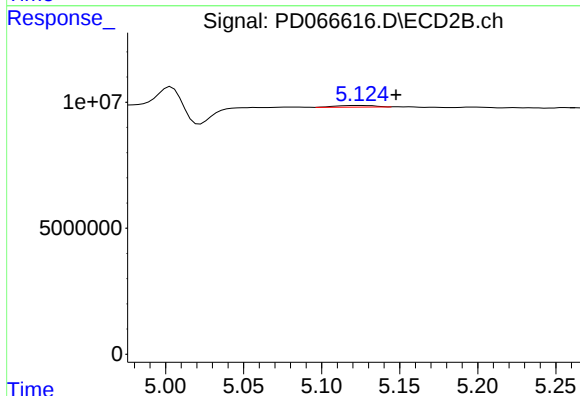


#4 Heptachlor

R.T.: 5.125 min
Delta R.T.: -0.023 min
Response: 1111723
Conc: 0.11 ng/ml

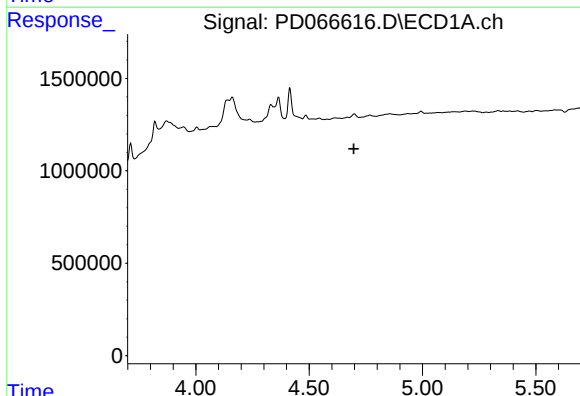


#5 Aldrin

R.T.: 0.000 min
Exp R.T.: 4.697 min
Response: 0
Conc: N.D.

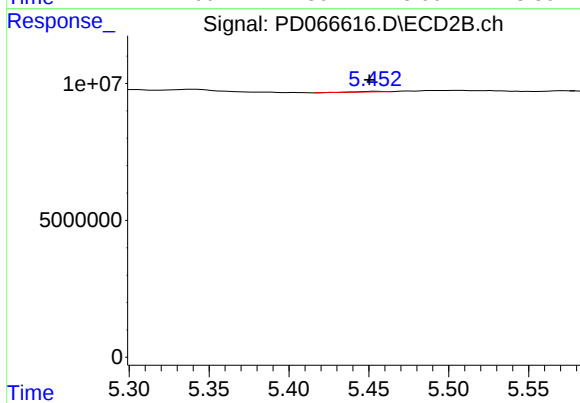

#5 Aldrin


R.T.: 5.455 min
Delta R.T.: 0.004 min
Response: 245825
Conc: 0.03 ng/ml

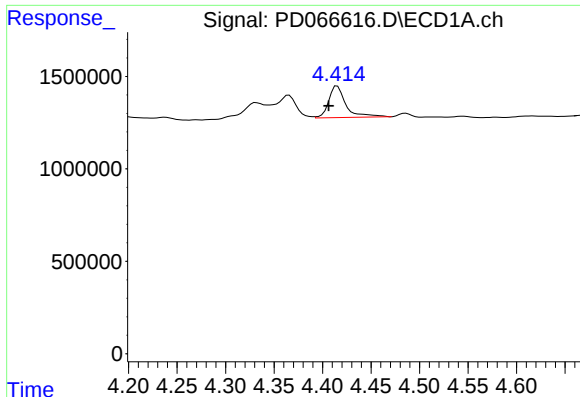

#6 beta-BHC


R.T.: 4.415 min
Delta R.T.: 0.009 min
Response: 2116335
Conc: 1.69 ng/ml

Instrument :
ECD_D
ClientSampleId :

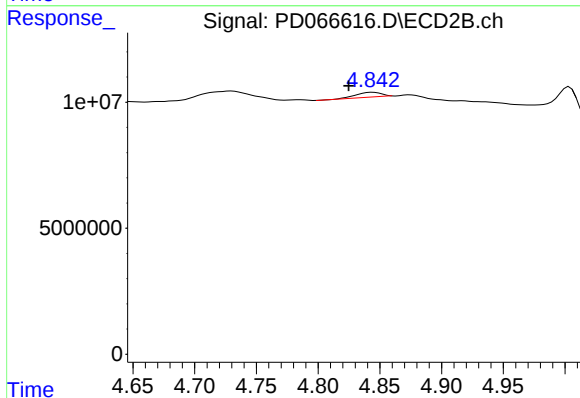


#6 beta-BHC

R.T.: 4.844 min
Delta R.T.: 0.020 min
Response: 2714780
Conc: 0.58 ng/ml

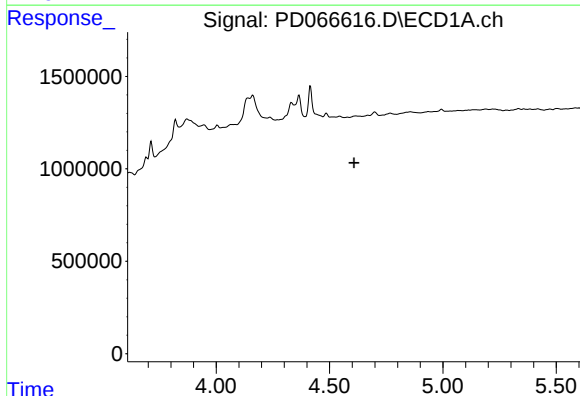


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.608 min
Response: 0
Conc: N.D.

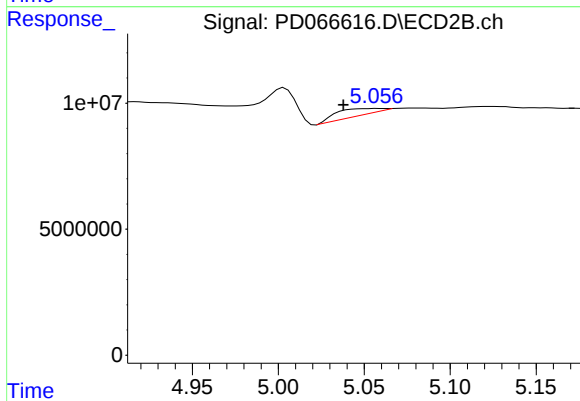

#7 delta-BHC


R.T.: 5.058 min
Delta R.T.: 0.020 min
Response: 4722518
Conc: 0.52 ng/ml

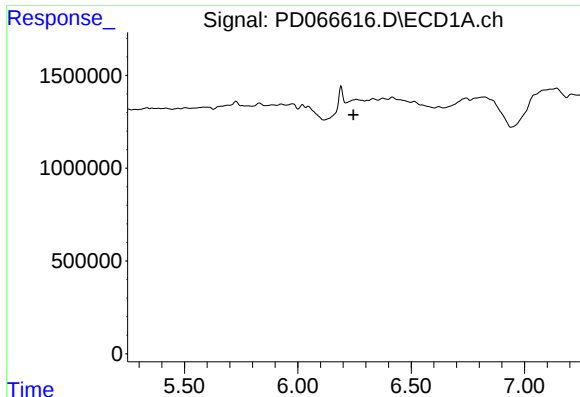

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.246 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

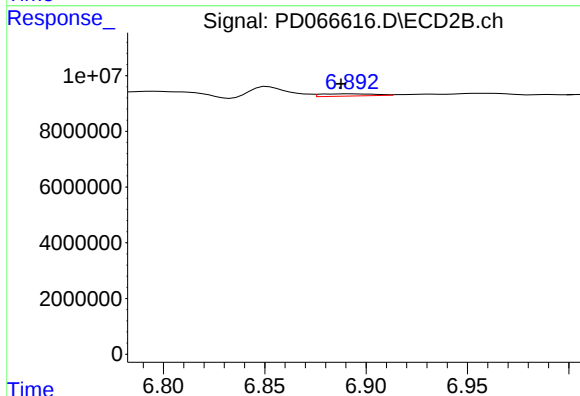


#15 Endosulfan II

R.T.: 6.893 min
Delta R.T.: 0.005 min
Response: 1526097
Conc: 0.22 ng/ml

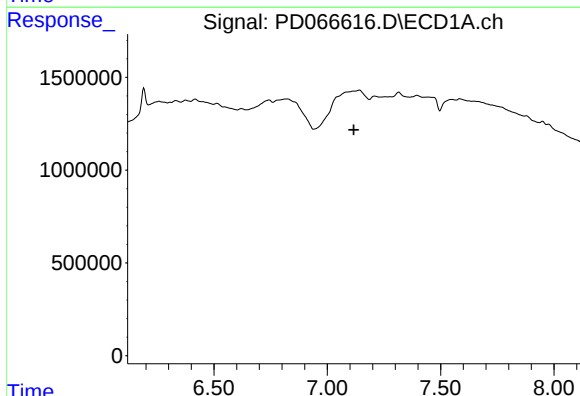


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 7.118 min
Response: 0
Conc: N.D.

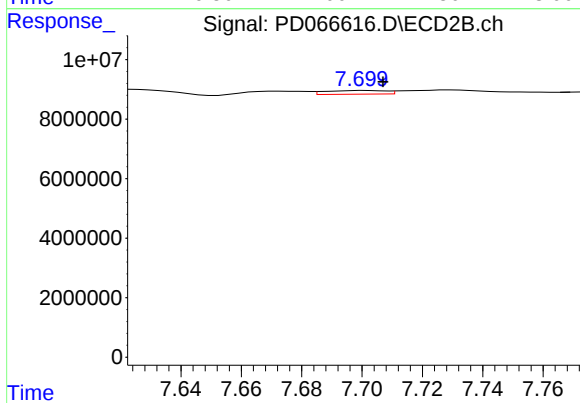

#21 Endrin ketone


R.T.: 7.701 min
Delta R.T.: -0.006 min
Response: 1709482
Conc: 0.20 ng/ml

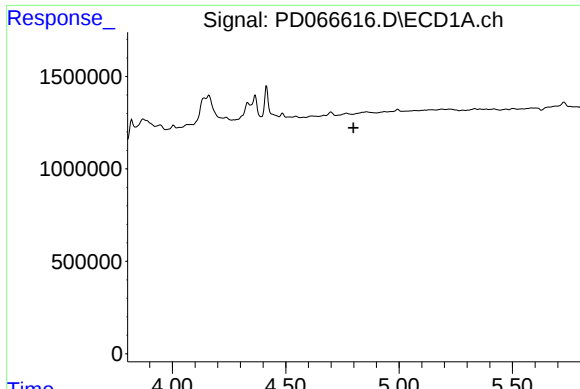

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.799 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

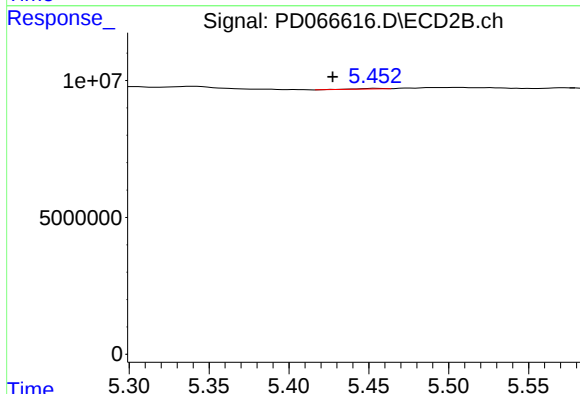


#24 Chlordane-2

R.T.: 5.455 min
Delta R.T.: 0.027 min
Response: 245825
Conc: 0.83 ng/ml

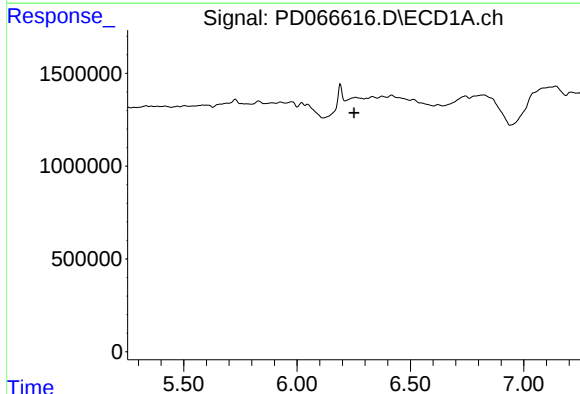


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.252 min
Response: 0
Conc: N.D.

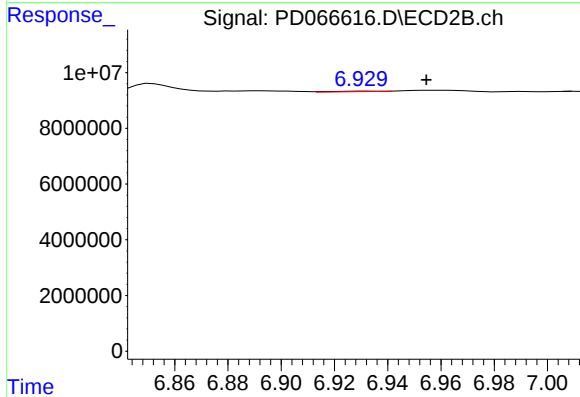

#27 Chlordane-5


R.T.: 6.931 min
Delta R.T.: -0.023 min
Response: 164987
Conc: 0.61 ng/ml

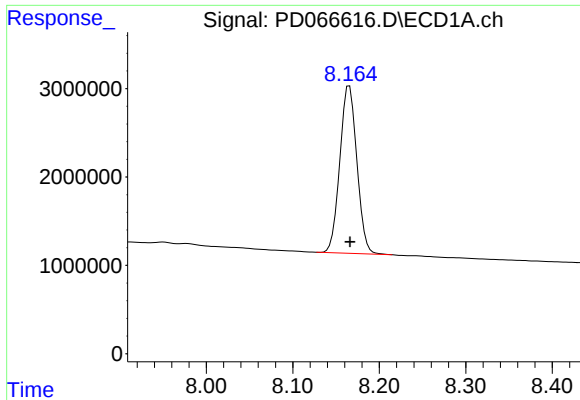

#28 Decachlorobiphenyl

R.T.: 8.165 min
Delta R.T.: -0.001 min
Response: 25749273
Conc: 22.29 ng/ml

Instrument :
ECD_D
ClientSampleId :

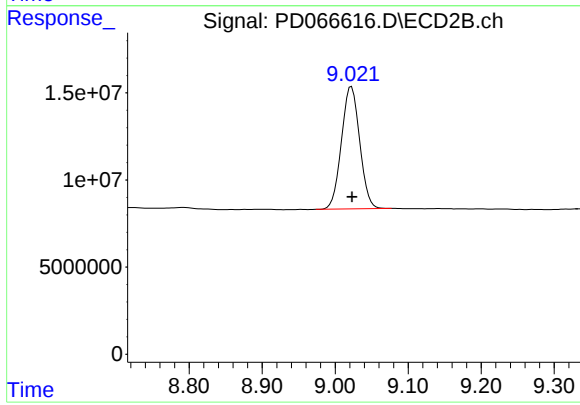

#28 Decachlorobiphenyl

R.T.: 9.022 min
Delta R.T.: 0.000 min
Response: 121862709
Conc: 22.62 ng/ml