

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102925\
 Data File : PD090917.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Oct 2025 13:20
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA4006

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 29 14:48:52 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102925CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 29 14:43:19 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.543	2.874	108.3E6	1109.1E6	39.755	39.849
27)	SA Decachlor...	9.062	8.059	326.5E6	2652.6E6	79.577	79.563
Target Compounds							
2)	A alpha-BHC	3.993	3.385	250.6E6	1881.3E6	39.890	39.775
3)	MA gamma-BHC...	4.323	3.721	236.3E6	1723.7E6	39.911	39.819
4)	MA Heptachlor	4.921	4.073	230.3E6	1736.7E6	39.783	39.885
9)	A Endosulfan I	6.066	5.237	189.8E6	1436.3E6	39.741	39.859
13)	MA Dieldrin	6.339	5.502	422.2E6	3176.8E6	79.790	79.945
14)	MA Endrin	6.566	5.779	354.2E6	2867.9E6	79.773	79.834
16)	A 4,4'-DDD	6.698	5.919	288.7E6	2593.7E6	79.686	80.064
17)	MA 4,4'-DDT	7.014	6.172	302.0E6	2753.1E6	79.735	79.905
20)	A Methoxychlor	7.487	6.742	775.4E6	5649.7E6	399.899	403.455

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102925\
Data File : PD090917.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Oct 2025 13:20
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 14:48:52 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102925CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 29 14:43:19 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

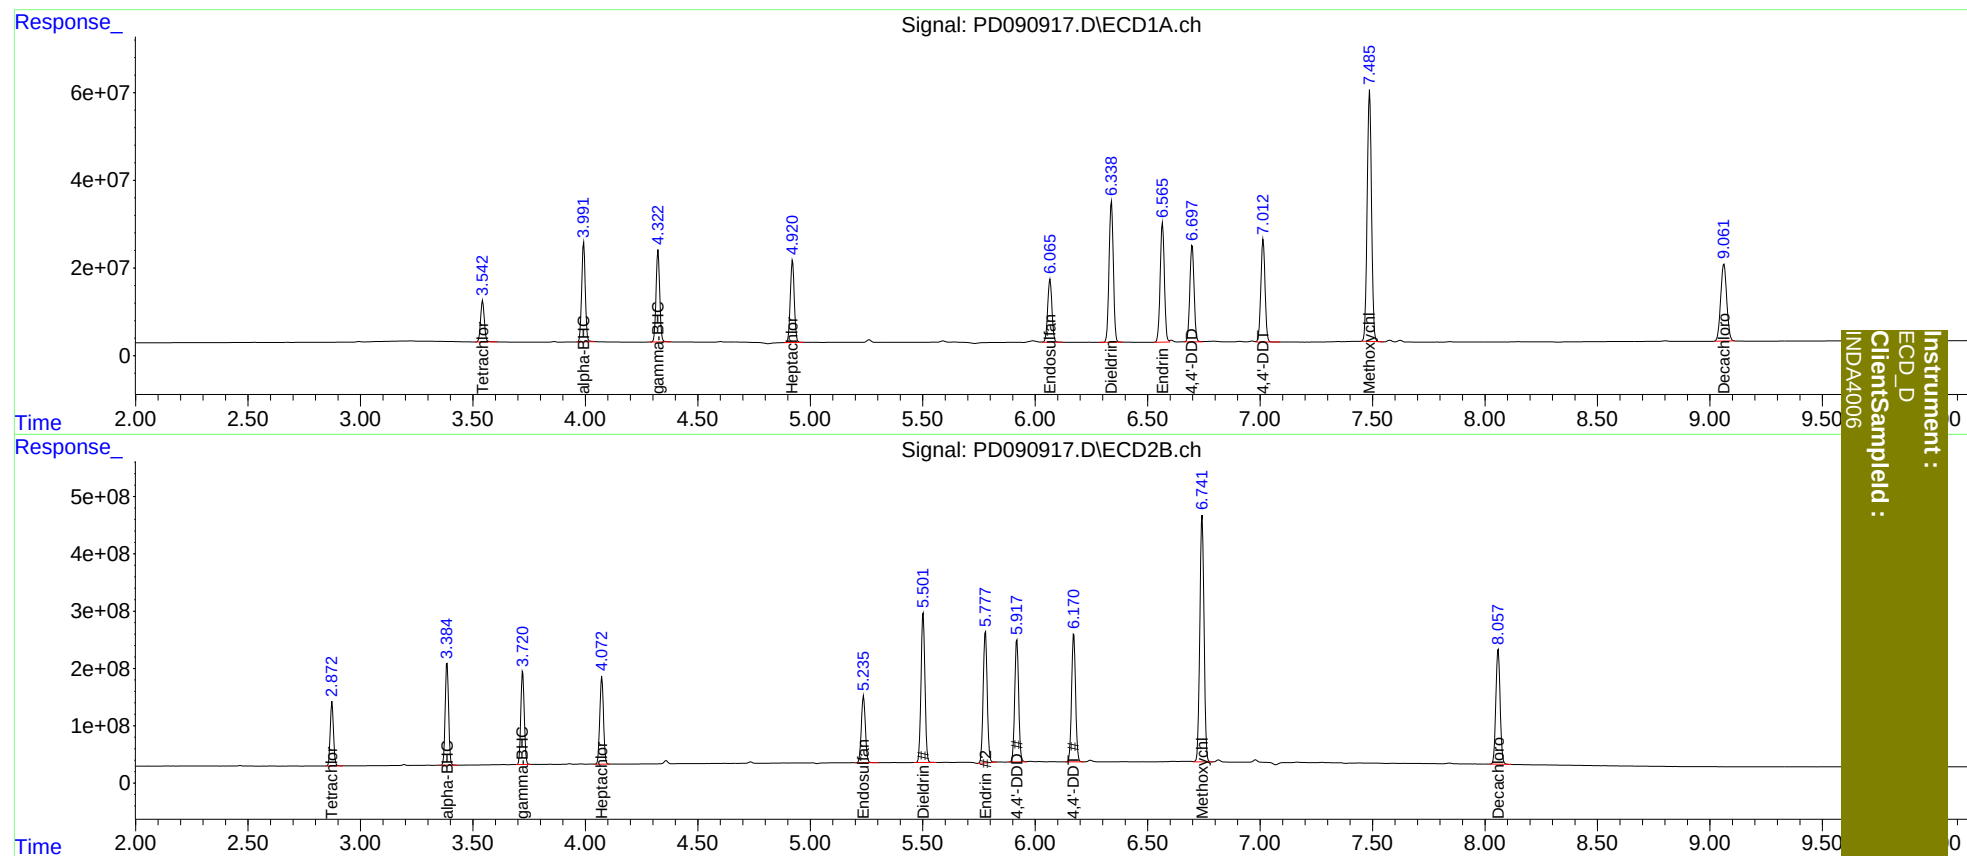

Instrument :
ECD_D
ClientSampled :
INDA4006