

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD103018\
 Data File : PD050115.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Oct 2018 9:06
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 09:46:16 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD103018.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 30 03:08:01 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.232	4.059	14091074	661.2E6	22.477	23.741
28)	SA Decachlor...	9.017	9.169	13317841	403.4E6	22.155	23.469
Target Compounds							
2)	A alpha-BHC	0.000	4.489f	0	9668969	N.D.	0.221 #
3)	MA gamma-BHC...	0.000	4.807f	0	4060178	N.D.	0.104 #
4)	MA Heptachlor	0.000	5.266	0	3229397	N.D.	0.086 #
6)	B beta-BHC	0.000	4.905	0	1266839	N.D.	0.079 #
8)	B Heptachlo...	0.000	6.003f	0	3247786	N.D.	0.102 #
9)	A Endosulfan I	6.339	0.000	68571	0	0.092	N.D. #
10)	B gamma-Chl...	6.218	0.000	452718	0	0.548	N.D. #
11)	B alpha-Chl...	6.266	0.000	888302	0	1.084	N.D. #
17)	MA 4,4'-DDT	0.000	7.253f	0	3308412	N.D.	0.179 #
24)	Chlordane-2	0.000	5.466	0	1078532	N.D.	0.877 #
25)	Chlordane-3	6.218	0.000	452718	0	5.158	N.D. #
26)	Chlordane-4	6.266	0.000	888302	0	12.261	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD103018\
Data File : PD050115.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Oct 2018 9:06
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 09:46:16 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD103018.M
Quant Title : GC Extractables
QLast Update : Tue Oct 30 03:08:01 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

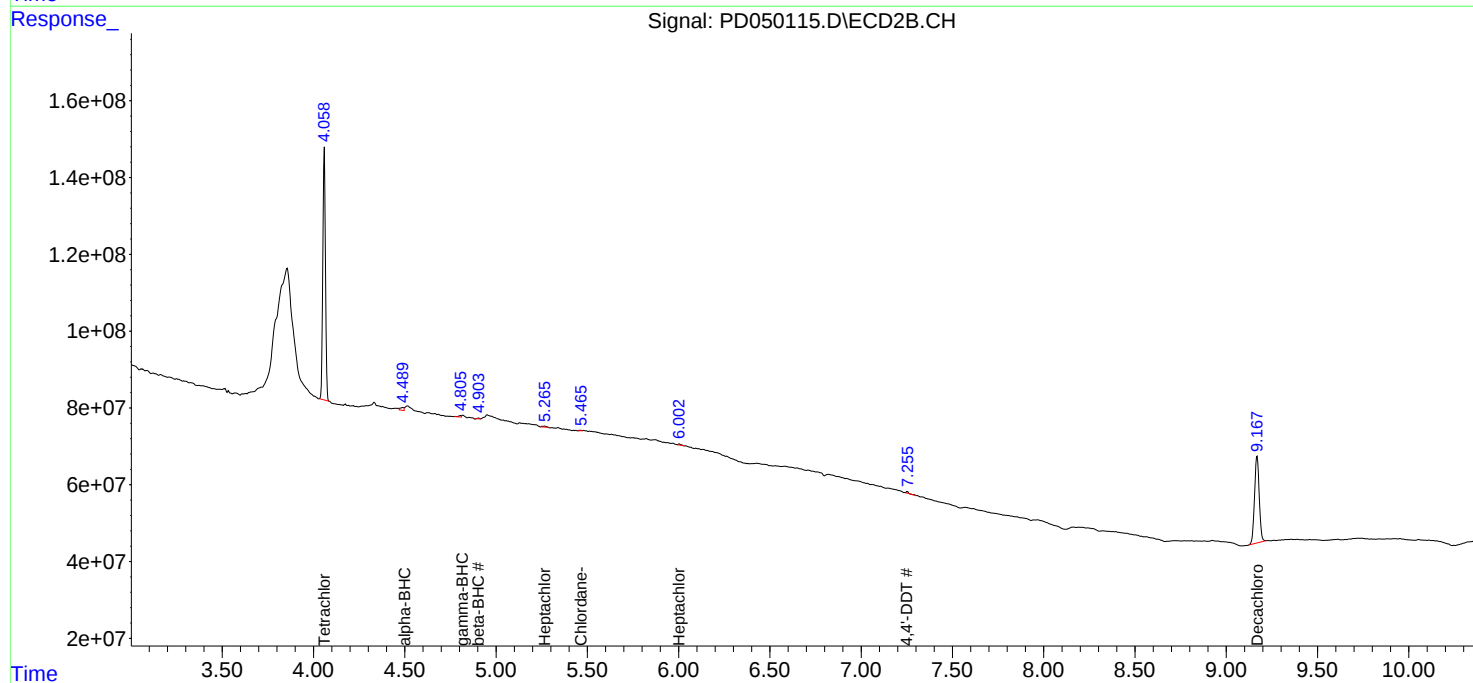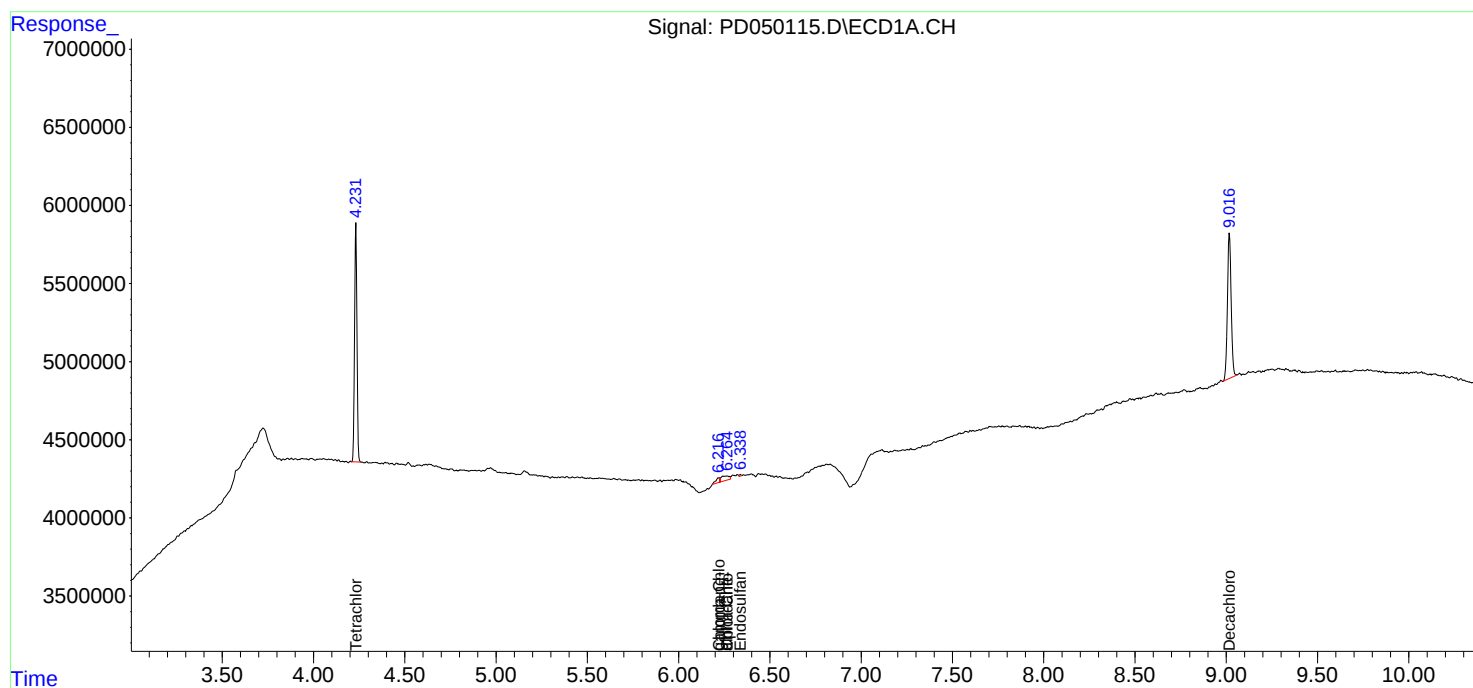


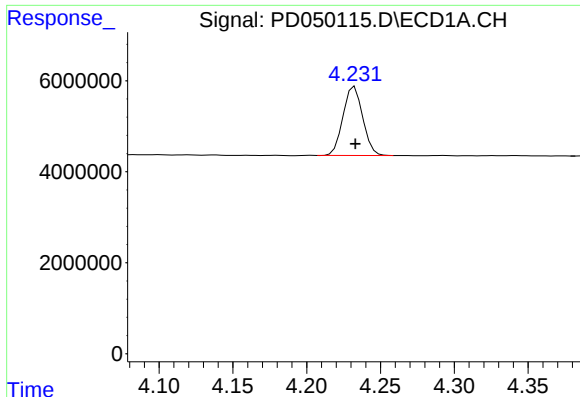

#1 Tetrachloro-m-xylene


R.T.: 4.232 min
Delta R.T.: 0.000 min
Response: 14091074
Conc: 22.48 ng/ml

Instrument :
ECD_D
ClientSampleId :

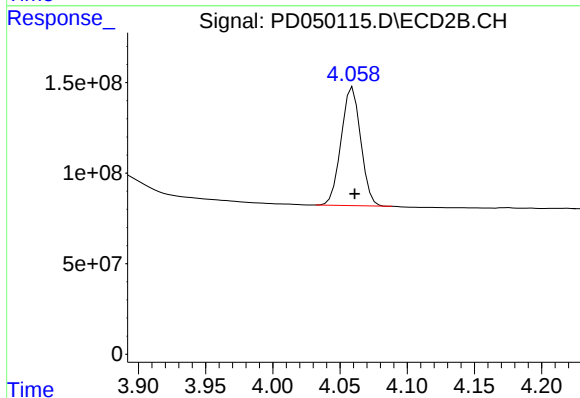


#1 Tetrachloro-m-xylene

R.T.: 4.059 min
Delta R.T.: -0.001 min
Response: 661189067
Conc: 23.74 ng/ml

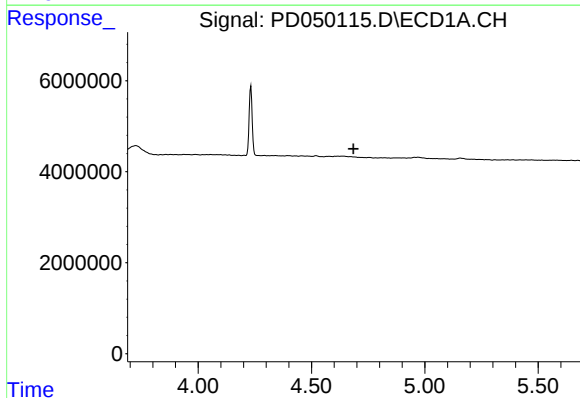


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 4.686 min
Response: 0
Conc: N.D.

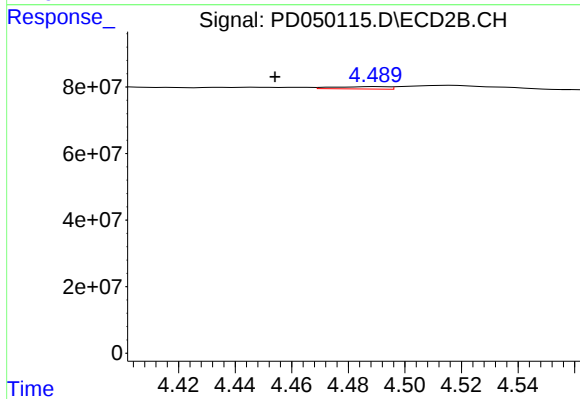

#2 alpha-BHC


R.T.: 4.489 min
Delta R.T.: 0.035 min
Response: 9668969
Conc: 0.22 ng/ml

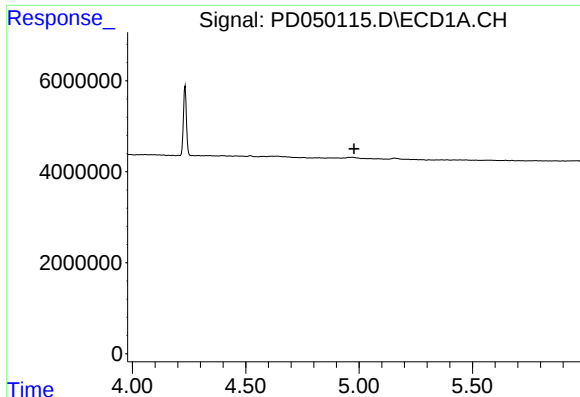

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.978 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

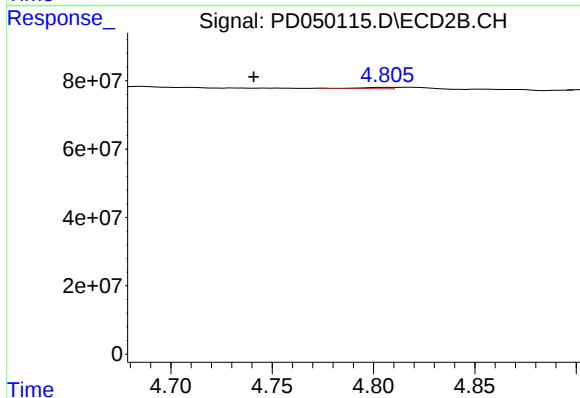


#3 gamma-BHC (Lindane)

R.T.: 4.807 min
Delta R.T.: 0.066 min
Response: 4060178
Conc: 0.10 ng/ml

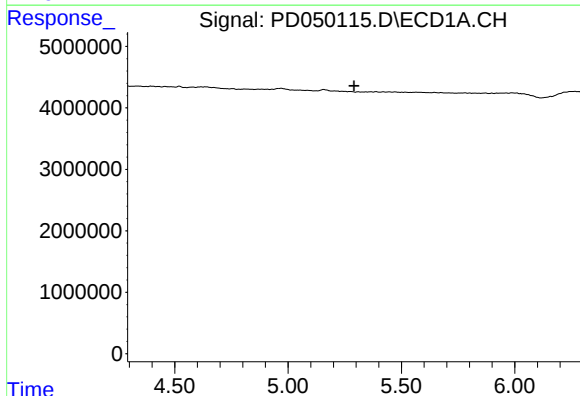


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 5.291 min
Response: 0
Conc: N.D.

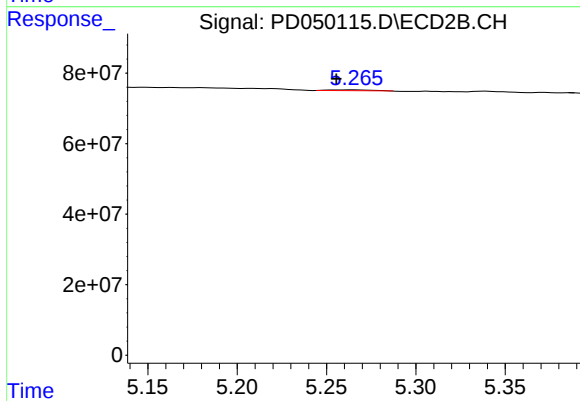

#4 Heptachlor


R.T.: 5.266 min
Delta R.T.: 0.010 min
Response: 3229397
Conc: 0.09 ng/ml

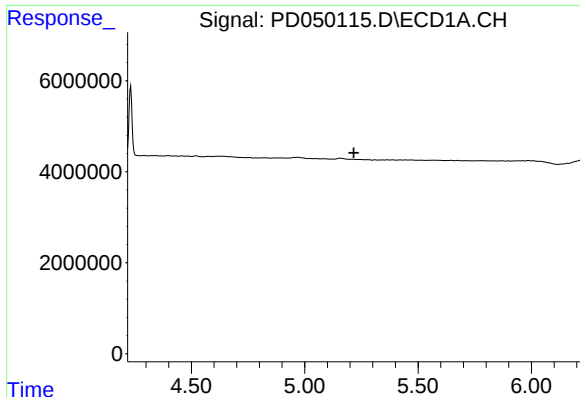

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 5.217 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

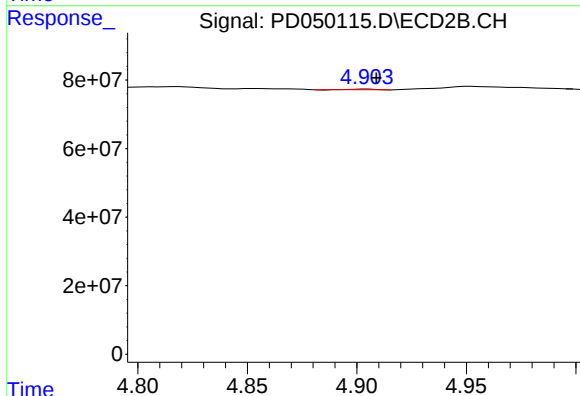


#6 beta-BHC

R.T.: 4.905 min
Delta R.T.: -0.004 min
Response: 1266839
Conc: 0.08 ng/ml

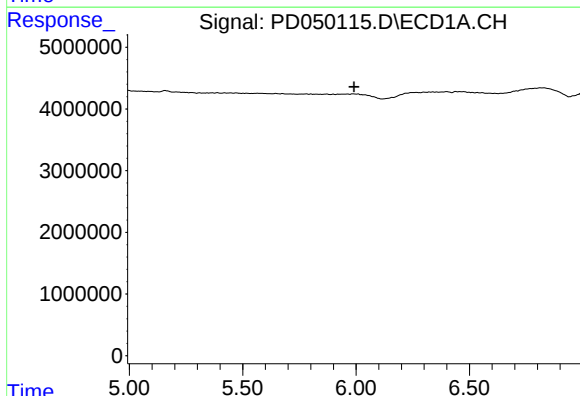


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.991 min
Response: 0
Conc: N.D.

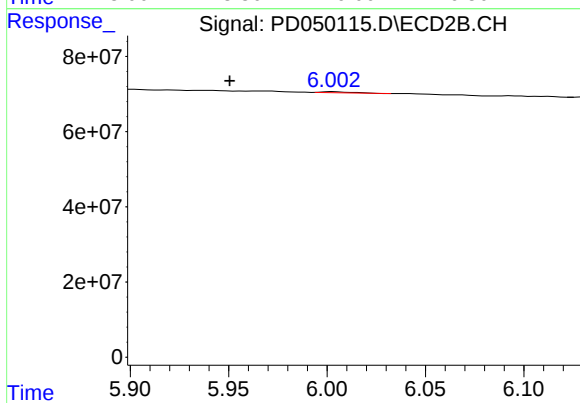

#8 Heptachlor epoxide


R.T.: 6.003 min
Delta R.T.: 0.053 min
Response: 3247786
Conc: 0.10 ng/ml

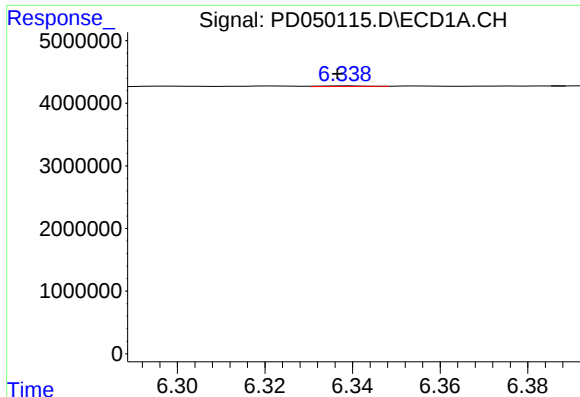

#9 Endosulfan I


R.T.: 6.339 min
Delta R.T.: 0.002 min
Response: 68571
Conc: 0.09 ng/ml

Instrument :
ECD_D
ClientSampleId :

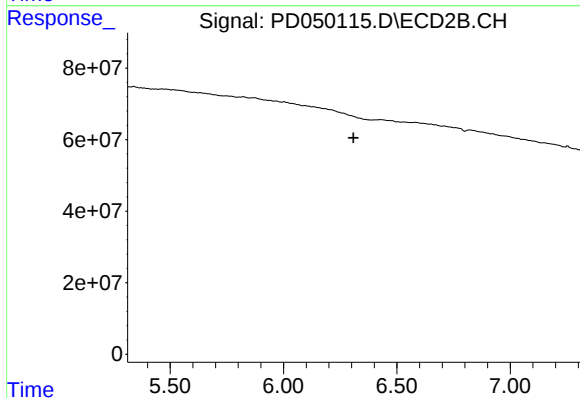


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.309 min
Response: 0
Conc: N.D.

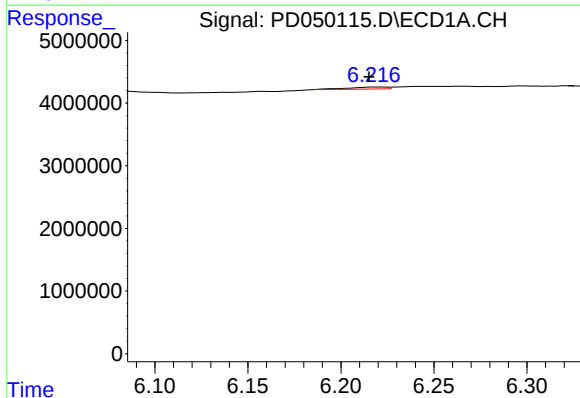


#10 gamma-Chlordane

R.T.: 6.218 min
Delta R.T.: 0.003 min
Response: 452718
Conc: 0.55 ng/ml

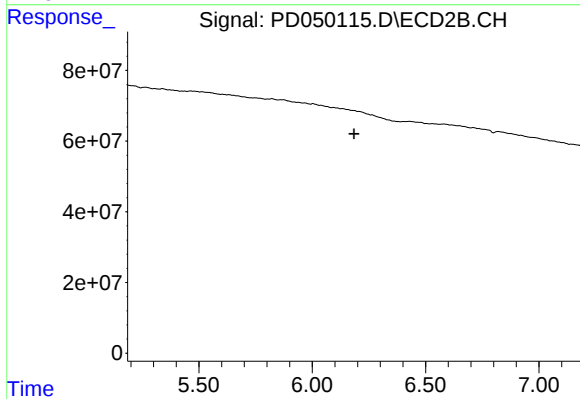

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.185 min
Response: 0
Conc: N.D.

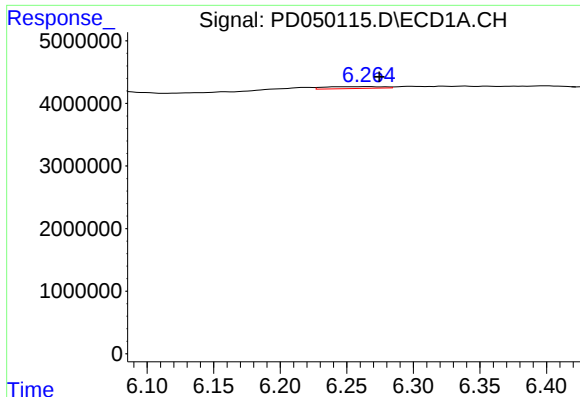

#11 alpha-Chlordane


R.T.: 6.266 min
Delta R.T.: -0.008 min
Response: 888302
Conc: 1.08 ng/ml

Instrument :
ECD_D
ClientSampleId :

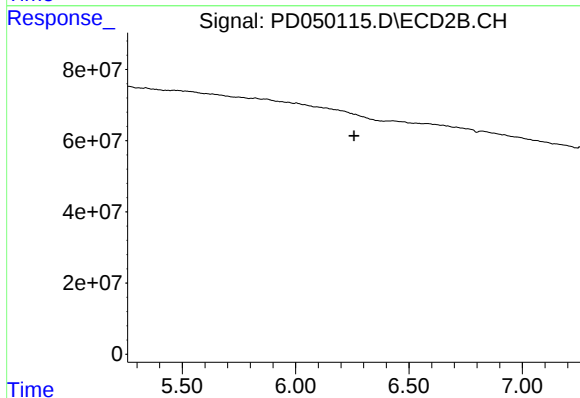


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.258 min
Response: 0
Conc: N.D.

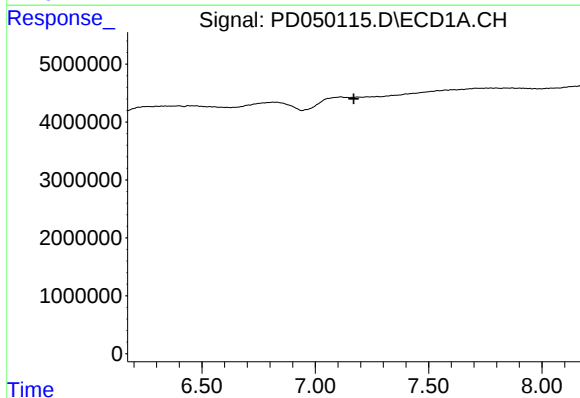


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.170 min
Response: 0
Conc: N.D.

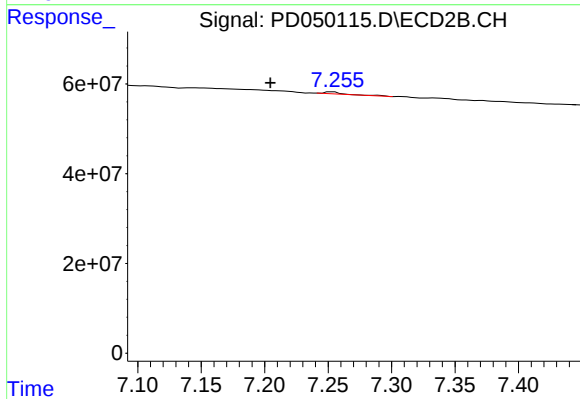

#17 4,4'-DDT


R.T.: 7.253 min
Delta R.T.: 0.049 min
Response: 3308412
Conc: 0.18 ng/ml

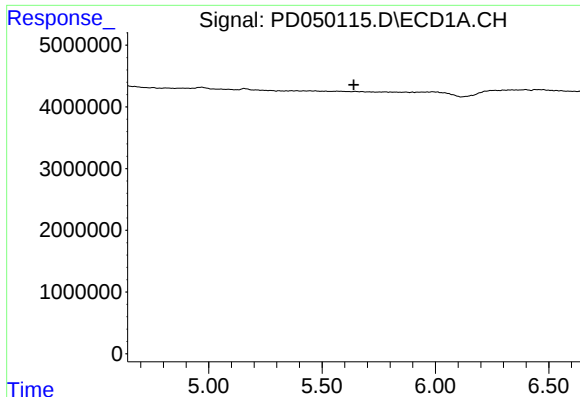

#24 Chlorine-2


R.T.: 0.000 min
Exp R.T.: 5.640 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

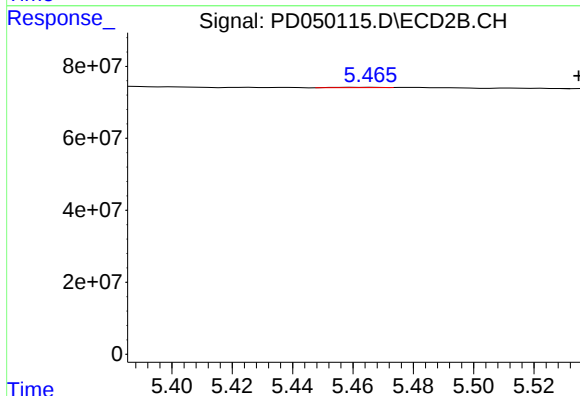


#24 Chlorine-2

R.T.: 5.466 min
Delta R.T.: -0.069 min
Response: 1078532
Conc: 0.88 ng/ml

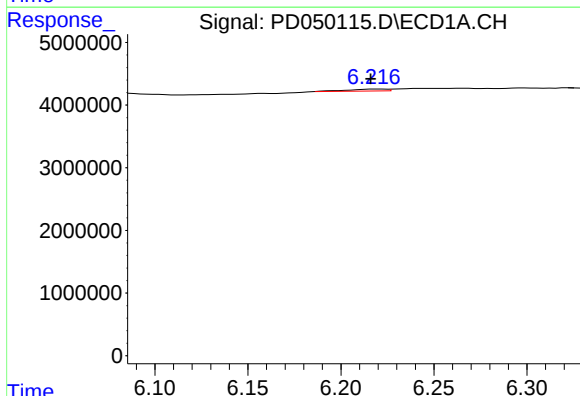


#25 Chlorine-3

R.T.: 6.218 min
Delta R.T.: 0.002 min
Response: 452718
Conc: 5.16 ng/ml

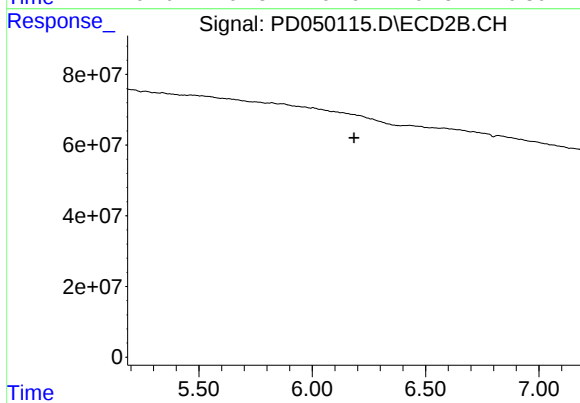

#25 Chlorine-3


R.T.: 0.000 min
Exp R.T.: 6.185 min
Response: 0
Conc: N.D.

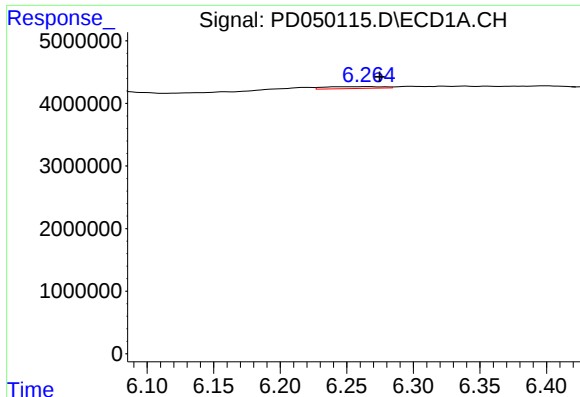

#26 Chlordane-4


R.T.: 6.266 min
Delta R.T.: -0.009 min
Response: 888302
Conc: 12.26 ng/ml

Instrument :
ECD_D
ClientSampleId :

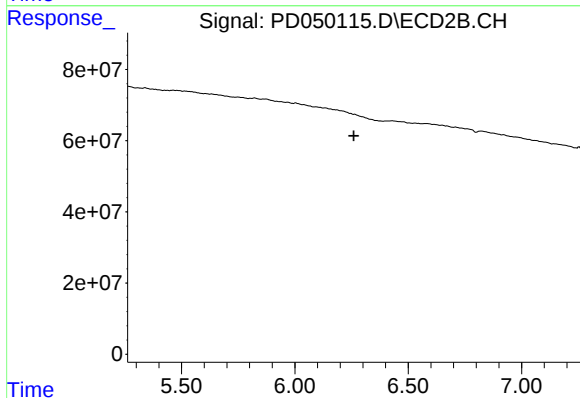


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 6.260 min
Response: 0
Conc: N.D.

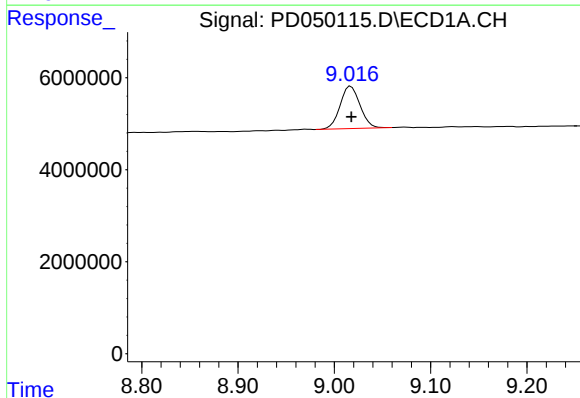

#28 Decachlorobiphenyl

R.T.: 9.017 min
Delta R.T.: 0.000 min
Response: 13317841
Conc: 22.16 ng/ml

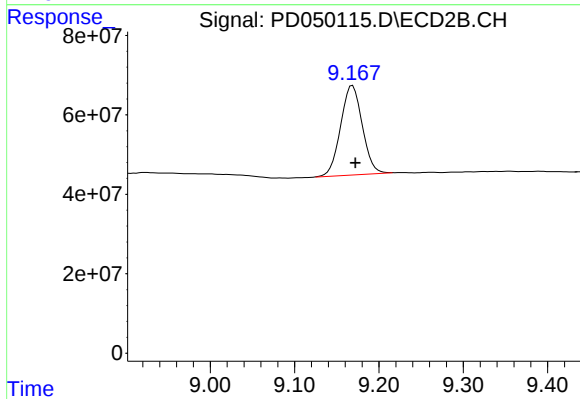

#28 Decachlorobiphenyl

R.T.: 9.169 min
Delta R.T.: -0.003 min
Response: 403395638
Conc: 23.47 ng/ml