

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD103021\
 Data File : PD066622.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Oct 2021 08:52
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 04:49:07 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102821.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 28 02:17:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.440	3.968	40613805	191.3E6	21.767	23.638
28)	SA Decachlor...	8.167	9.023	25768831	123.2E6	22.303	22.864
Target Compounds							
4)	MA Heptachlor	0.000	5.158	0	1087310	N.D.	0.111 #
5)	MB Aldrin	0.000	5.448	0	227137	N.D.	0.025 #
6)	B beta-BHC	4.416	4.843f	1677031	2247473	1.343	0.483 #
7)	B delta-BHC	0.000	5.060f	0	5609084	N.D.	0.614 #
15)	B Endosulfa...	0.000	6.895	0	996228	N.D.	0.141 #
21)	B Endrin ke...	0.000	7.706	0	5764108	N.D.	0.685 #
22)	Mirex	0.000	8.183f	0	2961602	N.D.	0.501 #
24)	Chlordane-2	0.000	5.448f	0	227137	N.D.	0.766 #
27)	Chlordane-5	0.000	6.931f	0	470416	N.D.	1.726 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD103021\
Data File : PD066622.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Oct 2021 08:52
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 04:49:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102821.M
Quant Title : GC Extractables
QLast Update : Thu Oct 28 02:17:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

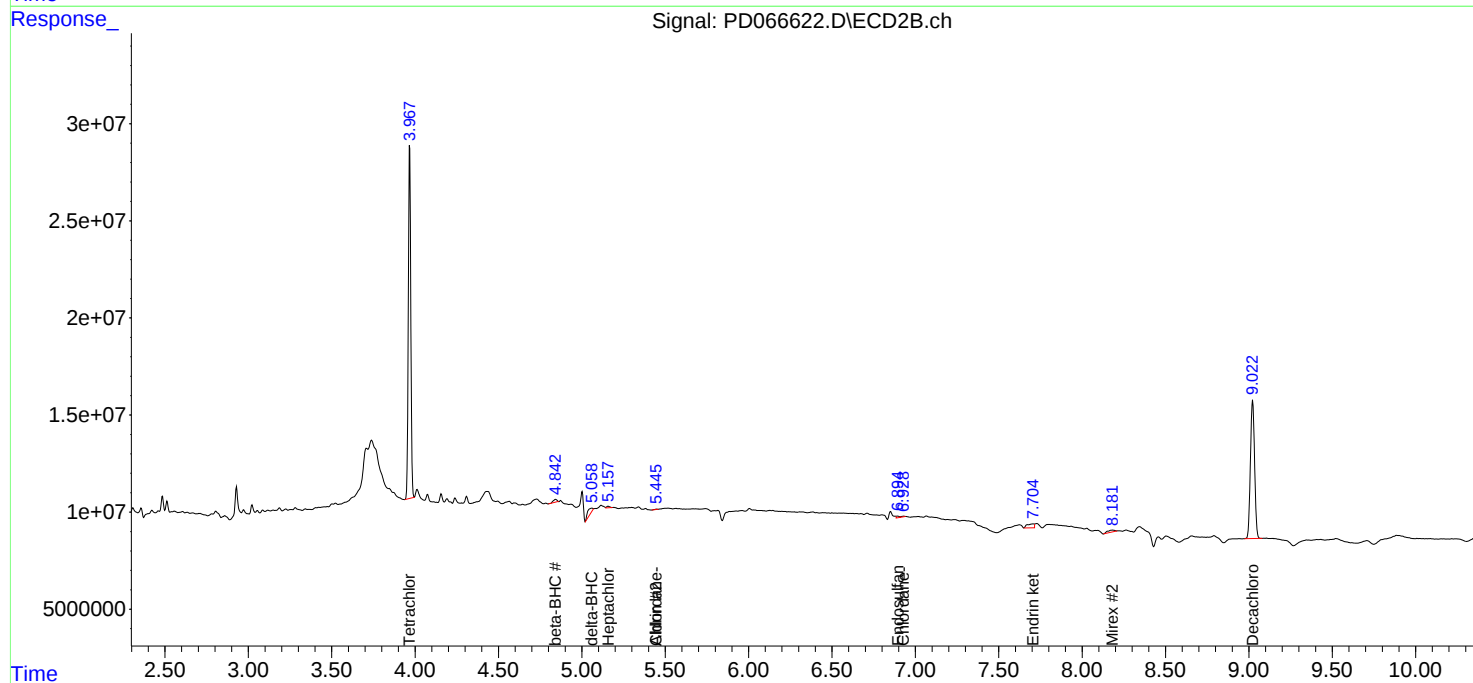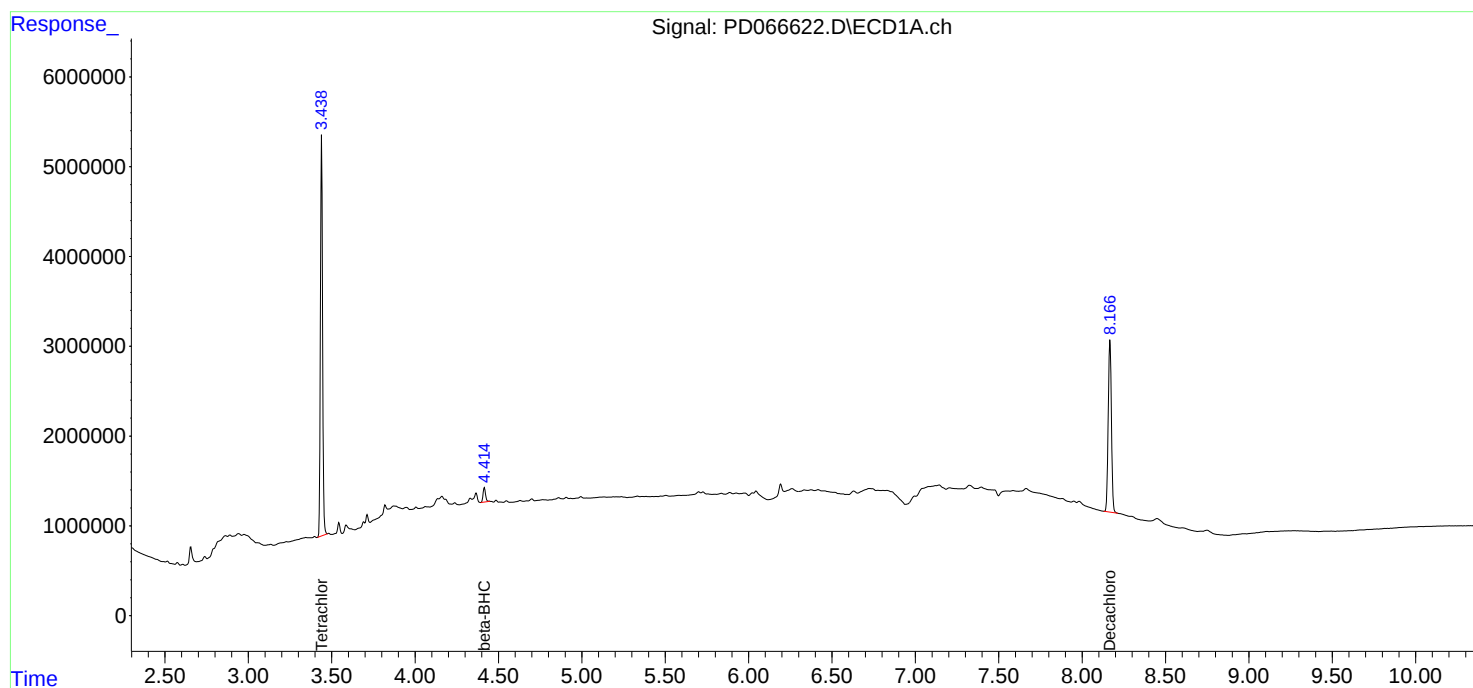


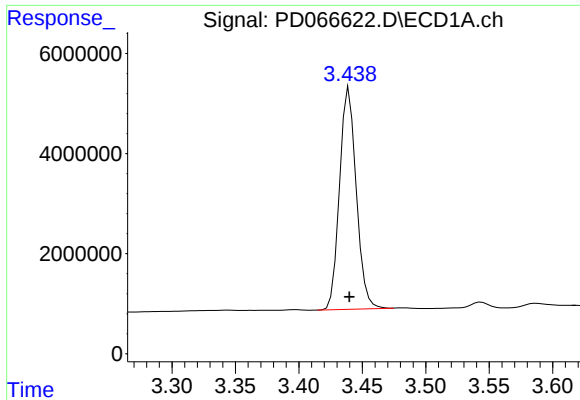

#1 Tetrachloro-m-xylene


R.T.: 3.440 min
Delta R.T.: 0.000 min
Response: 40613805
Conc: 21.77 ng/ml

Instrument :
ECD_D
ClientSampleId :

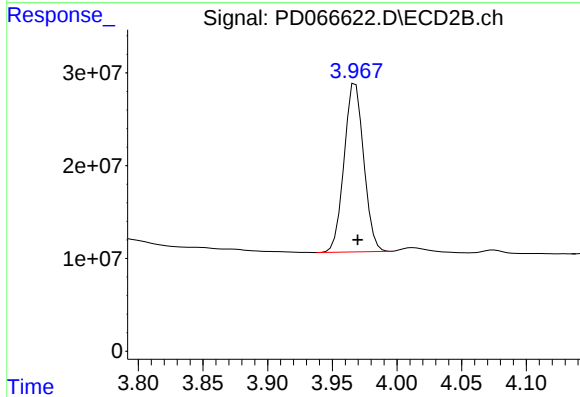


#1 Tetrachloro-m-xylene

R.T.: 3.968 min
Delta R.T.: -0.002 min
Response: 191281137
Conc: 23.64 ng/ml

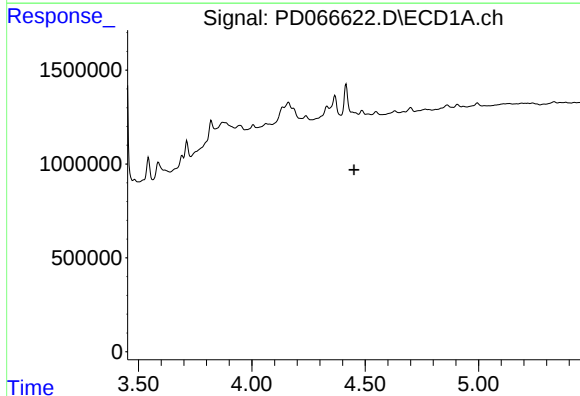


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.452 min
Response: 0
Conc: N.D.

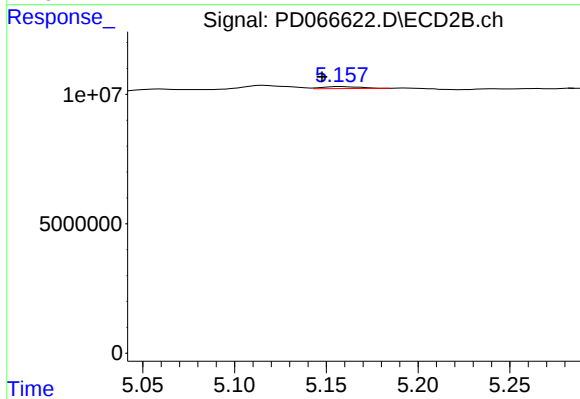

#4 Heptachlor


R.T.: 5.158 min
Delta R.T.: 0.011 min
Response: 1087310
Conc: 0.11 ng/ml

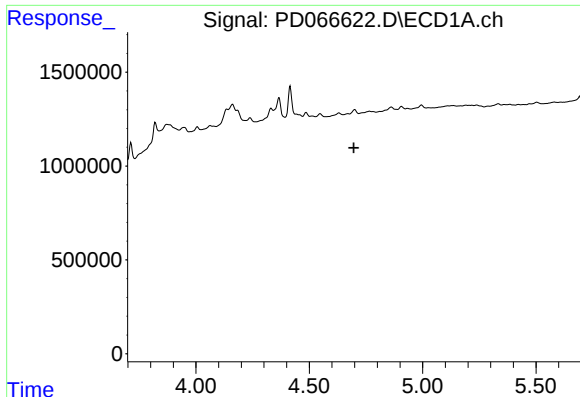

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 4.697 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

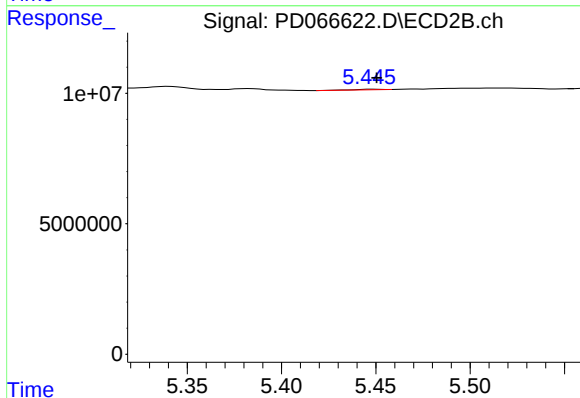


#5 Aldrin

R.T.: 5.448 min
Delta R.T.: -0.002 min
Response: 227137
Conc: 0.03 ng/ml

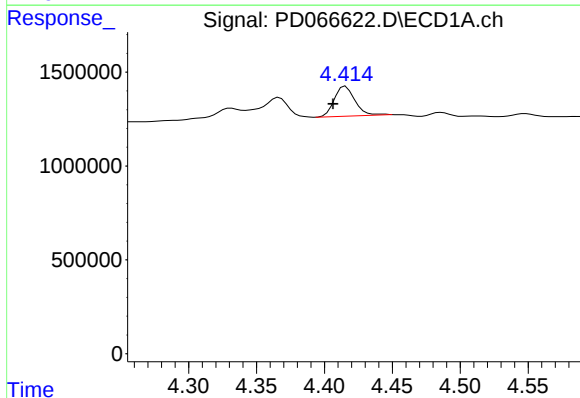


#6 beta-BHC

R.T.: 4.416 min
Delta R.T.: 0.009 min
Response: 1677031
Conc: 1.34 ng/ml

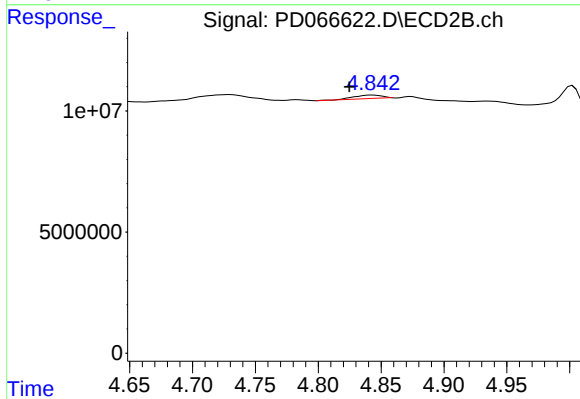

#6 beta-BHC


R.T.: 4.843 min
Delta R.T.: 0.019 min
Response: 2247473
Conc: 0.48 ng/ml

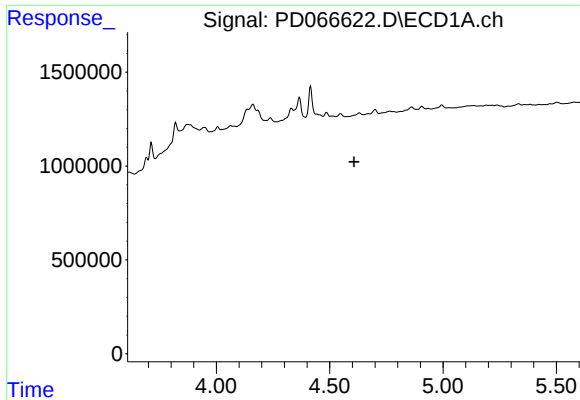

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.608 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

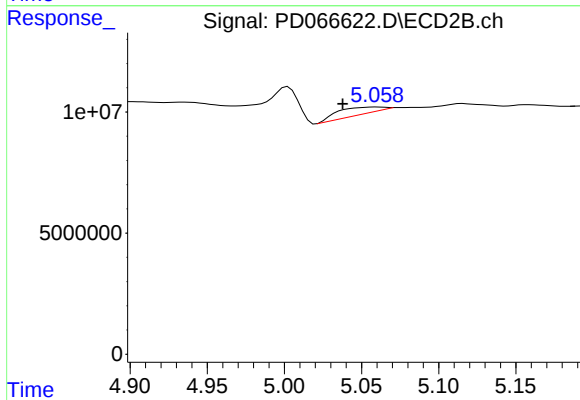


#7 delta-BHC

R.T.: 5.060 min
Delta R.T.: 0.022 min
Response: 5609084
Conc: 0.61 ng/ml

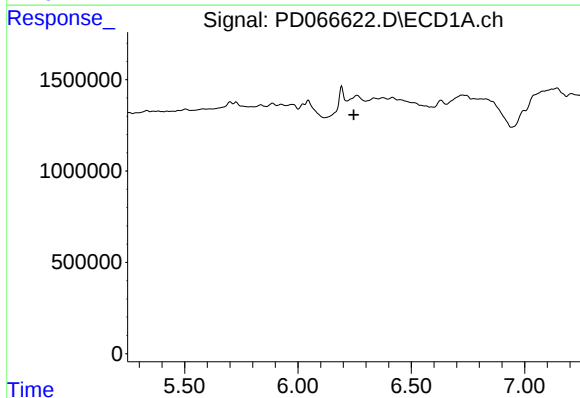


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.246 min
Response: 0
Conc: N.D.

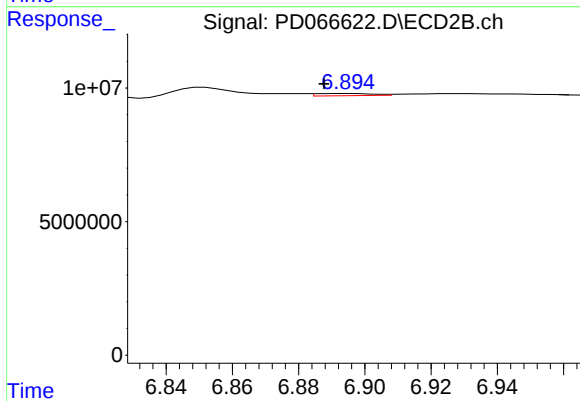

#15 Endosulfan II


R.T.: 6.895 min
Delta R.T.: 0.008 min
Response: 996228
Conc: 0.14 ng/ml

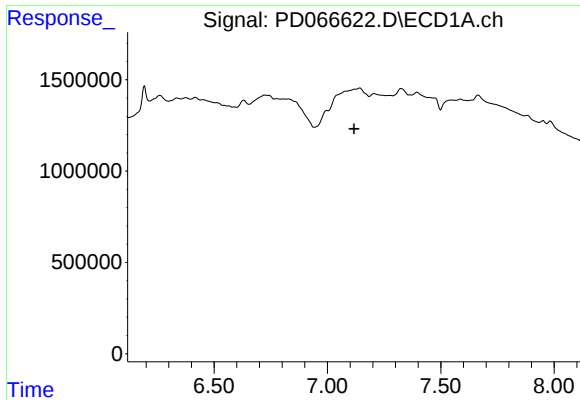

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.118 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

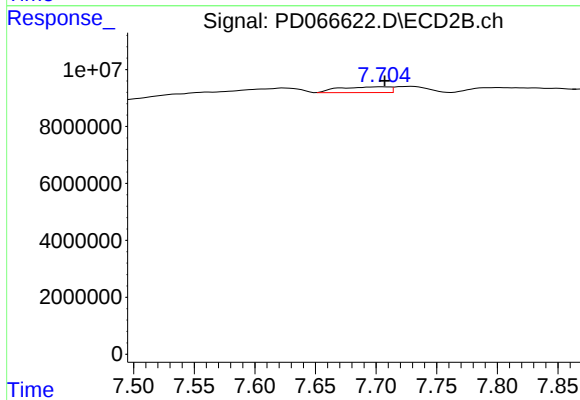


#21 Endrin ketone

R.T.: 7.706 min
Delta R.T.: -0.001 min
Response: 5764108
Conc: 0.69 ng/ml

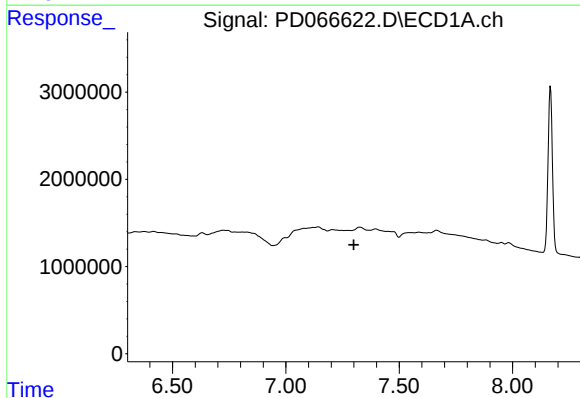


#22 Mirex

R.T.: 0.000 min
Exp R.T.: 7.299 min
Response: 0
Conc: N.D.

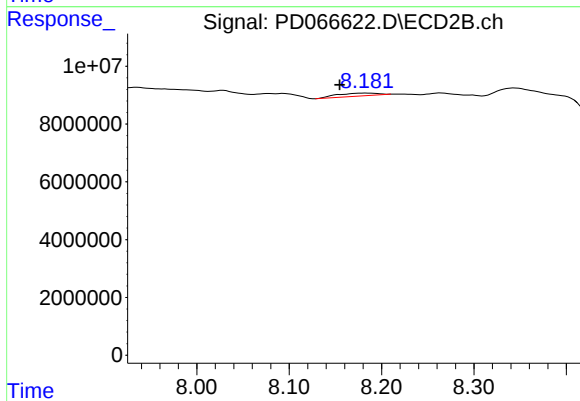

#22 Mirex


R.T.: 8.183 min
Delta R.T.: 0.028 min
Response: 2961602
Conc: 0.50 ng/ml

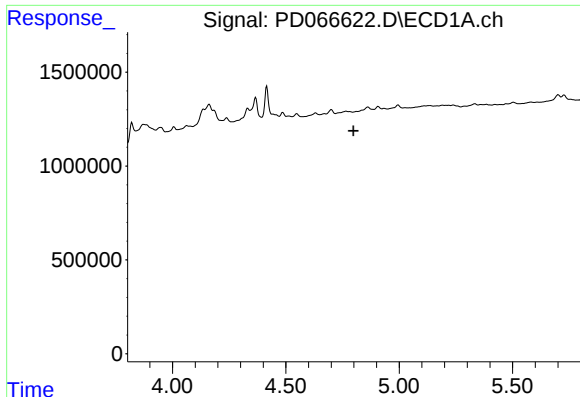

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.799 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

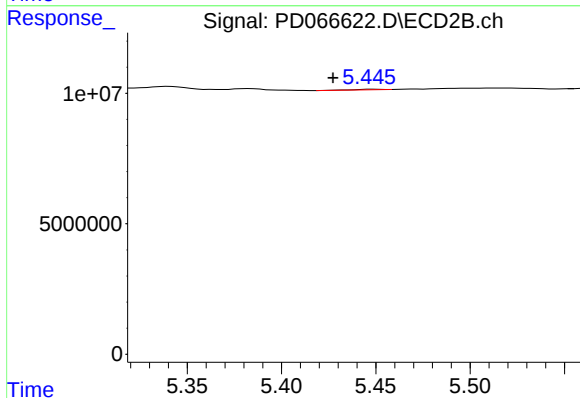


#24 Chlordane-2

R.T.: 5.448 min
Delta R.T.: 0.021 min
Response: 227137
Conc: 0.77 ng/ml

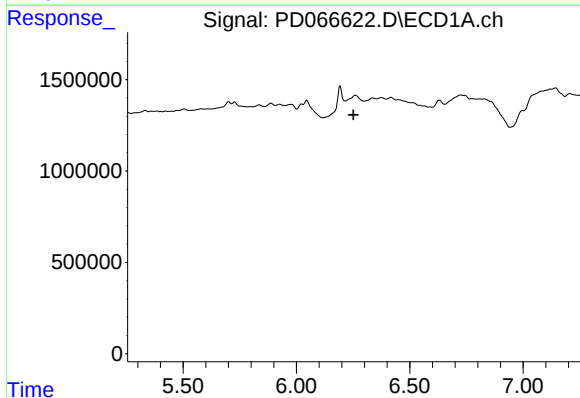


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.252 min
Response: 0
Conc: N.D.

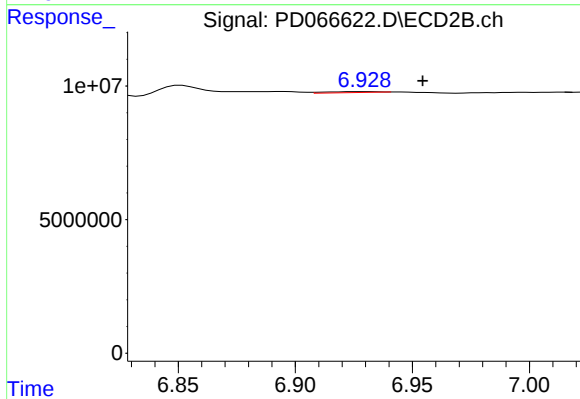

#27 Chlordane-5


R.T.: 6.931 min
Delta R.T.: -0.024 min
Response: 470416
Conc: 1.73 ng/ml

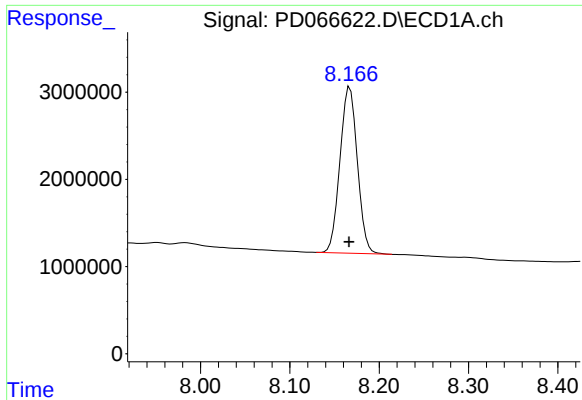

#28 Decachlorobiphenyl

R.T.: 8.167 min
Delta R.T.: 0.000 min
Response: 25768831
Conc: 22.30 ng/ml

Instrument :
ECD_D
ClientSampleId :

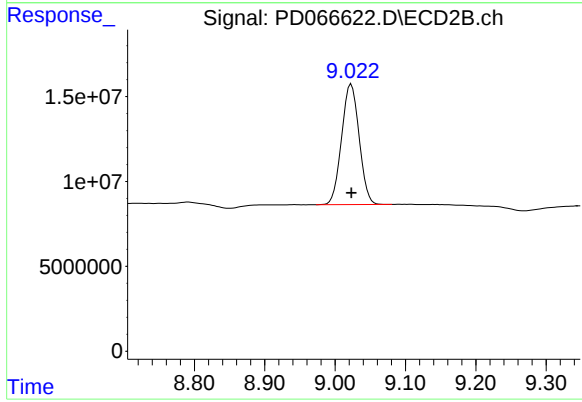

#28 Decachlorobiphenyl

R.T.: 9.023 min
Delta R.T.: 0.000 min
Response: 123152842
Conc: 22.86 ng/ml