

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD103021\
 Data File : PD066645.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Oct 2021 15:44
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 06:25:33 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102821.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 28 02:17:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.440	3.969	41023103	188.5E6	21.986	23.294
28)	SA Decachlor...	8.167	9.025	25629688	125.6E6	22.182	23.311
Target Compounds							
3)	MA gamma-BHC...	4.160	0.000	4231842	0	1.401	N.D. #
4)	MA Heptachlor	0.000	5.128f	0	1873045	N.D.	0.191 #
6)	B beta-BHC	4.415	4.846f	1967250	1941175	1.575	0.417 #
7)	B delta-BHC	0.000	5.057f	0	3303399	N.D.	0.361 #
8)	B Heptachlo...	0.000	5.859f	0	1310546	N.D.	0.181 #
15)	B Endosulfa...	0.000	6.892	0	1270051	N.D.	0.180 #
21)	B Endrin ke...	0.000	7.732f	0	1859520	N.D.	0.221 #
22)	Mirex	0.000	8.178f	0	579346	N.D.	0.098 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD103021\
Data File : PD066645.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Oct 2021 15:44
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 06:25:33 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102821.M
Quant Title : GC Extractables
QLast Update : Thu Oct 28 02:17:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

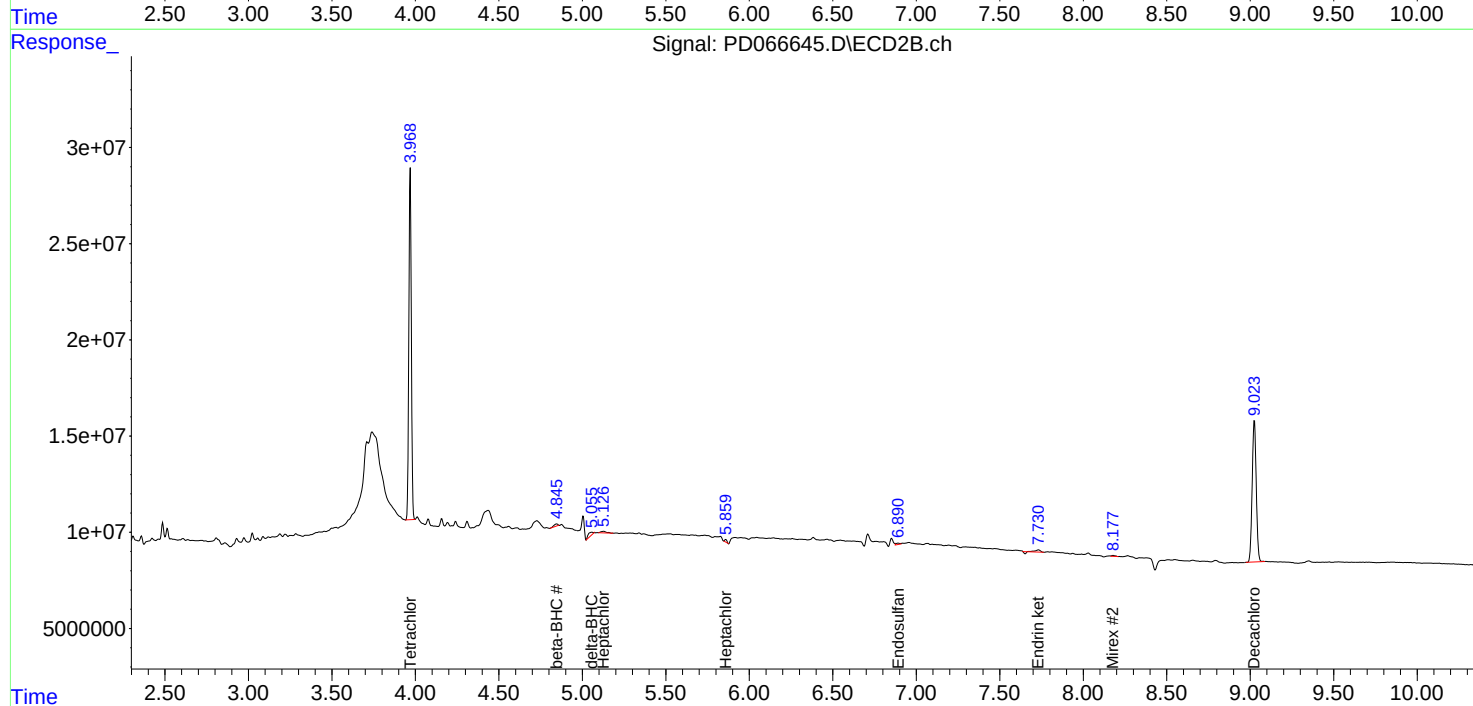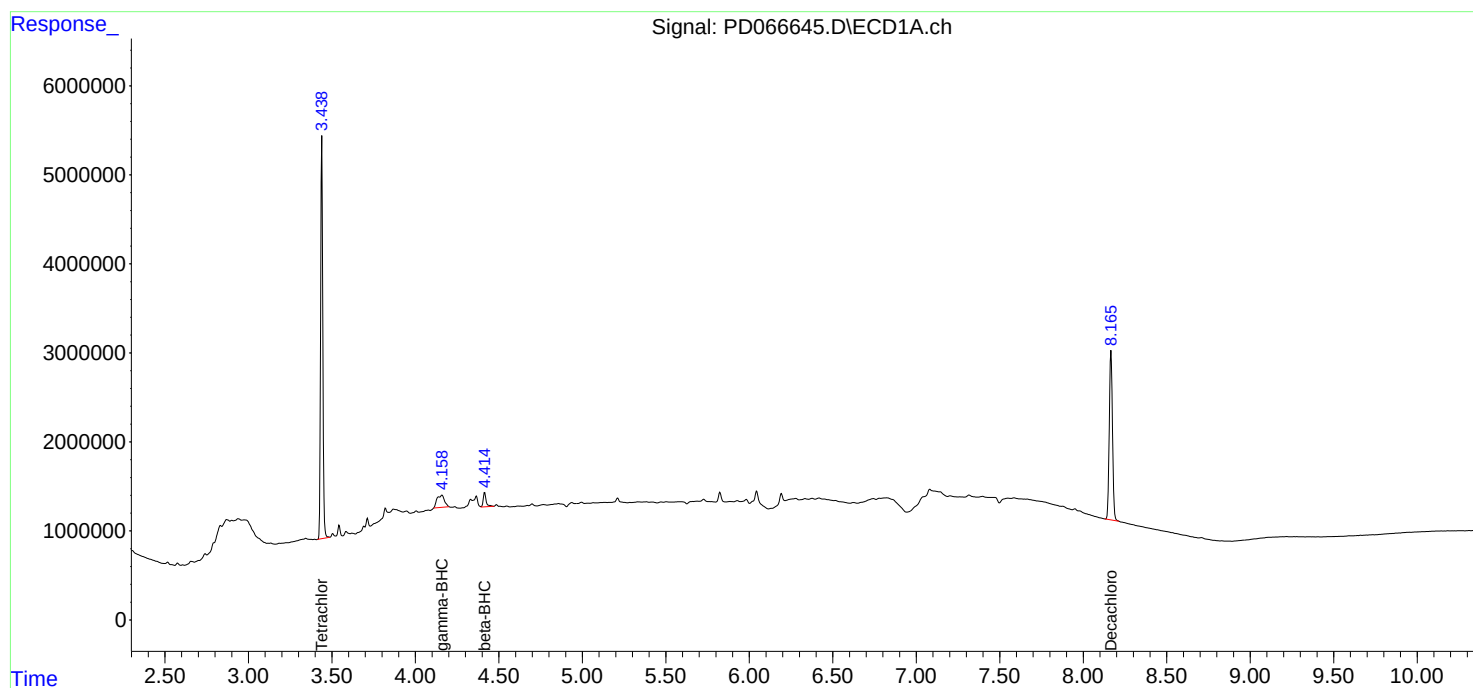


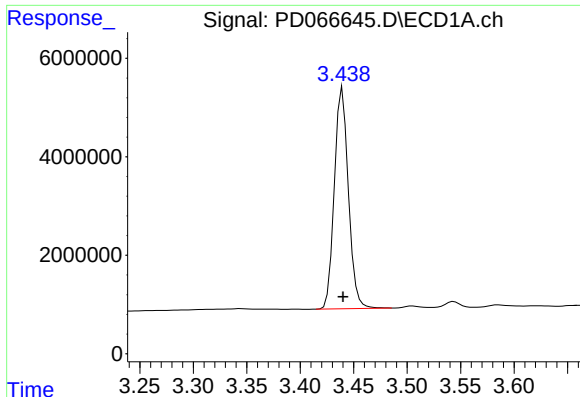

#1 Tetrachloro-m-xylene


R.T.: 3.440 min
Delta R.T.: 0.000 min
Response: 41023103
Conc: 21.99 ng/ml

Instrument :
ECD_D
ClientSampleId :

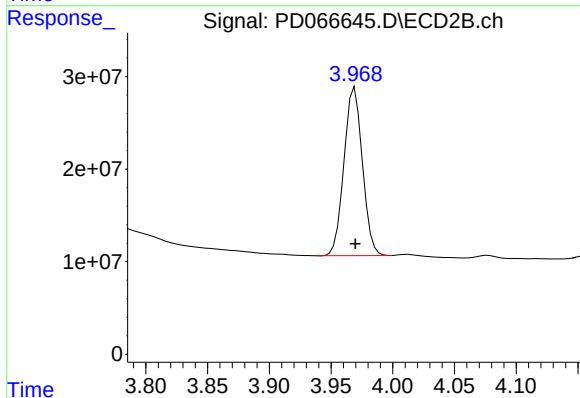


#1 Tetrachloro-m-xylene

R.T.: 3.969 min
Delta R.T.: 0.000 min
Response: 188498916
Conc: 23.29 ng/ml

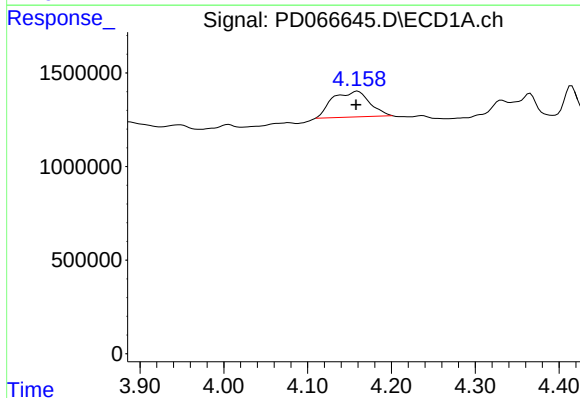


#3 gamma-BHC (Lindane)

R.T.: 4.160 min
Delta R.T.: 0.002 min
Response: 4231842
Conc: 1.40 ng/ml

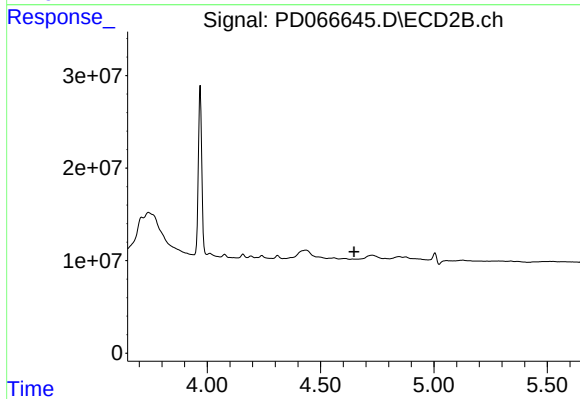

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.647 min
Response: 0
Conc: N.D.

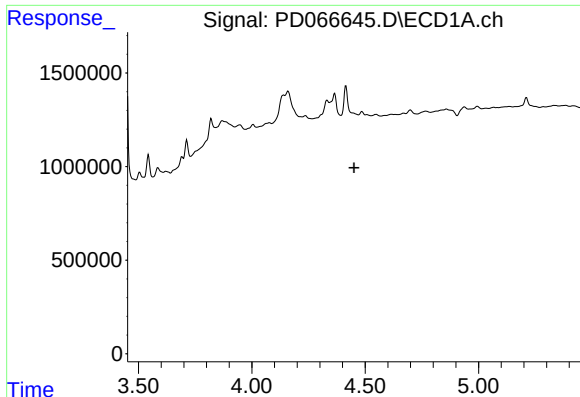

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.452 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

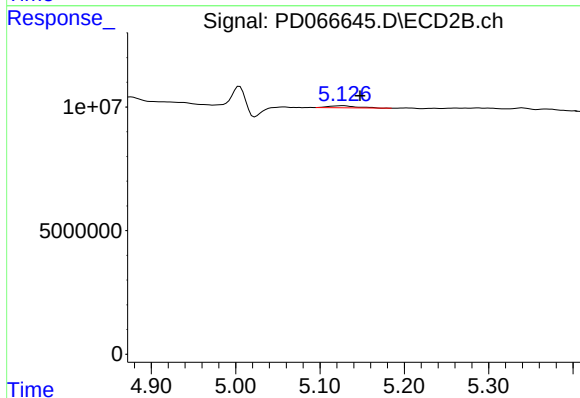


#4 Heptachlor

R.T.: 5.128 min
Delta R.T.: -0.020 min
Response: 1873045
Conc: 0.19 ng/ml

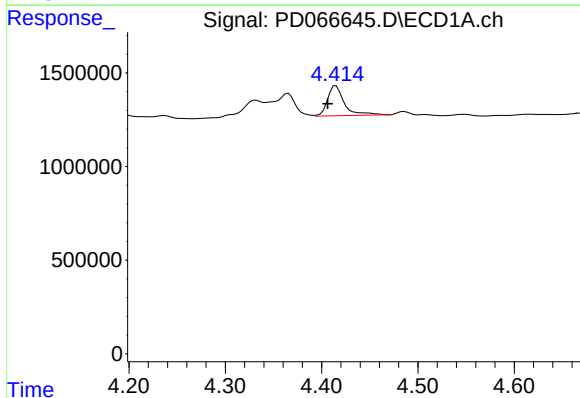


#6 beta-BHC

R.T.: 4.415 min
Delta R.T.: 0.009 min
Response: 1967250
Conc: 1.57 ng/ml

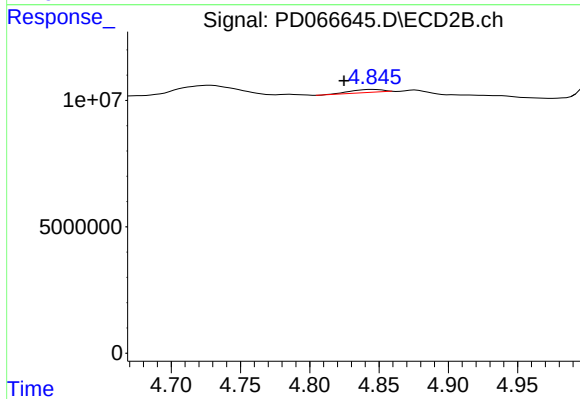

#6 beta-BHC


R.T.: 4.846 min
Delta R.T.: 0.022 min
Response: 1941175
Conc: 0.42 ng/ml

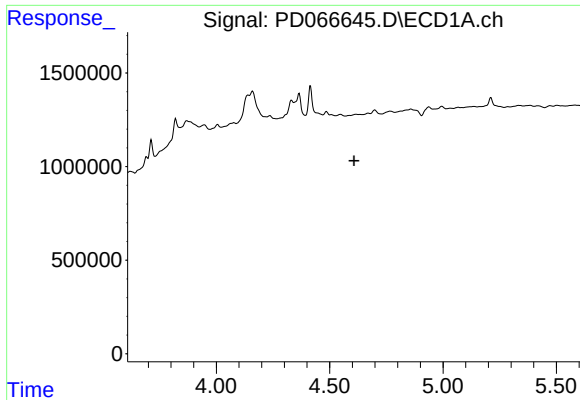

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.608 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

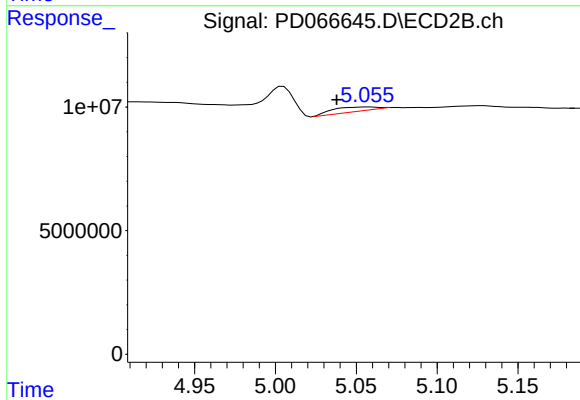


#7 delta-BHC

R.T.: 5.057 min
Delta R.T.: 0.020 min
Response: 3303399
Conc: 0.36 ng/ml

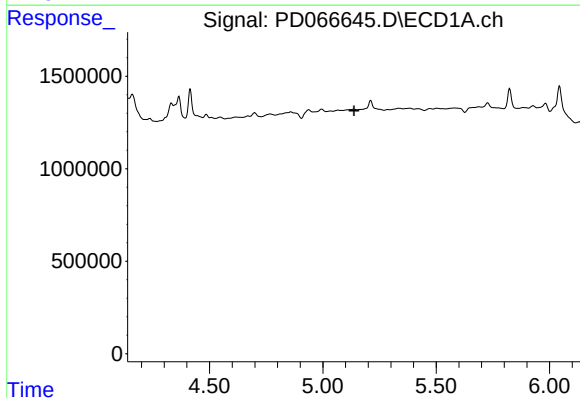


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.138 min
Response: 0
Conc: N.D.

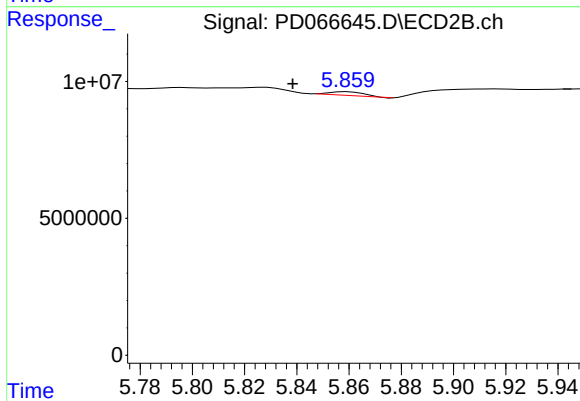

#8 Heptachlor epoxide


R.T.: 5.859 min
Delta R.T.: 0.021 min
Response: 1310546
Conc: 0.18 ng/ml

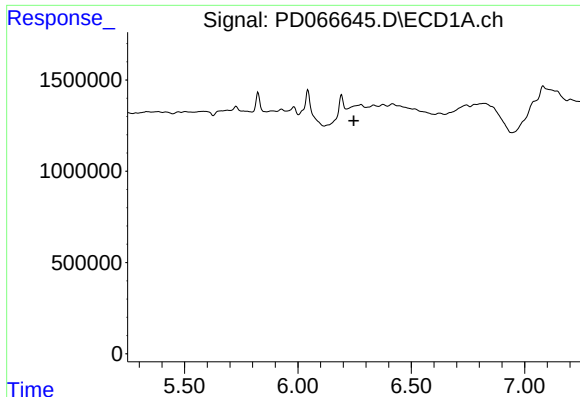

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.246 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

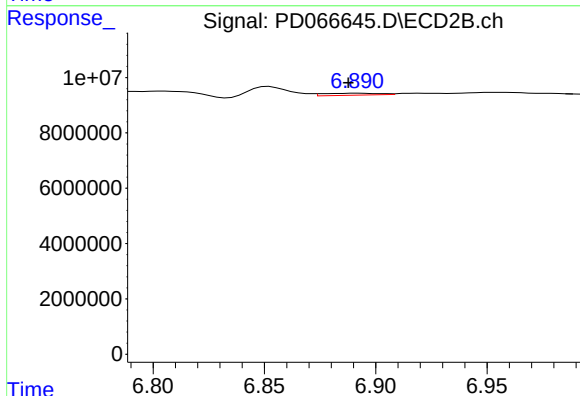


#15 Endosulfan II

R.T.: 6.892 min
Delta R.T.: 0.004 min
Response: 1270051
Conc: 0.18 ng/ml

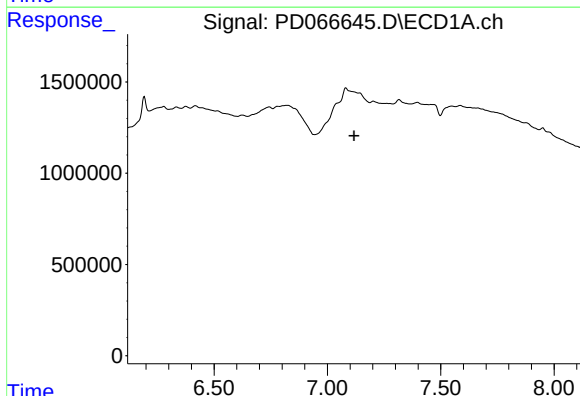


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 7.118 min
Response: 0
Conc: N.D.

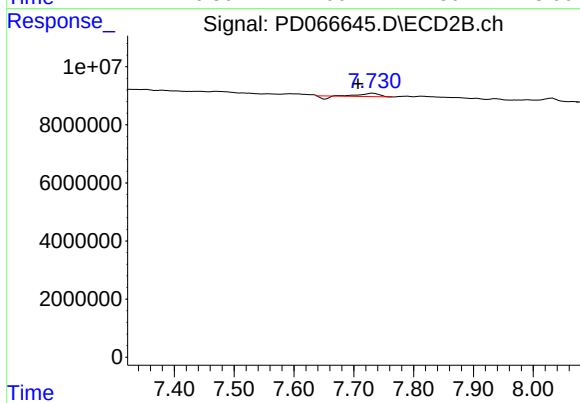

#21 Endrin ketone


R.T.: 7.732 min
Delta R.T.: 0.025 min
Response: 1859520
Conc: 0.22 ng/ml

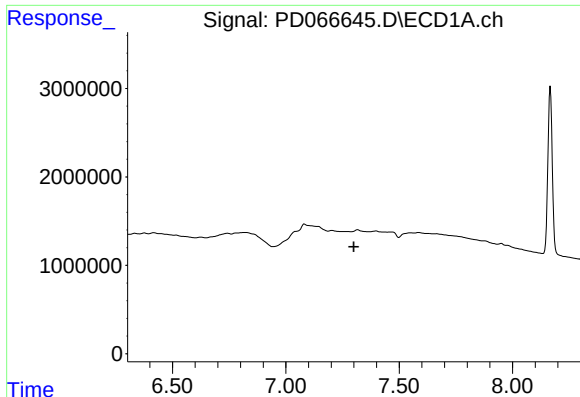

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 7.299 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

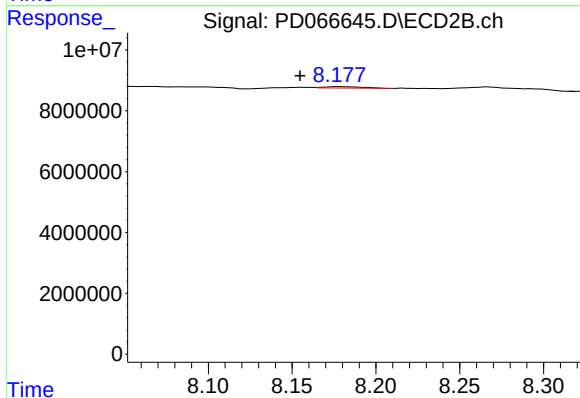


#22 Mirex

R.T.: 8.178 min
Delta R.T.: 0.023 min
Response: 579346
Conc: 0.10 ng/ml

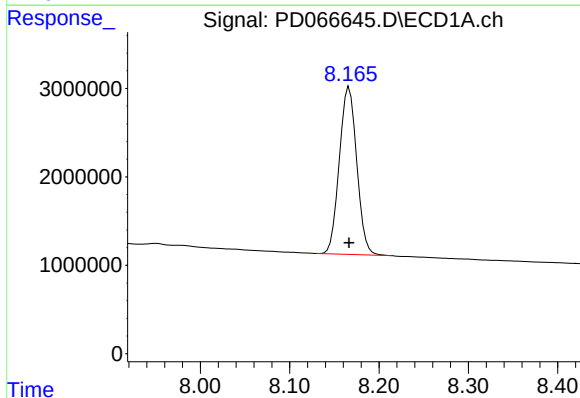

#28 Decachlorobiphenyl

R.T.: 8.167 min
Delta R.T.: 0.000 min
Response: 25629688
Conc: 22.18 ng/ml

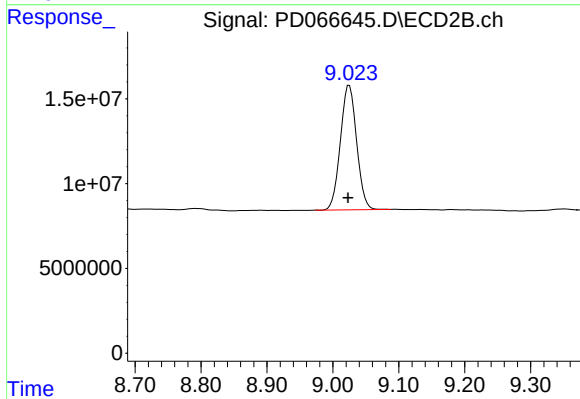

#28 Decachlorobiphenyl

R.T.: 9.025 min
Delta R.T.: 0.002 min
Response: 125564022
Conc: 23.31 ng/ml