

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD103023\
 Data File : PD079231.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Oct 2023 13:31
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 21:24:58 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102023.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 20 04:44:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.570	2.806	35154462	51973457	21.773	22.448
28)	SA Decachlor...	9.121	7.957	41915642	53350634	20.895	21.888
Target Compounds							
2)	A alpha-BHC	0.000	3.297	0	264731	N.D.	0.076 #
8)	B Heptachlo...	5.717	0.000	691661	0	0.295	N.D. #
10)	B gamma-Chl...	5.975	0.000	202789	0	0.088	N.D. #
11)	B alpha-Chl...	6.060	0.000	99579	0	0.044	N.D. #
14)	MA Endrin	0.000	5.692f	0	628296	N.D.	0.246 #
15)	B Endosulfa...	6.814f	0.000	33051	0	0.016	N.D. #
21)	B Endrin ke...	7.714f	0.000	85573	0	0.039	N.D. #
25)	Chlordane-3	5.975	0.000	202789	0	0.654	N.D. #
26)	Chlordane-4	6.060	0.000	99579	0	0.268	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD103023\
Data File : PD079231.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2023 13:31
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 21:24:58 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102023.M
Quant Title : GC Extractables
QLast Update : Fri Oct 20 04:44:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

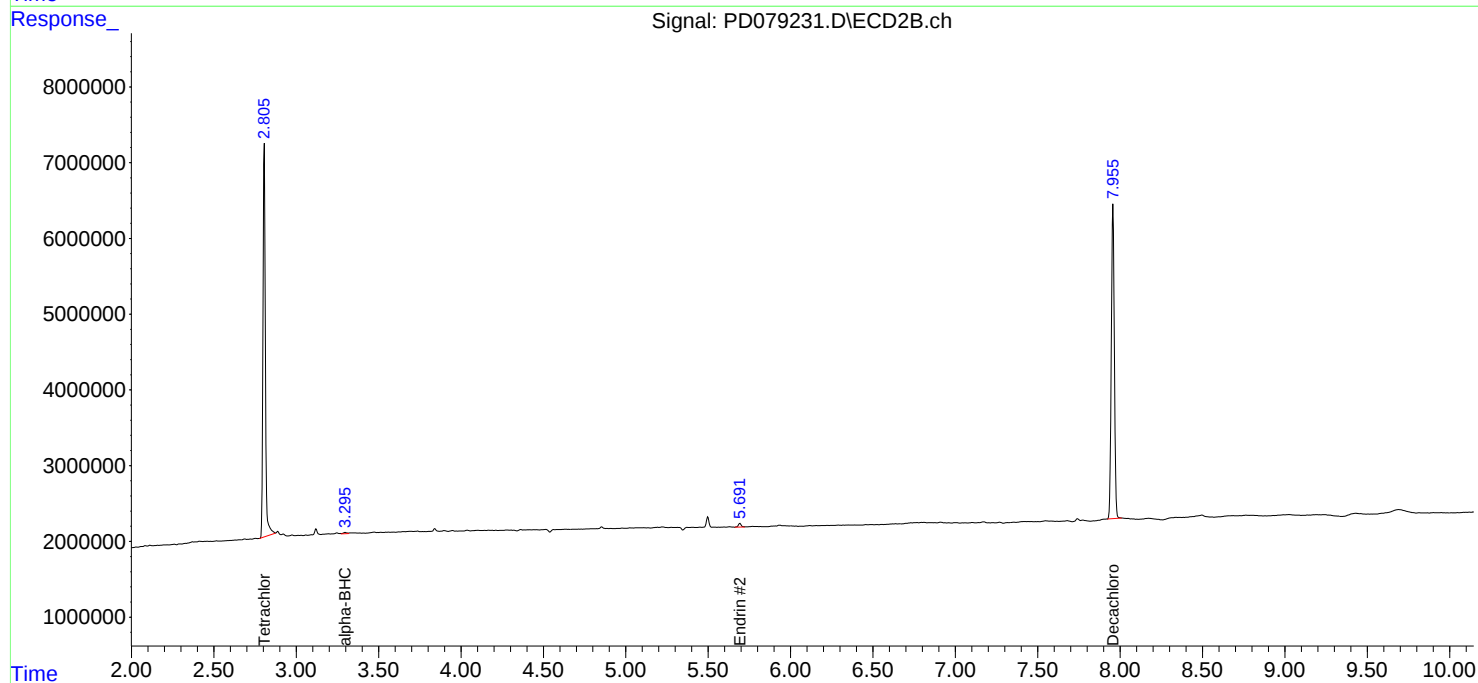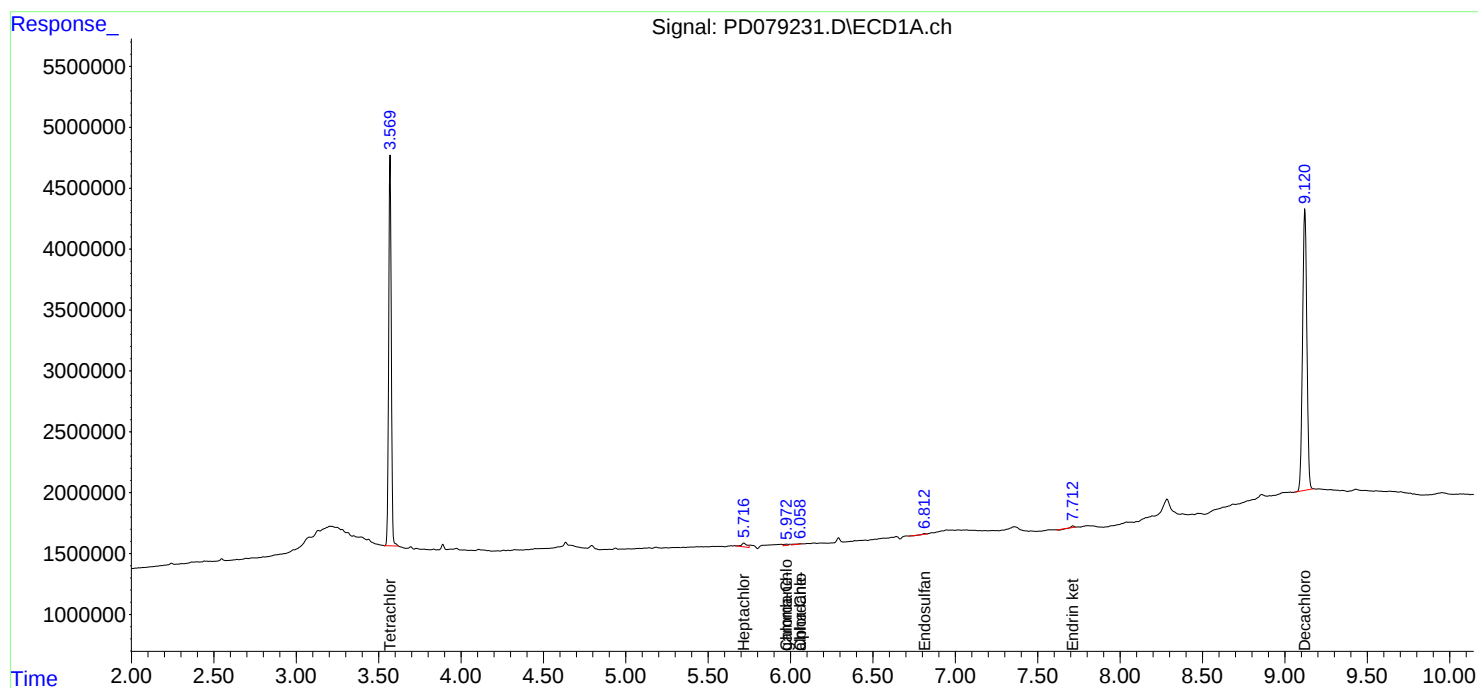


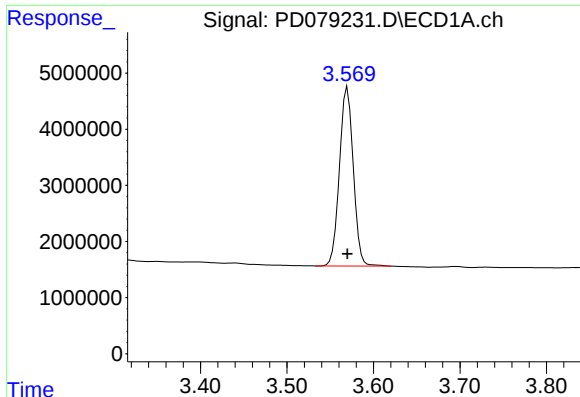

#1 Tetrachloro-m-xylene


R.T.: 3.570 min
Delta R.T.: 0.000 min
Response: 35154462
Conc: 21.77 ng/ml

Instrument :
ECD_D
ClientSampleId :

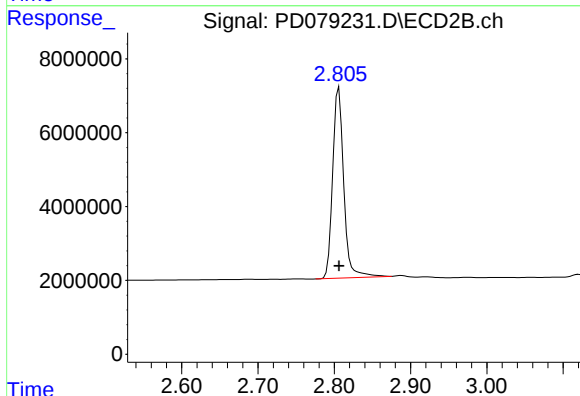


#1 Tetrachloro-m-xylene

R.T.: 2.806 min
Delta R.T.: 0.000 min
Response: 51973457
Conc: 22.45 ng/ml

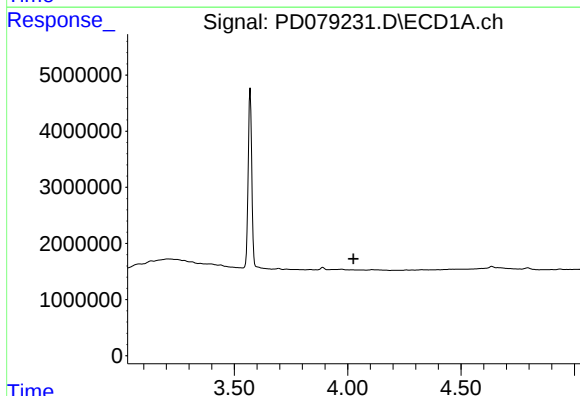


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 4.026 min
Response: 0
Conc: N.D.

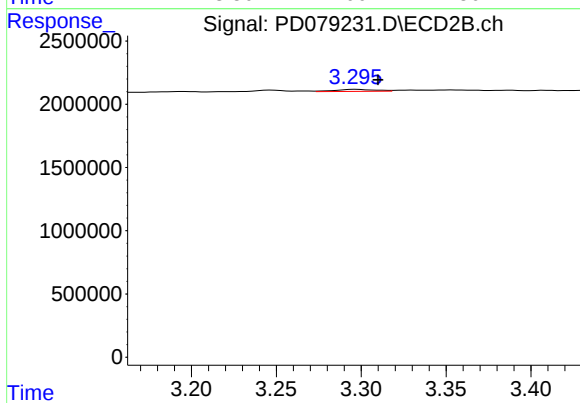

#2 alpha-BHC


R.T.: 3.297 min
Delta R.T.: -0.013 min
Response: 264731
Conc: 0.08 ng/ml

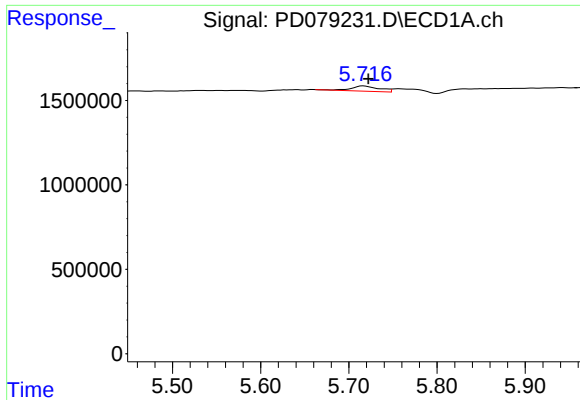

#8 Heptachlor epoxide


R.T.: 5.717 min
Delta R.T.: -0.006 min
Response: 691661
Conc: 0.30 ng/ml

Instrument :
ECD_D
ClientSampleId :

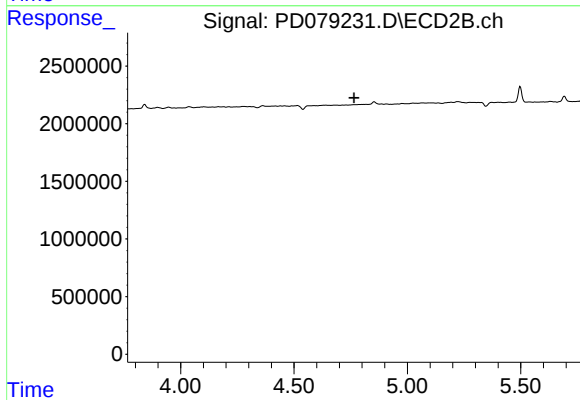


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.766 min
Response: 0
Conc: N.D.

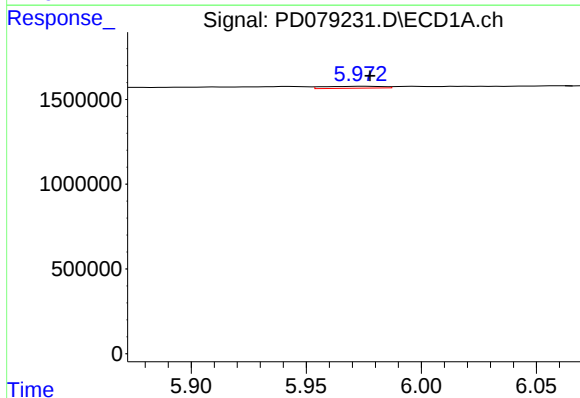


#10 gamma-Chlordane

R.T.: 5.975 min
Delta R.T.: -0.003 min
Response: 202789
Conc: 0.09 ng/ml

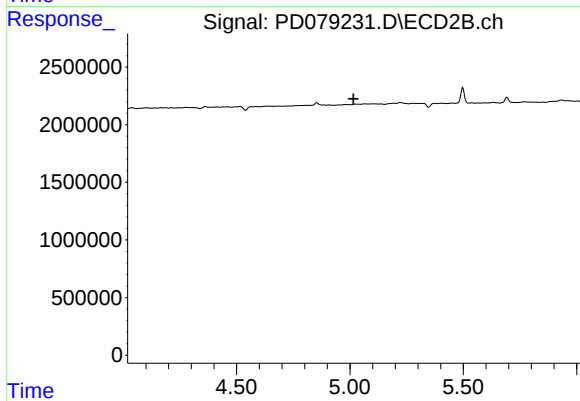

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.016 min
Response: 0
Conc: N.D.

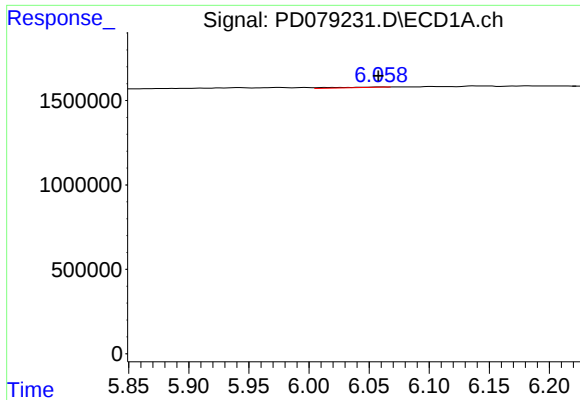

#11 alpha-Chlordane


R.T.: 6.060 min
Delta R.T.: 0.002 min
Response: 99579
Conc: 0.04 ng/ml

Instrument :
ECD_D
ClientSampleId :

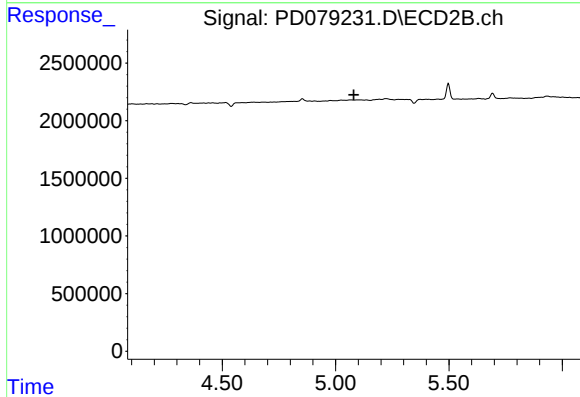


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.080 min
Response: 0
Conc: N.D.

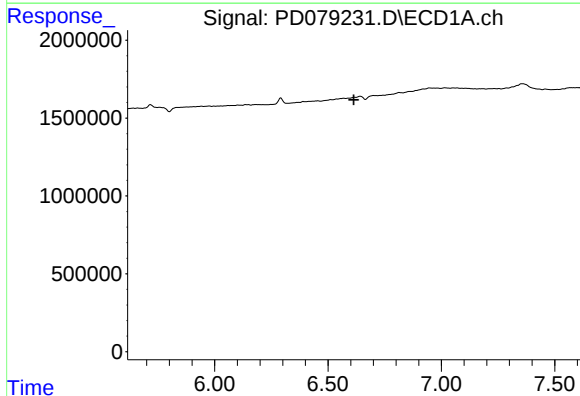


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.614 min
Response: 0
Conc: N.D.

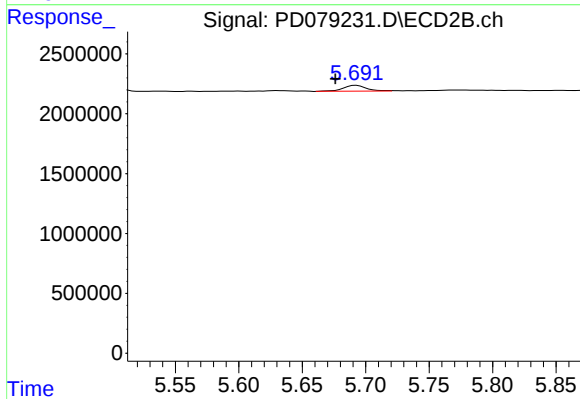

#14 Endrin


R.T.: 5.692 min
Delta R.T.: 0.016 min
Response: 628296
Conc: 0.25 ng/ml

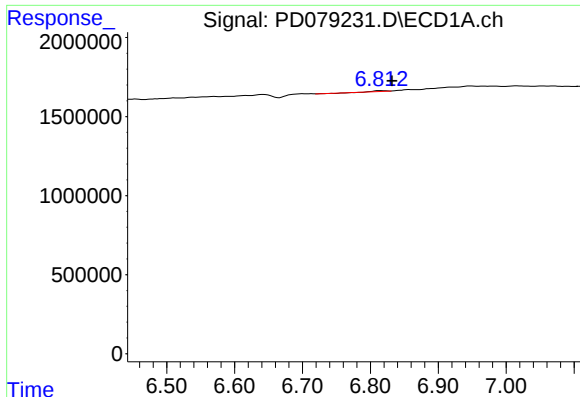

#15 Endosulfan II


R.T.: 6.814 min
Delta R.T.: -0.018 min
Response: 33051
Conc: 0.02 ng/ml

Instrument :
ECD_D
ClientSampleId :

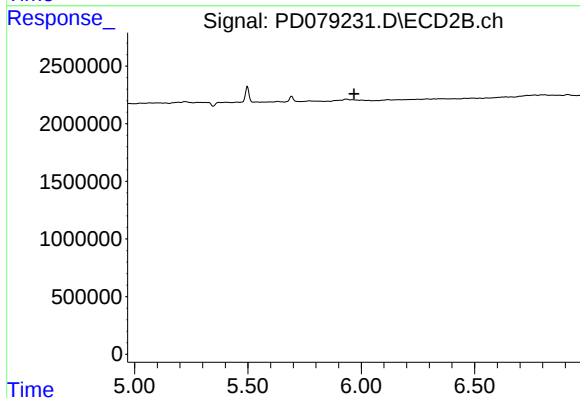


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.968 min
Response: 0
Conc: N.D.

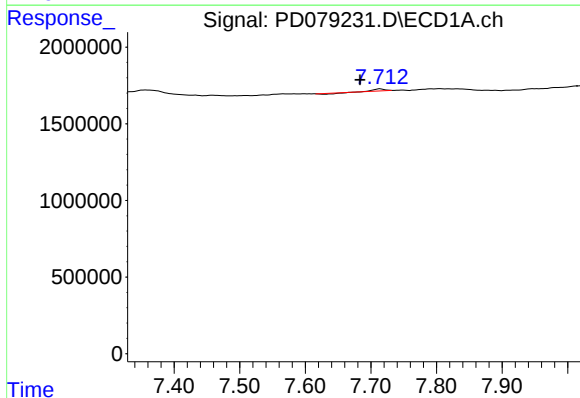


#21 Endrin ketone

R.T.: 7.714 min
Delta R.T.: 0.031 min
Response: 85573
Conc: 0.04 ng/ml

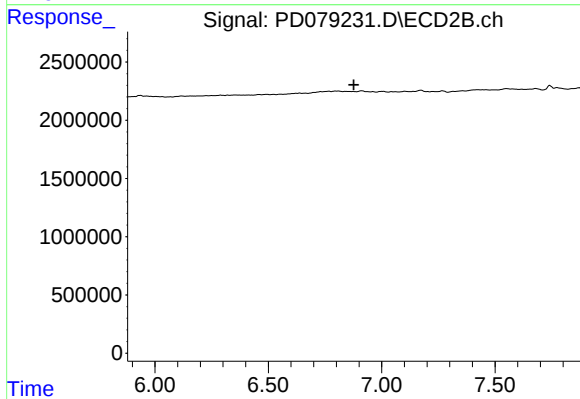

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 6.876 min
Response: 0
Conc: N.D.

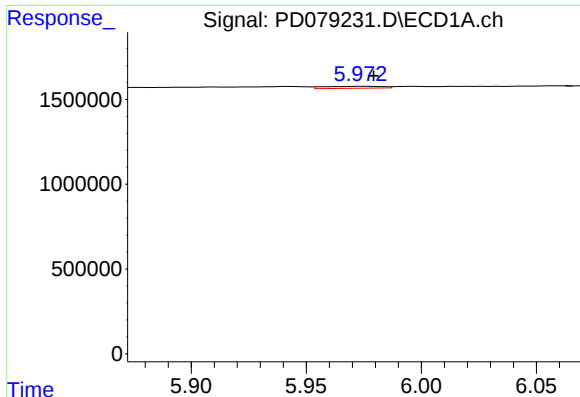

#25 Chlordane-3


R.T.: 5.975 min
Delta R.T.: -0.004 min
Response: 202789
Conc: 0.65 ng/ml

Instrument :
ECD_D
ClientSampleId :

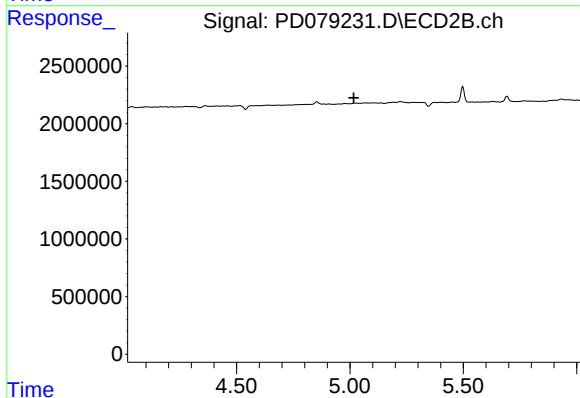


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.018 min
Response: 0
Conc: N.D.

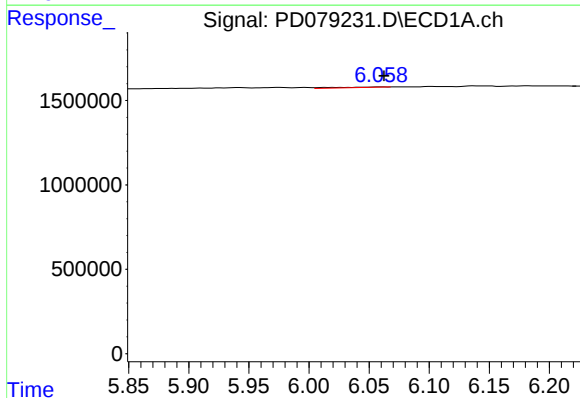


#26 Chlordane-4

R.T.: 6.060 min
Delta R.T.: -0.003 min
Response: 99579
Conc: 0.27 ng/ml

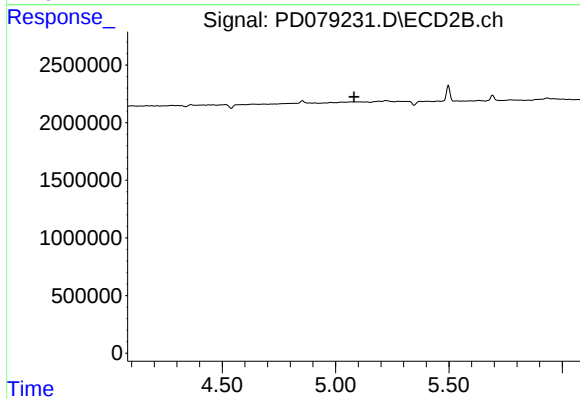

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 5.081 min
Response: 0
Conc: N.D.

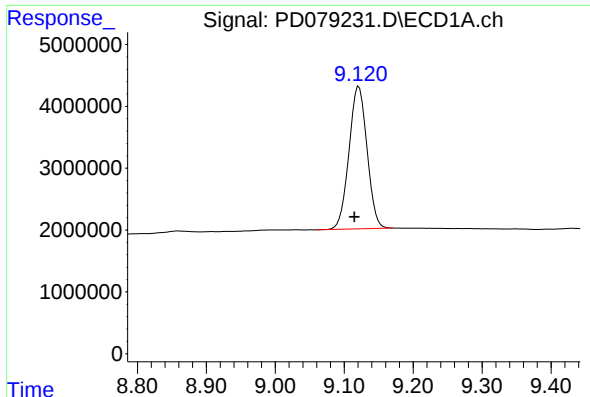

#28 Decachlorobiphenyl

R.T.: 9.121 min
Delta R.T.: 0.007 min
Response: 41915642
Conc: 20.89 ng/ml

Instrument :
ECD_D
ClientSampleId :

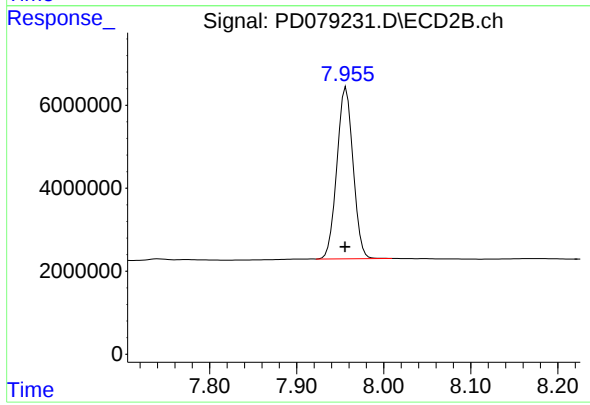

#28 Decachlorobiphenyl

R.T.: 7.957 min
Delta R.T.: 0.002 min
Response: 53350634
Conc: 21.89 ng/ml