

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD103023\
 Data File : PD079228.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Oct 2023 12:51
 Operator : AR\AJ
 Sample : 05142-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PSC-124037

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/31/2023
 Supervised By : mohammad ahmed 10/31/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 21:21:49 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102023.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 20 04:44:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.569	2.805	29497827	40012529	18.270m	17.282m
28) SA Decachlor...	9.121	7.957	29289400	36690476	14.601	15.053

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD103023\
Data File : PD079228.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2023 12:51
Operator : AR\AJ
Sample : 05142-01
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
PSC-124037


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 10/31/2023
Supervised By : mohammad ahmed 10/31/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 21:21:49 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102023.M
Quant Title : GC Extractables
QLast Update : Fri Oct 20 04:44:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

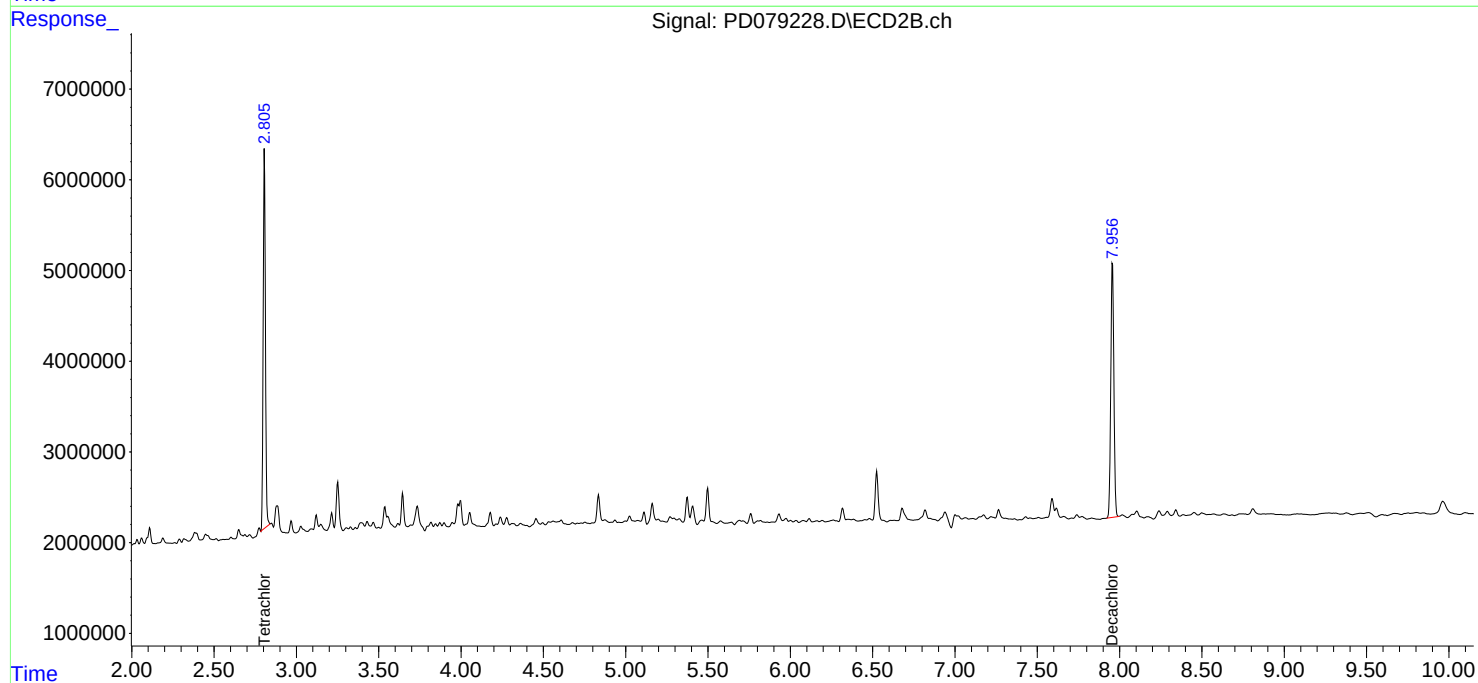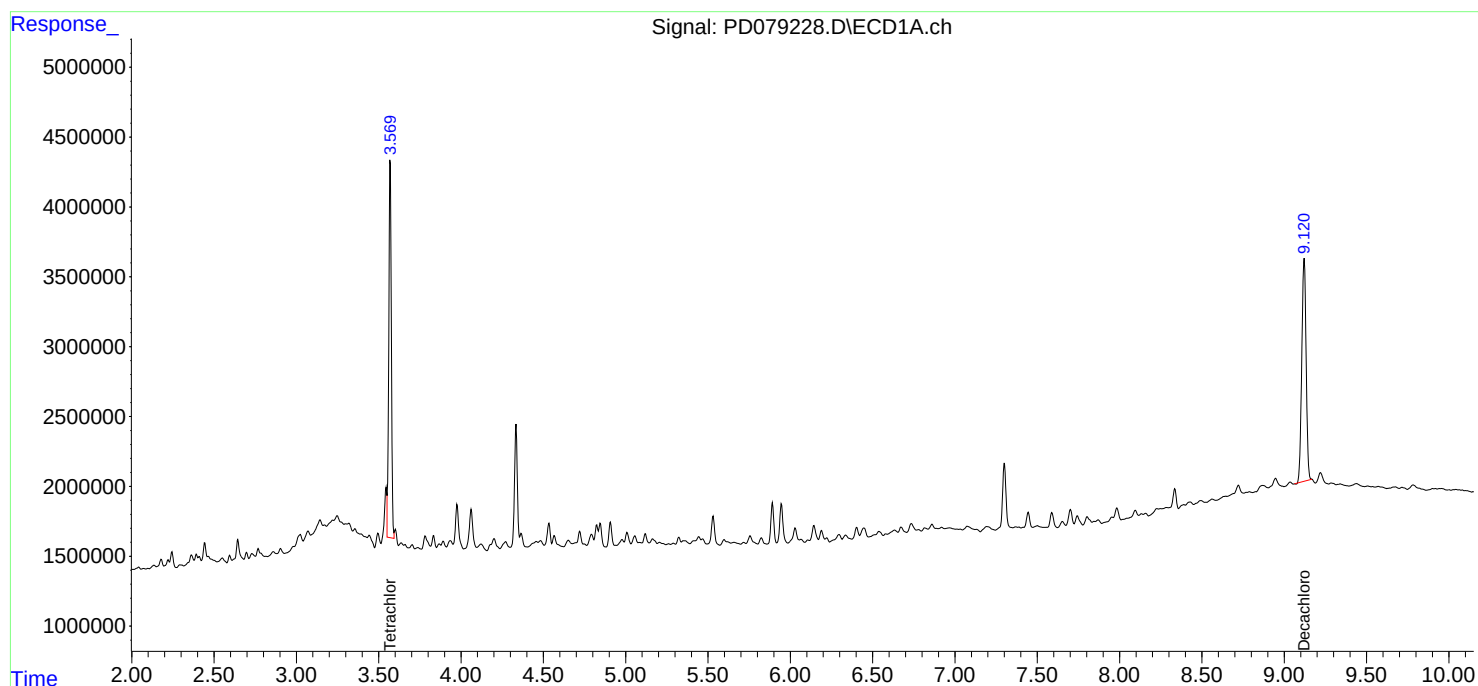

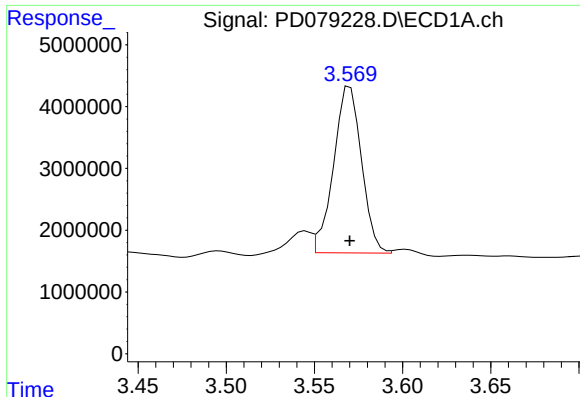


#1 Tetrachloro-m-xylene

R.T.: 3.569 min
Delta R.T.: -0.001 min
Response: 29497827
Conc: 18.27 ng/ml

Instrument :
ECD_D
ClientSampleId :
PSC-124037


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/31/2023
Supervised By :mohammad ahmed 10/31/2023

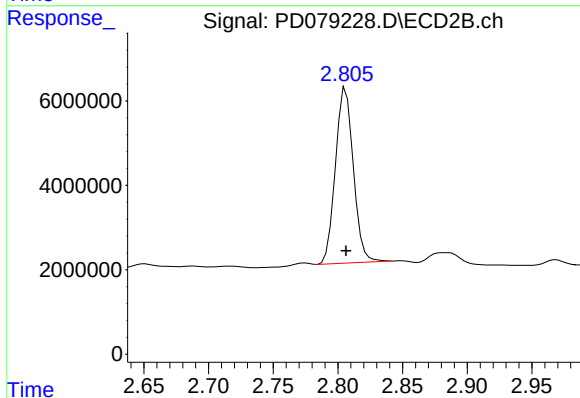


#1 Tetrachloro-m-xylene

R.T.: 2.805 min
Delta R.T.: -0.002 min
Response: 40012529
Conc: 17.28 ng/ml m

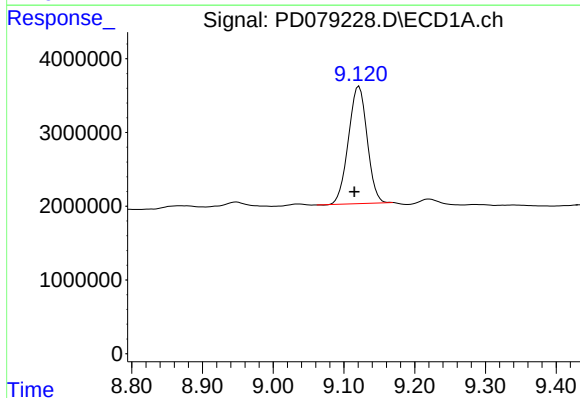

#28 Decachlorobiphenyl

R.T.: 9.121 min
Delta R.T.: 0.007 min
Response: 29289400
Conc: 14.60 ng/ml

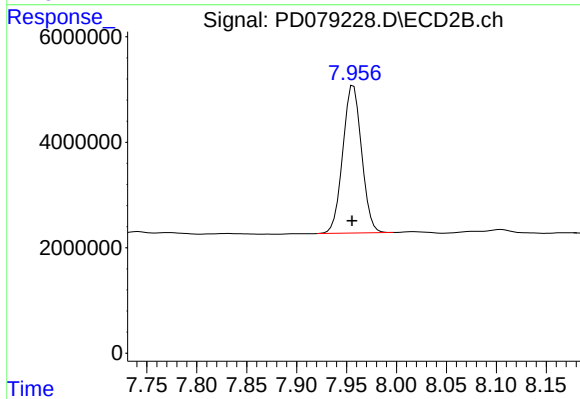

#28 Decachlorobiphenyl

R.T.: 7.957 min
Delta R.T.: 0.002 min
Response: 36690476
Conc: 15.05 ng/ml