

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD103024\
 Data File : PD086257.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Oct 2024 12:34
 Operator : AR\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 13:18:04 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD103024.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 31 11:38:14 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.561	2.889	29506536	210.0E6	20.200	21.232
28)	SA Decachlor...	9.095	8.097	39653450	226.5E6	20.684	21.143
Target Compounds							
9)	A Endosulfan I	6.091	5.263	22078553	134.8E6	9.618	10.851
10)	B gamma-Chl...	5.962	5.142	23293873	149.4E6	9.676	10.974
12)	B 4,4'-DDE	6.212	5.393	42284605	269.3E6	18.913	20.581
13)	MA Dieldrin	6.364	5.529	46413606	275.3E6	18.647	20.194
19)	B Endosulfa...	7.164	6.500	37133565	255.3E6	18.481	22.059
20)	A Methoxychlor	7.508	6.776	103.4E6	541.9E6	95.566	85.765
21)	B Endrin ke...	7.645	7.009	43868130	257.8E6	19.336	20.273



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD103024\
Data File : PD086257.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2024 12:34
Operator : AR\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 13:18:04 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD103024.M
Quant Title : GC Extractables
QLast Update : Thu Oct 31 11:38:14 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

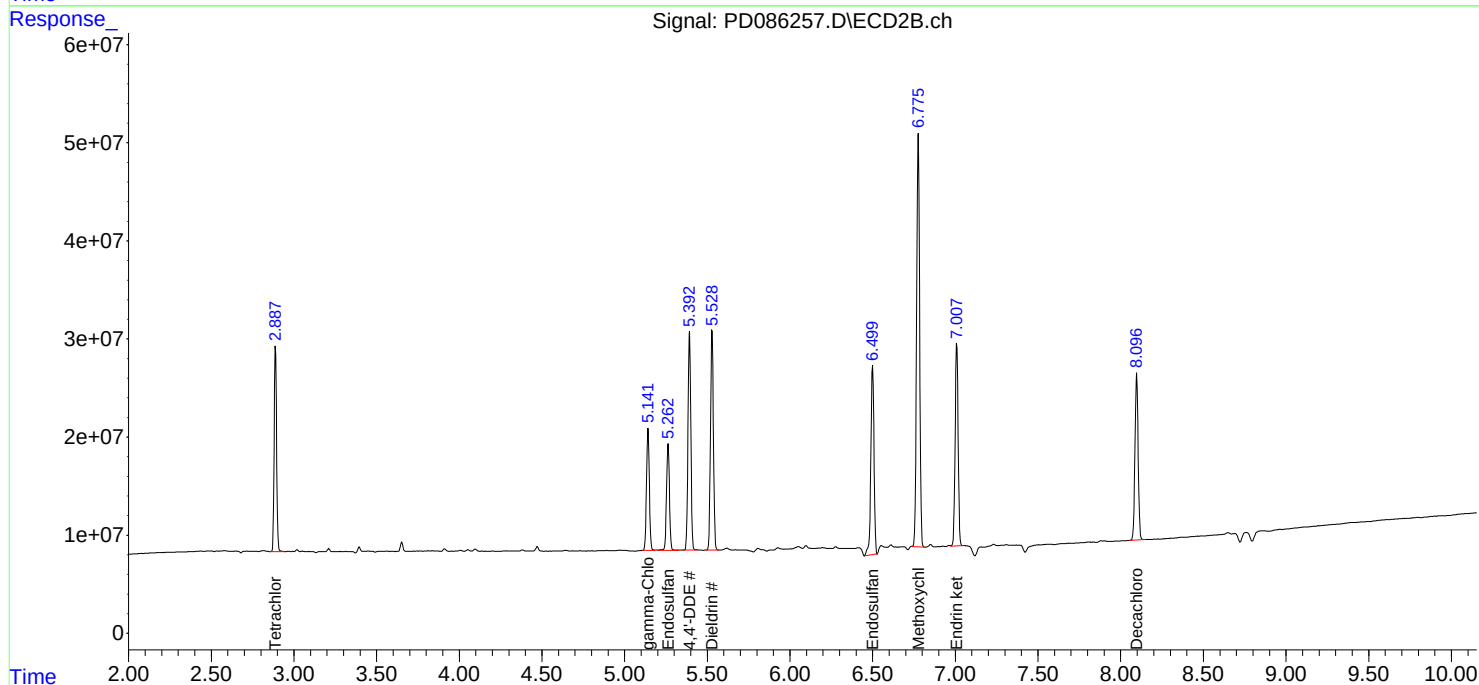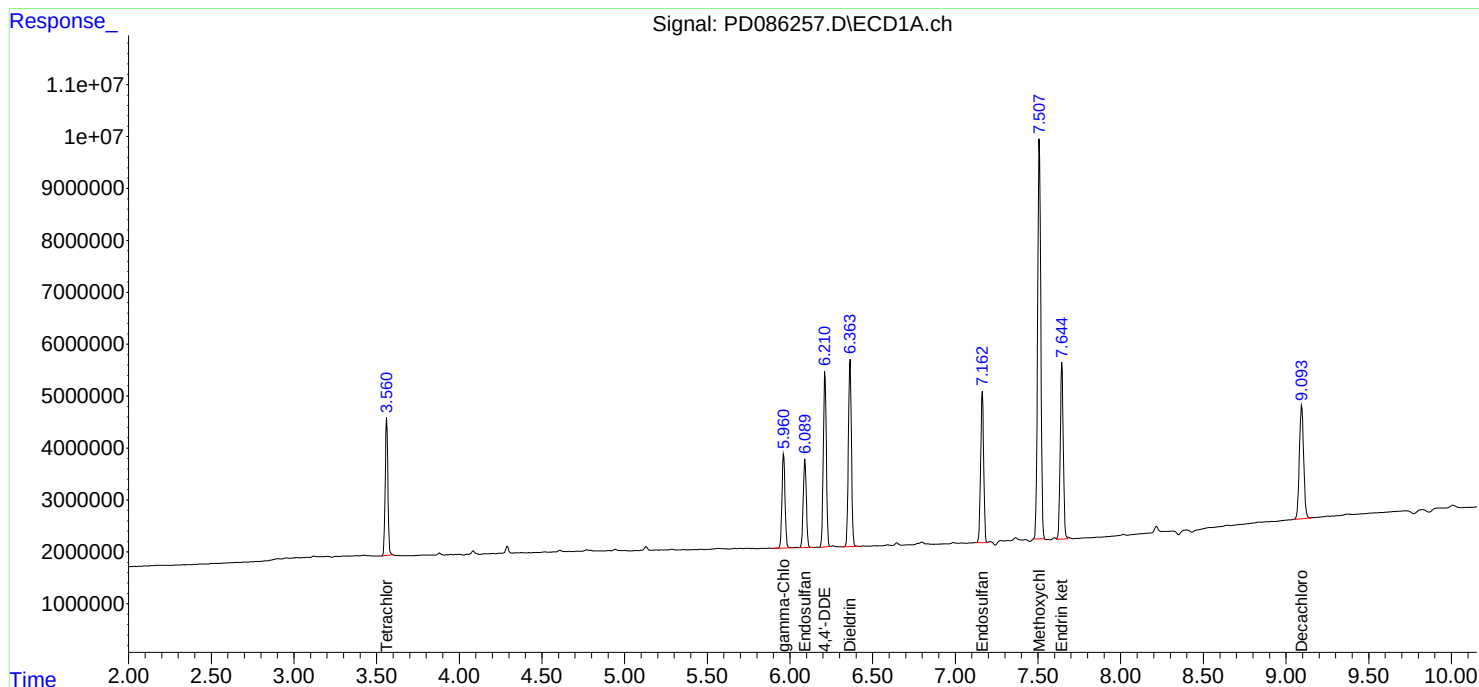


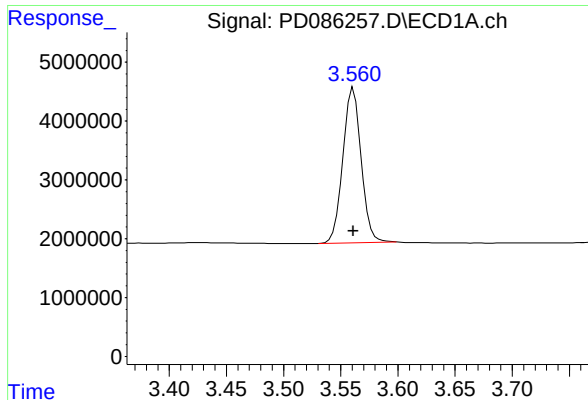

#1 Tetrachloro-m-xylene


R.T.: 3.561 min
Delta R.T.: 0.000 min
Response: 29506536
Conc: 20.20 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

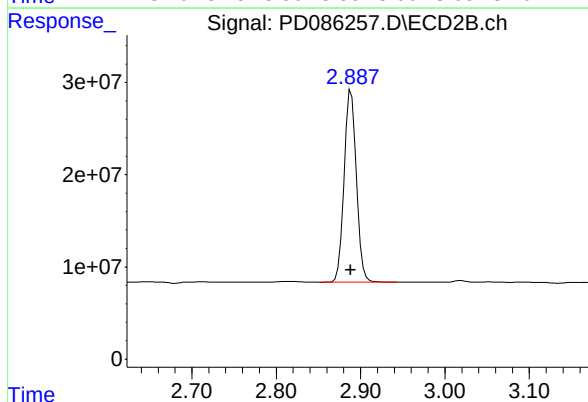


#1 Tetrachloro-m-xylene

R.T.: 2.889 min
Delta R.T.: 0.000 min
Response: 209967728
Conc: 21.23 ng/ml

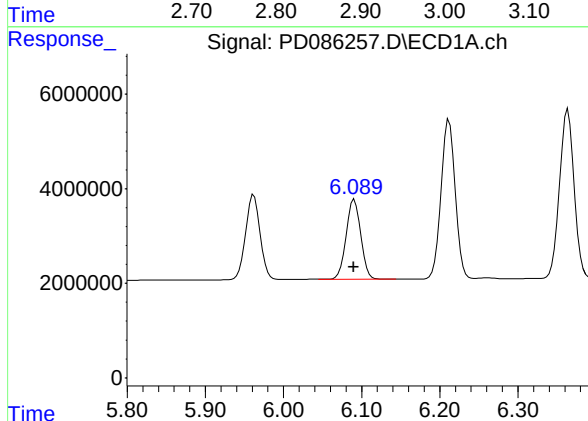


#9 Endosulfan I

R.T.: 6.091 min
Delta R.T.: 0.000 min
Response: 22078553
Conc: 9.62 ng/ml

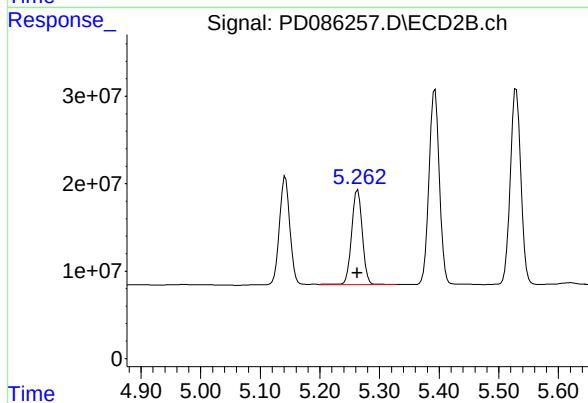

#9 Endosulfan I


R.T.: 5.263 min
Delta R.T.: 0.000 min
Response: 134812523
Conc: 10.85 ng/ml

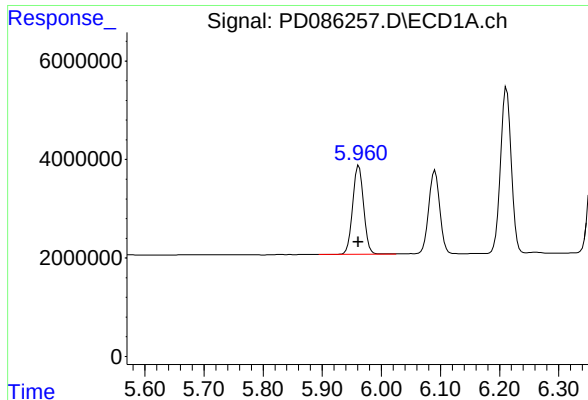

#10 gamma-Chlordane


R.T.: 5.962 min
Delta R.T.: 0.000 min
Response: 23293873
Conc: 9.68 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

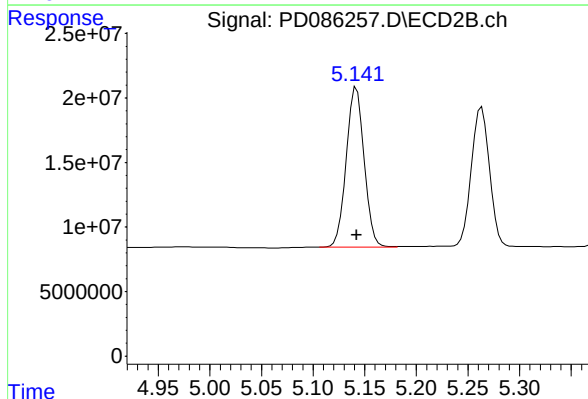


#10 gamma-Chlordane

R.T.: 5.142 min
Delta R.T.: 0.000 min
Response: 149378937
Conc: 10.97 ng/ml

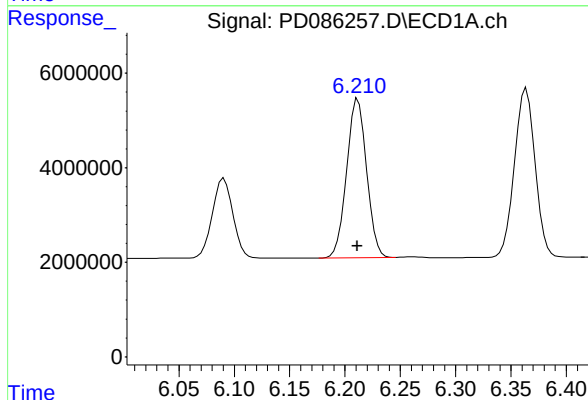


#12 4,4'-DDE

R.T.: 6.212 min
Delta R.T.: 0.000 min
Response: 42284605
Conc: 18.91 ng/ml

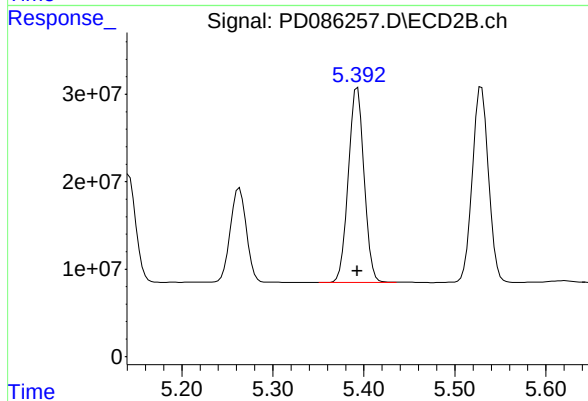

#12 4,4'-DDE


R.T.: 5.393 min
Delta R.T.: 0.000 min
Response: 269310271
Conc: 20.58 ng/ml

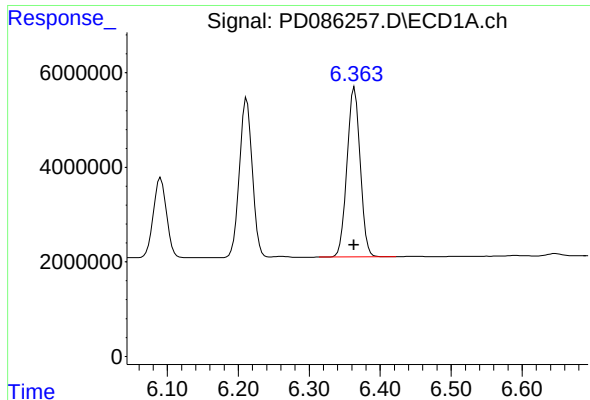

#13 Dieldrin


R.T.: 6.364 min
Delta R.T.: 0.000 min
Response: 46413606
Conc: 18.65 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

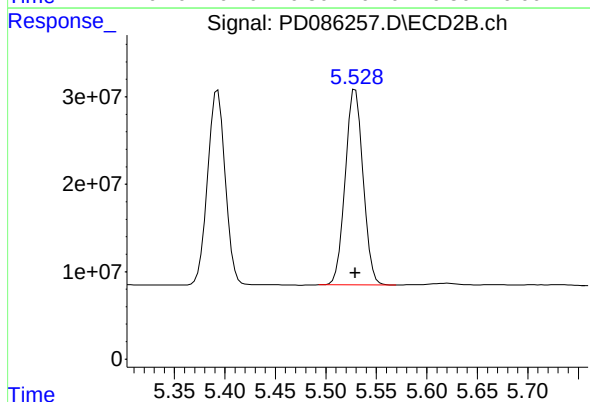


#13 Dieldrin

R.T.: 5.529 min
Delta R.T.: 0.000 min
Response: 275313335
Conc: 20.19 ng/ml

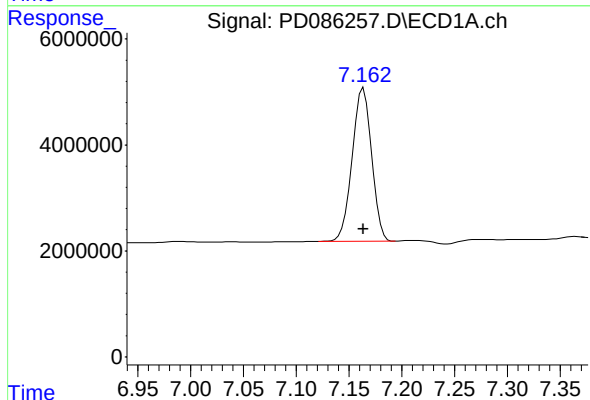


#19 Endosulfan Sulfate

R.T.: 7.164 min
Delta R.T.: 0.000 min
Response: 37133565
Conc: 18.48 ng/ml

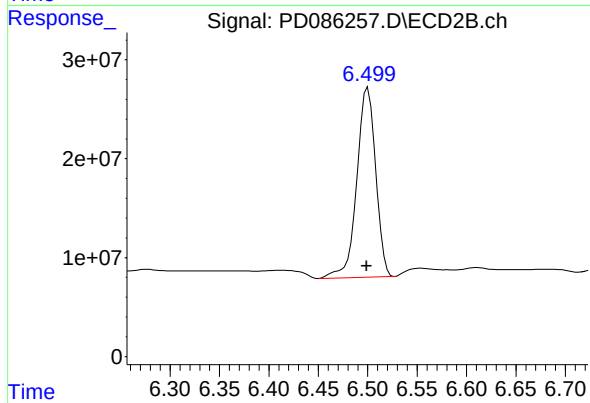

#19 Endosulfan Sulfate


R.T.: 6.500 min
Delta R.T.: 0.000 min
Response: 255333102
Conc: 22.06 ng/ml

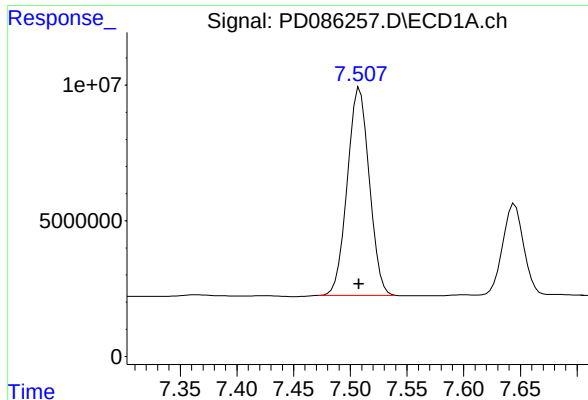

#20 Methoxychlor


R.T.: 7.508 min
Delta R.T.: 0.000 min
Response: 103350370
Conc: 95.57 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

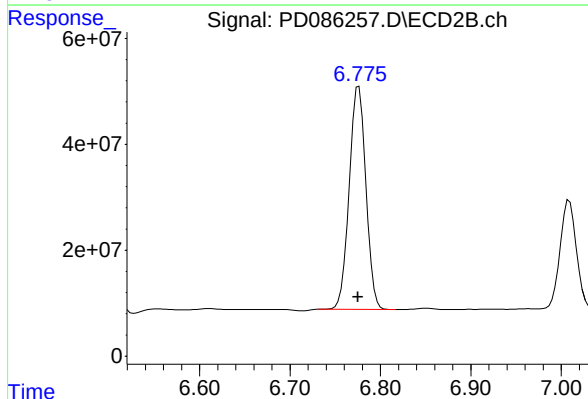


#20 Methoxychlor

R.T.: 6.776 min
Delta R.T.: 0.000 min
Response: 541924109
Conc: 85.77 ng/ml

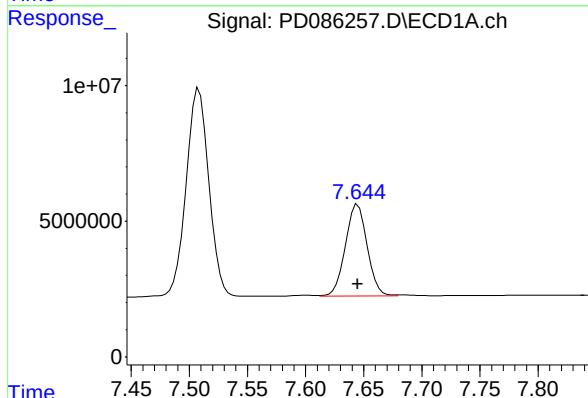


#21 Endrin ketone

R.T.: 7.645 min
Delta R.T.: 0.000 min
Response: 43868130
Conc: 19.34 ng/ml

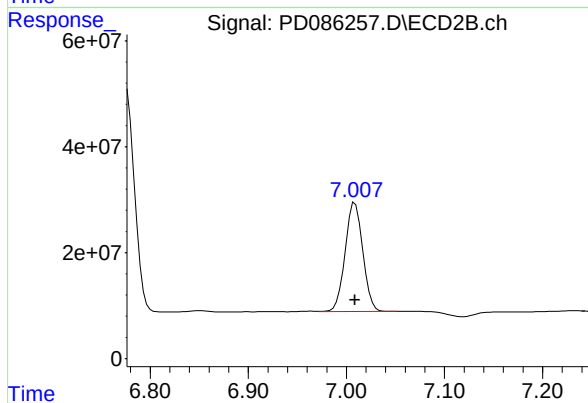

#21 Endrin ketone


R.T.: 7.009 min
Delta R.T.: 0.000 min
Response: 257809715
Conc: 20.27 ng/ml

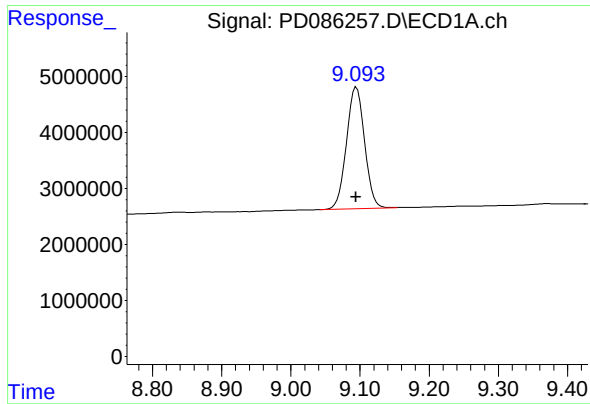

#28 Decachlorobiphenyl

R.T.: 9.095 min
Delta R.T.: 0.000 min
Response: 39653450
Conc: 20.68 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

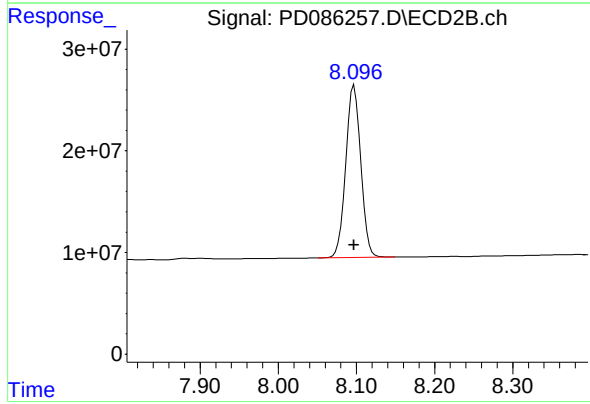

#28 Decachlorobiphenyl

R.T.: 8.097 min
Delta R.T.: 0.000 min
Response: 226487438
Conc: 21.14 ng/ml