

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD103024\
 Data File : PD086264.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Oct 2024 14:12
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 10:07:18 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD103024.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 31 10:02:31 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.562	2.889	105.4E6	833.7E6	73.598	73.591
28)	SA Decachlor...	9.095	8.098	137.3E6	748.9E6	73.865	73.423
Target Compounds							
23)	Chlordane-1	4.731	3.919	65279042	316.5E6	733.723	734.472
24)	Chlordane-2	5.258	4.502	67279688	331.4E6	736.986	733.330
25)	Chlordane-3	5.963	5.143	281.3E6	1011.3E6	737.502	737.519
26)	Chlordane-4	6.049	5.208	336.5E6	833.1E6	735.960	732.433
27)	Chlordane-5	6.888	5.878	58190438	272.2E6	737.896	726.055



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD103024\
Data File : PD086264.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2024 14:12
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 10:07:18 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD103024.M
Quant Title : GC Extractables
QLast Update : Thu Oct 31 10:02:31 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

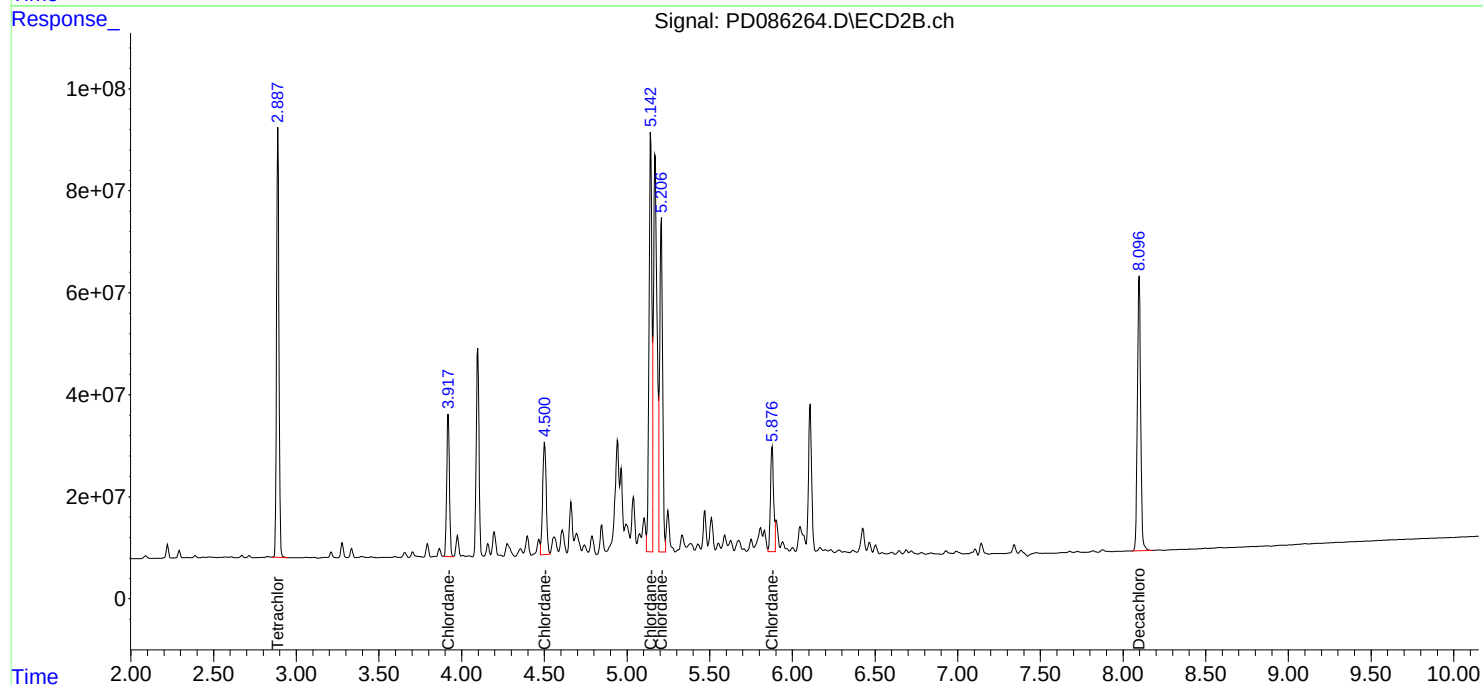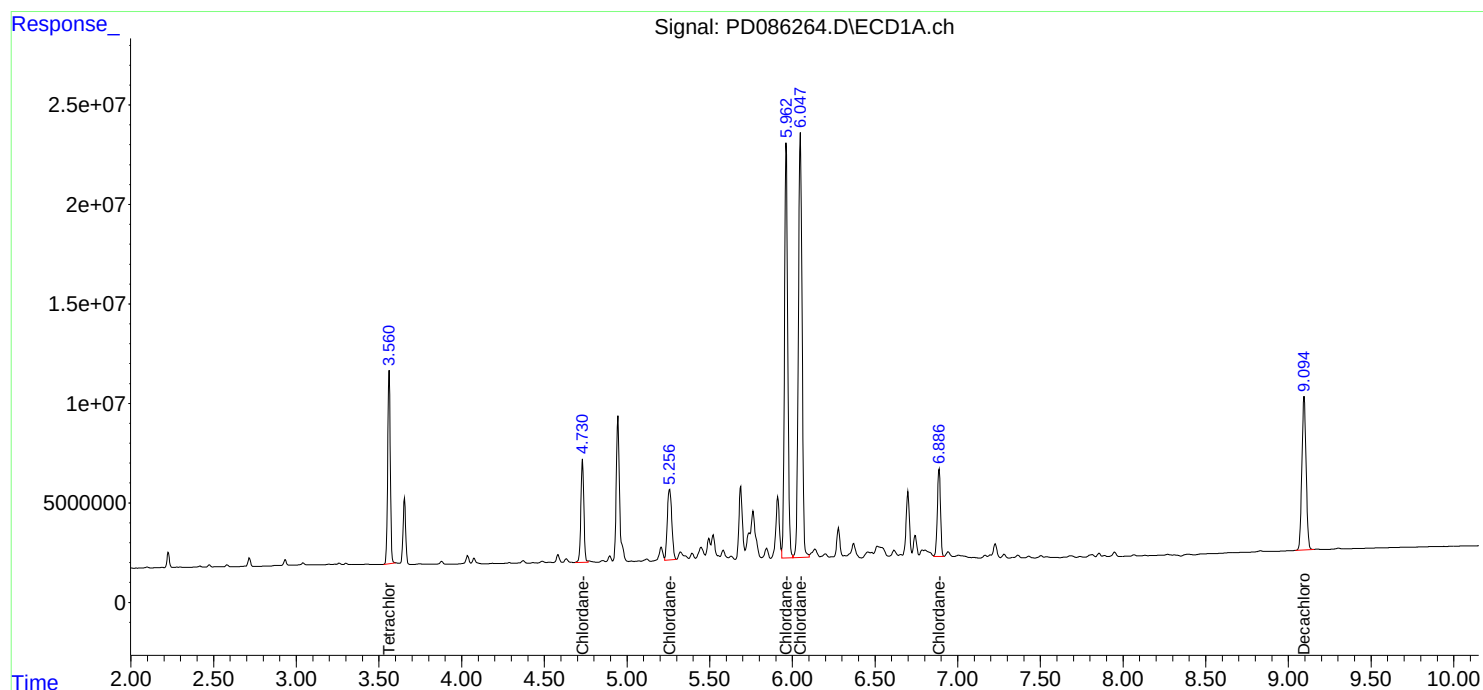


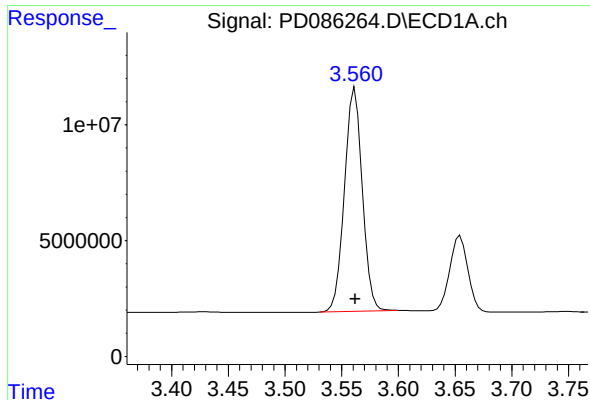

#1 Tetrachloro-m-xylene


R.T.: 3.562 min
Delta R.T.: 0.000 min
Response: 105416197
Conc: 73.60 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

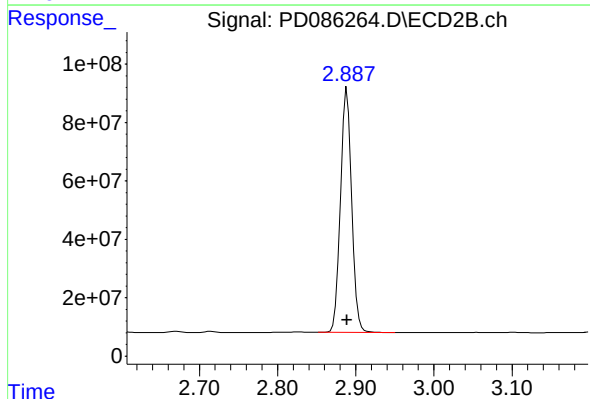


#1 Tetrachloro-m-xylene

R.T.: 2.889 min
Delta R.T.: 0.000 min
Response: 833676229
Conc: 73.59 ng/ml

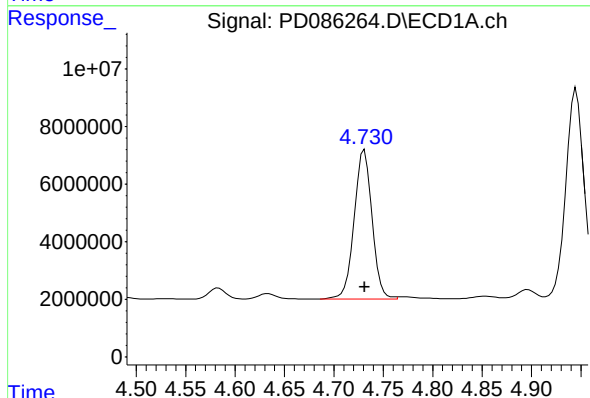


#23 Chlordane-1

R.T.: 4.731 min
Delta R.T.: 0.000 min
Response: 65279042
Conc: 733.72 ng/ml

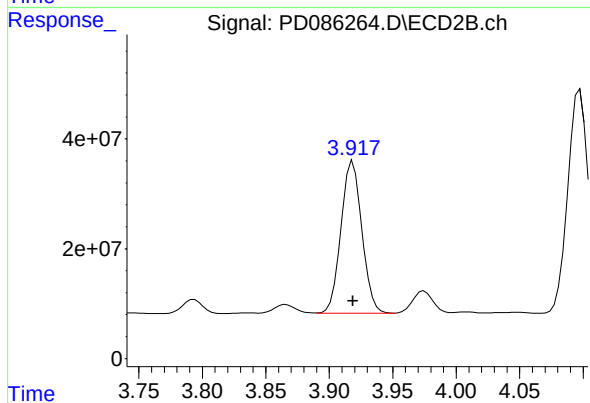

#23 Chlordane-1


R.T.: 3.919 min
Delta R.T.: 0.000 min
Response: 316486628
Conc: 734.47 ng/ml

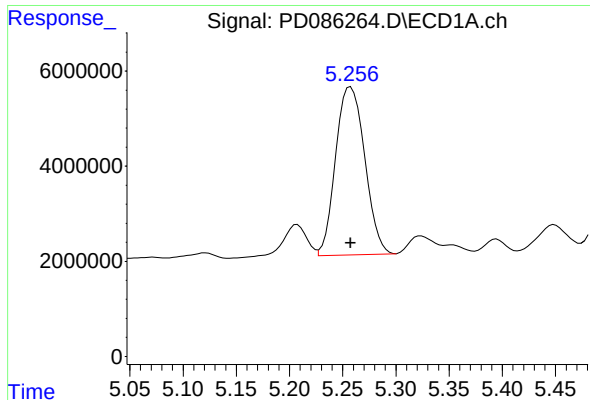

#24 Chlordane-2


R.T.: 5.258 min
Delta R.T.: 0.000 min
Response: 67279688
Conc: 736.99 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

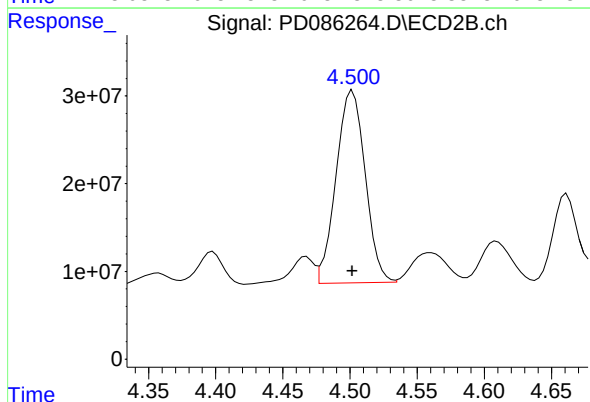


#24 Chlordane-2

R.T.: 4.502 min
Delta R.T.: 0.000 min
Response: 331430833
Conc: 733.33 ng/ml

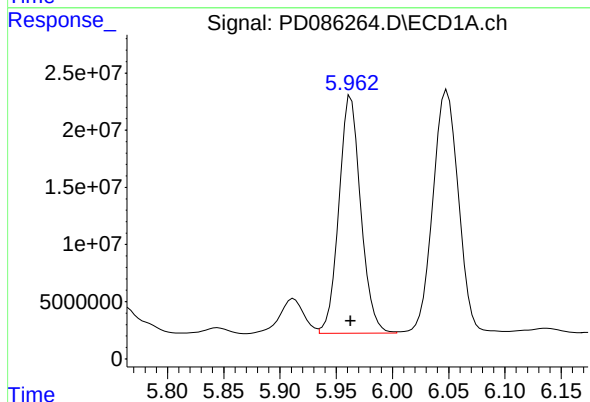


#25 Chlordane-3

R.T.: 5.963 min
Delta R.T.: 0.000 min
Response: 281318423
Conc: 737.50 ng/ml

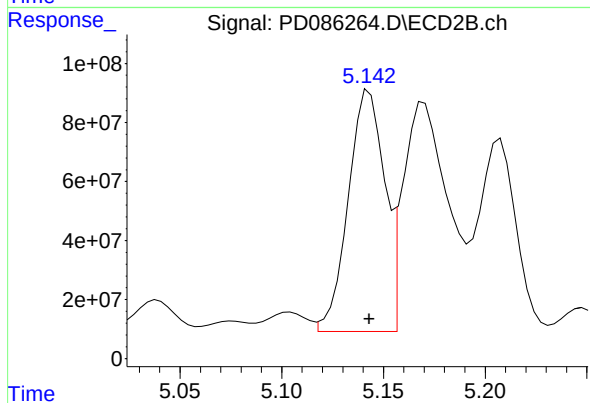

#25 Chlordane-3


R.T.: 5.143 min
Delta R.T.: 0.000 min
Response: 1011314659
Conc: 737.52 ng/ml

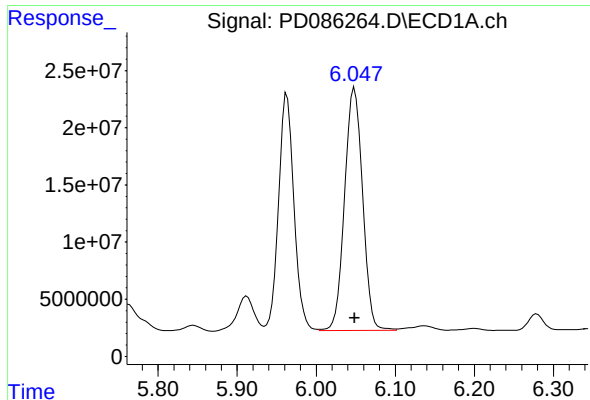

#26 Chlordane-4


R.T.: 6.049 min
Delta R.T.: 0.000 min
Response: 336503514
Conc: 735.96 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

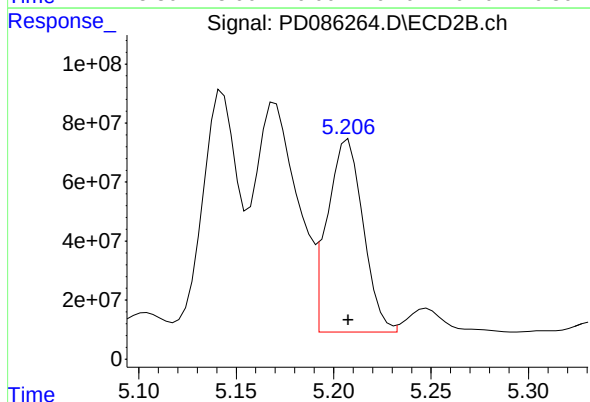


#26 Chlordane-4

R.T.: 5.208 min
Delta R.T.: 0.000 min
Response: 833077550
Conc: 732.43 ng/ml

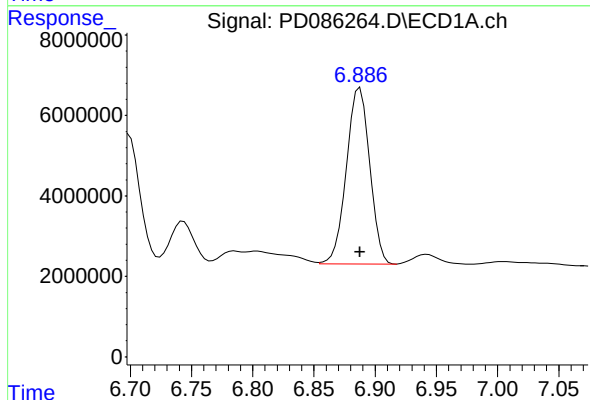


#27 Chlordane-5

R.T.: 6.888 min
Delta R.T.: 0.000 min
Response: 58190438
Conc: 737.90 ng/ml

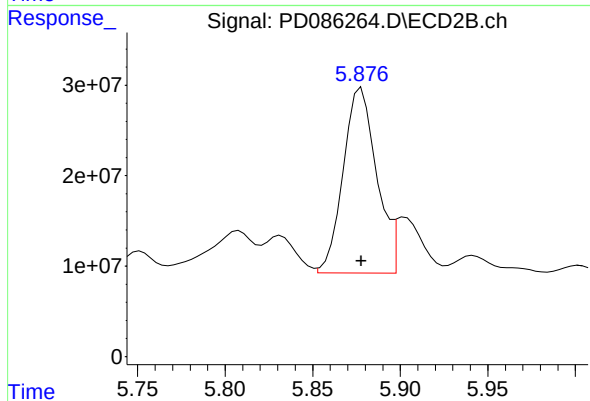

#27 Chlordane-5


R.T.: 5.878 min
Delta R.T.: 0.000 min
Response: 272171460
Conc: 726.05 ng/ml

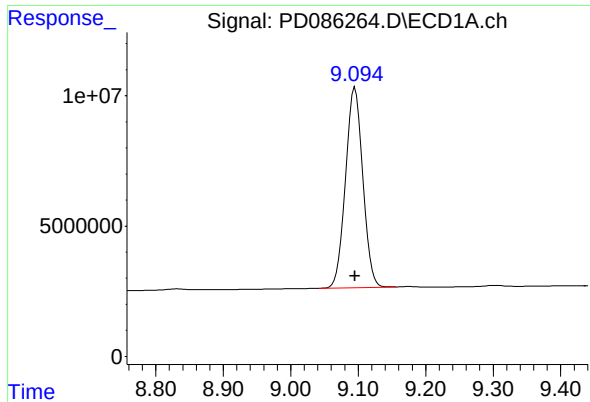

#28 Decachlorobiphenyl

R.T.: 9.095 min
Delta R.T.: 0.000 min
Response: 137276341
Conc: 73.87 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

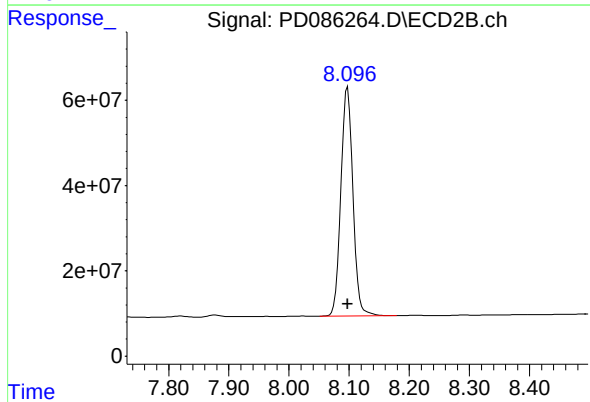

#28 Decachlorobiphenyl

R.T.: 8.098 min
Delta R.T.: 0.000 min
Response: 748944500
Conc: 73.42 ng/ml