

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD103024\
 Data File : PD086265.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Oct 2024 14:26
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 10:02:46 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD103024.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 31 10:02:31 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.562	2.889	71096699	577.0E6	50.000	50.000
28)	SA Decachlor...	9.096	8.098	93618220	525.0E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.731	3.919	43528262	220.6E6	500.000	500.000
24)	Chlordane-2	5.257	4.502	46381472	235.6E6	500.000	500.000
25)	Chlordane-3	5.963	5.143	185.8E6	701.6E6	500.000	500.000
26)	Chlordane-4	6.049	5.208	225.3E6	585.1E6	500.000	500.000
27)	Chlordane-5	6.888	5.878	38804306	192.5E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD103024\
Data File : PD086265.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2024 14:26
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 10:02:46 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD103024.M
Quant Title : GC Extractables
QLast Update : Thu Oct 31 10:02:31 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

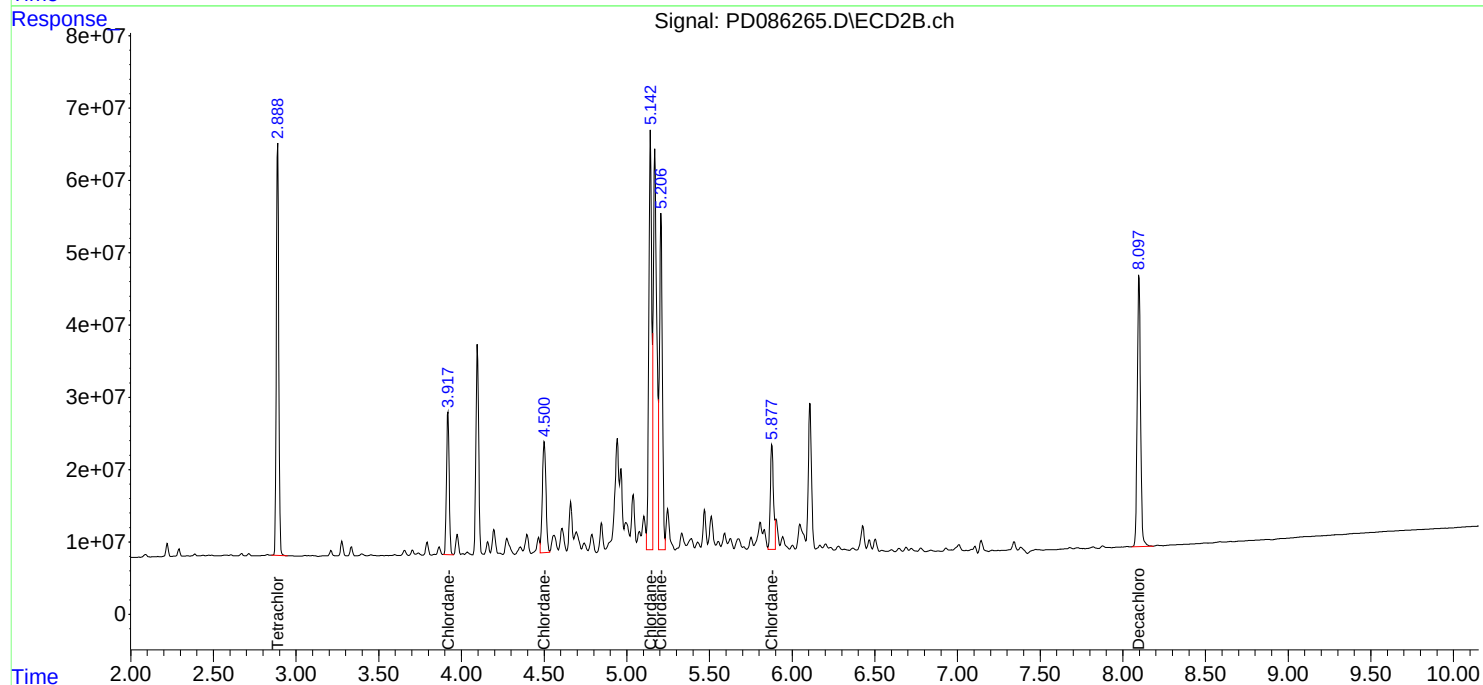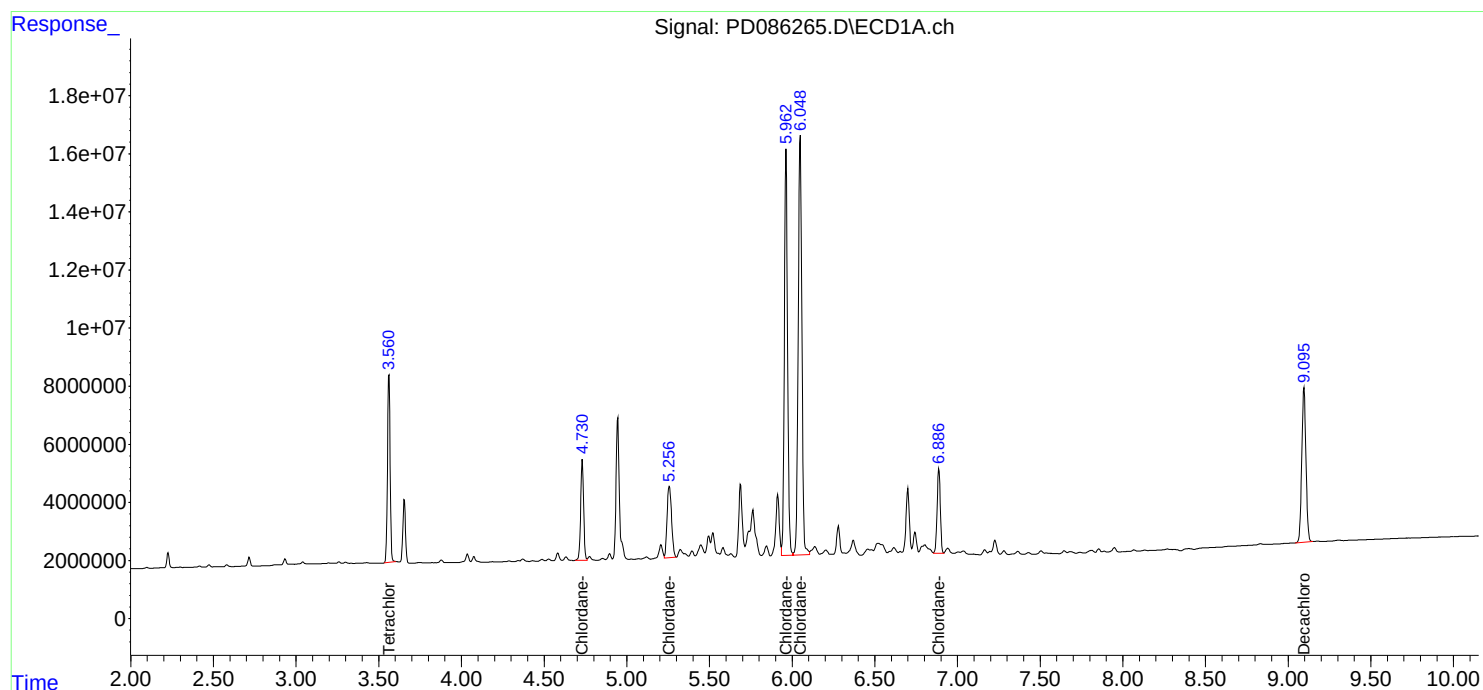


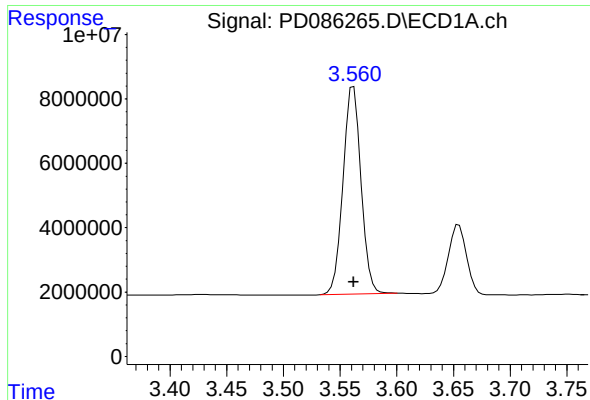

#1 Tetrachloro-m-xylene


R.T.: 3.562 min
Delta R.T.: 0.000 min
Response: 71096699
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

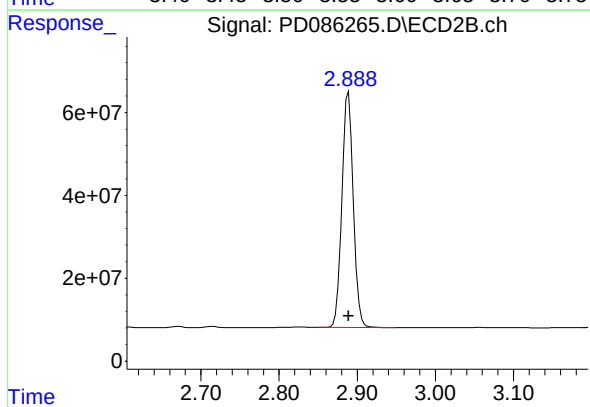


#1 Tetrachloro-m-xylene

R.T.: 2.889 min
Delta R.T.: 0.000 min
Response: 577001354
Conc: 50.00 ng/ml

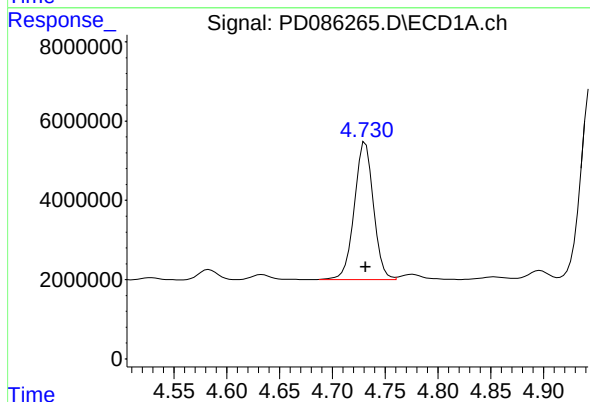


#23 Chlordane-1

R.T.: 4.731 min
Delta R.T.: 0.000 min
Response: 43528262
Conc: 500.00 ng/ml

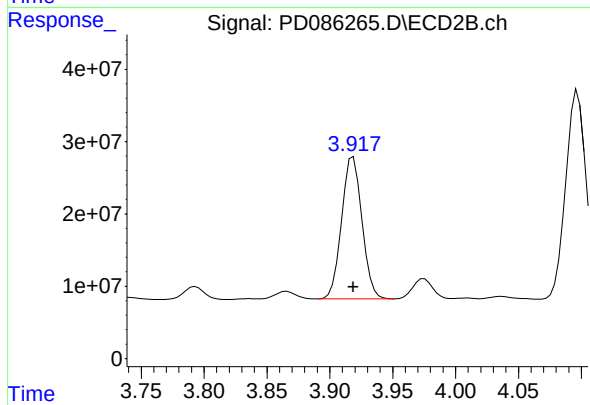

#23 Chlordane-1


R.T.: 3.919 min
Delta R.T.: 0.000 min
Response: 220577504
Conc: 500.00 ng/ml

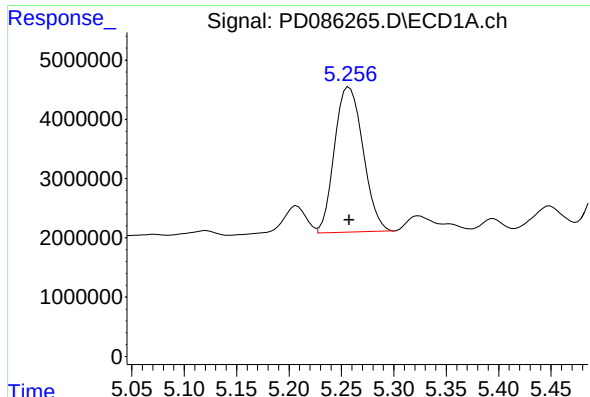

#24 Chlordane-2


R.T.: 5.257 min
Delta R.T.: 0.000 min
Response: 46381472
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

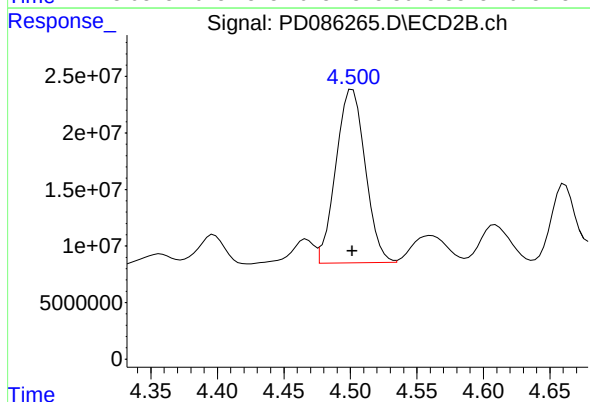


#24 Chlordane-2

R.T.: 4.502 min
Delta R.T.: 0.000 min
Response: 235599353
Conc: 500.00 ng/ml

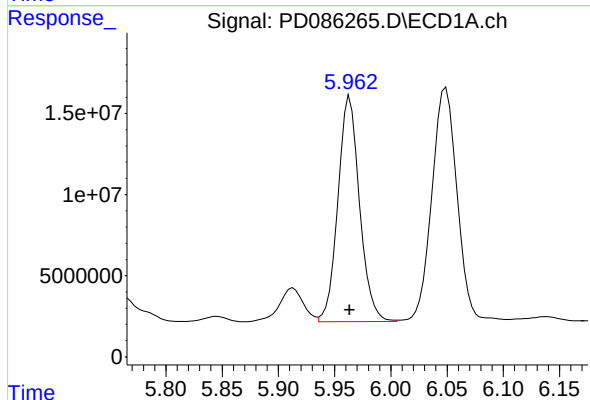


#25 Chlordane-3

R.T.: 5.963 min
Delta R.T.: 0.000 min
Response: 185832496
Conc: 500.00 ng/ml

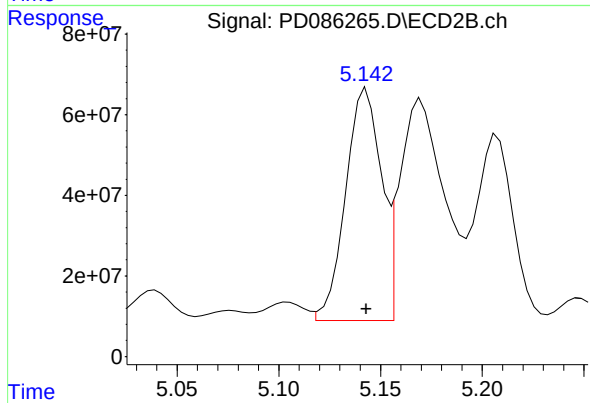

#25 Chlordane-3


R.T.: 5.143 min
Delta R.T.: 0.000 min
Response: 701628212
Conc: 500.00 ng/ml

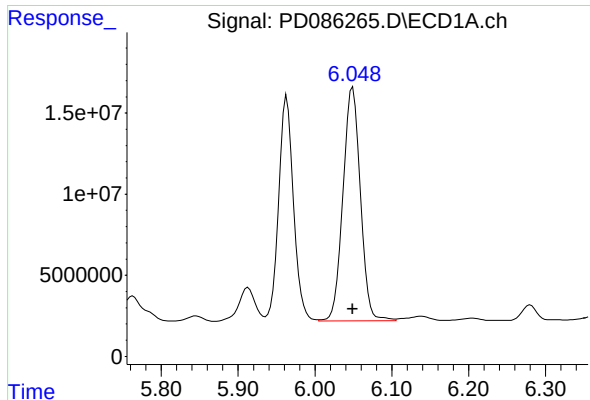

#26 Chlordane-4


R.T.: 6.049 min
Delta R.T.: 0.000 min
Response: 225337182
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

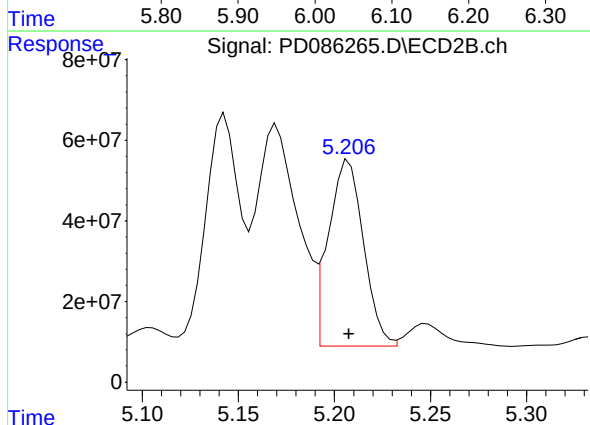


#26 Chlordane-4

R.T.: 5.208 min
Delta R.T.: 0.000 min
Response: 585143738
Conc: 500.00 ng/ml

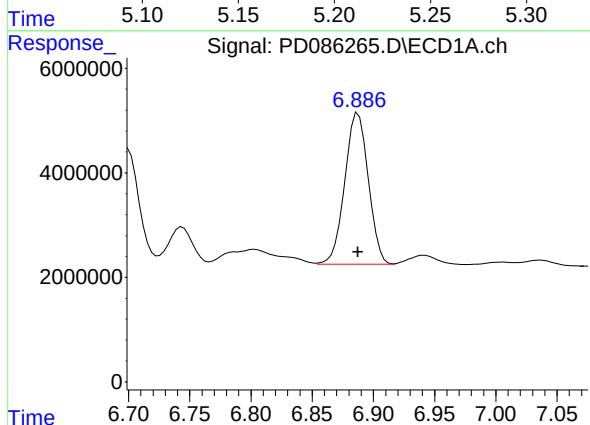


#27 Chlordane-5

R.T.: 6.888 min
Delta R.T.: 0.000 min
Response: 38804306
Conc: 500.00 ng/ml

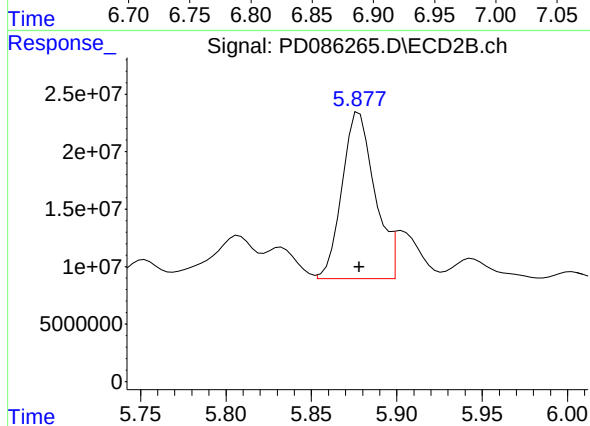

#27 Chlordane-5


R.T.: 5.878 min
Delta R.T.: 0.000 min
Response: 192457713
Conc: 500.00 ng/ml

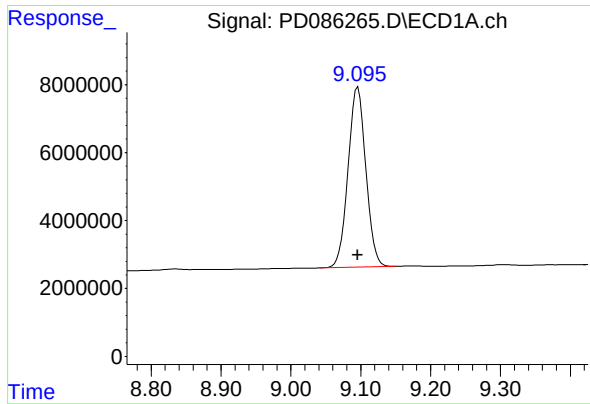

#28 Decachlorobiphenyl

R.T.: 9.096 min
Delta R.T.: 0.000 min
Response: 93618220
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

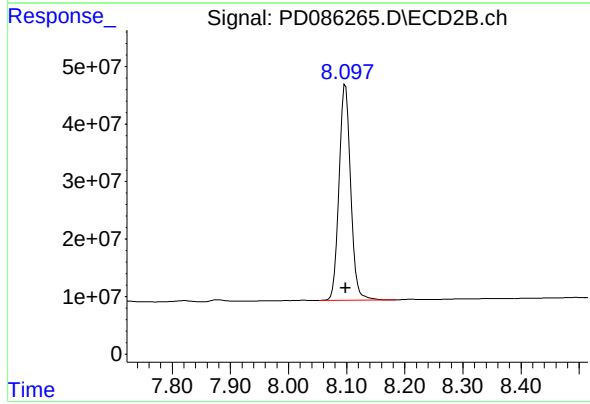

#28 Decachlorobiphenyl

R.T.: 8.098 min
Delta R.T.: 0.000 min
Response: 525005692
Conc: 50.00 ng/ml