

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD103024\
 Data File : PD086266.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Oct 2024 14:40
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 10:09:15 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD103024.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 31 10:02:31 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.562	2.889	36177665	305.6E6	25.193	26.456
28) SA Decachlor...	9.095	8.097	48802729	284.6E6	25.933	27.116
Target Compounds						
23) Chlordane-1	4.730	3.918	21963312	118.0E6	247.640	267.397
24) Chlordane-2	5.258	4.502	24330198	128.4E6	262.185	274.738
25) Chlordane-3	5.963	5.143	90679802	373.9E6	240.680	266.641
26) Chlordane-4	6.049	5.207	111.8E6	314.7E6	245.852	269.486
27) Chlordane-5	6.888	5.878	19532385	103.2E6	248.259	268.535



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD103024\
Data File : PD086266.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2024 14:40
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 10:09:15 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD103024.M
Quant Title : GC Extractables
QLast Update : Thu Oct 31 10:02:31 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

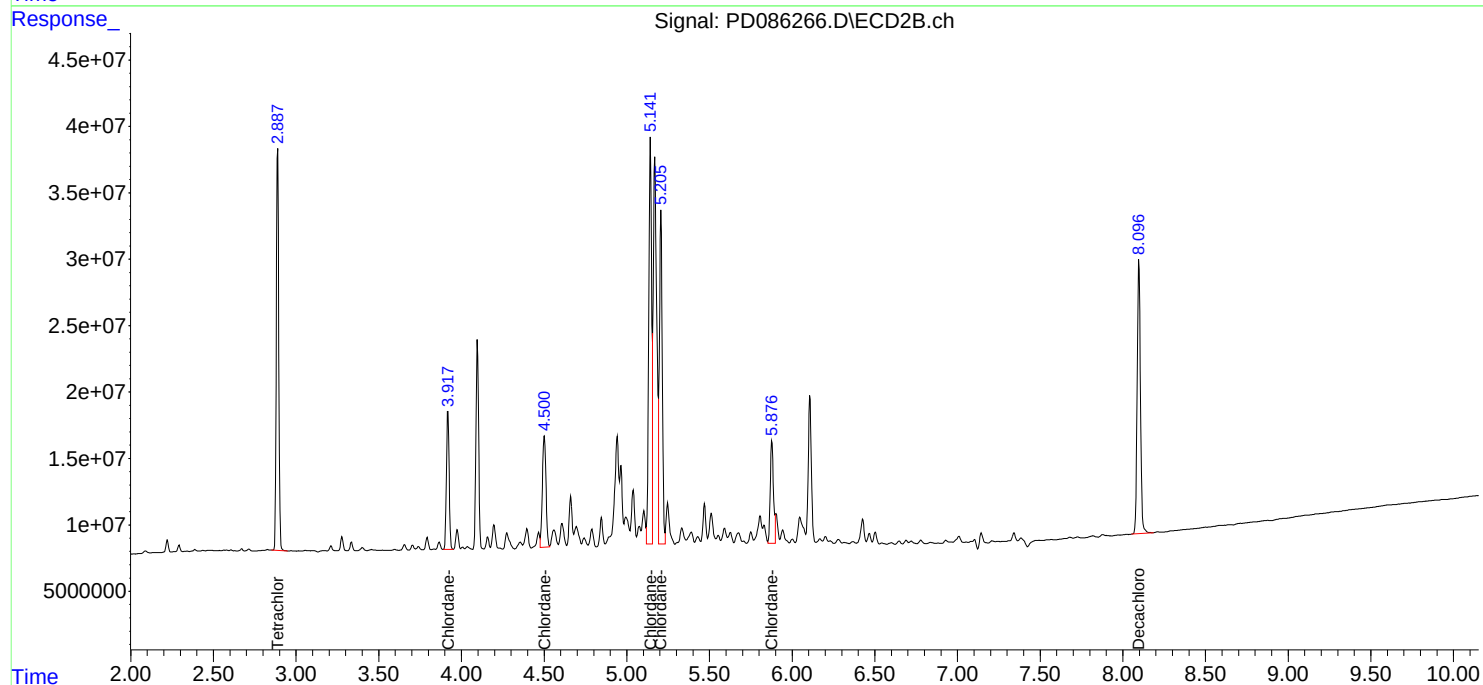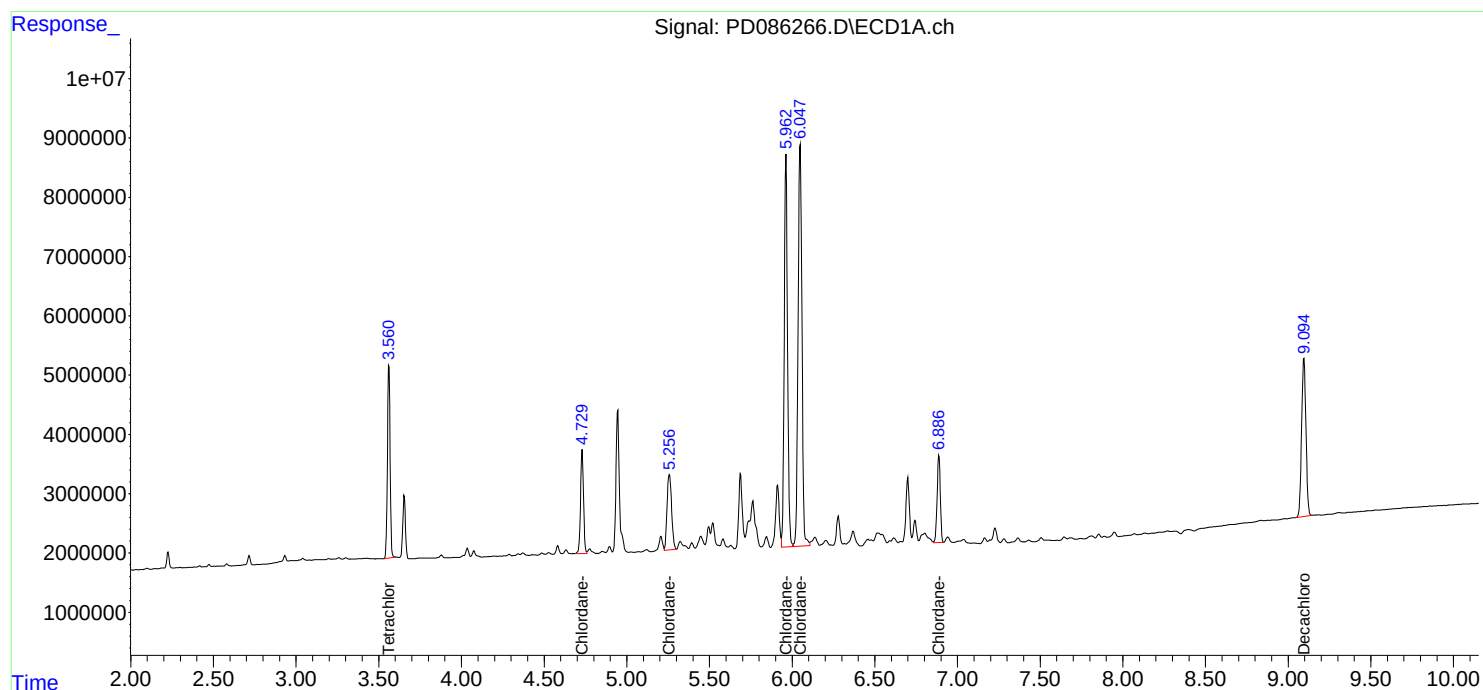


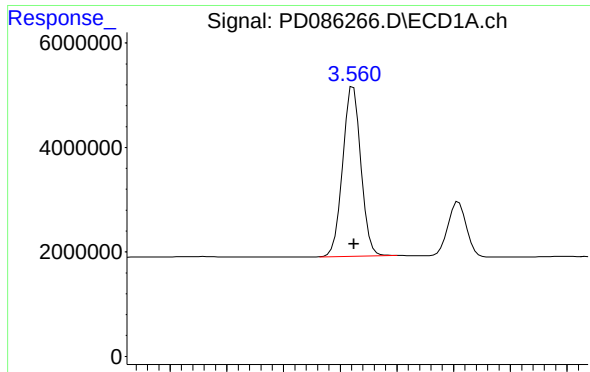

#1 Tetrachloro-m-xylene


R.T.: 3.562 min
Delta R.T.: 0.000 min
Response: 36177665
Conc: 25.19 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

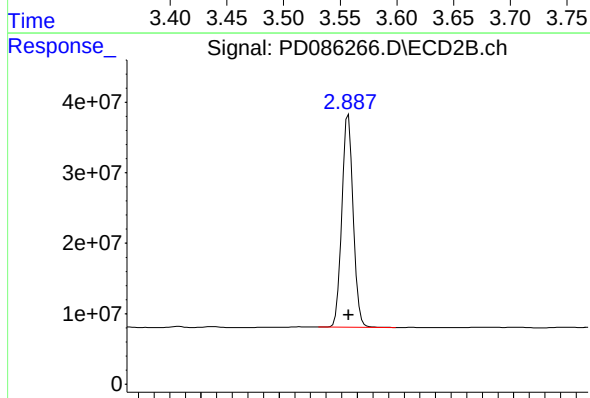


#1 Tetrachloro-m-xylene

R.T.: 2.889 min
Delta R.T.: 0.000 min
Response: 305643302
Conc: 26.46 ng/ml

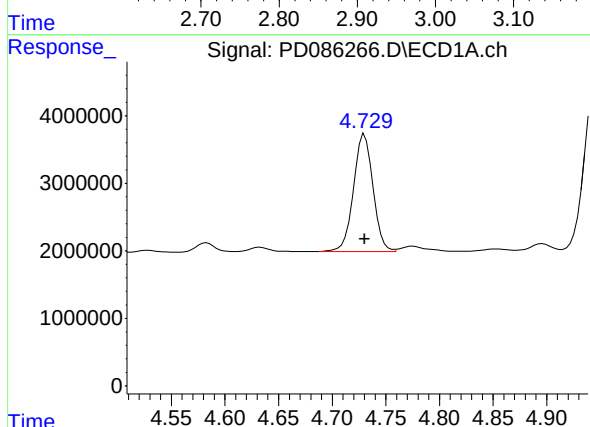


#23 Chlordane-1

R.T.: 4.730 min
Delta R.T.: 0.000 min
Response: 21963312
Conc: 247.64 ng/ml

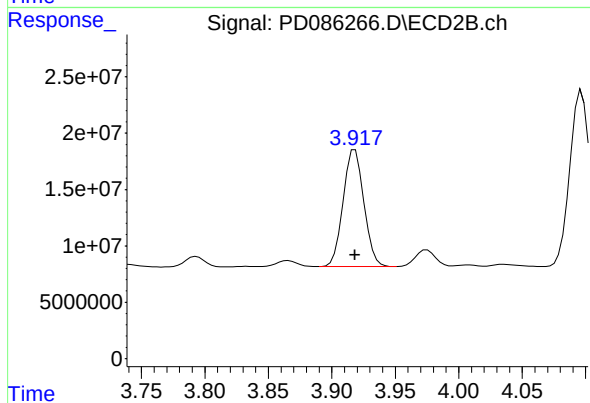

#23 Chlordane-1


R.T.: 3.918 min
Delta R.T.: 0.000 min
Response: 117958409
Conc: 267.40 ng/ml

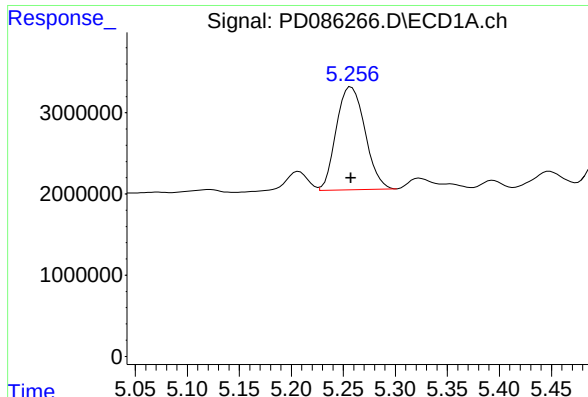

#24 Chlordane-2


R.T.: 5.258 min
Delta R.T.: 0.000 min
Response: 24330198
Conc: 262.18 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

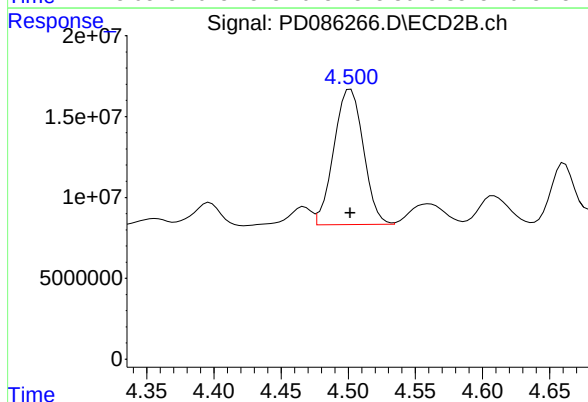


#24 Chlordane-2

R.T.: 4.502 min
Delta R.T.: 0.000 min
Response: 128403881
Conc: 274.74 ng/ml

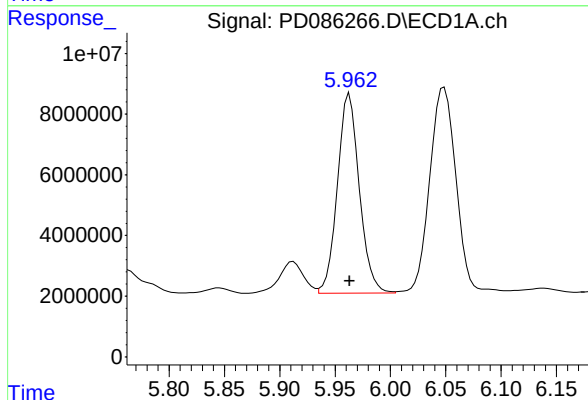


#25 Chlordane-3

R.T.: 5.963 min
Delta R.T.: 0.000 min
Response: 90679802
Conc: 240.68 ng/ml

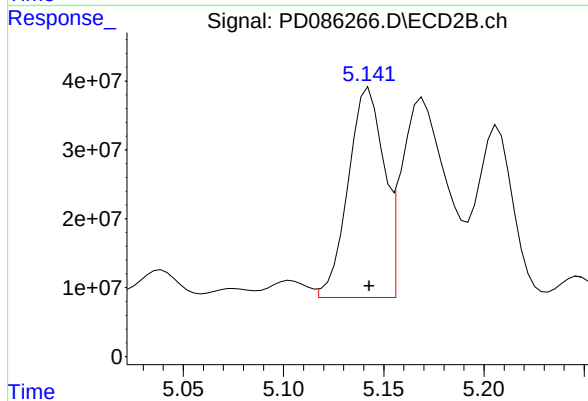

#25 Chlordane-3


R.T.: 5.143 min
Delta R.T.: 0.000 min
Response: 373925601
Conc: 266.64 ng/ml

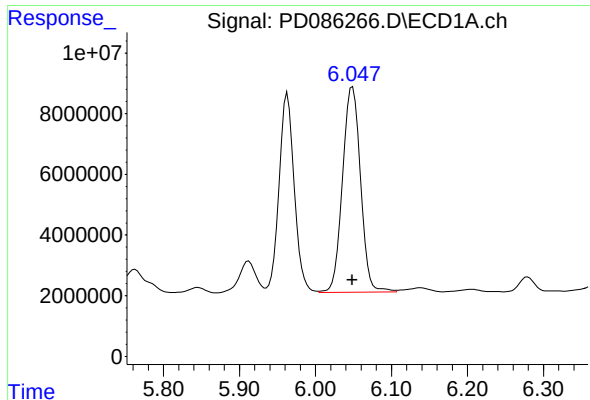

#26 Chlordane-4


R.T.: 6.049 min
Delta R.T.: 0.000 min
Response: 111792966
Conc: 245.85 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

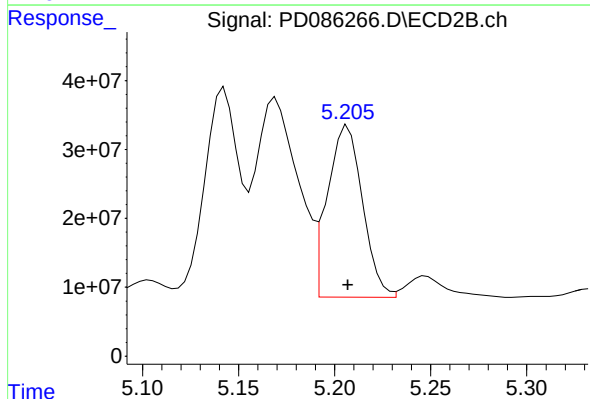


#26 Chlordane-4

R.T.: 5.207 min
Delta R.T.: 0.000 min
Response: 314692802
Conc: 269.49 ng/ml

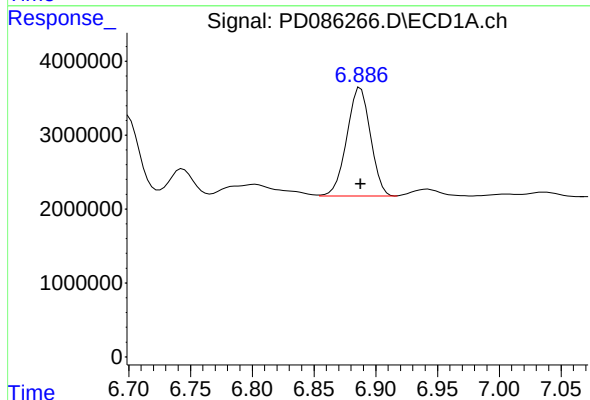


#27 Chlordane-5

R.T.: 6.888 min
Delta R.T.: 0.000 min
Response: 19532385
Conc: 248.26 ng/ml

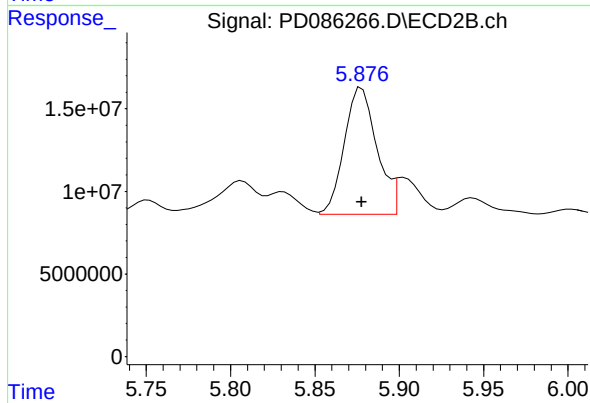

#27 Chlordane-5


R.T.: 5.878 min
Delta R.T.: 0.000 min
Response: 103214989
Conc: 268.54 ng/ml

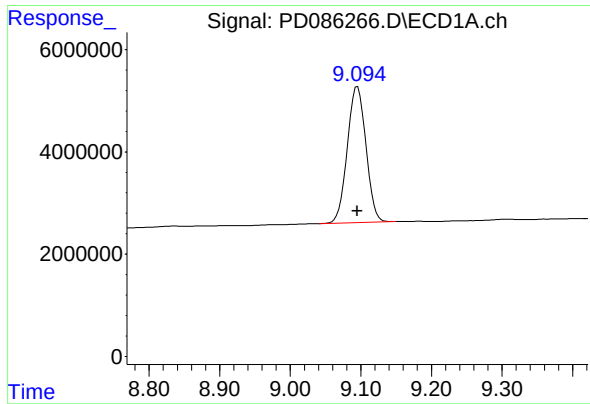

#28 Decachlorobiphenyl

R.T.: 9.095 min
Delta R.T.: 0.000 min
Response: 48802729
Conc: 25.93 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

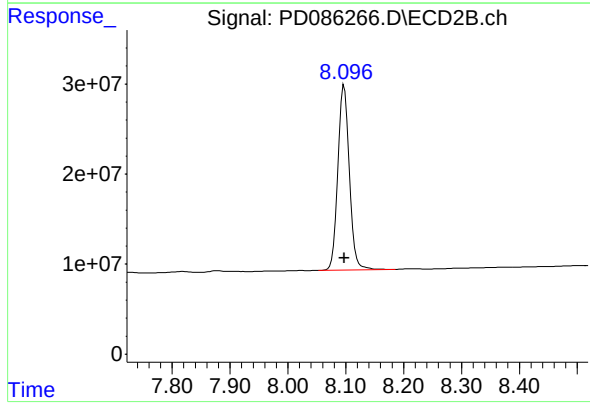

#28 Decachlorobiphenyl

R.T.: 8.097 min
Delta R.T.: 0.000 min
Response: 284619962
Conc: 27.12 ng/ml