

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD103024\
 Data File : PD086267.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Oct 2024 14:54
 Operator : AR\AJ
 Sample : PCHLORICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 10:11:05 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD103024.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 31 10:02:31 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.561	2.889	8037522	71405098	5.467	5.902
28) SA Decachlor...	9.095	8.098	10575177	68856091	5.484	6.175
Target Compounds						
23) Chlordane-1	4.730	3.919	4754081	28031358	52.841	60.278
24) Chlordane-2	5.257	4.502	5861698	30369750	60.006	61.307
25) Chlordane-3	5.962	5.143	19223804	91752623	50.815	61.625
26) Chlordane-4	6.048	5.207	23911299	80492839	52.047	64.078
27) Chlordane-5	6.888	5.878	4377445	25190304	54.411	61.703



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD103024\
Data File : PD086267.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2024 14:54
Operator : AR\AJ
Sample : PCHLORICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 10:11:05 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD103024.M
Quant Title : GC Extractables
QLast Update : Thu Oct 31 10:02:31 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

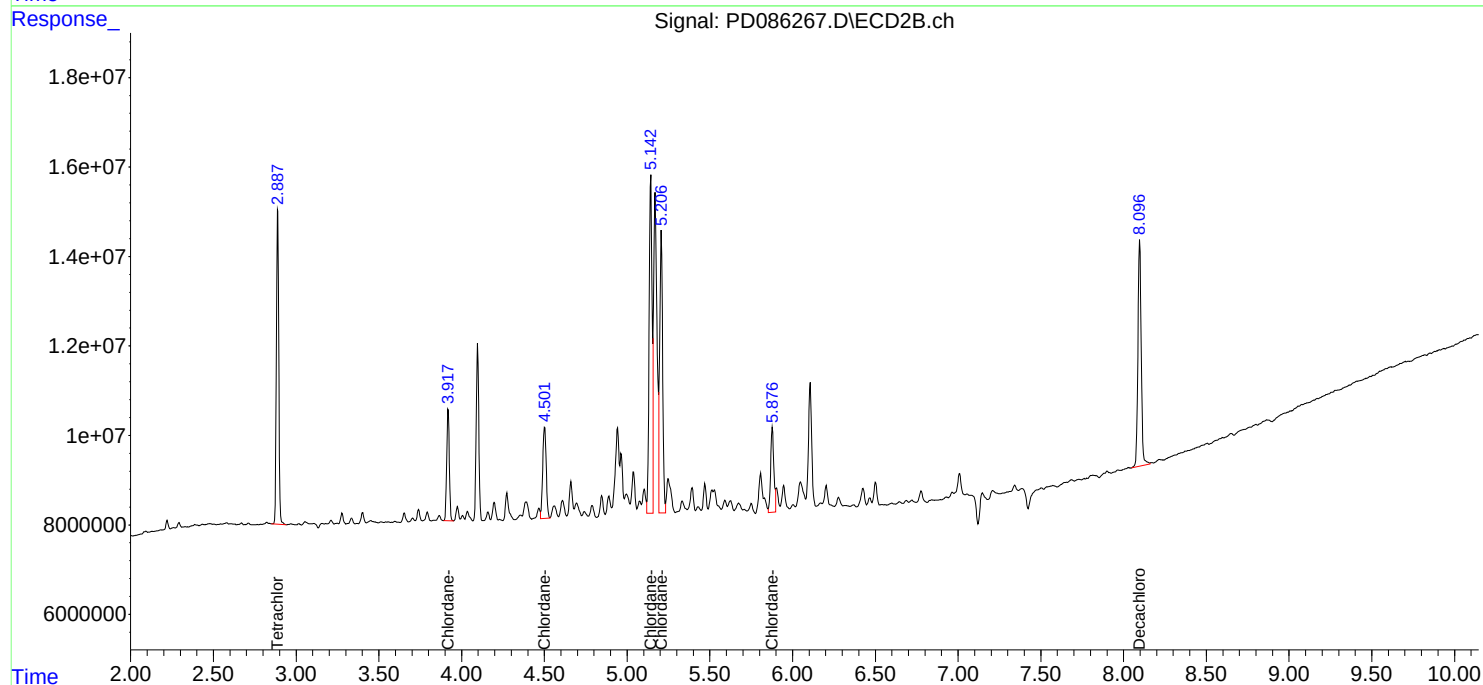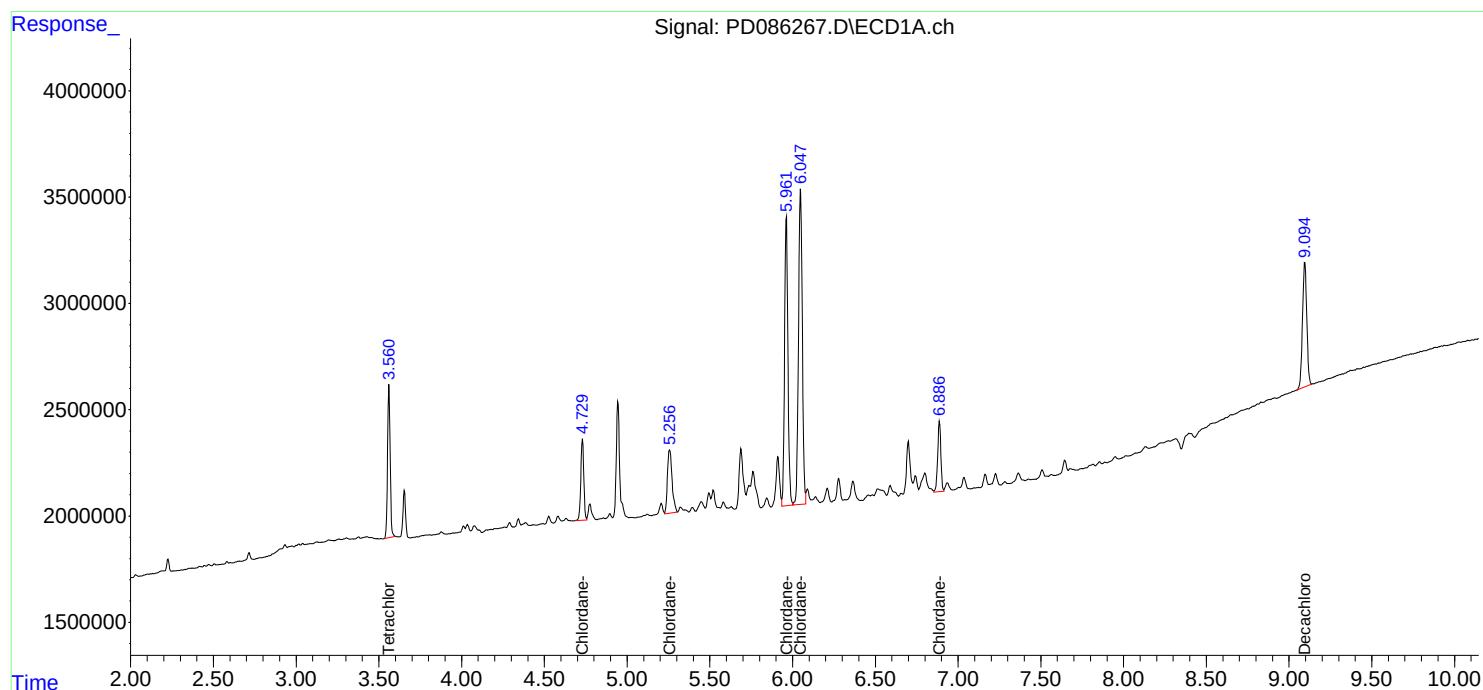


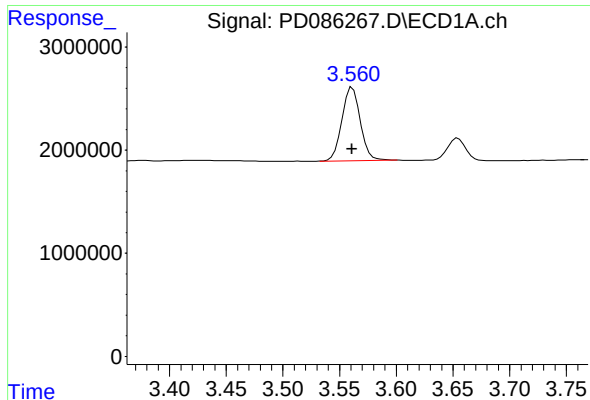

#1 Tetrachloro-m-xylene


R.T.: 3.561 min
Delta R.T.: 0.000 min
Response: 8037522
Conc: 5.47 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

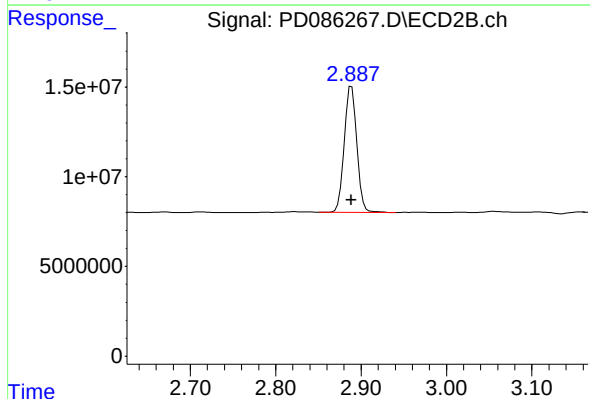


#1 Tetrachloro-m-xylene

R.T.: 2.889 min
Delta R.T.: 0.000 min
Response: 71405098
Conc: 5.90 ng/ml

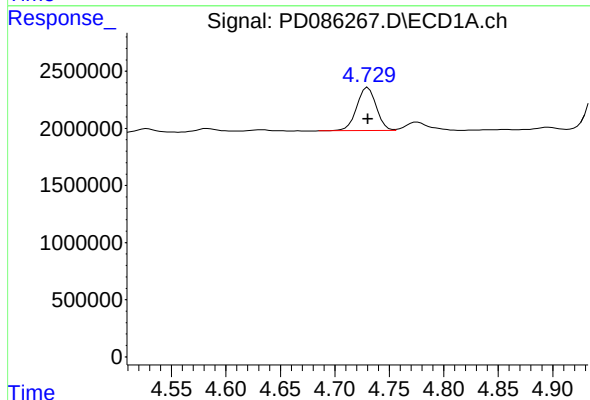


#23 Chlordane-1

R.T.: 4.730 min
Delta R.T.: 0.000 min
Response: 4754081
Conc: 52.84 ng/ml

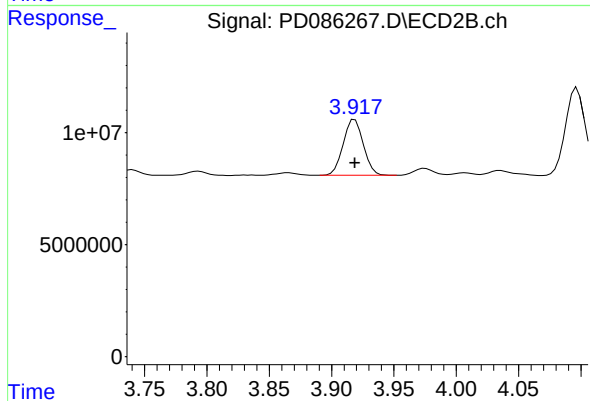

#23 Chlordane-1


R.T.: 3.919 min
Delta R.T.: 0.000 min
Response: 28031358
Conc: 60.28 ng/ml

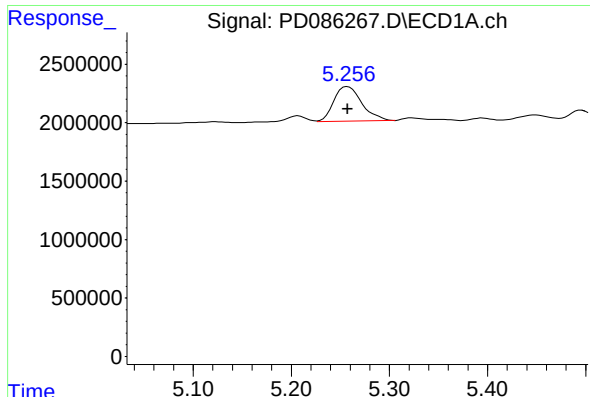

#24 Chlordane-2


R.T.: 5.257 min
Delta R.T.: 0.000 min
Response: 5861698
Conc: 60.01 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

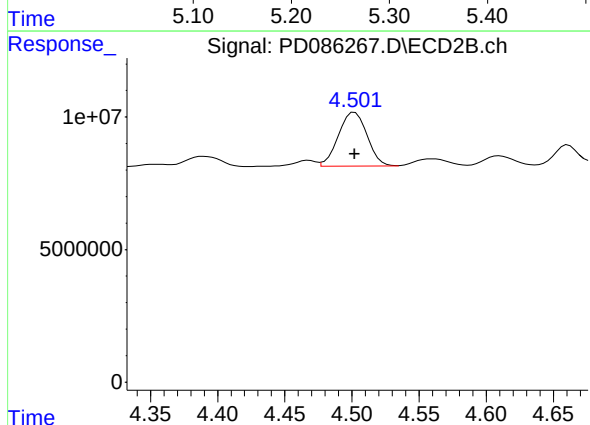


#24 Chlordane-2

R.T.: 4.502 min
Delta R.T.: 0.000 min
Response: 30369750
Conc: 61.31 ng/ml

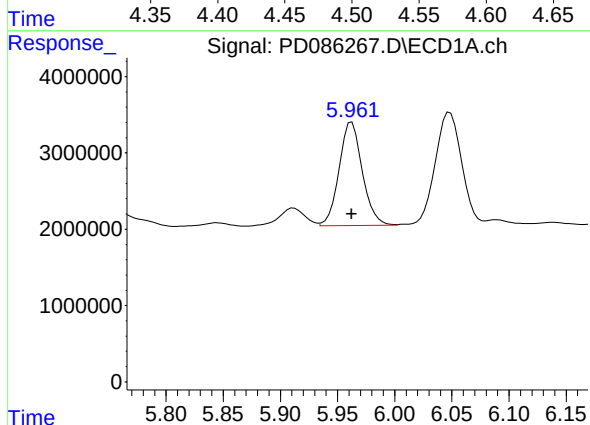


#25 Chlordane-3

R.T.: 5.962 min
Delta R.T.: 0.000 min
Response: 19223804
Conc: 50.82 ng/ml

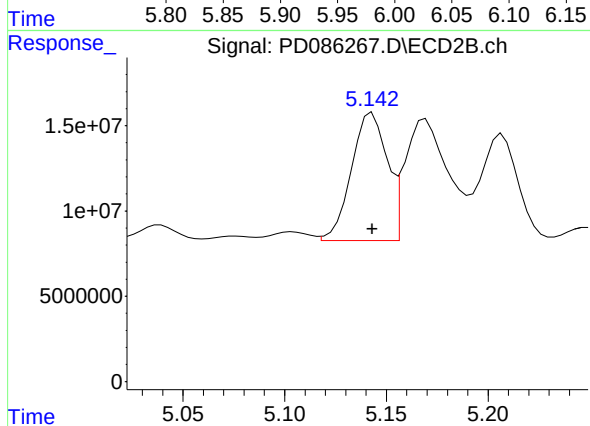

#25 Chlordane-3


R.T.: 5.143 min
Delta R.T.: 0.000 min
Response: 91752623
Conc: 61.62 ng/ml

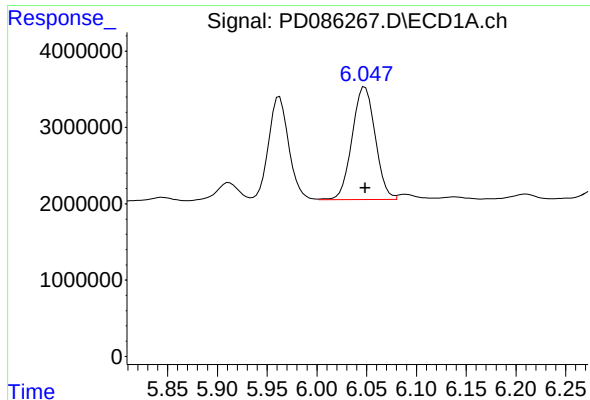

#26 Chlordane-4


R.T.: 6.048 min
Delta R.T.: 0.000 min
Response: 23911299
Conc: 52.05 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

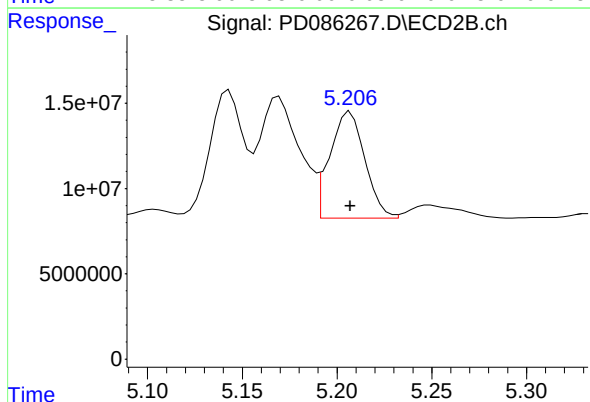


#26 Chlordane-4

R.T.: 5.207 min
Delta R.T.: 0.000 min
Response: 80492839
Conc: 64.08 ng/ml

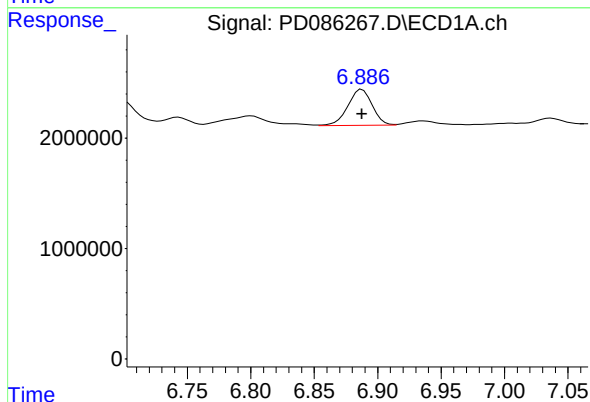


#27 Chlordane-5

R.T.: 6.888 min
Delta R.T.: 0.000 min
Response: 4377445
Conc: 54.41 ng/ml

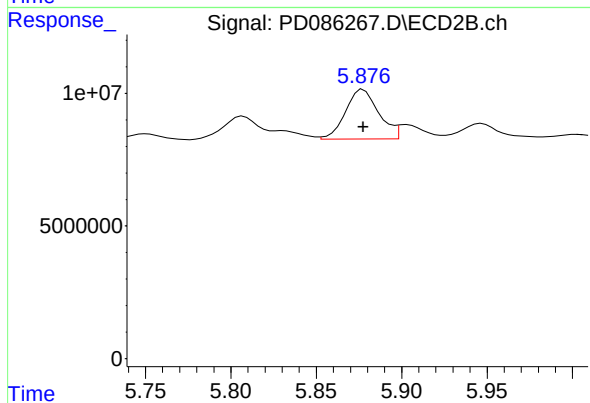

#27 Chlordane-5


R.T.: 5.878 min
Delta R.T.: 0.000 min
Response: 25190304
Conc: 61.70 ng/ml

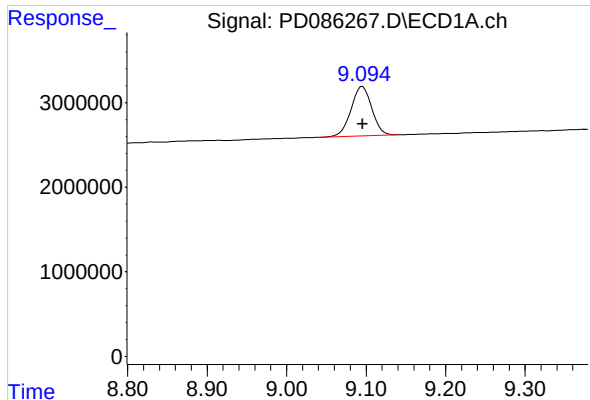

#28 Decachlorobiphenyl

R.T.: 9.095 min
Delta R.T.: 0.000 min
Response: 10575177
Conc: 5.48 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

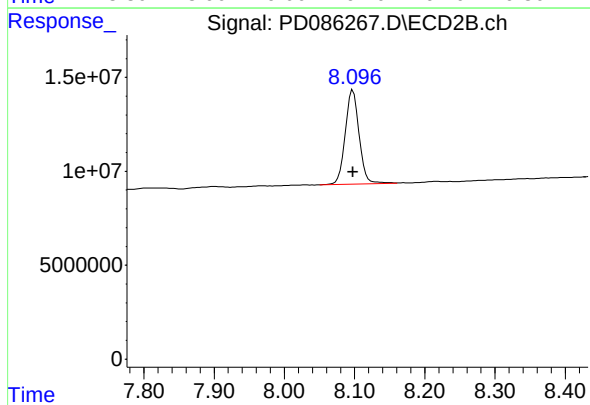

#28 Decachlorobiphenyl

R.T.: 8.098 min
Delta R.T.: 0.000 min
Response: 68856091
Conc: 6.17 ng/ml