

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD103024\
 Data File : PD086274.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Oct 2024 16:47
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ICVPD103024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 10:12:40 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD103024.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 31 10:11:59 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.561	2.889	73081001	594.2E6	49.704	49.115
28) SA Decachlor...	9.095	8.098	96167810	541.3E6	49.866	48.542
Target Compounds						
23) Chlordane-1	4.731	3.918	44889841	228.6E6	498.949	491.658
24) Chlordane-2	5.258	4.501	47672959	242.7E6	488.027	489.911
25) Chlordane-3	5.963	5.143	191.7E6	727.5E6	506.700	488.643
26) Chlordane-4	6.049	5.207	231.8E6	604.6E6	504.518	481.268
27) Chlordane-5	6.888	5.878	39862414	198.6E6	495.483	486.400



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD103024\
Data File : PD086274.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2024 16:47
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
ICVPD103024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 10:12:40 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD103024.M
Quant Title : GC Extractables
QLast Update : Thu Oct 31 10:11:59 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

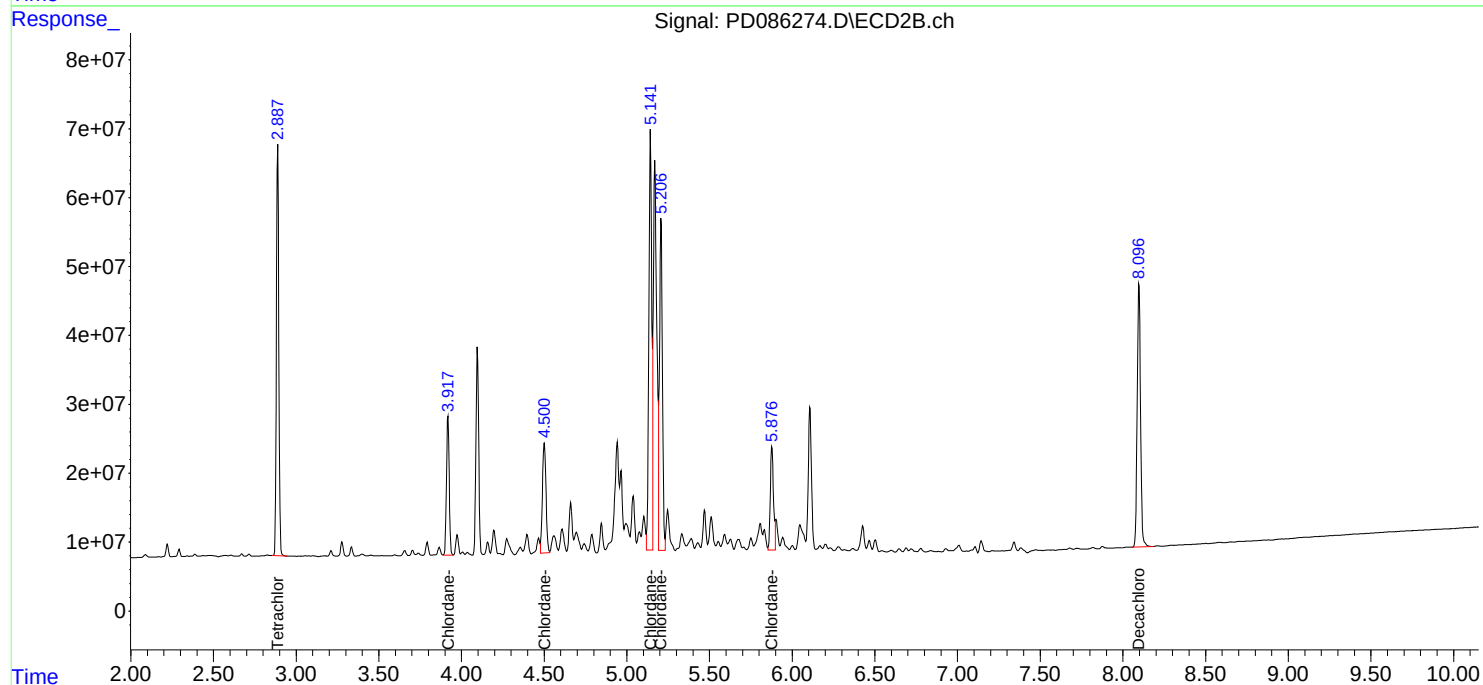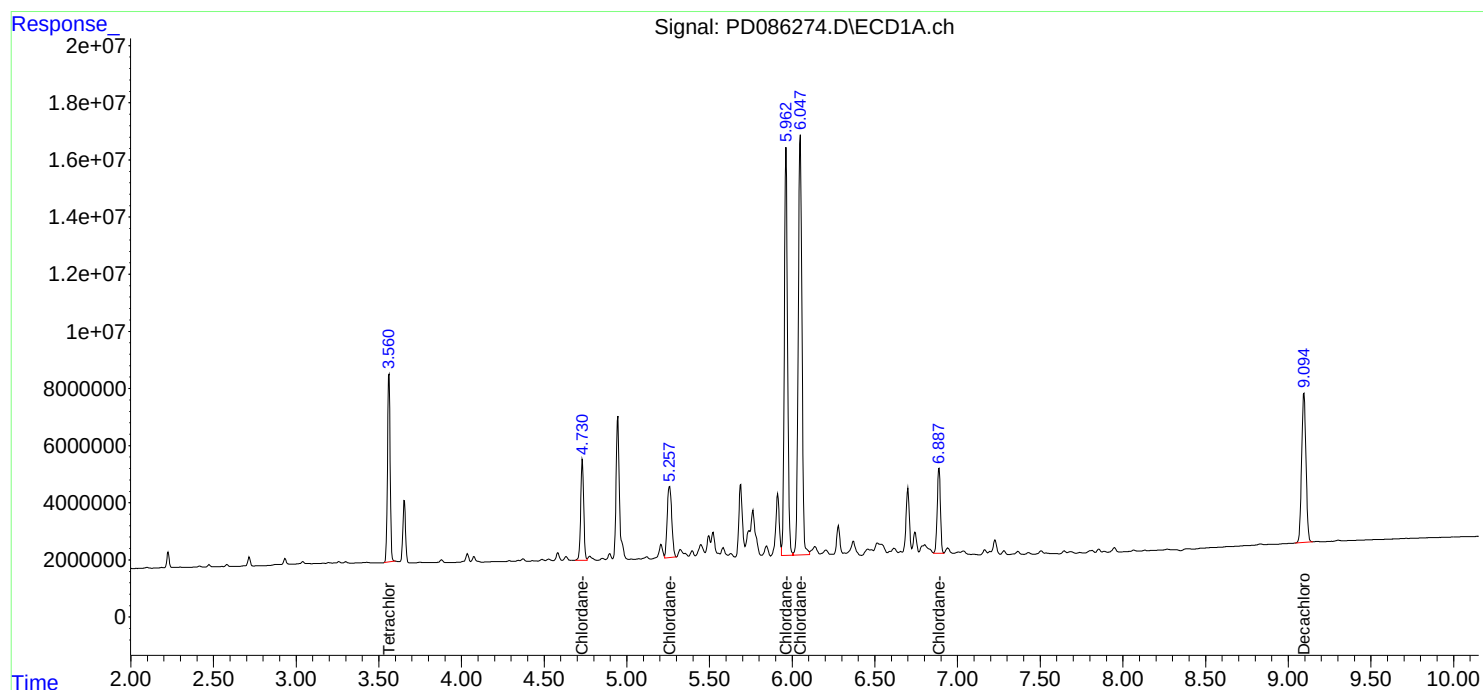


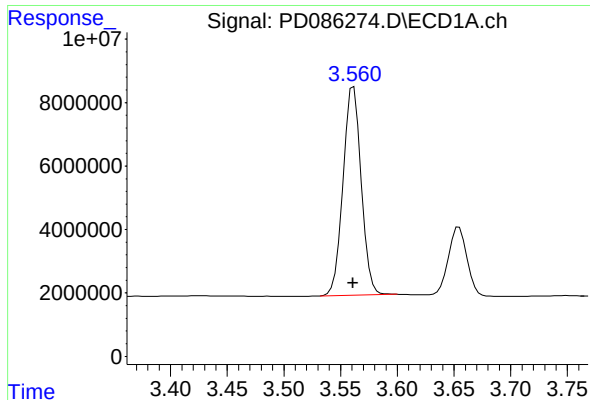

#1 Tetrachloro-m-xylene


R.T.: 3.561 min
Delta R.T.: 0.000 min
Response: 73081001
Conc: 49.70 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD103024

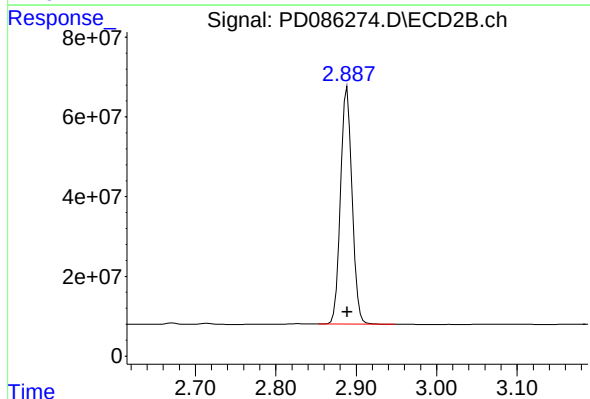


#1 Tetrachloro-m-xylene

R.T.: 2.889 min
Delta R.T.: 0.000 min
Response: 594220771
Conc: 49.12 ng/ml

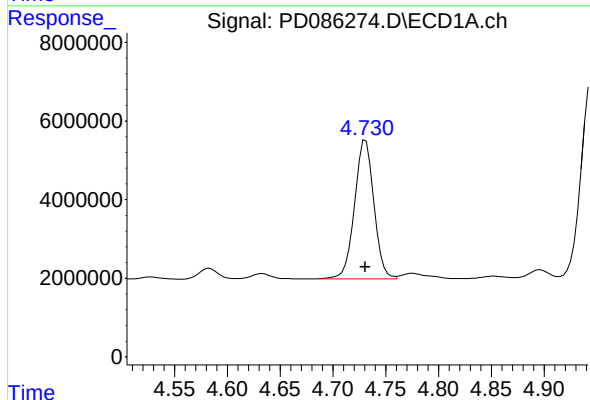


#23 Chlordane-1

R.T.: 4.731 min
Delta R.T.: 0.000 min
Response: 44889841
Conc: 498.95 ng/ml

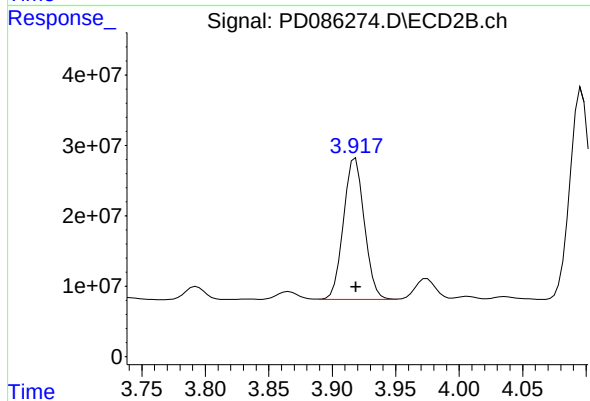

#23 Chlordane-1


R.T.: 3.918 min
Delta R.T.: 0.000 min
Response: 228637789
Conc: 491.66 ng/ml

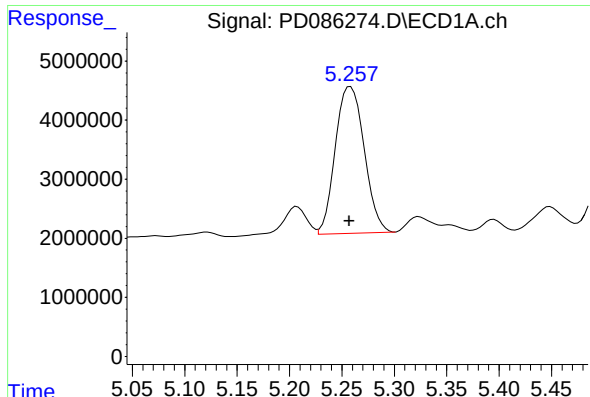

#24 Chlordane-2


R.T.: 5.258 min
Delta R.T.: 0.000 min
Response: 47672959
Conc: 488.03 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD103024

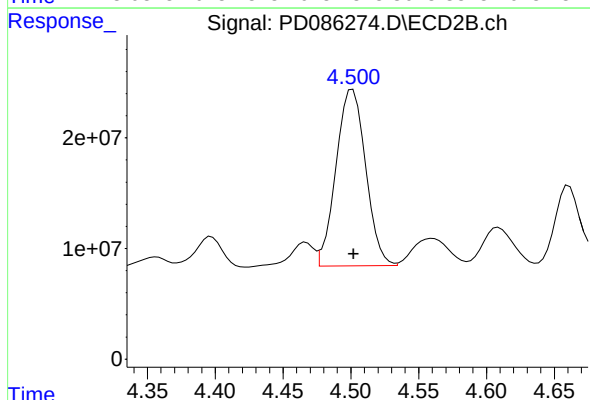


#24 Chlordane-2

R.T.: 4.501 min
Delta R.T.: 0.000 min
Response: 242689195
Conc: 489.91 ng/ml

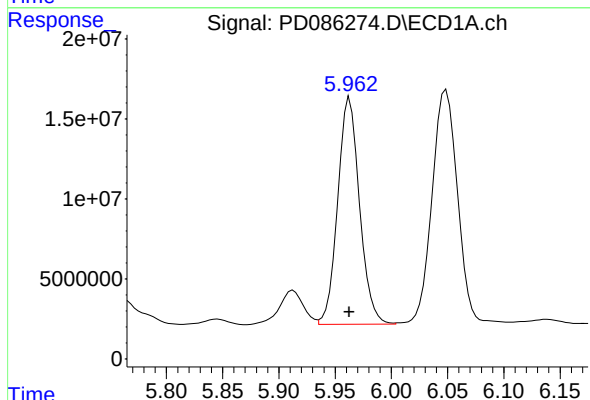


#25 Chlordane-3

R.T.: 5.963 min
Delta R.T.: 0.000 min
Response: 191688235
Conc: 506.70 ng/ml

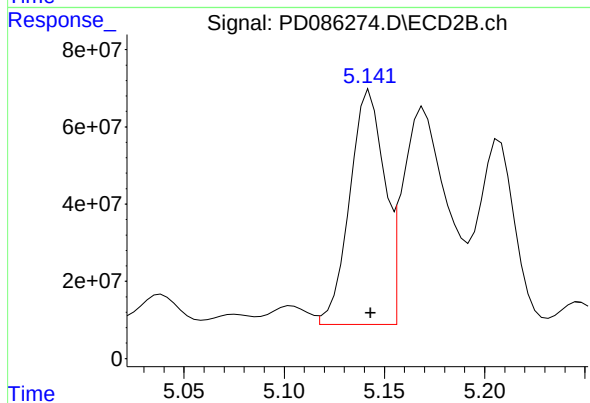

#25 Chlordane-3


R.T.: 5.143 min
Delta R.T.: 0.000 min
Response: 727538216
Conc: 488.64 ng/ml

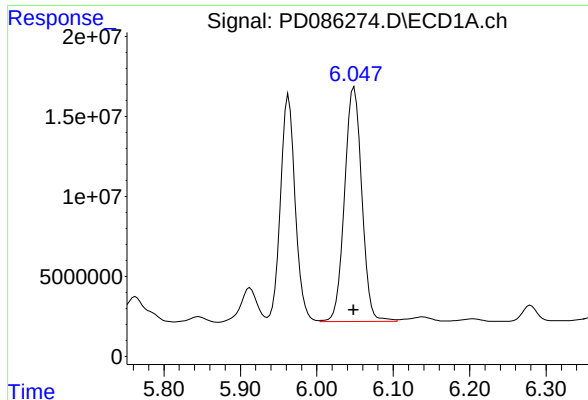

#26 Chlordane-4


R.T.: 6.049 min
Delta R.T.: 0.000 min
Response: 231784526
Conc: 504.52 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD103024

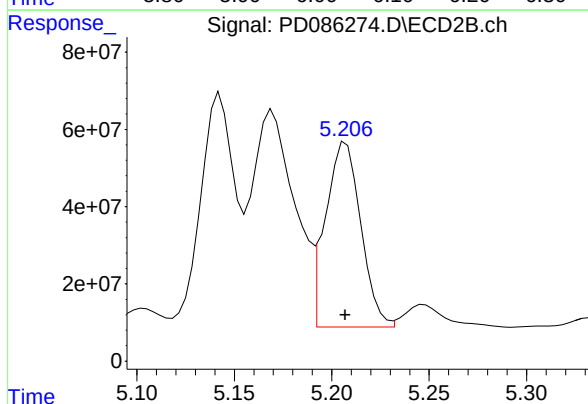


#26 Chlordane-4

R.T.: 5.207 min
Delta R.T.: 0.000 min
Response: 604556124
Conc: 481.27 ng/ml

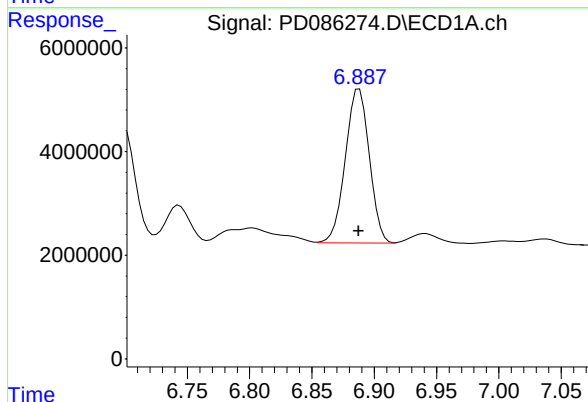


#27 Chlordane-5

R.T.: 6.888 min
Delta R.T.: 0.000 min
Response: 39862414
Conc: 495.48 ng/ml

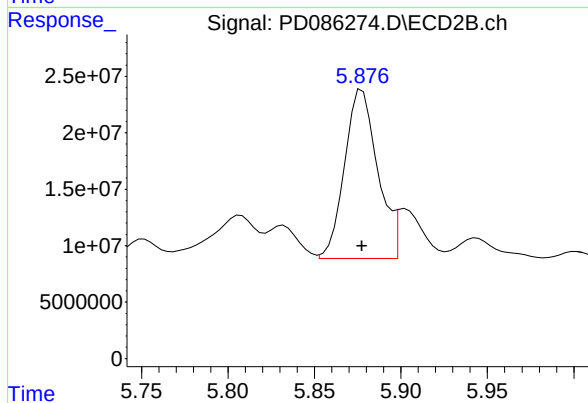

#27 Chlordane-5


R.T.: 5.878 min
Delta R.T.: 0.000 min
Response: 198573447
Conc: 486.40 ng/ml

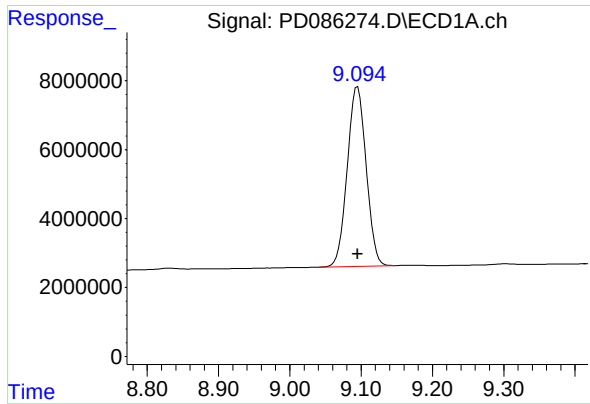

#28 Decachlorobiphenyl

R.T.: 9.095 min
Delta R.T.: 0.000 min
Response: 96167810
Conc: 49.87 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD103024

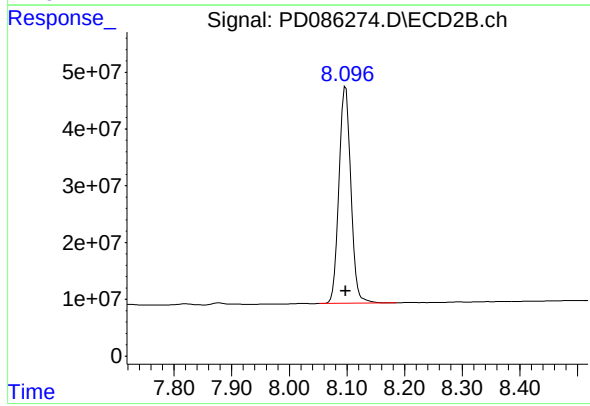

#28 Decachlorobiphenyl

R.T.: 8.098 min
Delta R.T.: 0.000 min
Response: 541318014
Conc: 48.54 ng/ml