

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD103119\
 Data File : PD055707.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Oct 2019 19:40
 Operator : SG\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA401

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 07:18:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD103119CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 31 07:11:18 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.289	3.963	33838030	46506979	38.447	38.031
27)	SA Decachlor...	7.963	8.997	72952550	101.8E6	74.827	73.828
Target Compounds							
2)	A alpha-BHC	3.716	4.349	49860395	67991449	40.267	39.263
3)	MA gamma-BHC...	3.992	4.632	46464620	66101293	37.967	39.543
4)	MA Heptachlor	4.277	5.138	42500715	68445595	38.530	38.217
9)	A Endosulfan I	5.283	6.180	39309088	60617732	38.485	38.132
13)	MA Dieldrin	5.523	6.436	90104946	136.4E6	79.257	78.341
14)	MA Endrin	5.776	6.653	75196805	110.5E6	78.216	77.743
16)	A 4,4'-DDD	5.911	6.775	66814086	109.4E6	79.725	79.341
17)	MA 4,4'-DDT	6.146	7.073	65100584	111.1E6	82.561	79.960
20)	A Methoxychlor	6.694	7.529	163.7E6	296.6E6	386.462	379.348


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD103119\
Data File : PD055707.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2019 19:40
Operator : SG\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
INDA401

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 07:18:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD103119CLP.M
Quant Title : GC Extractables
QLast Update : Thu Oct 31 07:11:18 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

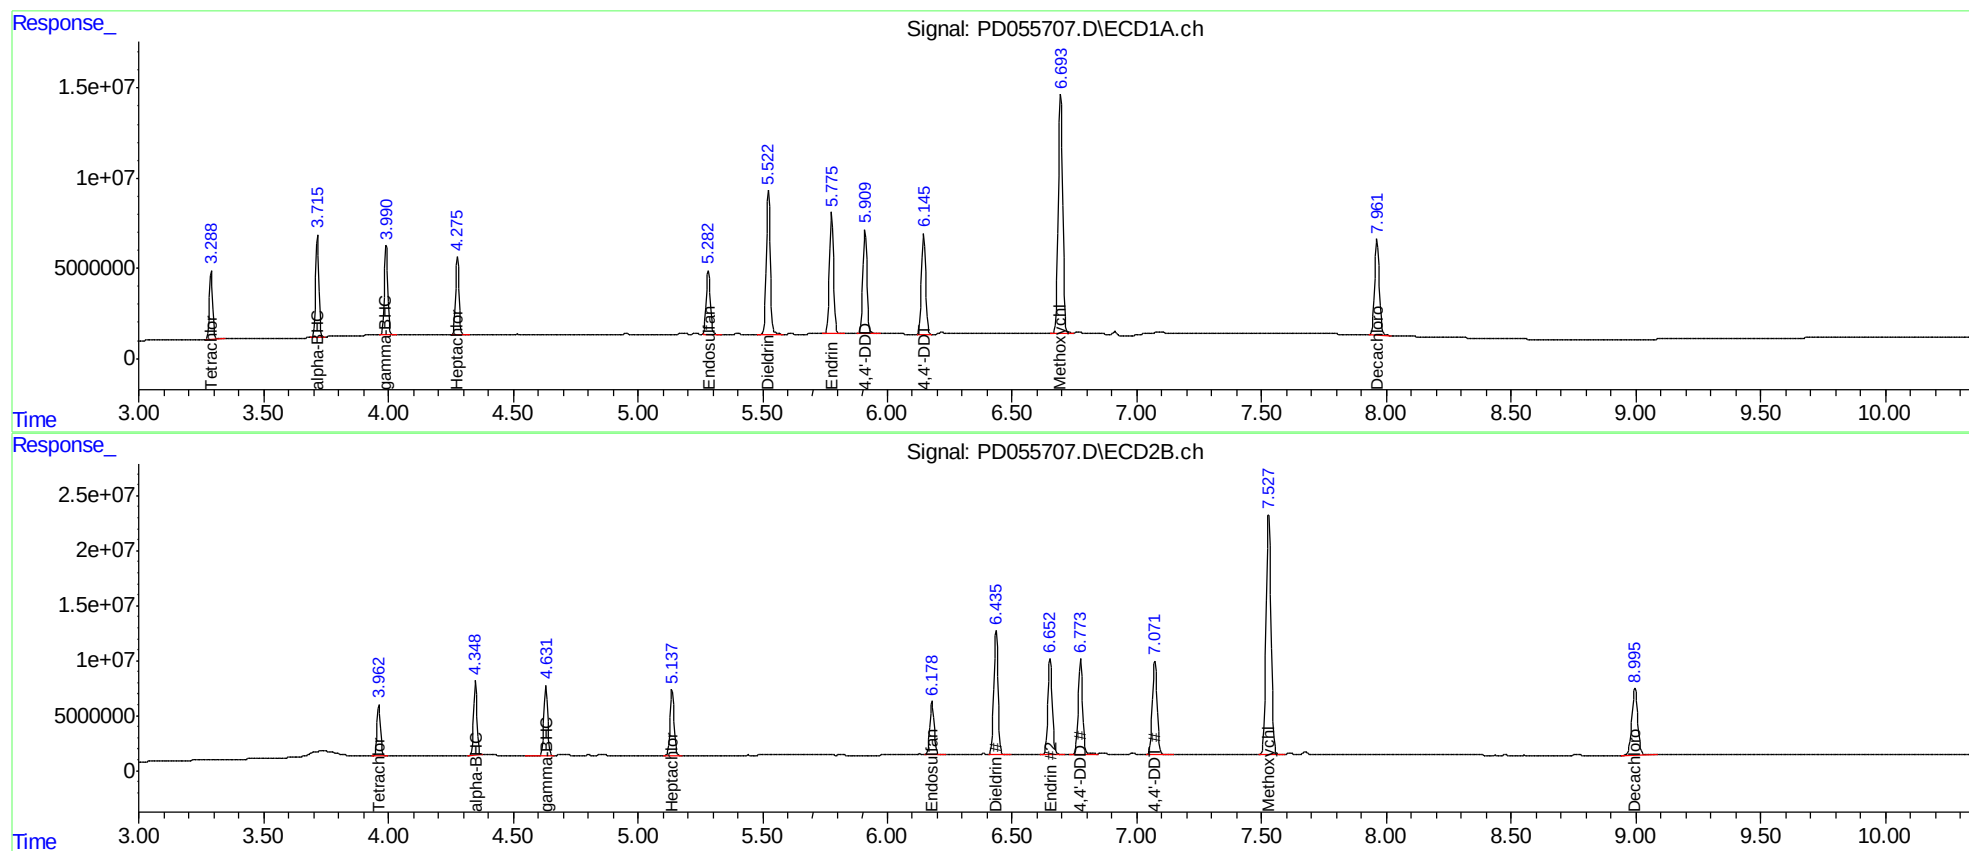


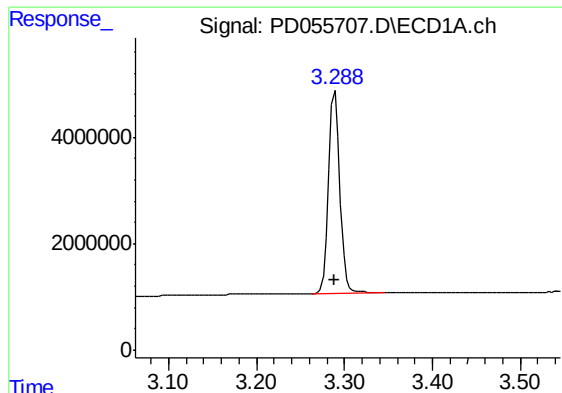

#1 Tetrachloro-m-xylene


R.T.: 3.289 min
Delta R.T.: 0.000 min
Response: 33838030
Conc: 38.45 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA401

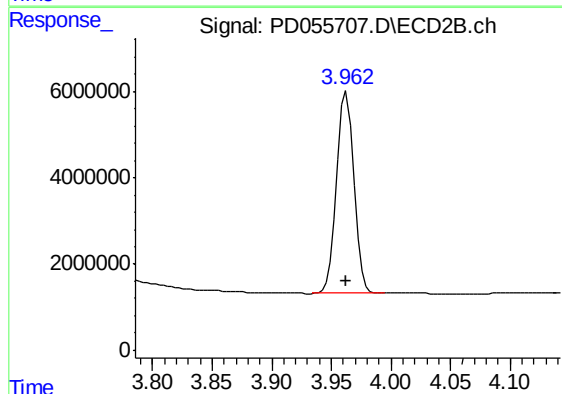


#1 Tetrachloro-m-xylene

R.T.: 3.963 min
Delta R.T.: 0.000 min
Response: 46506979
Conc: 38.03 ng/ml

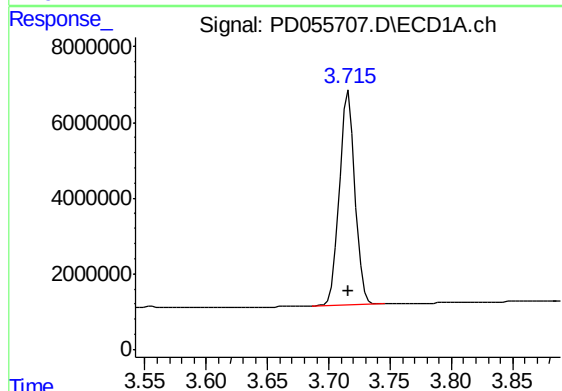


#2 alpha-BHC

R.T.: 3.716 min
Delta R.T.: 0.000 min
Response: 49860395
Conc: 40.27 ng/ml

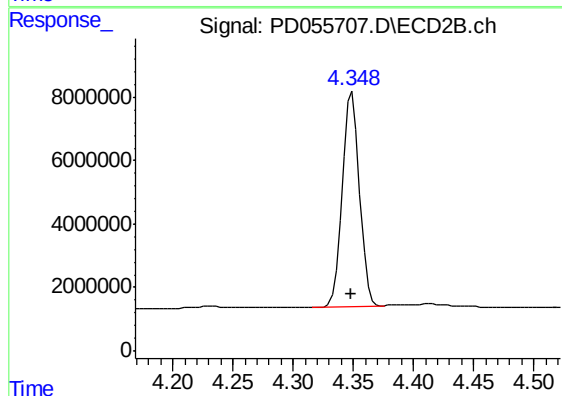

#2 alpha-BHC


R.T.: 4.349 min
Delta R.T.: 0.000 min
Response: 67991449
Conc: 39.26 ng/ml

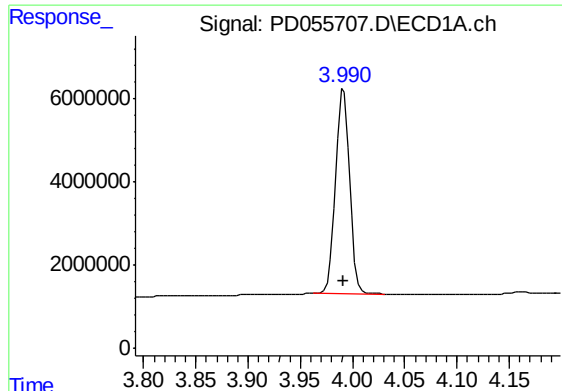

#3 gamma-BHC (Lindane)


R.T.: 3.992 min
Delta R.T.: 0.000 min
Response: 46464620
Conc: 37.97 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA401

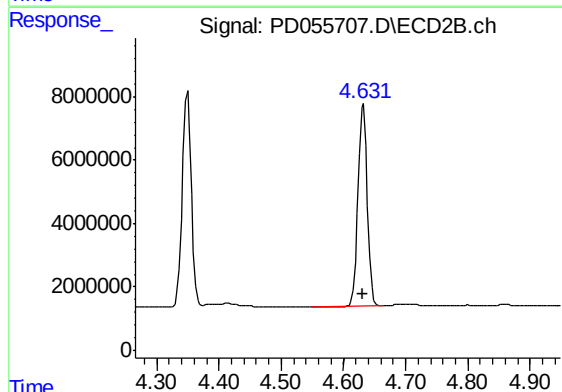


#3 gamma-BHC (Lindane)

R.T.: 4.632 min
Delta R.T.: 0.000 min
Response: 66101293
Conc: 39.54 ng/ml

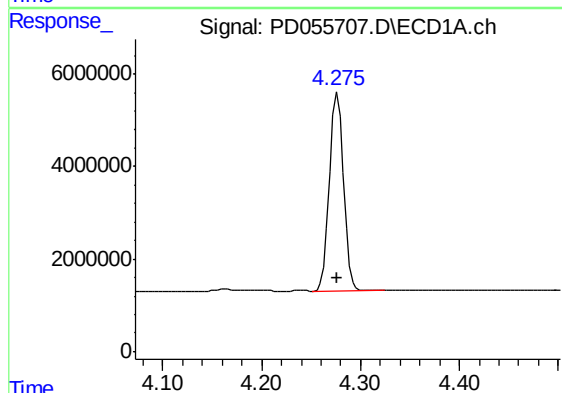


#4 Heptachlor

R.T.: 4.277 min
Delta R.T.: 0.000 min
Response: 42500715
Conc: 38.53 ng/ml

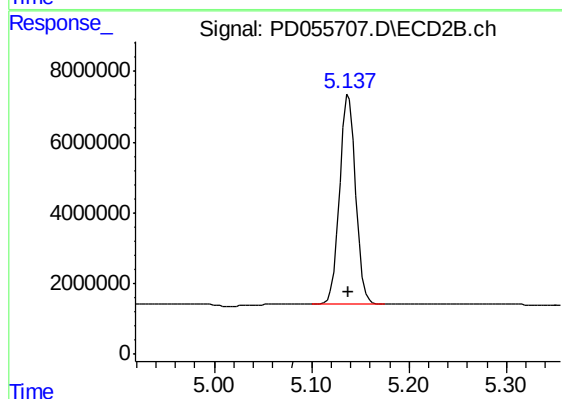

#4 Heptachlor


R.T.: 5.138 min
Delta R.T.: 0.000 min
Response: 68445595
Conc: 38.22 ng/ml

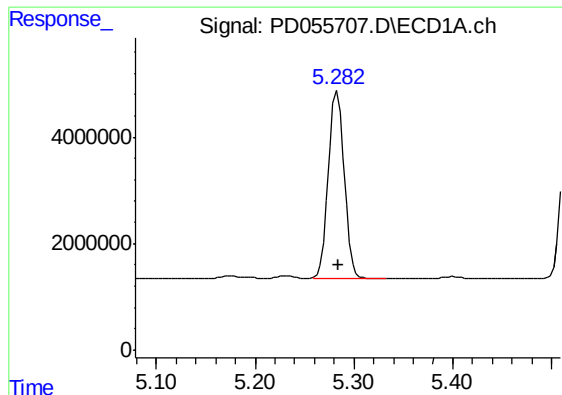

#9 Endosulfan I


R.T.: 5.283 min
Delta R.T.: 0.000 min
Response: 39309088
Conc: 38.49 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA401

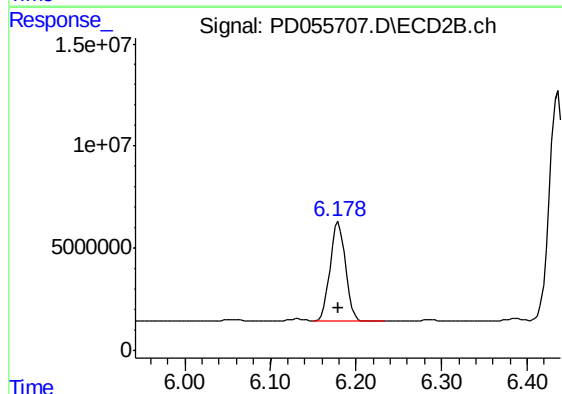


#9 Endosulfan I

R.T.: 6.180 min
Delta R.T.: 0.000 min
Response: 60617732
Conc: 38.13 ng/ml

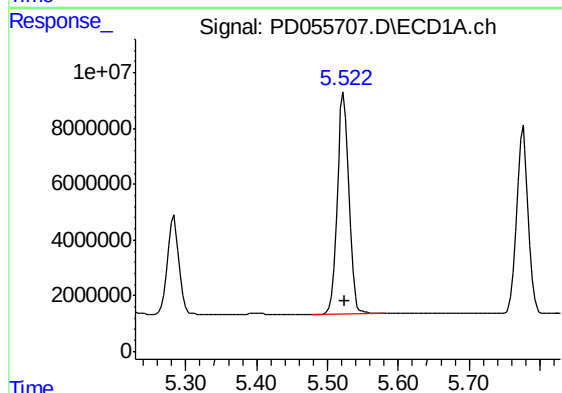


#13 Dieldrin

R.T.: 5.523 min
Delta R.T.: 0.000 min
Response: 90104946
Conc: 79.26 ng/ml

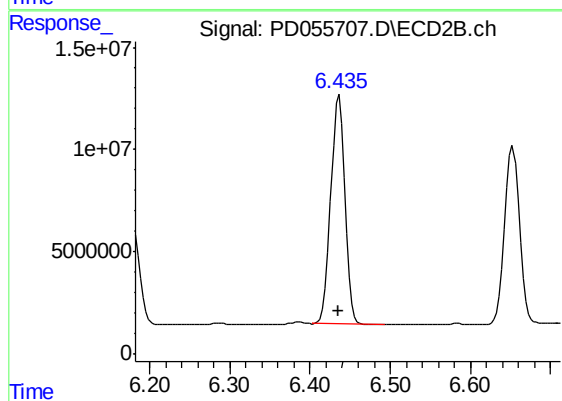

#13 Dieldrin


R.T.: 6.436 min
Delta R.T.: 0.000 min
Response: 136370158
Conc: 78.34 ng/ml

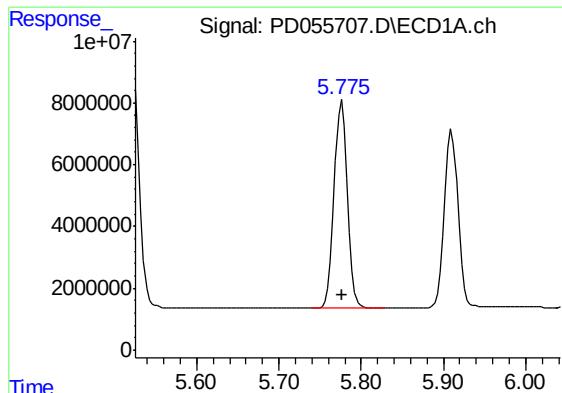

#14 Endrin


R.T.: 5.776 min
Delta R.T.: 0.000 min
Response: 75196805
Conc: 78.22 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA401

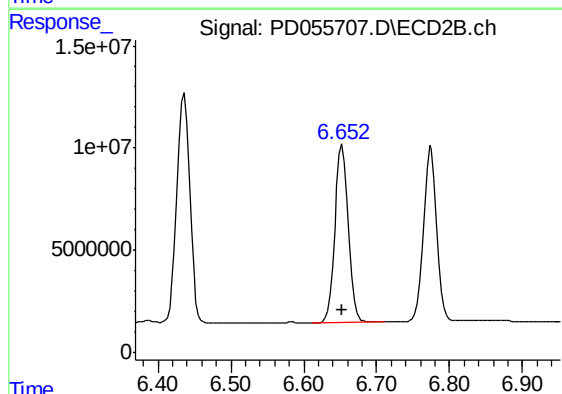


#14 Endrin

R.T.: 6.653 min
Delta R.T.: 0.000 min
Response: 110479248
Conc: 77.74 ng/ml

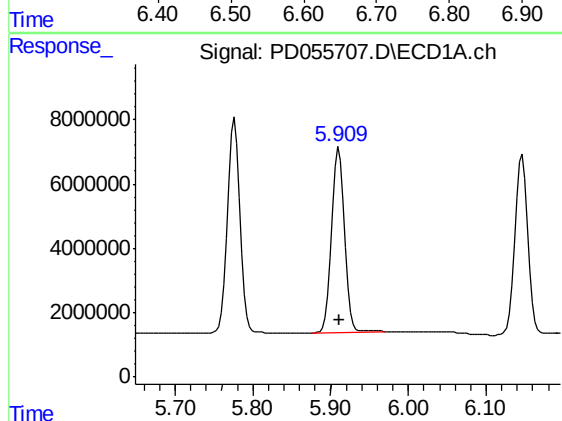


#16 4,4'-DDD

R.T.: 5.911 min
Delta R.T.: 0.000 min
Response: 66814086
Conc: 79.73 ng/ml

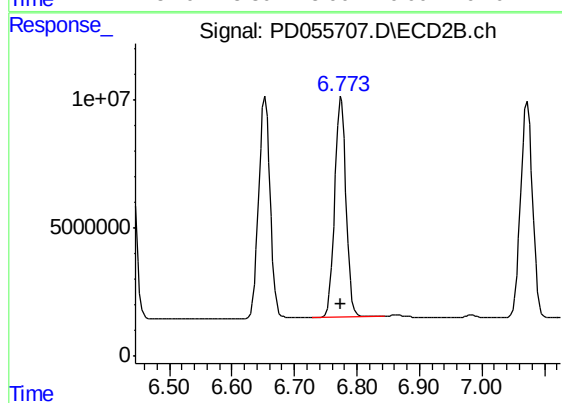

#16 4,4'-DDD


R.T.: 6.775 min
Delta R.T.: 0.000 min
Response: 109358407
Conc: 79.34 ng/ml

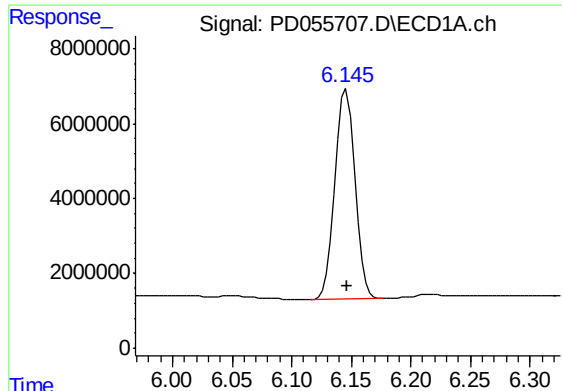

#17 4,4'-DDT


R.T.: 6.146 min
Delta R.T.: 0.000 min
Response: 65100584
Conc: 82.56 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA401

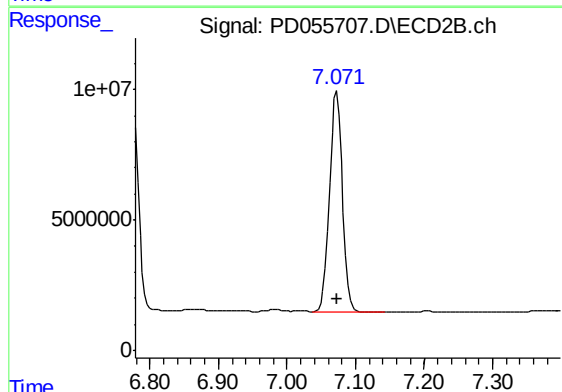


#17 4,4'-DDT

R.T.: 7.073 min
Delta R.T.: 0.000 min
Response: 111136865
Conc: 79.96 ng/ml

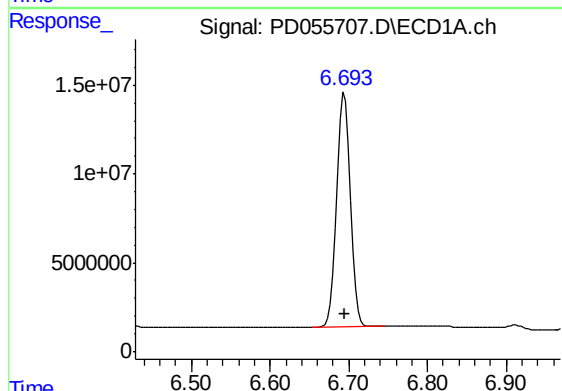


#20 Methoxychlor

R.T.: 6.694 min
Delta R.T.: 0.000 min
Response: 163711424
Conc: 386.46 ng/ml

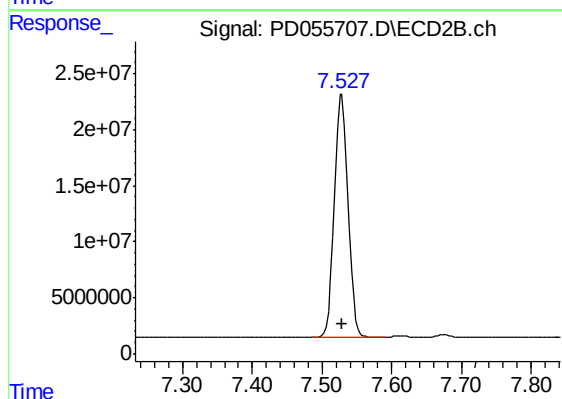

#20 Methoxychlor


R.T.: 7.529 min
Delta R.T.: 0.000 min
Response: 296575045
Conc: 379.35 ng/ml

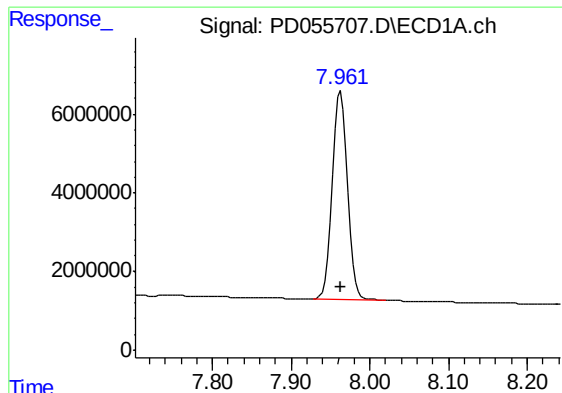

#27 Decachlorobiphenyl

R.T.: 7.963 min
Delta R.T.: 0.000 min
Response: 72952550
Conc: 74.83 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA401

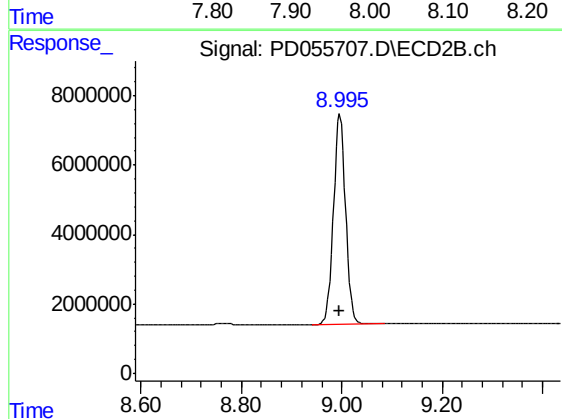

#27 Decachlorobiphenyl

R.T.: 8.997 min
Delta R.T.: 0.000 min
Response: 101847247
Conc: 73.83 ng/ml