

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD103122\
 Data File : PD072709.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Oct 2022 17:58
 Operator : AR\AJ
 Sample : N5301-10
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DBWU8

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 11/01/2022
 Supervised By :Ankita Jodhani 11/01/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 22:20:41 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102622CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 26 16:50:44 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.704	3.465	41096613	636.2E6	17.676	15.876
27)	SA Decachlor...	7.836	8.919	61787942	323.3E6	31.477	34.380
Target Compounds							
2)	A alpha-BHC	3.208	3.928	160.4E6	2046.0E6	45.940	38.569m
6)	B beta-BHC	3.840	4.479	39088744	428.3E6	25.728	25.244

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD103122\
Data File : PD072709.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Oct 2022 17:58
Operator : AR\AJ
Sample : N5301-10
Misc :
ALS Vial : 33 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 22:20:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102622CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 26 16:50:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

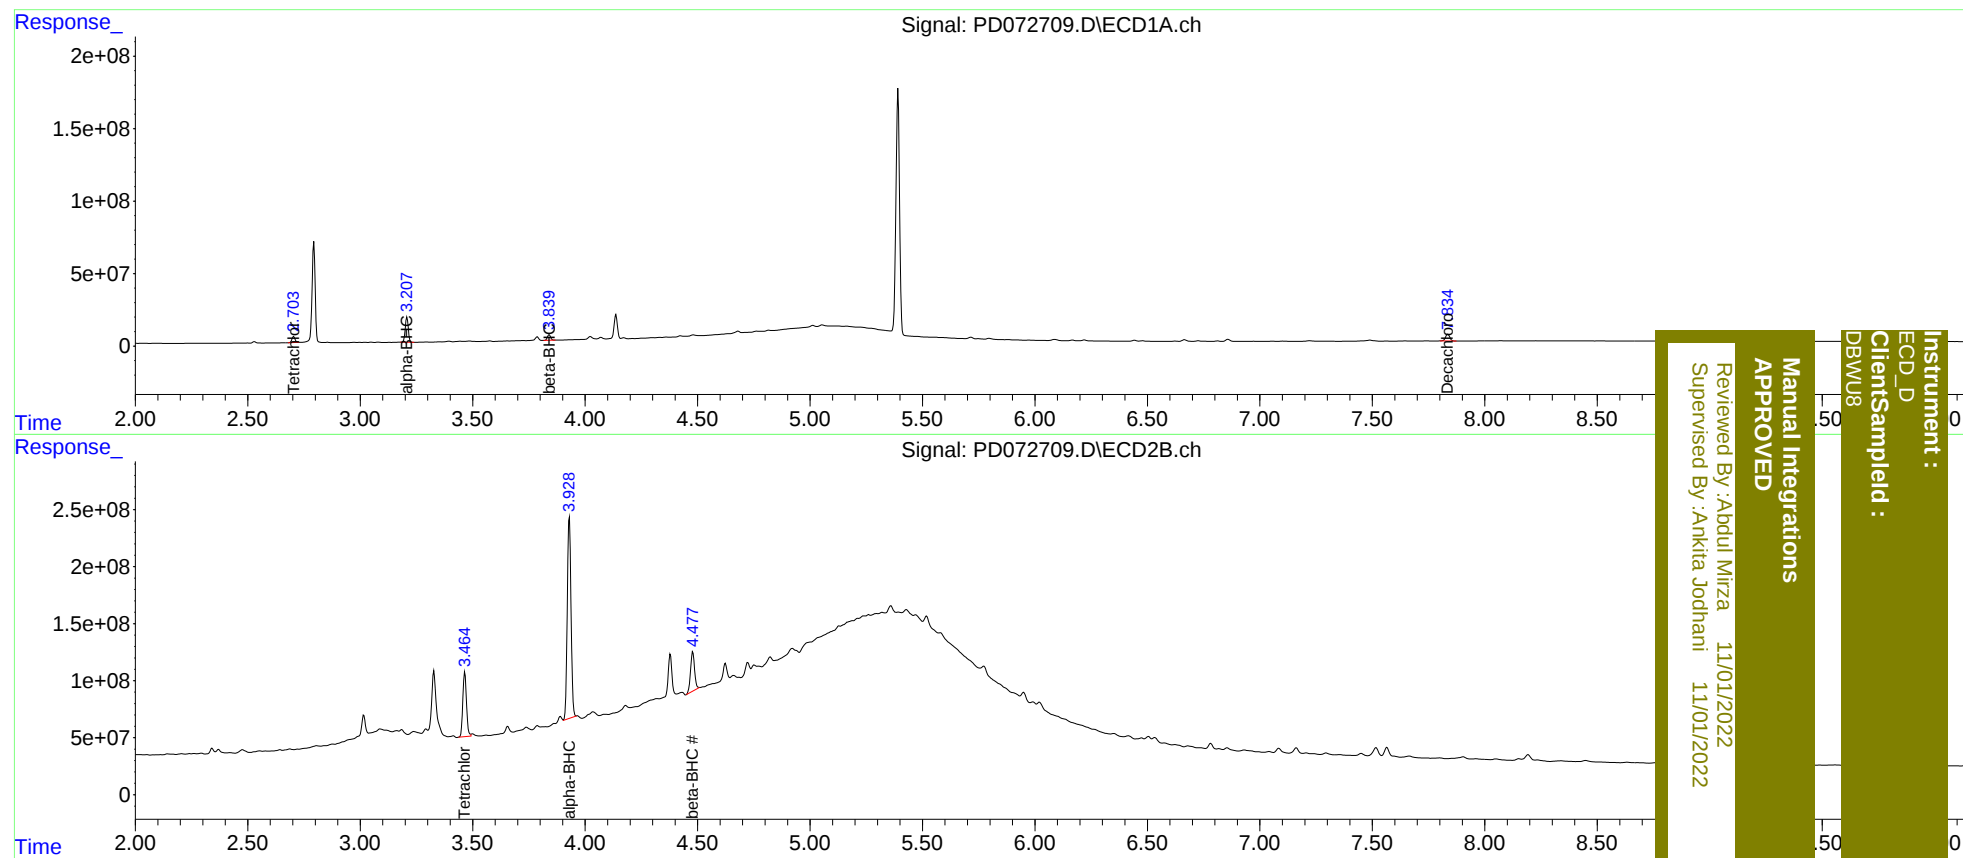

Reviewed By: Abdul Mirza 11/01/2022
Supervised By: Ankita Jodhani 11/01/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
DBWU8