

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD103122\
 Data File : PD072685.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Oct 2022 12:12
 Operator : AR\AJ
 Sample : N5276-06MS
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EW4W5MS

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 11/01/2022
 Supervised By :Ankita Jodhani 11/01/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 22:12:15 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102622CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 26 16:50:44 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.703	3.466	40376832	842.5E6	17.367	21.026
27)	SA Decachlor...	7.837	8.920	73847961	370.3E6	37.621	39.373
Target Compounds							
2)	A alpha-BHC	3.207	3.929	152.9E6	1967.7E6	43.785	37.093
3)	MA gamma-BHC...	3.538	4.263	149.2E6	1686.7E6	47.086	39.690
4)	MA Heptachlor	3.871	4.830	152.6E6	1197.4E6	47.033	40.272
5)	MB Aldrin	4.150	5.169	151.1E6	1040.1E6	47.711	41.500
6)	B beta-BHC	3.840	4.478	66677777	698.2E6	43.887	41.152
7)	B delta-BHC	4.070	4.722	20634892	230.8E6	6.156	6.750
8)	B Heptachlo...	4.655	5.601	139.8E6	898.2E6	49.159	43.442
9)	A Endosulfan I	5.025	5.985	129.9E6	819.0E6	51.194	47.271
10)	B trans-Chl...	4.904	5.854	141.6E6	870.8E6	48.246	43.479
11)	B cis-Chlor...	4.967	5.930	136.5E6	848.3E6	47.807	43.525
12)	B 4,4'-DDE	5.156	6.103	279.0E6	1680.9E6	102.482	94.131
13)	MA Dieldrin	5.290	6.263	294.9E6	1692.4E6	107.034	94.978
14)	MA Endrin	5.568	6.494	278.4E6	1406.3E6	114.860	96.132
15)	B Endosulfa...	5.865	6.722	241.6E6	1429.0E6	102.739	100.031m
16)	A 4,4'-DDD	5.714	6.628	221.5E6	1318.8E6	104.008	97.714
17)	MA 4,4'-DDT	5.963	6.936	223.9E6	1365.3E6	103.337	101.015
18)	B Endrin al...	6.048	6.855	177.9E6	1057.3E6	90.345	88.233
19)	B Endosulfa...	6.271	7.088	161.5E6	920.5E6	70.539	69.935
20)	A Methoxychlor	6.547	7.416	581.4E6	2954.1E6	500.832	488.387
21)	B Endrin ke...	6.781	7.578	279.9E6	1461.3E6	104.924	102.012

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD103122\
Data File : PD072685.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Oct 2022 12:12
Operator : AR\AJ
Sample : N5276-06MS
Misc :
ALS Vial : 10 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 22:12:15 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102622CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 26 16:50:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

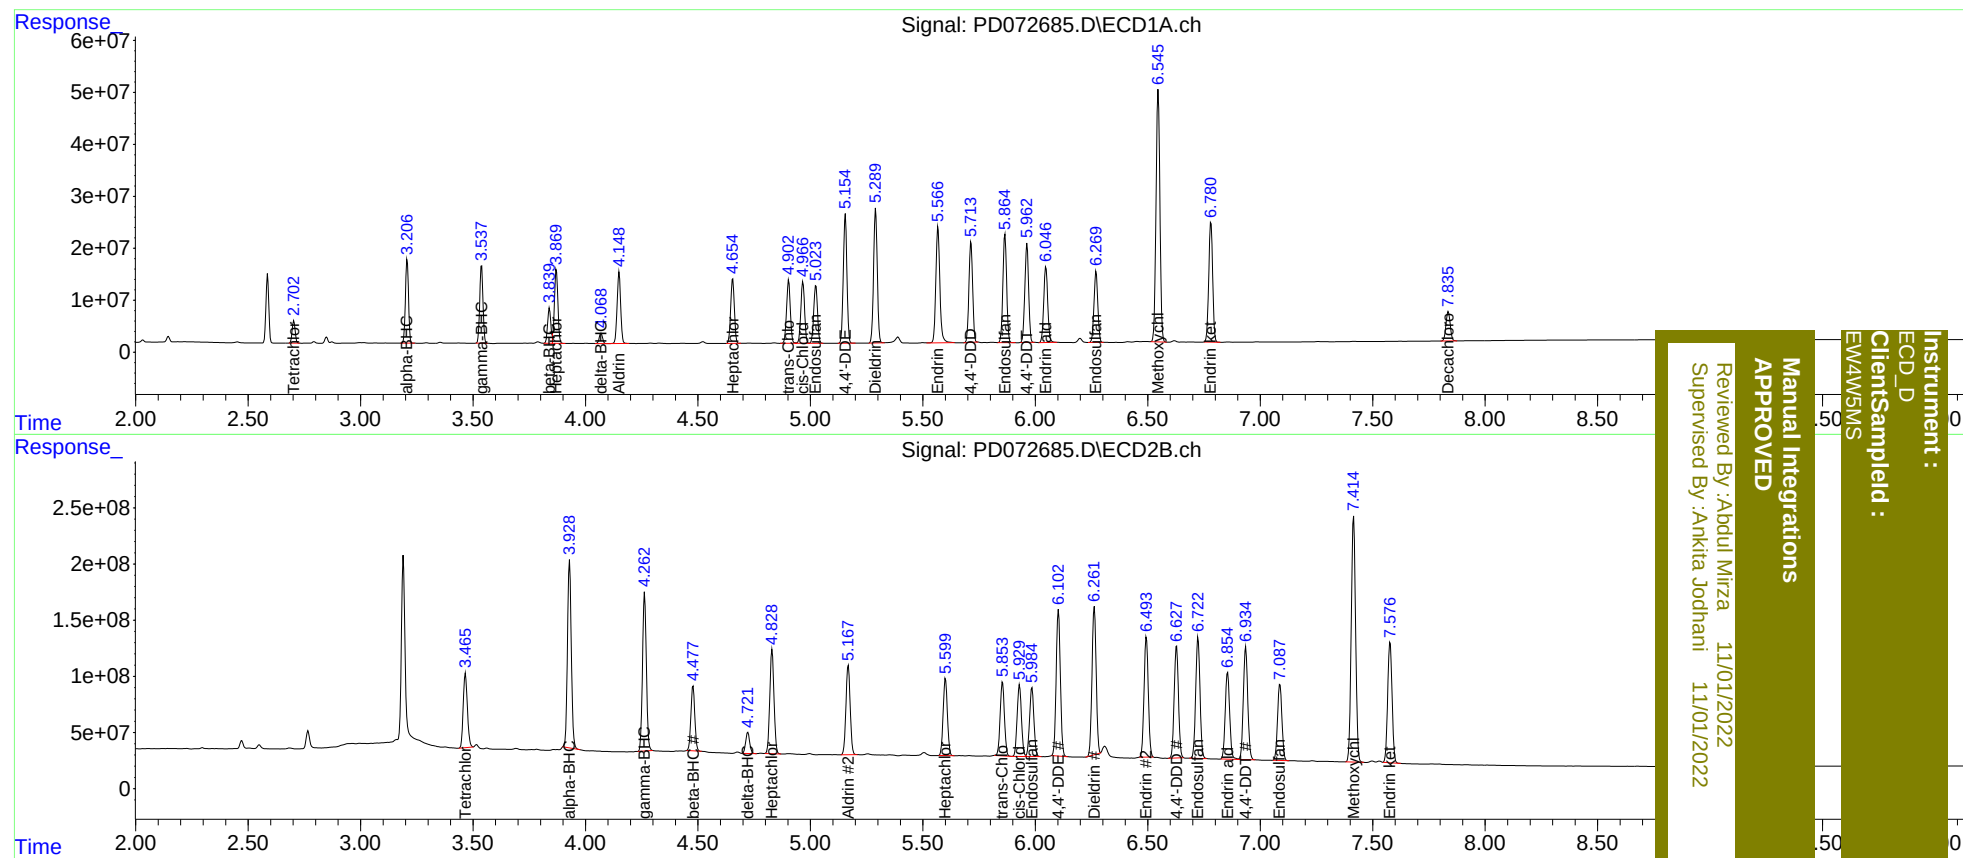

Instrument :
ECD_D
ClientSampled :
EW4W5MS

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 11/01/2022
Supervised By: Ankita Jodhani 11/01/2022