

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD103122\
 Data File : PD072686.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Oct 2022 12:25
 Operator : AR\AJ
 Sample : N5276-07MSD
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EW4W5MSD

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 11/01/2022
 Supervised By :Ankita Jodhani 11/01/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 22:12:39 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102622CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 26 16:50:44 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.704	3.467	40607444	847.7E6	17.466	21.154
27)	SA Decachlor...	7.837	8.920	73583598	369.3E6	37.487	39.267
Target Compounds							
2)	A alpha-BHC	3.208	3.930	153.5E6	1988.0E6	43.969	37.476
3)	MA gamma-BHC...	3.539	4.263	149.6E6	1697.6E6	47.200	39.946
4)	MA Heptachlor	3.871	4.830	154.2E6	1203.9E6	47.528	40.490
5)	MB Aldrin	4.150	5.169	152.0E6	1050.2E6	47.991	41.902
6)	B beta-BHC	3.840	4.478	67142614	695.5E6	44.193	40.995
7)	B delta-BHC	4.070	4.722	20765440	235.1E6	6.195	6.877
8)	B Heptachlo...	4.655	5.601	140.5E6	905.5E6	49.418	43.791
9)	A Endosulfan I	5.025	5.986	130.5E6	820.9E6	51.432	47.380
10)	B trans-Chl...	4.904	5.855	142.4E6	874.8E6	48.517	43.678
11)	B cis-Chlor...	4.967	5.931	137.1E6	848.9E6	48.013	43.556
12)	B 4,4'-DDE	5.156	6.104	280.4E6	1691.1E6	103.001	94.701
13)	MA Dieldrin	5.291	6.263	296.5E6	1696.0E6	107.628	95.181
14)	MA Endrin	5.568	6.495	279.8E6	1409.6E6	115.442	96.352
15)	B Endosulfa...	5.866	6.723	244.2E6	1412.6E6	103.843	98.884m
16)	A 4,4'-DDD	5.715	6.629	220.9E6	1324.2E6	103.733	98.121
17)	MA 4,4'-DDT	5.964	6.936	225.4E6	1363.8E6	104.031	100.900
18)	B Endrin al...	6.048	6.856	178.2E6	1058.6E6	90.487	88.340
19)	B Endosulfa...	6.272	7.089	161.6E6	923.2E6	70.585	70.143
20)	A Methoxychlor	6.547	7.417	586.0E6	2970.7E6	504.768	491.131
21)	B Endrin ke...	6.782	7.579	280.5E6	1460.5E6	105.146	101.962

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD103122\
Data File : PD072686.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Oct 2022 12:25
Operator : AR\AJ
Sample : N5276-07MSD
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 22:12:39 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102622CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 26 16:50:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

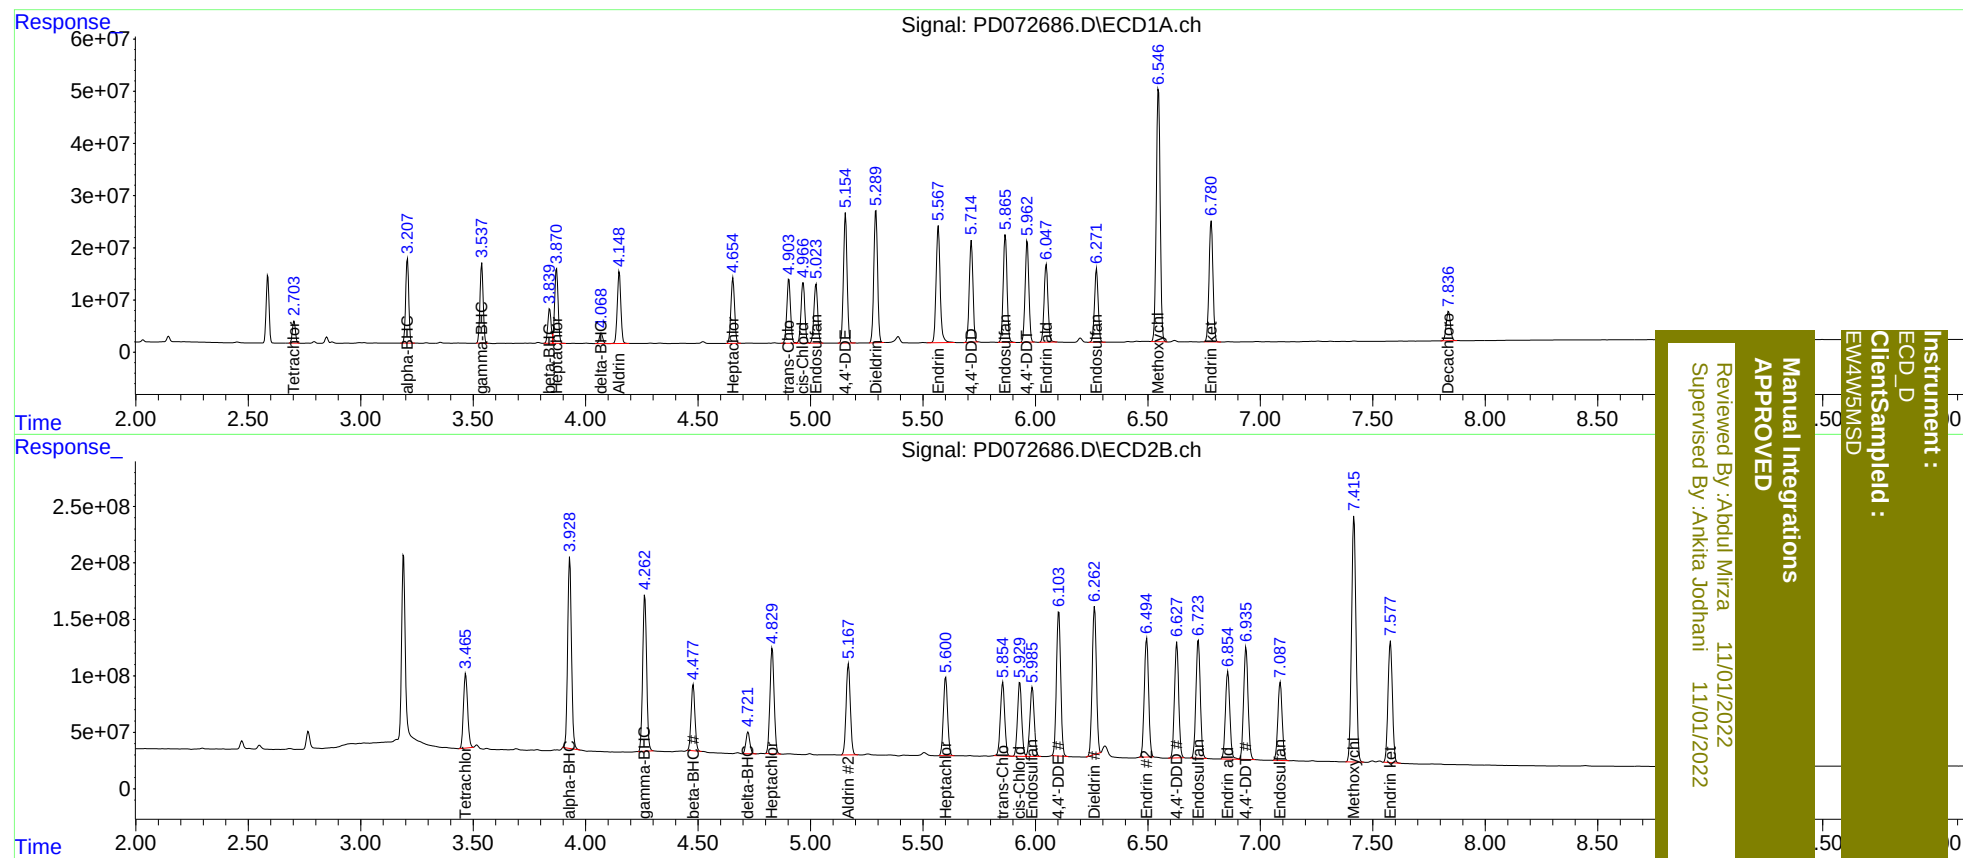

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 11/01/2022
Supervised By: Ankita Jodhani 11/01/2022

Instrument :
ECD_D
Client Sampled :
EW4W/MSD