

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD103123\
 Data File : PD079280.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Oct 2023 00:45
 Operator : AR\AJ
 Sample : PB156683BL
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 05:44:43 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101723CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 17 09:38:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.570	2.806	29205417	43710295	19.043	20.157
27) SA Decachlor...	9.118	7.954	42352450	53010469	22.330	22.729
Target Compounds						
3) MA gamma-BHC...	0.000	3.658	0	316903	N.D.	<MDL
15) B Endosulfa...	0.000	5.931f	0	403116	N.D.	0.169


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD103123\
Data File : PD079280.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Oct 2023 00:45
Operator : AR\AJ
Sample : PB156683BL
Misc :
ALS Vial : 45 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 05:44:43 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101723CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 17 09:38:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

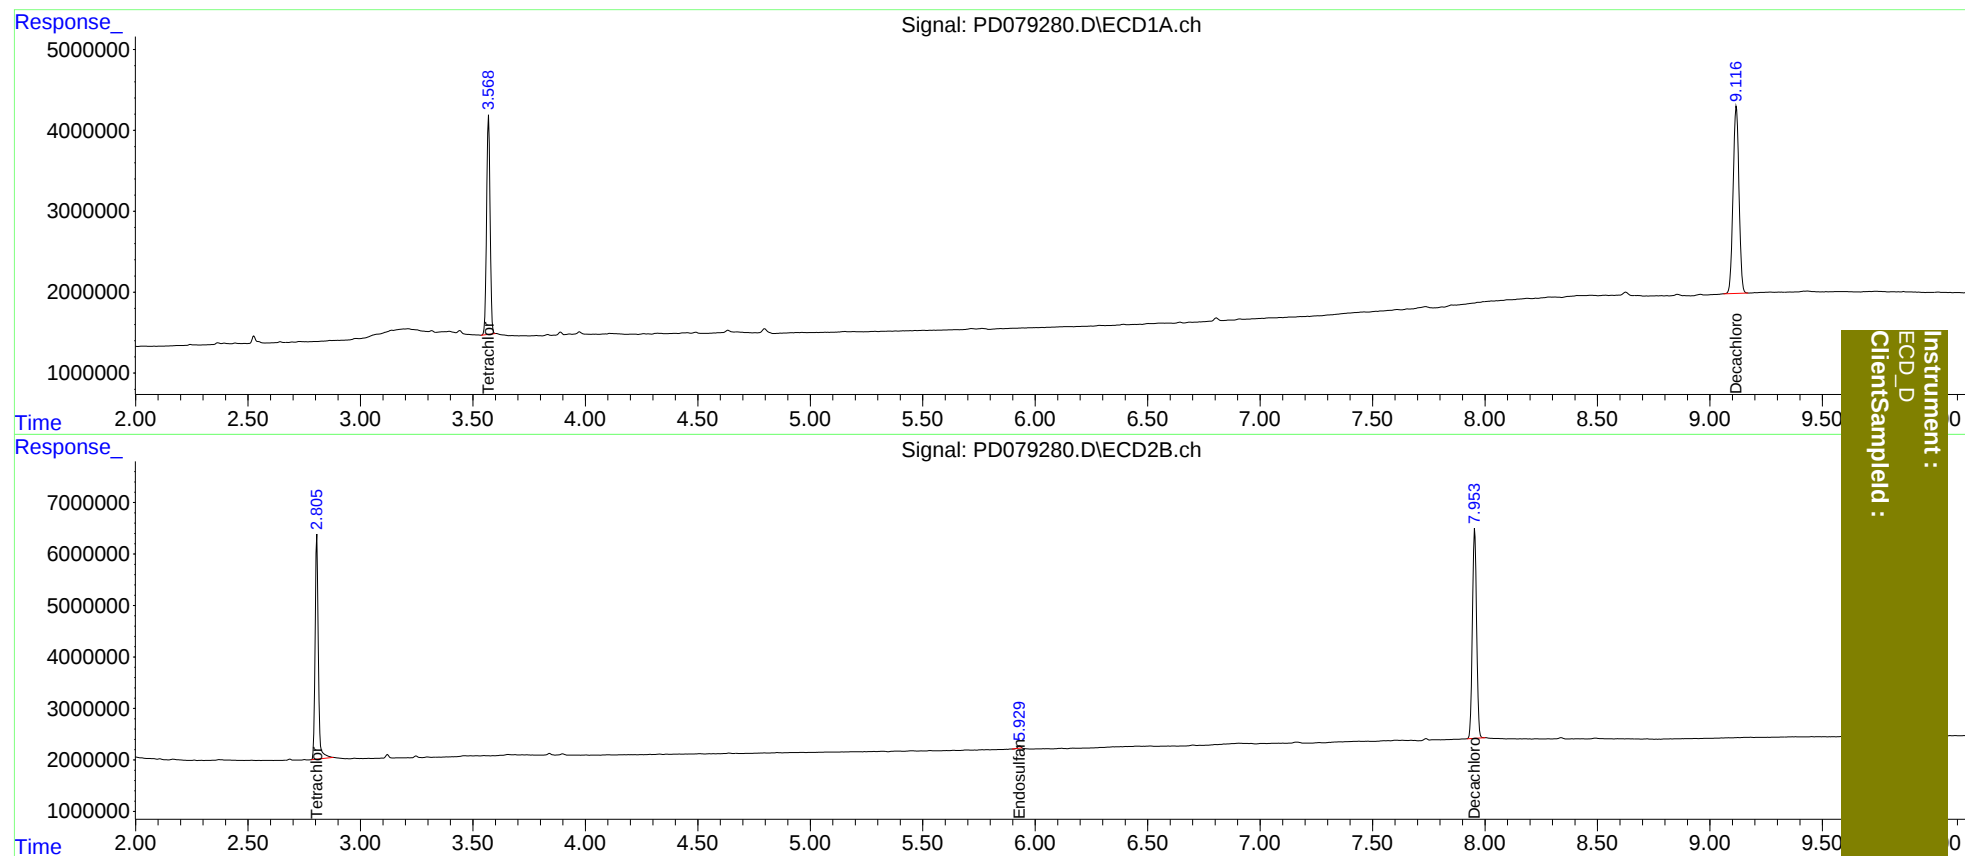


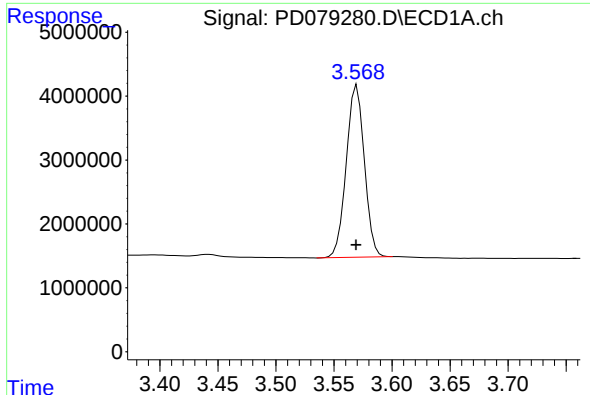

#1 Tetrachloro-m-xylene


R.T.: 3.570 min
Delta R.T.: 0.000 min
Response: 29205417
Conc: 19.04 ng/ml

Instrument :
ECD_D
ClientSampleId :

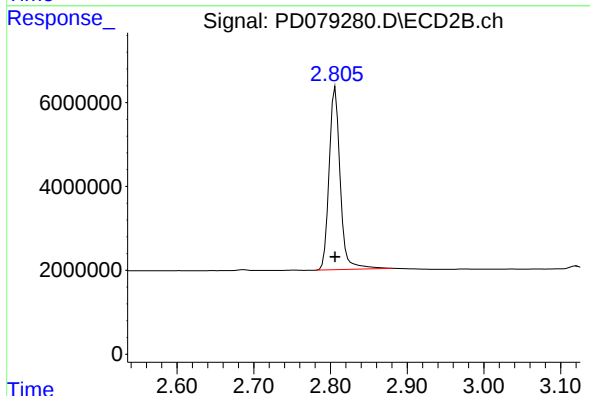


#1 Tetrachloro-m-xylene

R.T.: 2.806 min
Delta R.T.: 0.000 min
Response: 43710295
Conc: 20.16 ng/ml

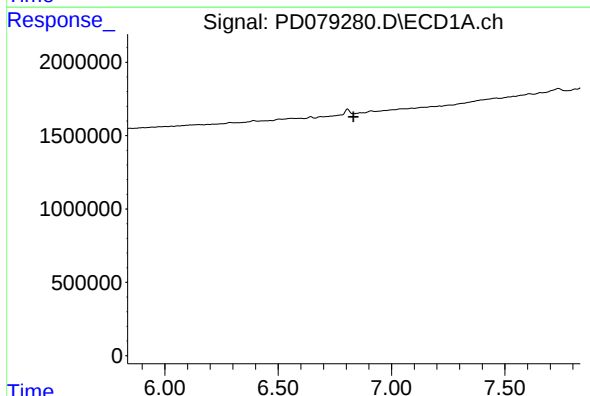


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.833 min
Response: 0
Conc: N.D.

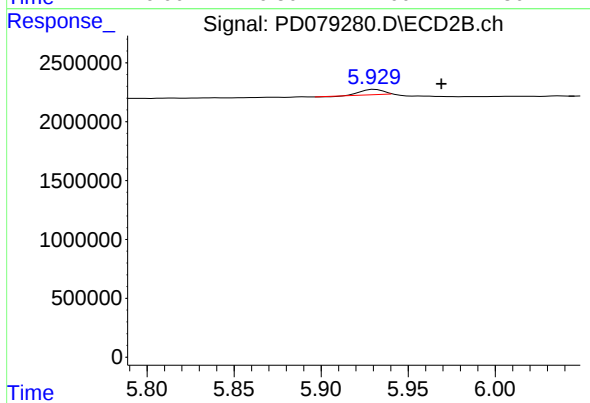

#15 Endosulfan II


R.T.: 5.931 min
Delta R.T.: -0.038 min
Response: 403116
Conc: 0.17 ng/ml

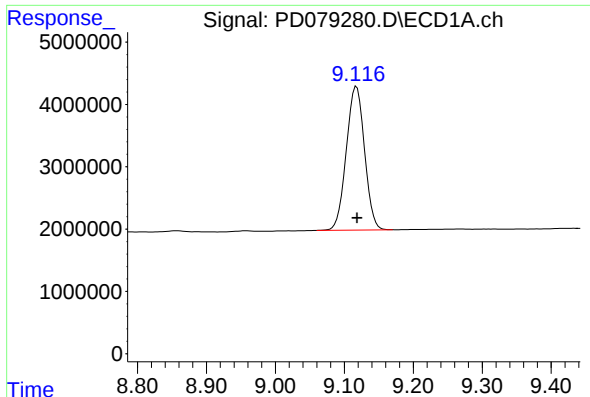

#27 Decachlorobiphenyl

R.T.: 9.118 min
Delta R.T.: 0.000 min
Response: 42352450
Conc: 22.33 ng/ml

Instrument :
ECD_D
ClientSampleId :

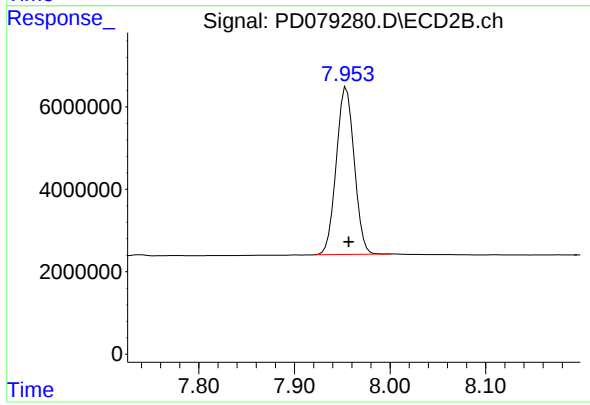

#27 Decachlorobiphenyl

R.T.: 7.954 min
Delta R.T.: -0.002 min
Response: 53010469
Conc: 22.73 ng/ml