

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD103123\
 Data File : PD079239.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Oct 2023 15:39
 Operator : AR\AJ
 Sample : 05044-02MS
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BHEE3MS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 21:26:23 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101723CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 17 09:38:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.570	2.806	29447613	42403927	19.200	19.554
2)	SA Decachlor...	9.121	7.957	32444606	41030247	17.106	17.592
Target Compounds							
2)	A alpha-BHC	4.027	3.310	140.4E6	190.1E6	53.889	55.762
3)	MA gamma-BHC...	4.361	3.640	126.6E6	167.8E6	50.861	51.913
4)	MA Heptachlor	4.955	3.983	128.2E6	157.4E6	48.117	51.767
5)	MB Aldrin	5.298	4.264	119.7E6	153.9E6	48.402	49.949
6)	B beta-BHC	4.554	3.934	52218786	70775071	45.794	48.934
7)	B delta-BHC	4.804	4.166	129.0E6	171.9E6	49.165	52.425
8)	B Heptachlo...	5.725	4.766	116.9E6	153.6E6	48.683	53.225
9)	A Endosulfan I	6.112	5.137	110.4E6	142.2E6	51.537	55.995
10)	B trans-Chl...	5.981	5.017	110.8E6	147.2E6	50.013	53.153
11)	B cis-Chlor...	6.061	5.081	111.8E6	148.9E6	49.190	52.589
12)	B 4,4'-DDE	6.231	5.270	215.3E6	291.0E6	104.494	111.266
13)	MA Dieldrin	6.388	5.402	240.8E6	325.9E6	105.984	110.666
14)	MA Endrin	6.618	5.677	207.5E6	293.2E6	109.613	116.197
15)	B Endosulfa...	6.835	5.969	205.6E6	274.7E6	103.667	115.446
16)	A 4,4'-DDD	6.748	5.824	177.2E6	241.8E6	105.409	109.495
17)	MA 4,4'-DDT	7.064	6.075	192.2E6	252.6E6	107.353	112.122
18)	B Endrin al...	6.966	6.149	150.3E6	197.6E6	99.088	106.636
19)	B Endosulfa...	7.200	6.371	193.4E6	254.0E6	100.651	110.226
20)	A Methoxychlor	7.538	6.651	481.3E6	617.9E6	501.670	506.804
21)	B Endrin ke...	7.687	6.878	211.3E6	293.3E6	101.148	111.149

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD103123\
Data File : PD079239.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2023 15:39
Operator : AR\AJ
Sample : 05044-02MS
Misc :
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 21:26:23 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101723CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 17 09:38:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

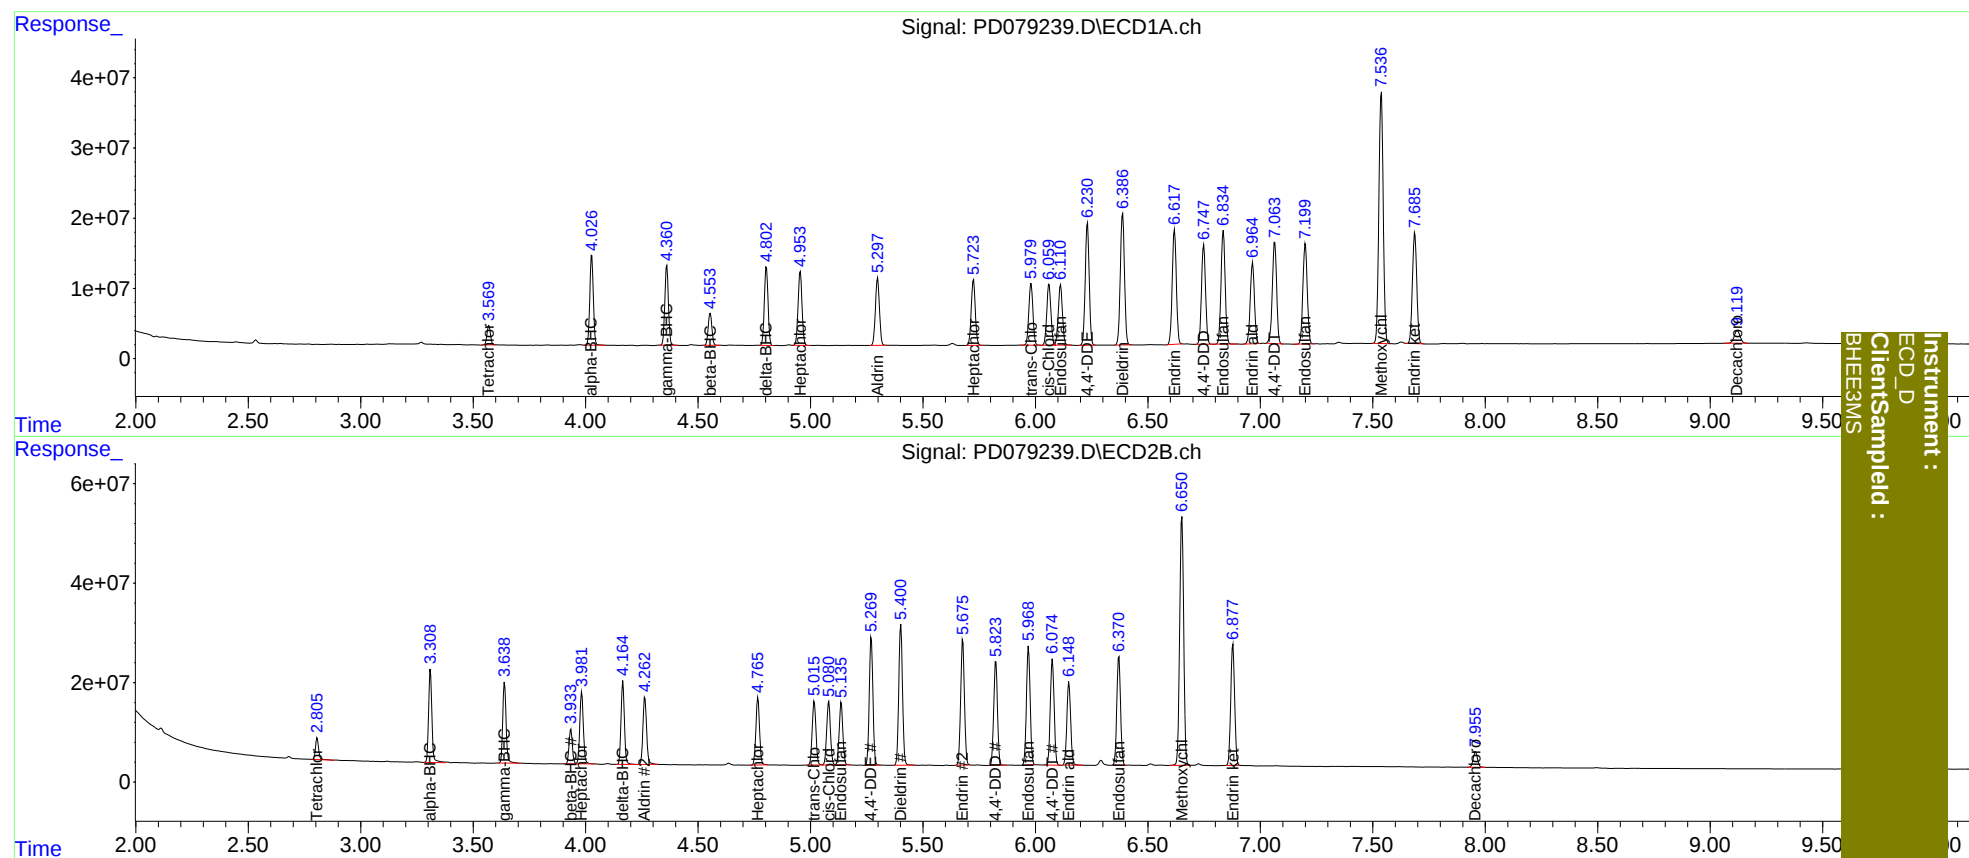

Instrument :
ECD_D
ClientSampled :
BHEE3MS