

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD103123\
 Data File : PD079240.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Oct 2023 15:52
 Operator : AR\AJ
 Sample : 05044-03MSD
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BHEE3MSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 21:26:47 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101723CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 17 09:38:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.571	2.807	29262286	42412425	19.080	19.558
2)	SA Decachlor...	9.121	7.958	32200474	40782751	16.977	17.486
Target Compounds							
2)	A alpha-BHC	4.027	3.310	139.8E6	188.9E6	53.672	55.406
3)	MA gamma-BHC...	4.362	3.640	125.4E6	166.9E6	50.389	51.628
4)	MA Heptachlor	4.954	3.983	123.4E6	156.2E6	46.332	51.359
5)	MB Aldrin	5.299	4.264	117.2E6	152.8E6	47.419	49.606
6)	B beta-BHC	4.554	3.934	51567107	69921898	45.222	48.344
7)	B delta-BHC	4.804	4.166	127.0E6	170.3E6	48.413	51.919
8)	B Heptachlo...	5.725	4.766	115.1E6	152.4E6	47.930	52.793
9)	A Endosulfan I	6.112	5.137	108.9E6	140.8E6	50.847	55.451
10)	B trans-Chl...	5.981	5.017	109.3E6	145.8E6	49.327	52.657
11)	B cis-Chlor...	6.061	5.081	110.5E6	147.5E6	48.613	52.084
12)	B 4,4'-DDE	6.231	5.270	212.3E6	287.8E6	103.065	110.041
13)	MA Dieldrin	6.387	5.402	237.1E6	323.4E6	104.387	109.808
14)	MA Endrin	6.618	5.677	205.1E6	291.5E6	108.336	115.536
15)	B Endosulfa...	6.835	5.970	203.3E6	273.2E6	102.520	114.810
16)	A 4,4'-DDD	6.748	5.825	175.0E6	239.6E6	104.094	108.462
17)	MA 4,4'-DDT	7.064	6.077	190.7E6	250.6E6	106.516	111.216
18)	B Endrin al...	6.965	6.149	148.5E6	196.8E6	97.905	106.226
19)	B Endosulfa...	7.200	6.372	191.6E6	252.5E6	99.703	109.572
20)	A Methoxychlor	7.538	6.652	478.4E6	616.1E6	498.689	505.299
21)	B Endrin ke...	7.687	6.879	210.4E6	291.9E6	100.699	110.608

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD103123\
Data File : PD079240.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2023 15:52
Operator : AR\AJ
Sample : 05044-03MSD
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 21:26:47 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101723CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 17 09:38:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

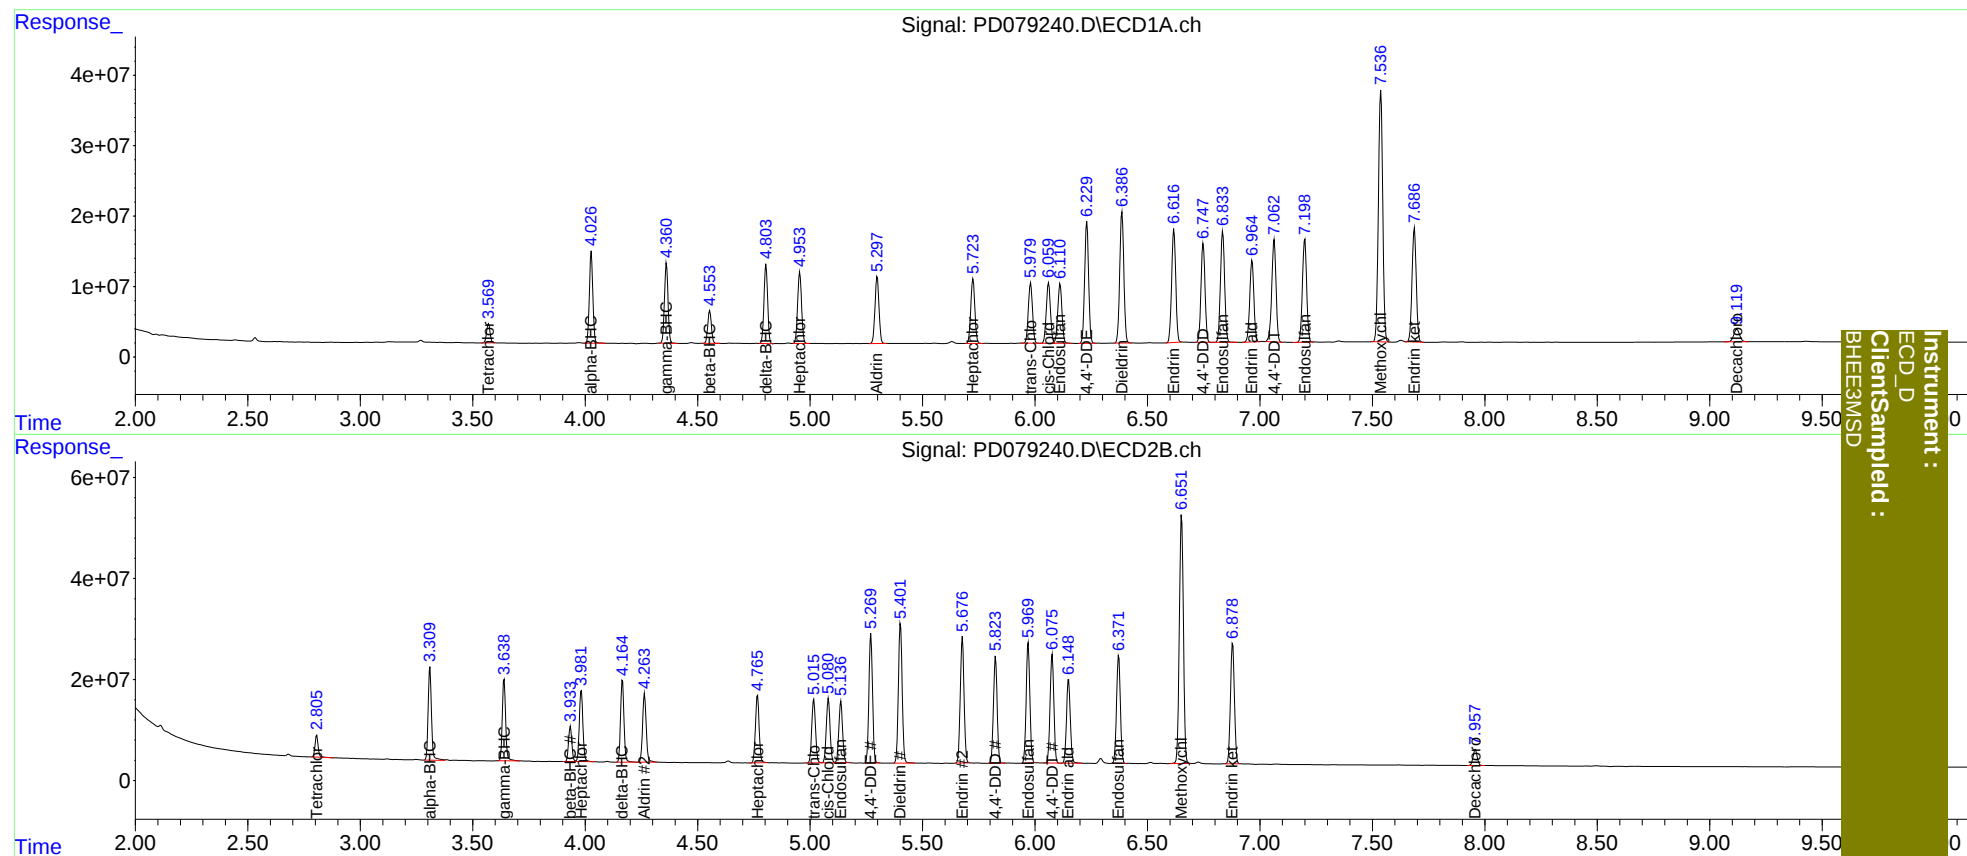

Instrument :
ECD_D
ClientSampled :
BHEE3MSD