

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110119\
 Data File : PD055724.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Oct 2019 23:38
 Operator : SG\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 06:35:13 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110119.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 31 06:31:17 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.289	3.963	44881968	57782290	50.000	50.000
28)	SA Decachlor...	7.964	8.998	45434720	65807605	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.130	4.951	13227479	22619673	500.000	500.000
24)	Chlordane-2	4.621	5.415	15293967	24938790	500.000	500.000
25)	Chlordane-3	5.176	6.059	47441808	106.9E6	500.000	500.000
26)	Chlordane-4	5.232	6.133	41553073	127.2E6	500.000	500.000
27)	Chlordane-5	6.055	6.933	15388218	22979962	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110119\
Data File : PD055724.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2019 23:38
Operator : SG\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 06:35:13 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110119.M
Quant Title : GC Extractables
QLast Update : Thu Oct 31 06:31:17 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

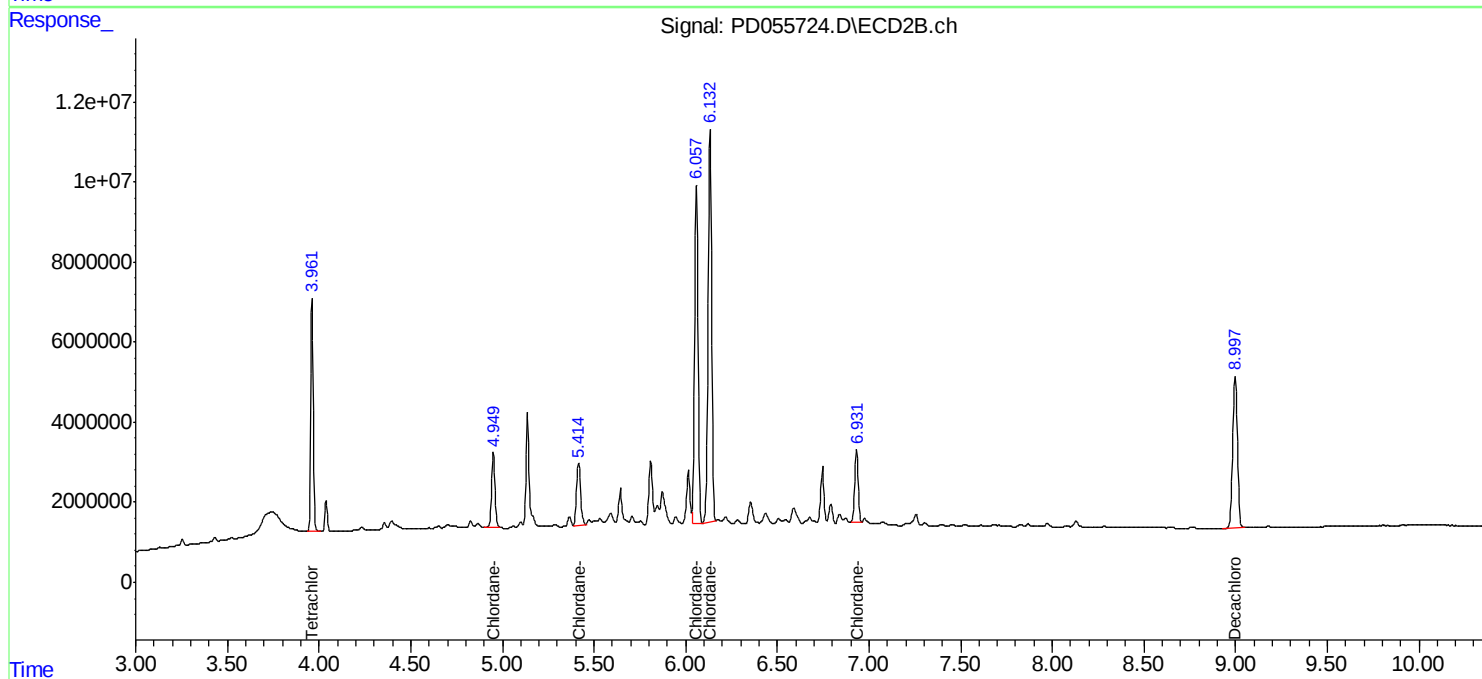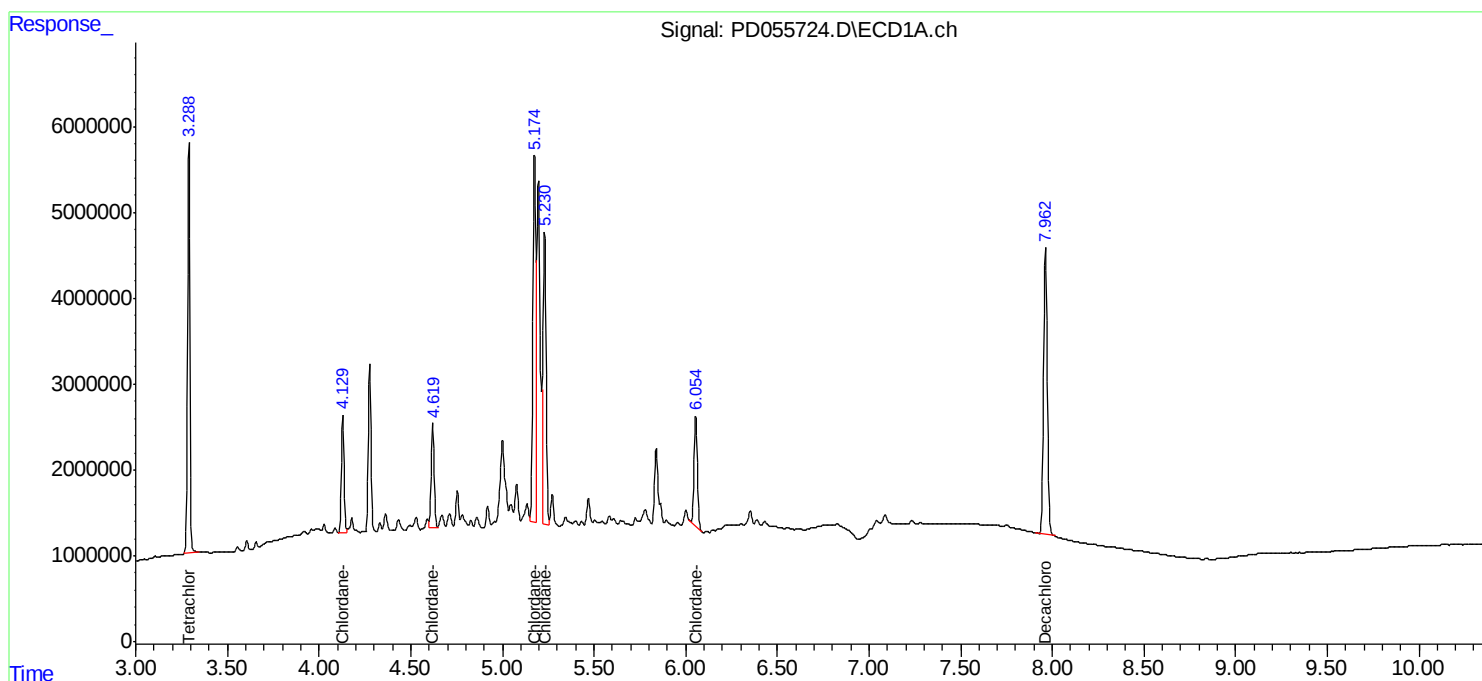


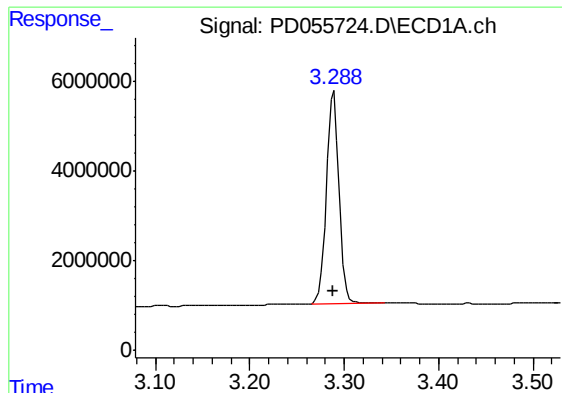

#1 Tetrachloro-m-xylene


R.T.: 3.289 min
Delta R.T.: 0.000 min
Response: 44881968
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

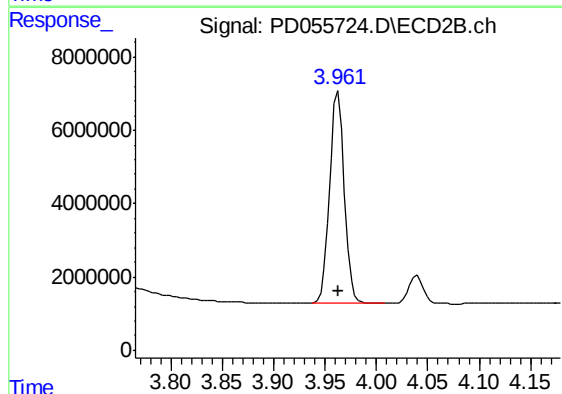


#1 Tetrachloro-m-xylene

R.T.: 3.963 min
Delta R.T.: 0.000 min
Response: 57782290
Conc: 50.00 ng/ml

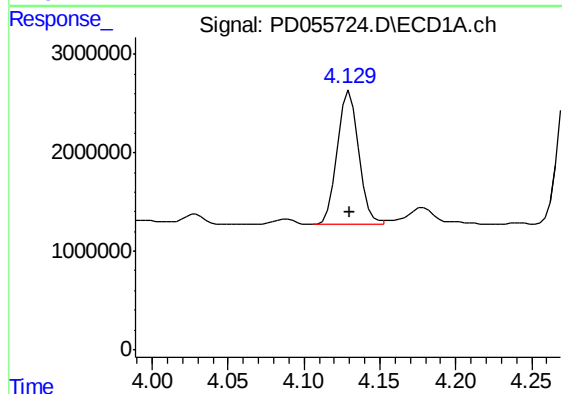


#23 Chlordane-1

R.T.: 4.130 min
Delta R.T.: 0.000 min
Response: 13227479
Conc: 500.00 ng/ml

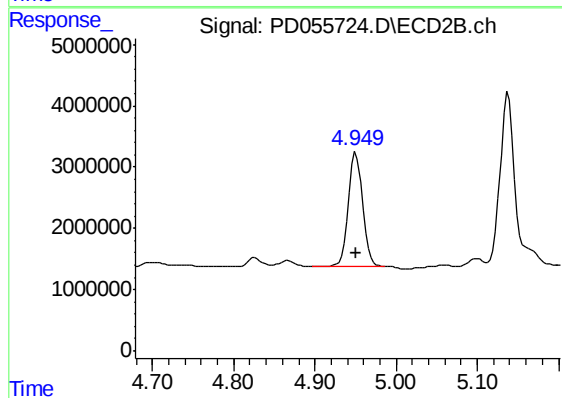

#23 Chlordane-1


R.T.: 4.951 min
Delta R.T.: 0.000 min
Response: 22619673
Conc: 500.00 ng/ml

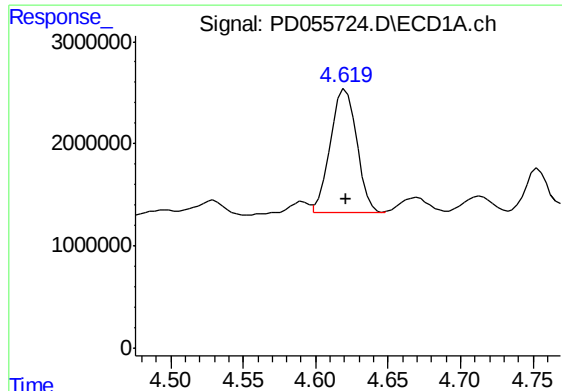

#24 Chlordane-2


R.T.: 4.621 min
Delta R.T.: 0.000 min
Response: 15293967
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

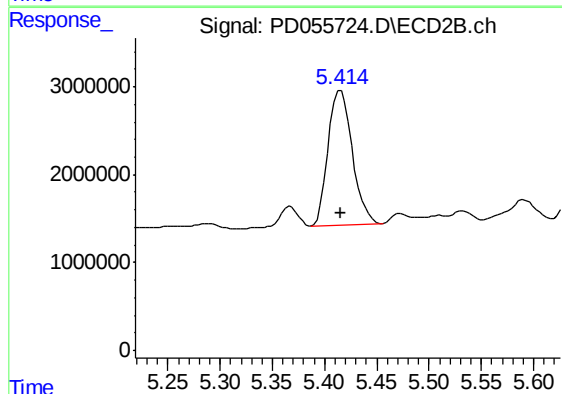


#24 Chlordane-2

R.T.: 5.415 min
Delta R.T.: 0.000 min
Response: 24938790
Conc: 500.00 ng/ml

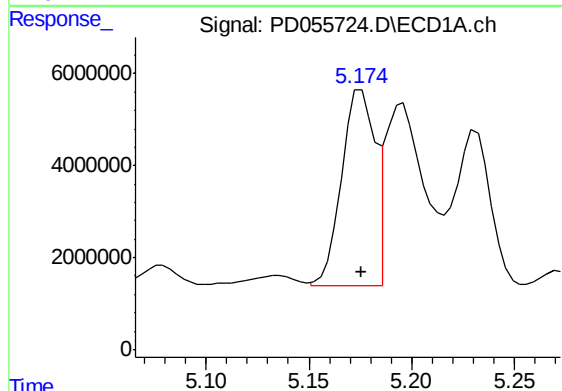


#25 Chlordane-3

R.T.: 5.176 min
Delta R.T.: 0.000 min
Response: 47441808
Conc: 500.00 ng/ml

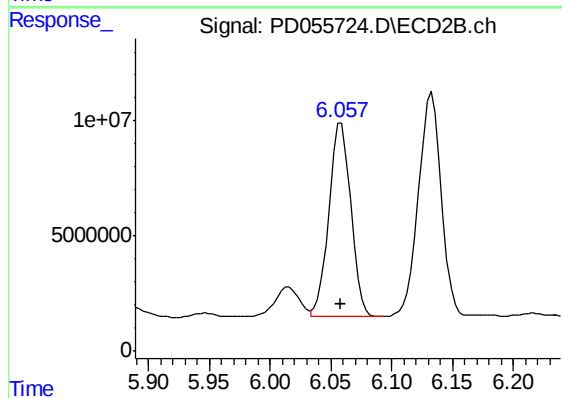

#25 Chlordane-3


R.T.: 6.059 min
Delta R.T.: 0.000 min
Response: 106902754
Conc: 500.00 ng/ml

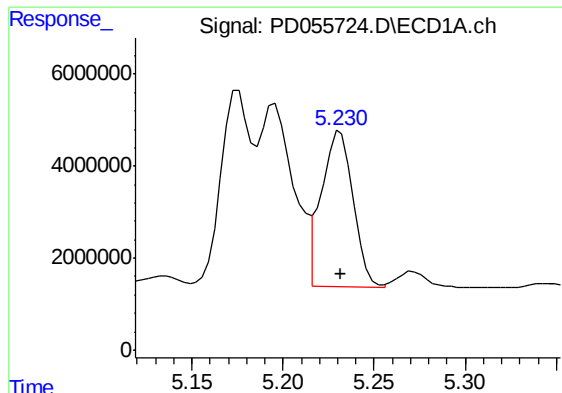

#26 Chlordane-4


R.T.: 5.232 min
Delta R.T.: 0.000 min
Response: 41553073
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

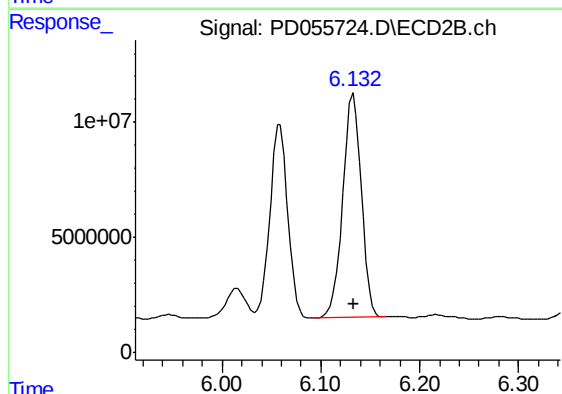


#26 Chlordane-4

R.T.: 6.133 min
Delta R.T.: 0.000 min
Response: 127241718
Conc: 500.00 ng/ml

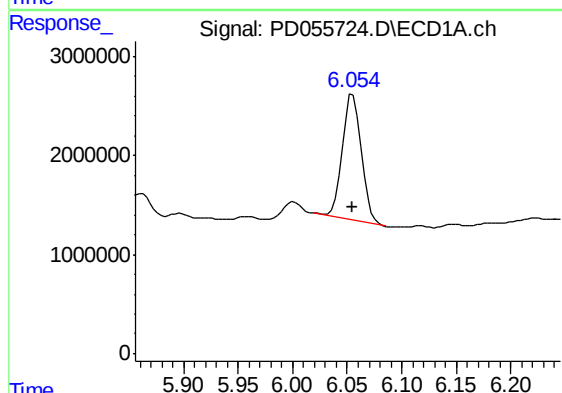


#27 Chlordane-5

R.T.: 6.055 min
Delta R.T.: 0.000 min
Response: 15388218
Conc: 500.00 ng/ml

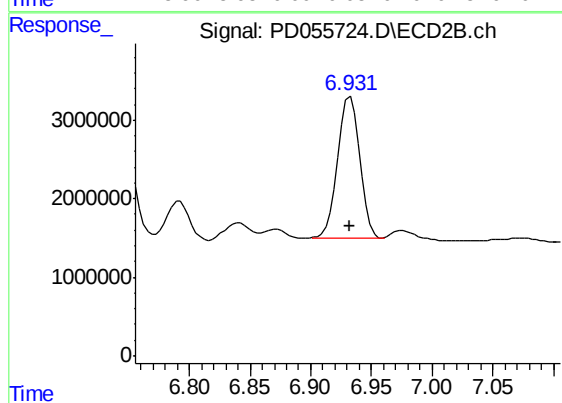

#27 Chlordane-5


R.T.: 6.933 min
Delta R.T.: 0.000 min
Response: 22979962
Conc: 500.00 ng/ml

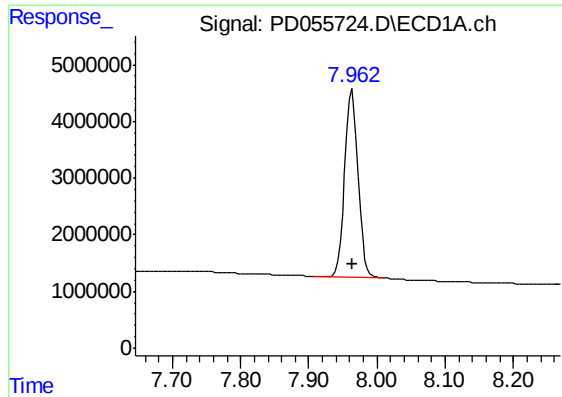

#28 Decachlorobiphenyl

R.T.: 7.964 min
Delta R.T.: 0.000 min
Response: 45434720
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

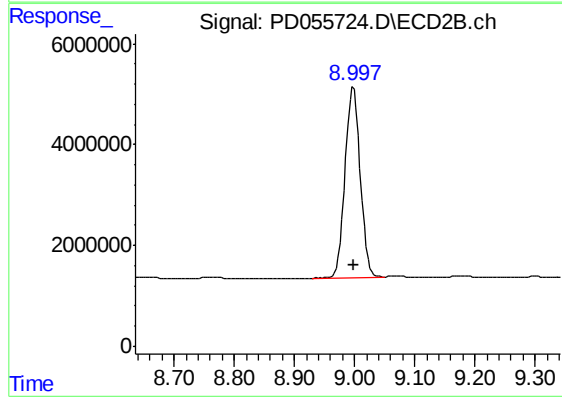

#28 Decachlorobiphenyl

R.T.: 8.998 min
Delta R.T.: 0.000 min
Response: 65807605
Conc: 50.00 ng/ml