

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110119\
 Data File : PD055726.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Oct 2019 00:06
 Operator : SG\AJ
 Sample : PCHLORICC050
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 06:35:37 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110119.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 31 06:31:17 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.289	3.963	5130940	6891492	5.716	5.963
28)	SA Decachlor...	7.963	8.999	5845541	8895835	6.433	6.759
Target Compounds							
25)	Chlordane-3	5.176	6.059	5066765	12256072	53.400	57.323
26)	Chlordane-4	5.232	6.133	4588092	14971520	55.208	58.831



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110119\
Data File : PD055726.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Oct 2019 00:06
Operator : SG\AJ
Sample : PCHLORICC050
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 06:35:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110119.M
Quant Title : GC Extractables
QLast Update : Thu Oct 31 06:31:17 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

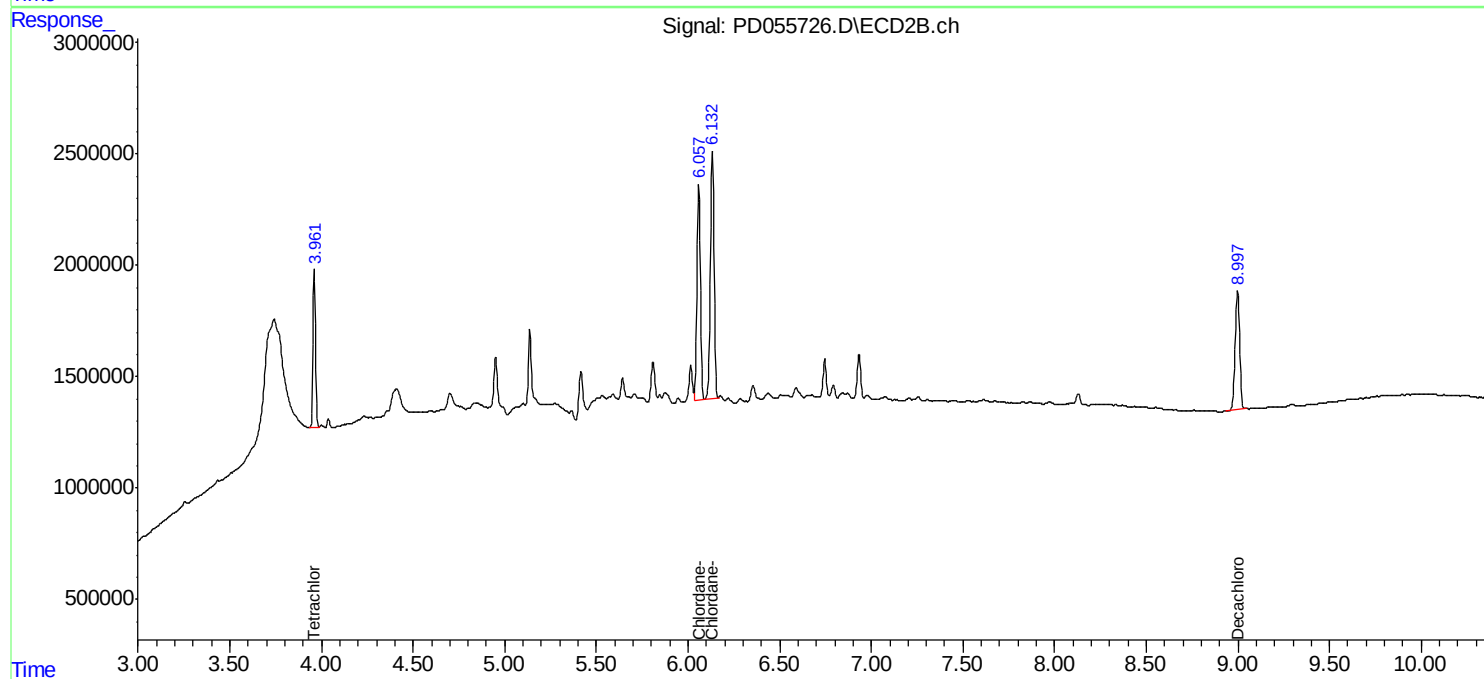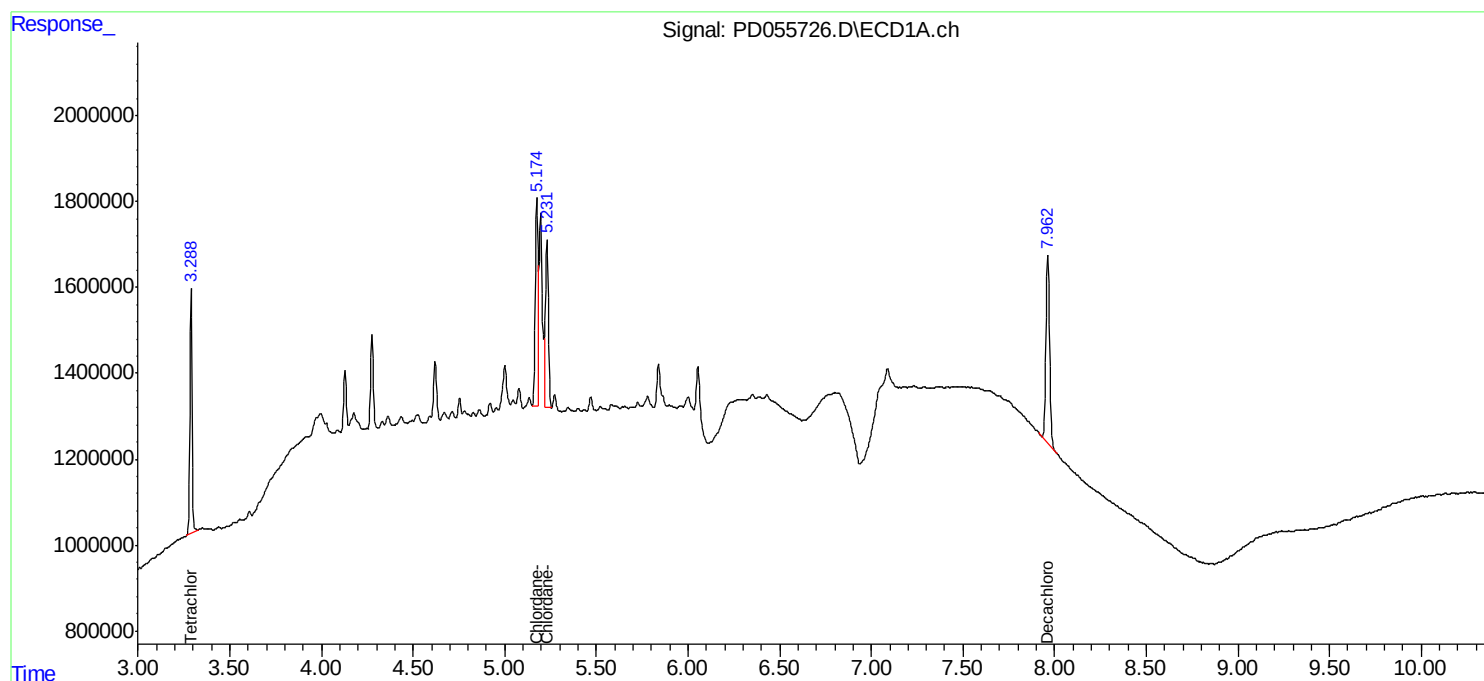


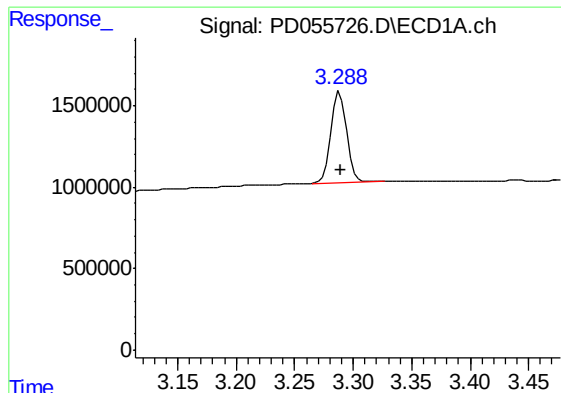

#1 Tetrachloro-m-xylene


R.T.: 3.289 min
Delta R.T.: 0.000 min
Response: 5130940
Conc: 5.72 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

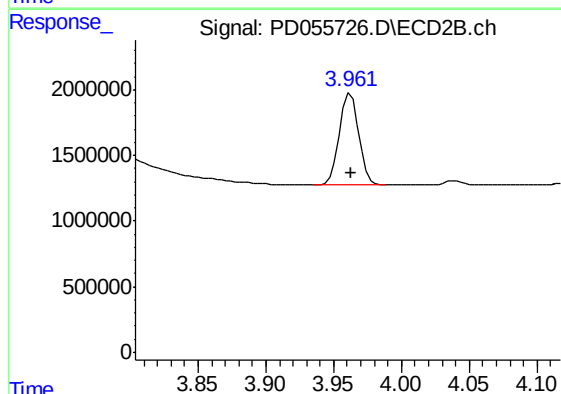


#1 Tetrachloro-m-xylene

R.T.: 3.963 min
Delta R.T.: 0.000 min
Response: 6891492
Conc: 5.96 ng/ml

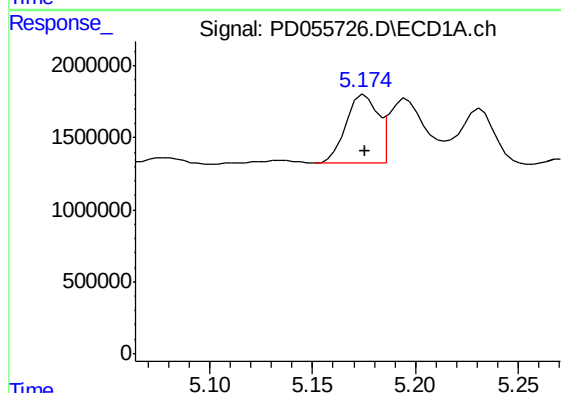


#25 Chlordane-3

R.T.: 5.176 min
Delta R.T.: 0.000 min
Response: 5066765
Conc: 53.40 ng/ml

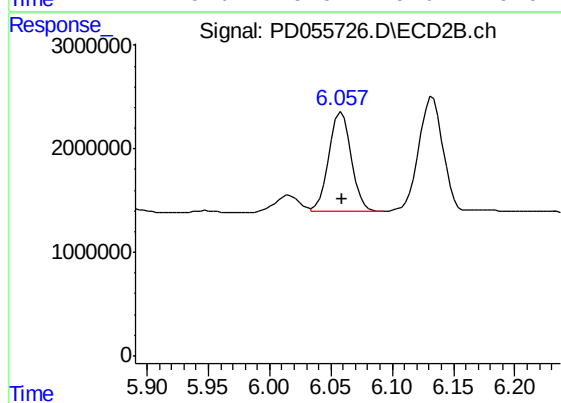

#25 Chlordane-3


R.T.: 6.059 min
Delta R.T.: 0.000 min
Response: 12256072
Conc: 57.32 ng/ml

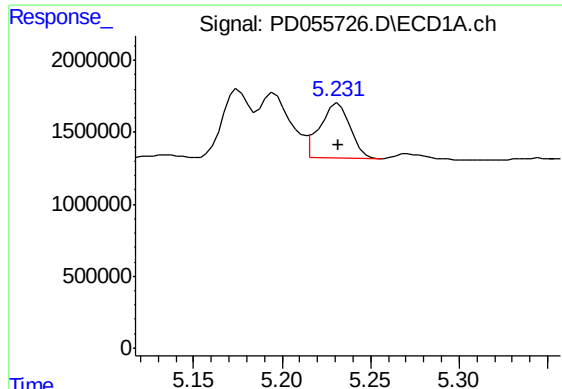

#26 Chlordane-4


R.T.: 5.232 min
Delta R.T.: 0.000 min
Response: 4588092
Conc: 55.21 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

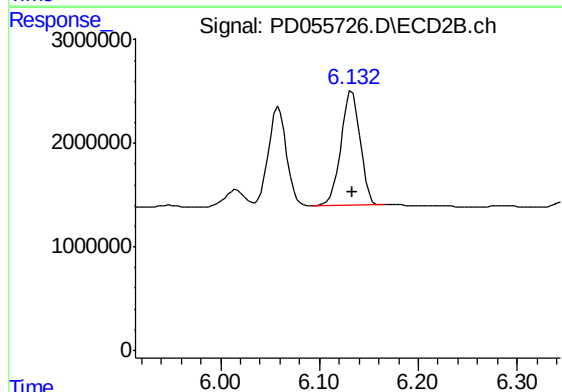


#26 Chlordane-4

R.T.: 6.133 min
Delta R.T.: 0.000 min
Response: 14971520
Conc: 58.83 ng/ml

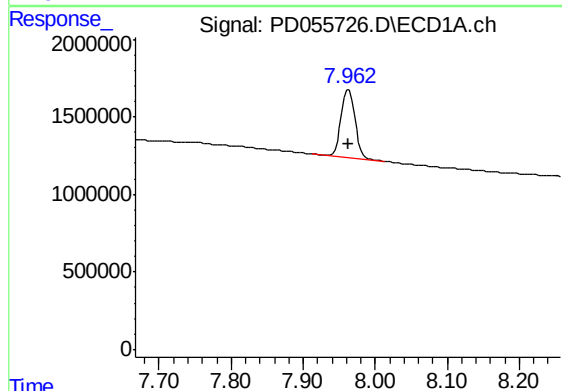

#28 Decachlorobiphenyl

R.T.: 7.963 min
Delta R.T.: 0.000 min
Response: 5845541
Conc: 6.43 ng/ml

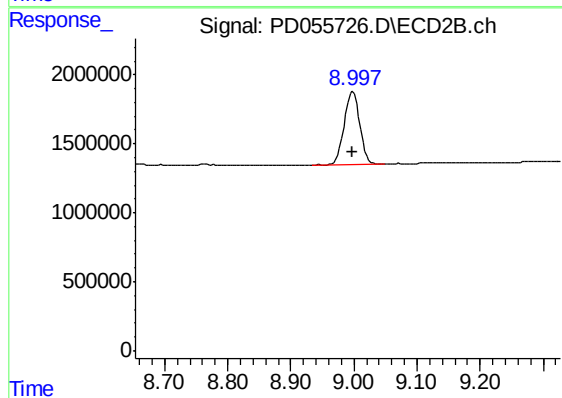

#28 Decachlorobiphenyl

R.T.: 8.999 min
Delta R.T.: 0.000 min
Response: 8895835
Conc: 6.76 ng/ml