

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110119\
 Data File : PD055757.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Oct 2019 13:32
 Operator : SG\AJ
 Sample : PB123927BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PB123927BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 04:03:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110119.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 31 06:48:28 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.290	3.963	22113960	31363947	25.940	26.043
28)	SA Decachlor...	7.966	8.998	23500656	34000189	24.841	24.433
Target Compounds							
11)	B alpha-Chl...	0.000	6.108f	0	5851616	N.D.	3.406 #
19)	B Endosulfa...	6.415	0.000	3833318	0	4.279	N.D. #
22)	Mirex	7.100	0.000	656375	0	0.796	N.D. #
26)	Chlordane-4	0.000	6.108f	0	5851616	N.D.	22.245 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110119\
Data File : PD055757.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Oct 2019 13:32
Operator : SG\AJ
Sample : PB123927BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleID :
PB123927BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 04:03:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110119.M
Quant Title : GC Extractables
QLast Update : Thu Oct 31 06:48:28 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

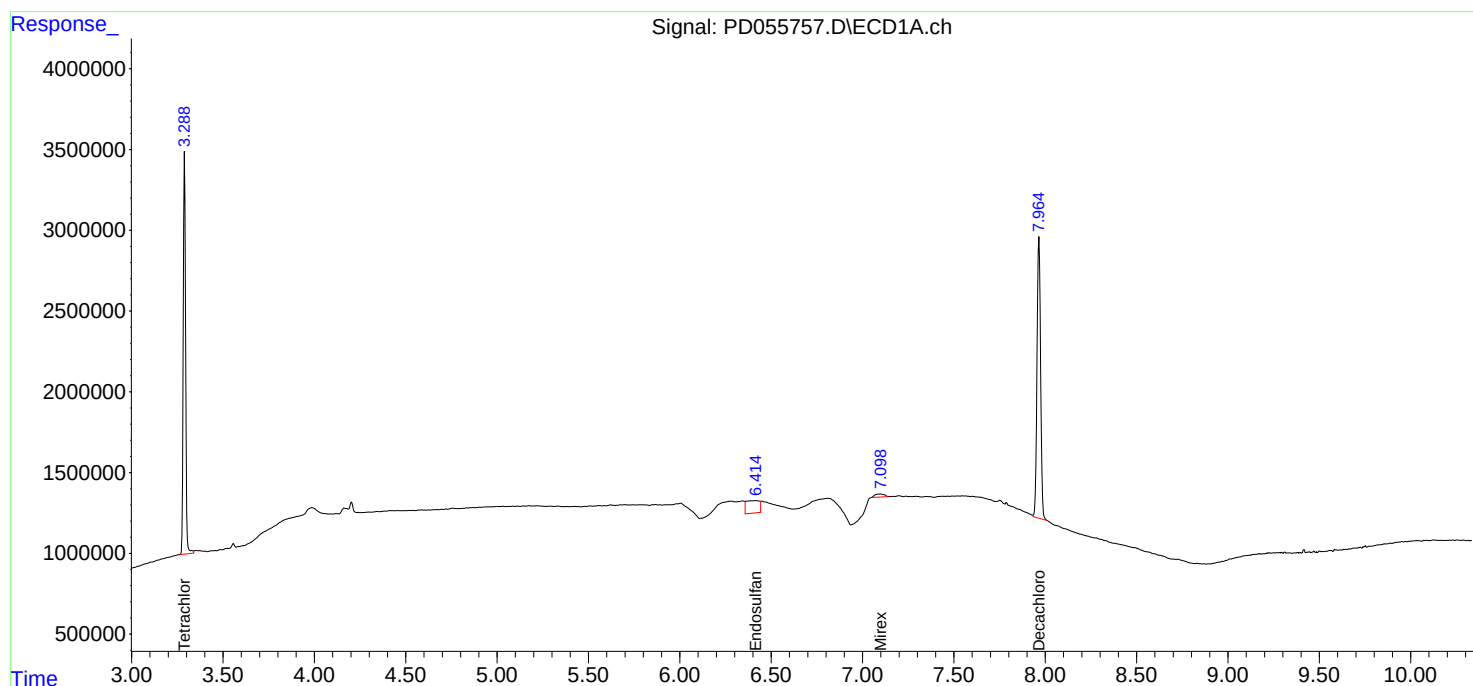


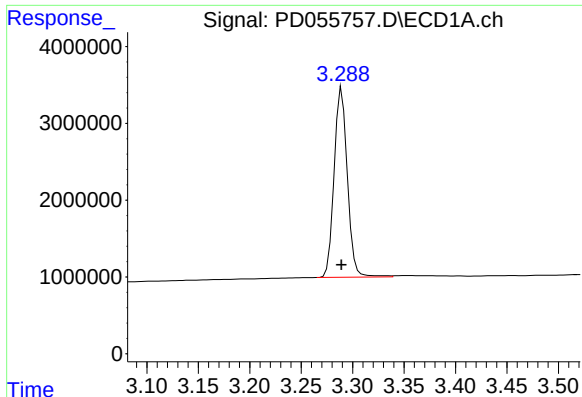

#1 Tetrachloro-m-xylene


R.T.: 3.290 min
Delta R.T.: 0.000 min
Response: 22113960
Conc: 25.94 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB123927BL

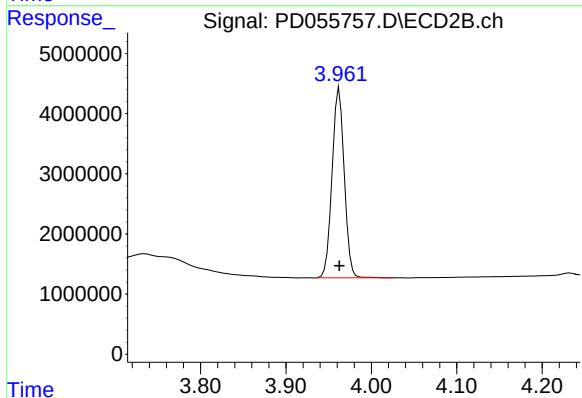


#1 Tetrachloro-m-xylene

R.T.: 3.963 min
Delta R.T.: 0.000 min
Response: 31363947
Conc: 26.04 ng/ml

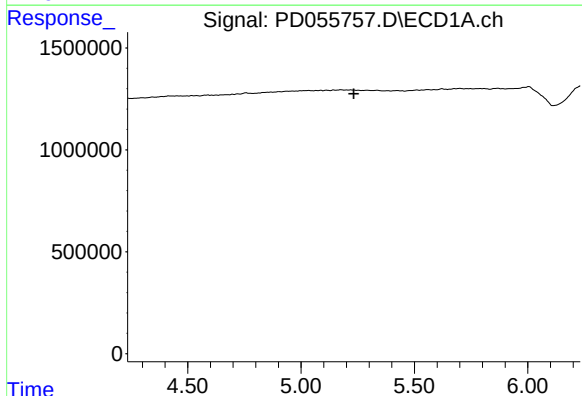


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.232 min
Response: 0
Conc: N.D.

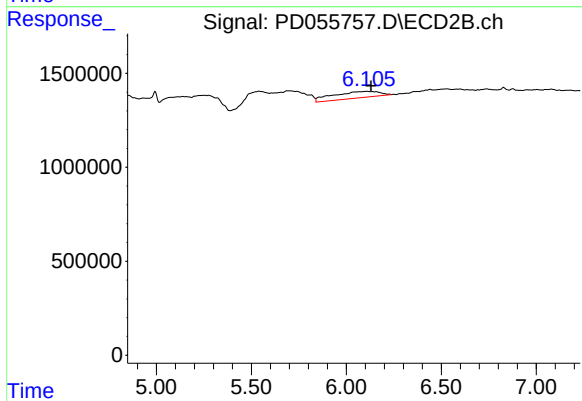

#11 alpha-Chlordane

R.T.: 6.108 min
Delta R.T.: -0.022 min
Response: 5851616
Conc: 3.41 ng/ml

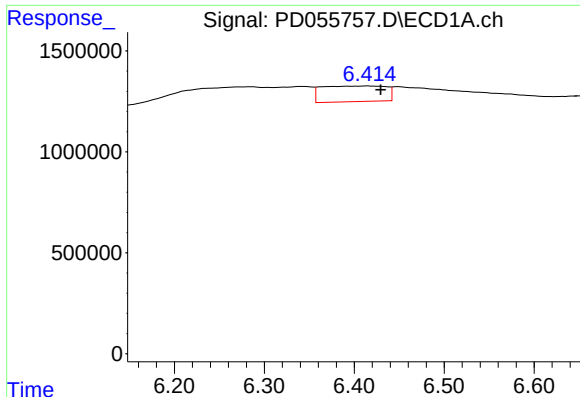

#19 Endosulfan Sulfate


R.T.: 6.415 min

Delta R.T.: -0.014 min

Response: 3833318

Conc: 4.28 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB123927BL

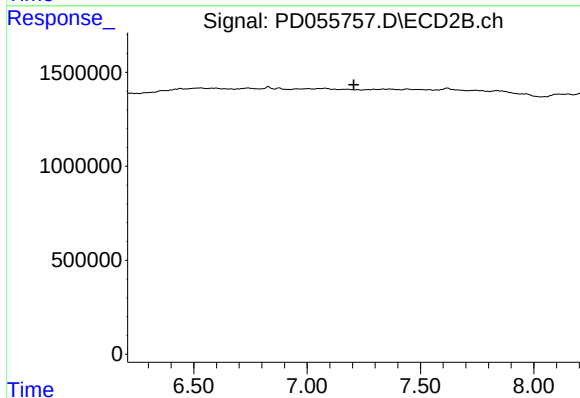


#19 Endosulfan Sulfate

R.T.: 0.000 min

Exp R.T. : 7.207 min

Response: 0

Conc: N.D.

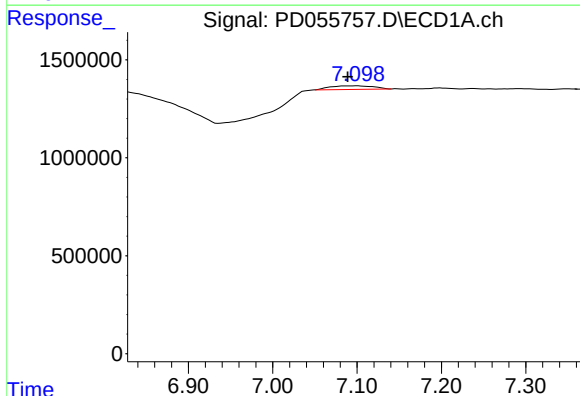


#22 Mirex

R.T.: 7.100 min

Delta R.T.: 0.011 min

Response: 656375

Conc: 0.80 ng/ml

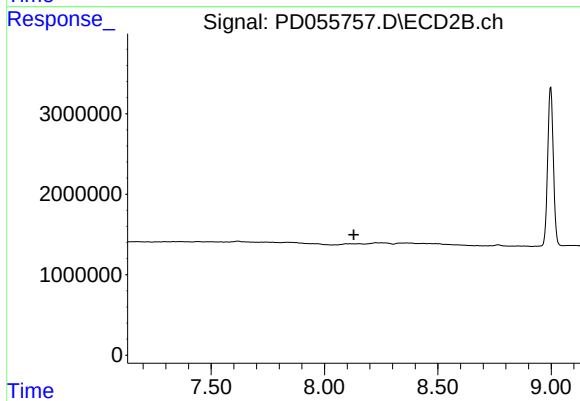


#22 Mirex

R.T.: 0.000 min

Exp R.T. : 8.130 min

Response: 0


Conc: N.D.

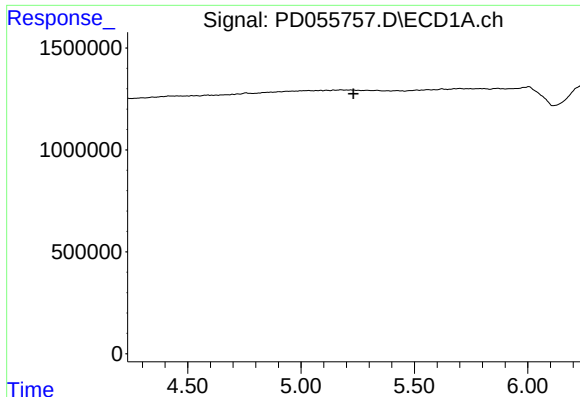

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.232 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PB123927BL

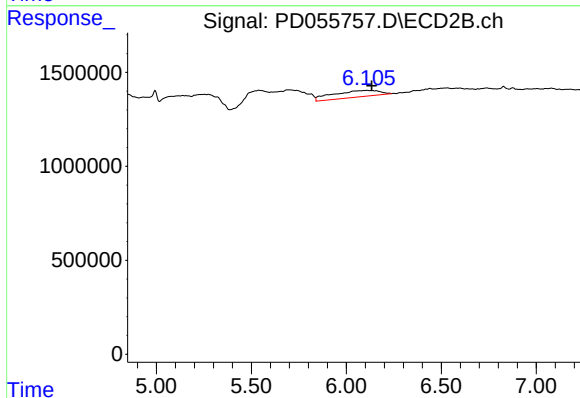


#26 Chlordane-4

R.T.: 6.108 min
Delta R.T.: -0.025 min
Response: 5851616
Conc: 22.25 ng/ml

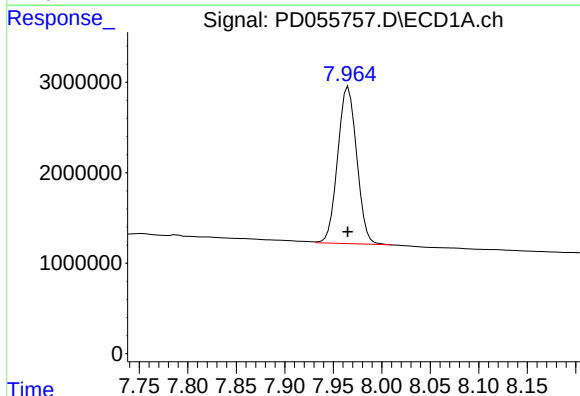

#28 Decachlorobiphenyl

R.T.: 7.966 min
Delta R.T.: 0.000 min
Response: 23500656
Conc: 24.84 ng/ml

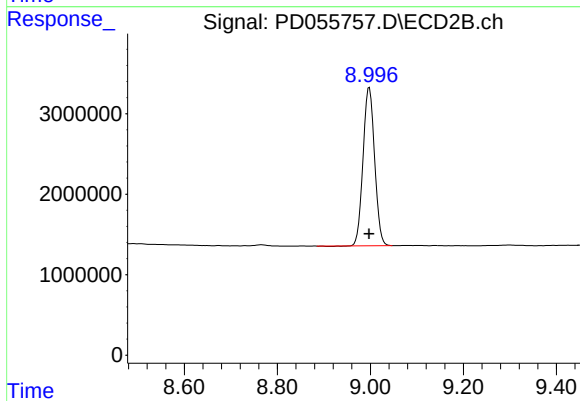

#28 Decachlorobiphenyl

R.T.: 8.998 min
Delta R.T.: 0.000 min
Response: 34000189
Conc: 24.43 ng/ml