

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110119\
 Data File : PD055714.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Oct 2019 21:18
 Operator : SG\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 I.BLK

Manual Integrations
 APPROVED

Ankita
 11/1/2019 12:19:10 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 07:18:27 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110119.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 31 06:48:28 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.289	3.963	21773936	30166239	25.541	25.048
28)	SA Decachlor...	7.963	8.996	23702078	34916579	25.054	25.091m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110119\
Data File : PD055714.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2019 21:18
Operator : SG\AJ
Sample : I.BLK
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Ankita
11/1/2019 12:19:10 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 07:18:27 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110119.M
Quant Title : GC Extractables
QLast Update : Thu Oct 31 06:48:28 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

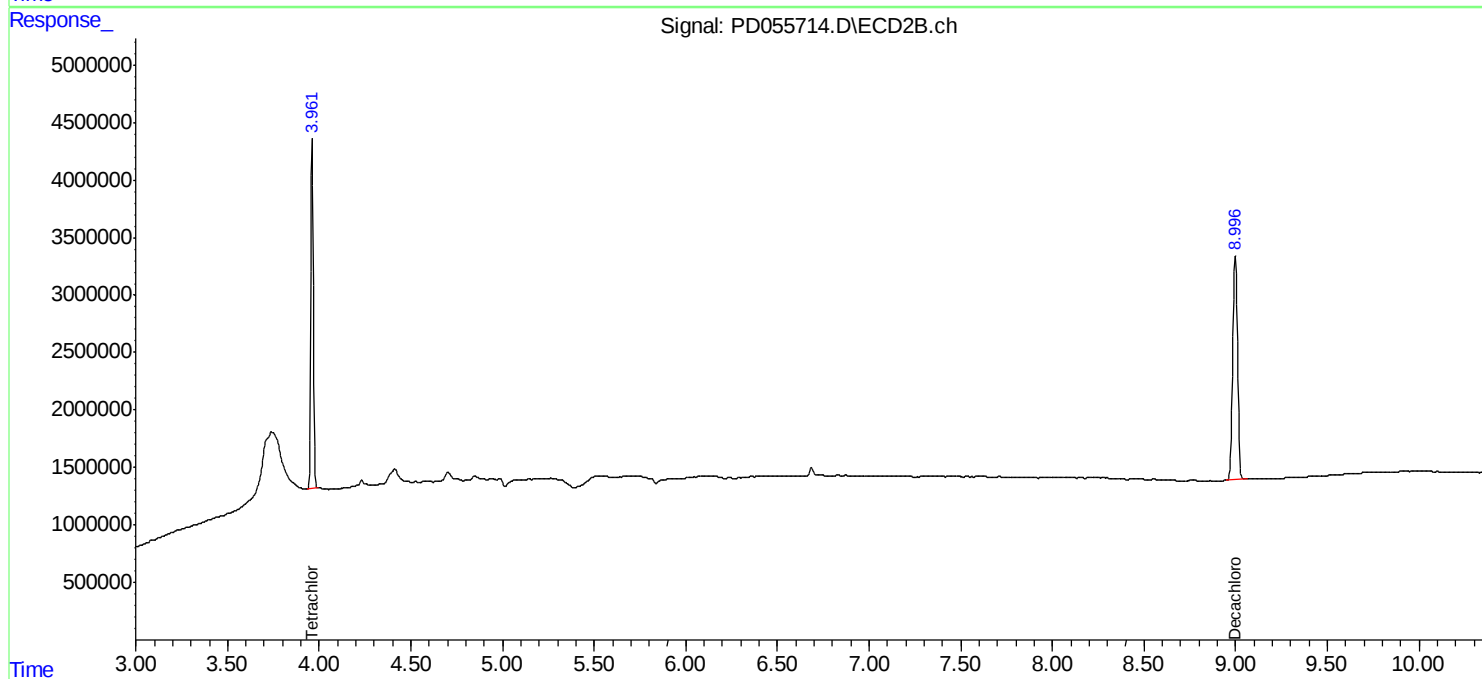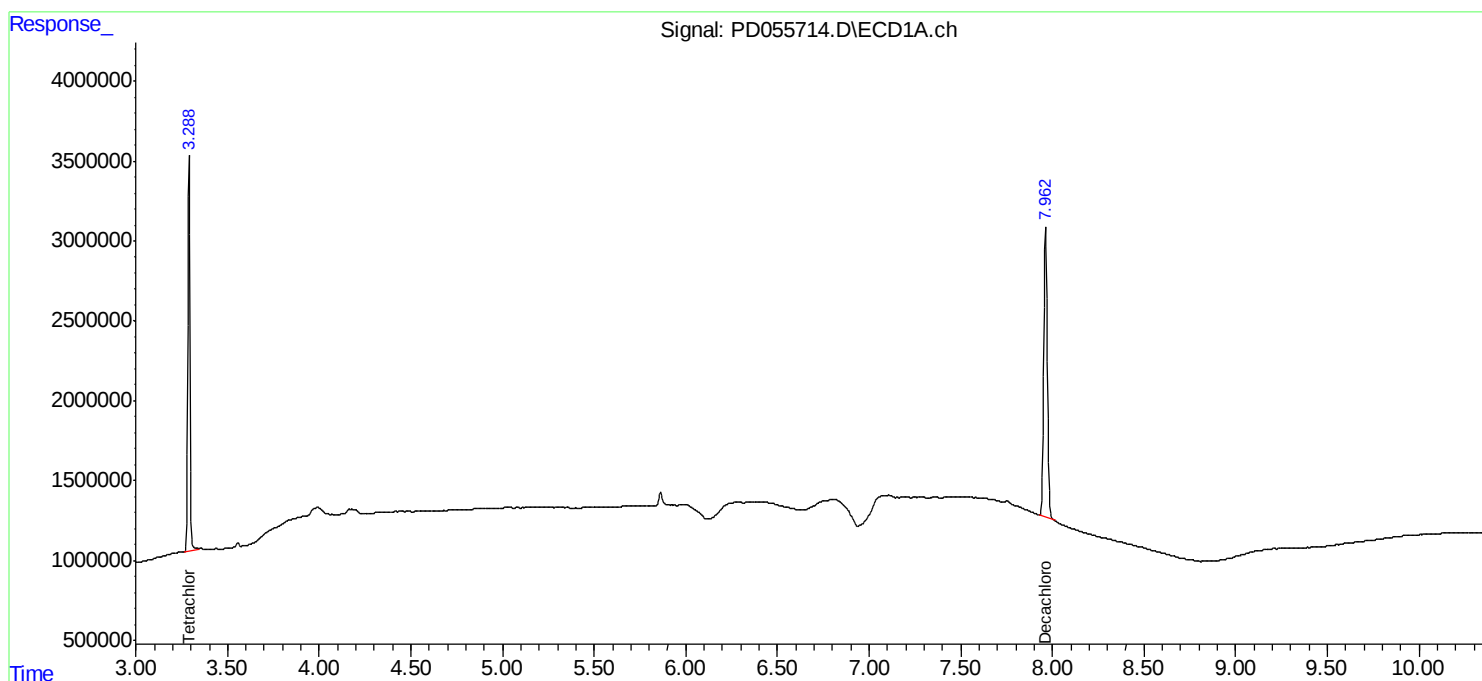

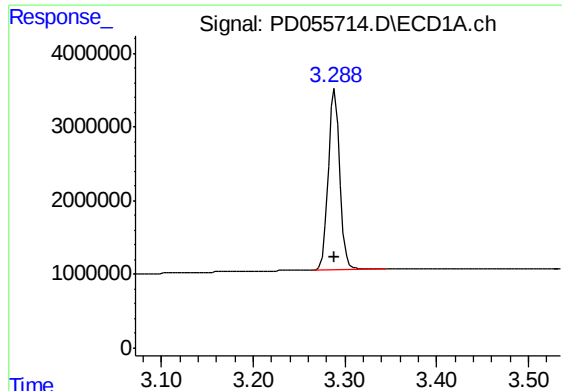


#1 Tetrachloro-m-xylene

R.T.: 3.289 min
Delta R.T.: 0.000 min
Response: 21773936
Conc: 25.54 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Ankita
11/1/2019 12:19:10 PM

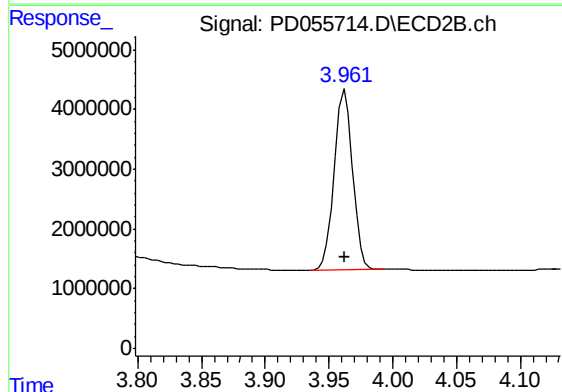


#1 Tetrachloro-m-xylene

R.T.: 3.963 min
Delta R.T.: 0.000 min
Response: 30166239
Conc: 25.05 ng/ml

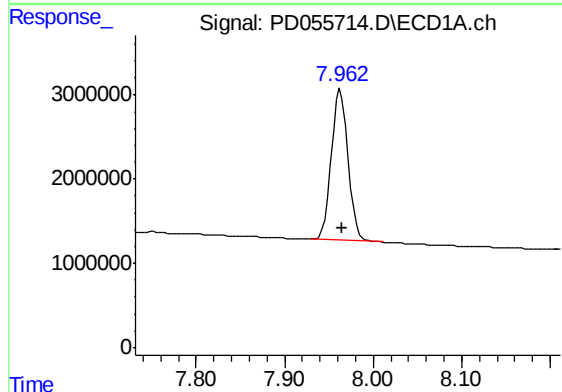

#28 Decachlorobiphenyl

R.T.: 7.963 min
Delta R.T.: -0.002 min
Response: 23702078
Conc: 25.05 ng/ml

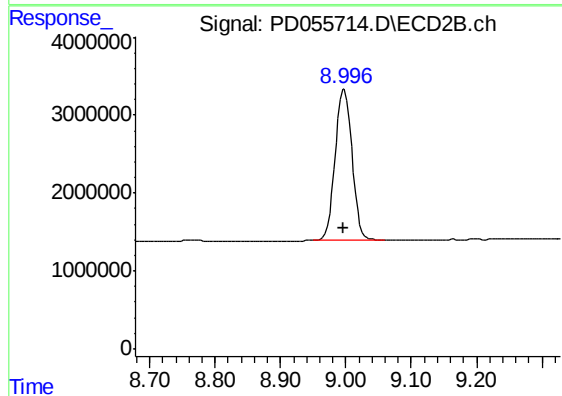

#28 Decachlorobiphenyl

R.T.: 8.996 min
Delta R.T.: 0.000 min
Response: 34916579
Conc: 25.09 ng/ml m