

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110119\
 Data File : PD055722.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Oct 2019 23:10
 Operator : SG\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 06:34:52 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110119.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 31 06:31:17 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.289	3.962	92245034	116.1E6	102.764	100.470
28)	SA Decachlor...	7.964	8.997	87504674	123.8E6	96.297	94.044
Target Compounds							
23)	Chlordane-1	4.130	4.950	26663977	45501010	1007.901	1005.784
24)	Chlordane-2	4.619	5.415	31047985	46927460	1015.040m	940.853
25)	Chlordane-3	5.176	6.058	97918356	218.2E6	1031.984	1020.547
26)	Chlordane-4	5.232	6.133	83678020	259.7E6	1006.881	1020.694
27)	Chlordane-5	6.055	6.933	30791499	46555553	1000.489	1012.960



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110119\
Data File : PD055722.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2019 23:10
Operator : SG\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 06:34:52 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110119.M
Quant Title : GC Extractables
QLast Update : Thu Oct 31 06:31:17 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

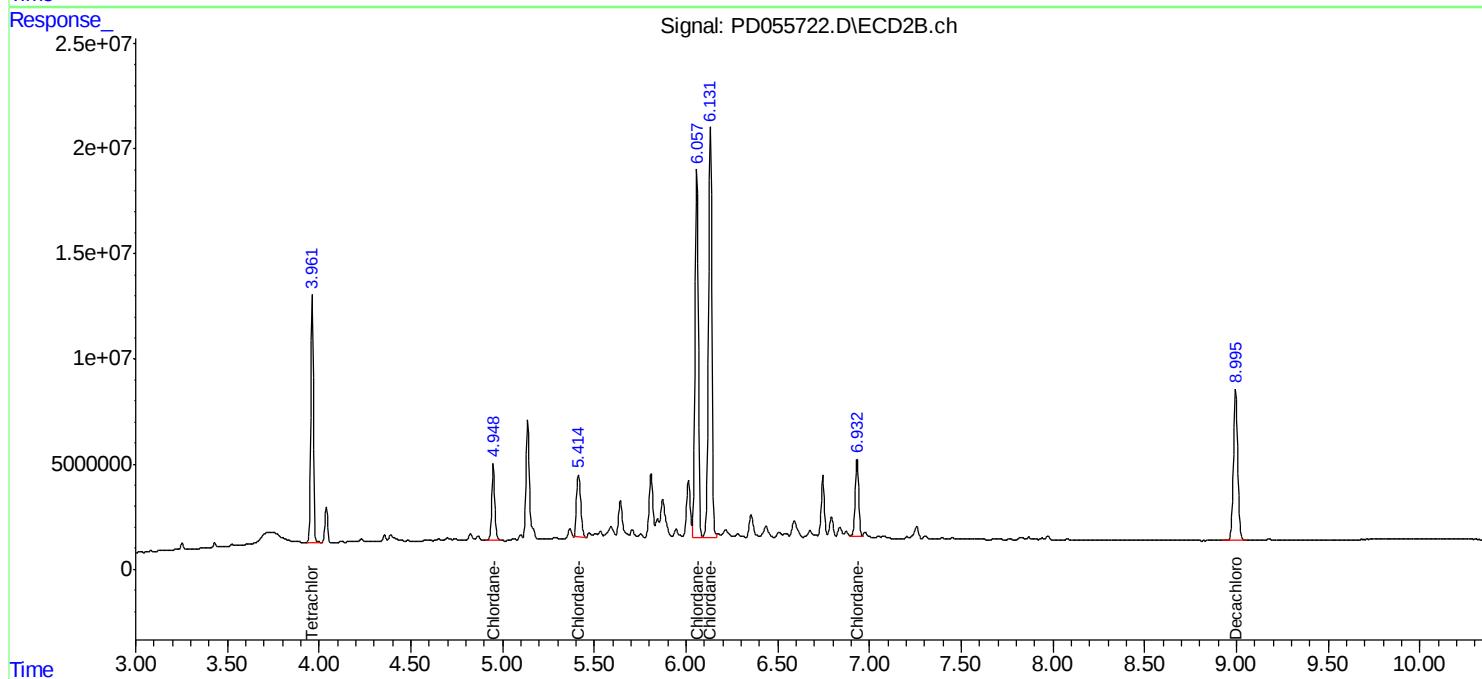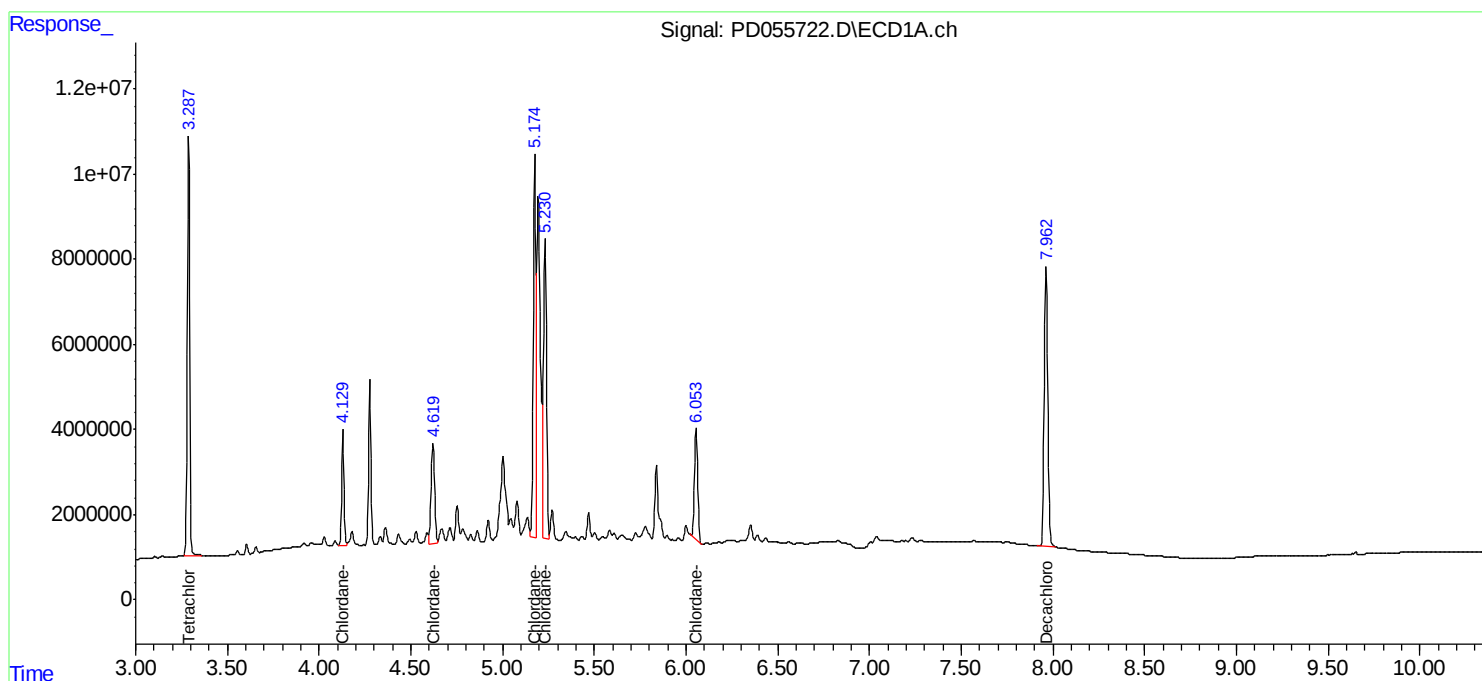


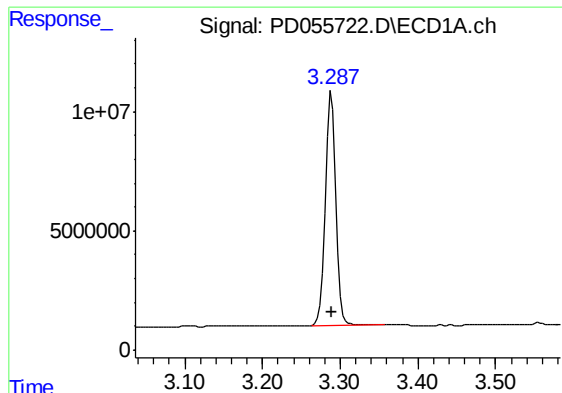

#1 Tetrachloro-m-xylene


R.T.: 3.289 min
Delta R.T.: 0.000 min
Response: 92245034
Conc: 102.76 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

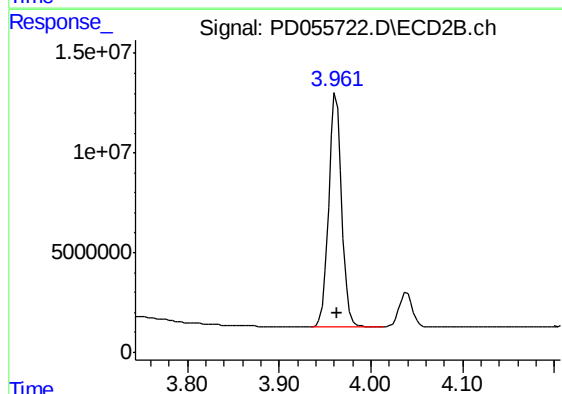


#1 Tetrachloro-m-xylene

R.T.: 3.962 min
Delta R.T.: 0.000 min
Response: 116108221
Conc: 100.47 ng/ml

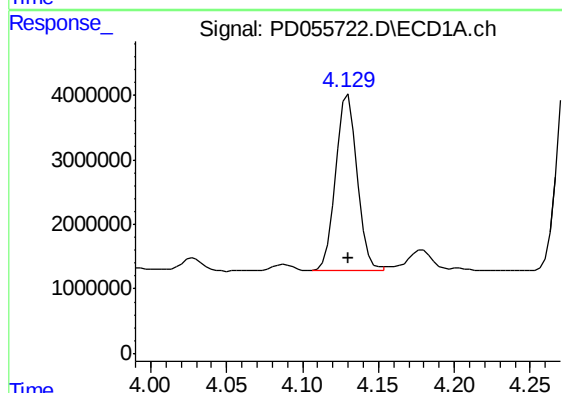


#23 Chlordane-1

R.T.: 4.130 min
Delta R.T.: 0.000 min
Response: 26663977
Conc: 1007.90 ng/ml

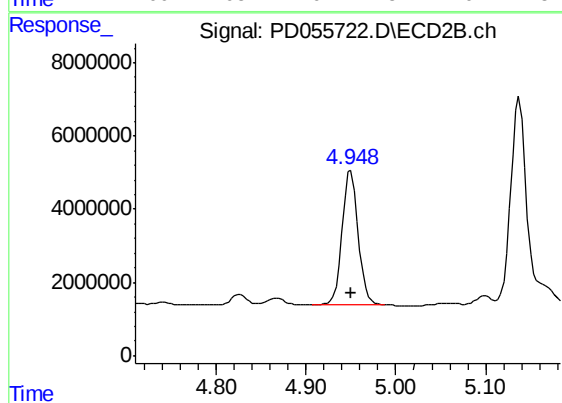

#23 Chlordane-1


R.T.: 4.950 min
Delta R.T.: 0.000 min
Response: 45501010
Conc: 1005.78 ng/ml

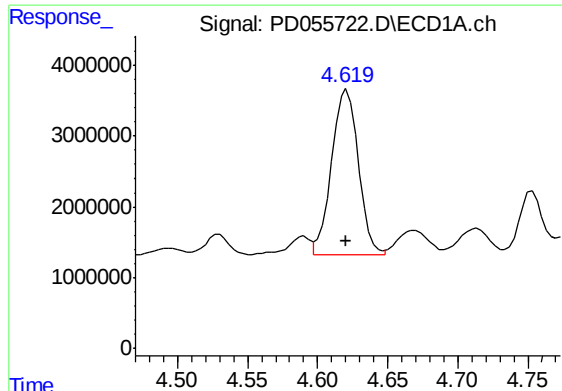

#24 Chlordane-2


R.T.: 4.619 min
Delta R.T.: -0.001 min
Response: 31047985
Conc: 1015.04 ng/ml m

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

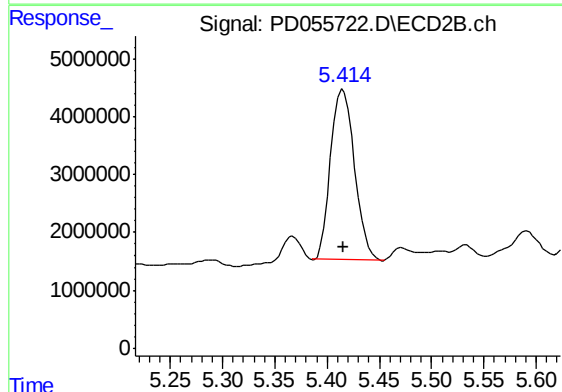


#24 Chlordane-2

R.T.: 5.415 min
Delta R.T.: 0.000 min
Response: 46927460
Conc: 940.85 ng/ml

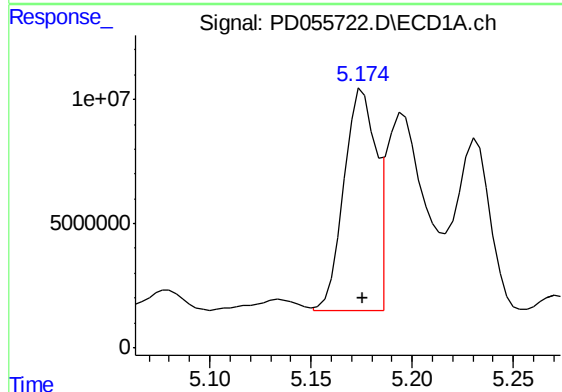


#25 Chlordane-3

R.T.: 5.176 min
Delta R.T.: 0.000 min
Response: 97918356
Conc: 1031.98 ng/ml

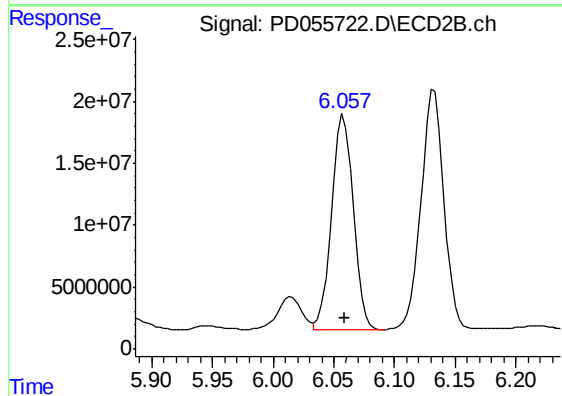

#25 Chlordane-3


R.T.: 6.058 min
Delta R.T.: 0.000 min
Response: 218198603
Conc: 1020.55 ng/ml

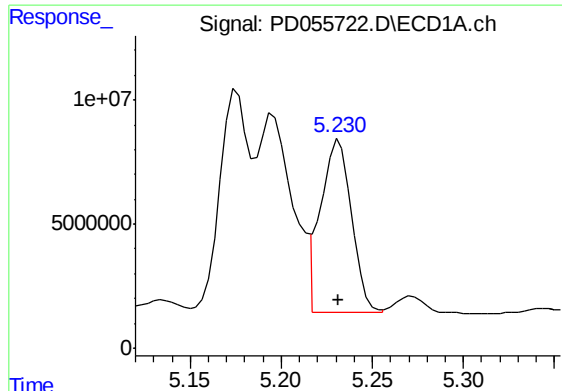

#26 Chlordane-4


R.T.: 5.232 min
Delta R.T.: 0.000 min
Response: 83678020
Conc: 1006.88 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

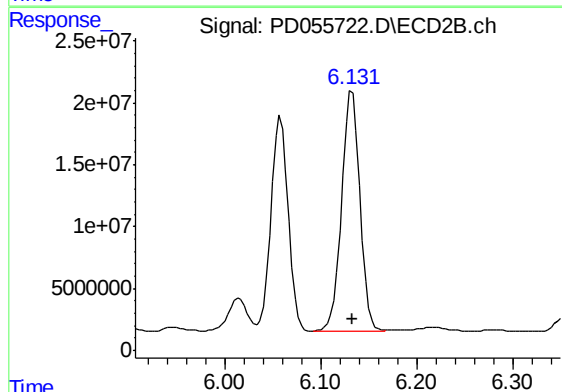


#26 Chlordane-4

R.T.: 6.133 min
Delta R.T.: 0.000 min
Response: 259749656
Conc: 1020.69 ng/ml

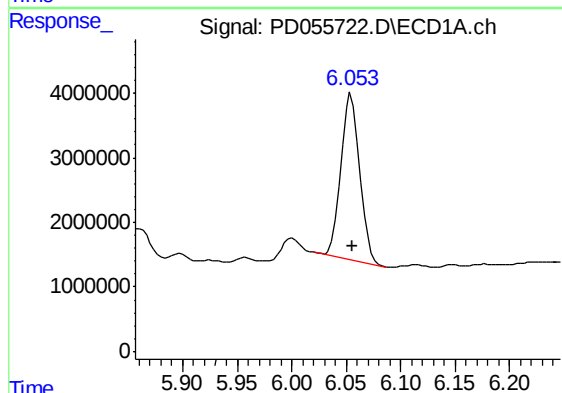


#27 Chlordane-5

R.T.: 6.055 min
Delta R.T.: 0.000 min
Response: 30791499
Conc: 1000.49 ng/ml

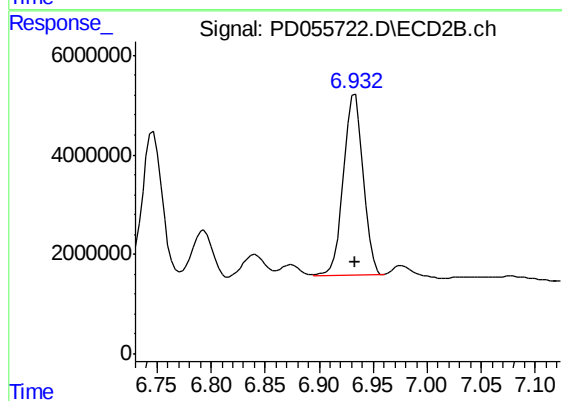

#27 Chlordane-5


R.T.: 6.933 min
Delta R.T.: 0.000 min
Response: 46555553
Conc: 1012.96 ng/ml

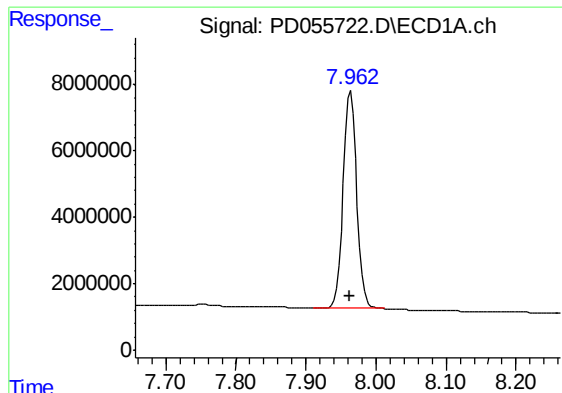

#28 Decachlorobiphenyl

R.T.: 7.964 min
Delta R.T.: 0.000 min
Response: 87504674
Conc: 96.30 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

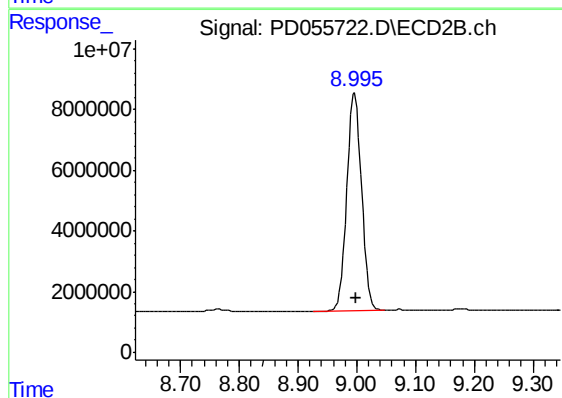

#28 Decachlorobiphenyl

R.T.: 8.997 min
Delta R.T.: -0.001 min
Response: 123775899
Conc: 94.04 ng/ml